
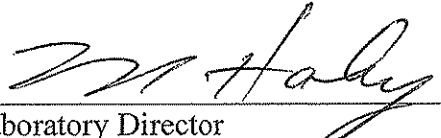



FACILITY SOP ATTACHMENT

SOP NUMBER: IR-QAM, 01/31/2009		CHANGE FORM ID: CF1
SOP TITLE: Quality Assurance Manual		
REASON FOR ADDITION OR CHANGE (Use additional sheets if necessary): Updates and additions		
CHANGE OR ADDITION (Use additional sheets if necessary): The following changes have been made:		
Section	Description	Type of Change
Title Page	Title Page	Revised signatories
Table of Contents	SOP and Policy Reference	Revised list to reflect new SOP file names
4.2.9	LIMS Administrator	LIMS administered by corporate
Figure 4-1	Corp Org Chart	Update
5.3	QA Support Documents	Addition of QAS
Table 16-1	Audit Types	Revised 2009 types and frequency
16.2.1.1	Technical Audits	Replaced method/instrument/analyst with technical by method
Figure 17-1	Monthly QA Report	Update
Figure 17-2	QA Metrics	Update
20.7.10	MDL MLD Frequency <i>do 11/16/09</i>	Annual verification
Table 20-1	SOP List	Update
Table 21-1	Laboratory Equipment List	Update
24.2.3	Project Receipt Checklist	Addition
Figure 24-5	Sample Acceptance Policy	Update
Figure 24-6	Project Receipt Checklist	Formerly "cooler receipt form"
Appendix 2	Irvine Org Chart	Update
Prepared By: D. Dawes		
*APPROVED BY:		
		Date <i>11/16/09</i>
Quality Assurance Manager		
		Date <i>11/16/09</i>
Laboratory Director		

**UNCONTROLLED
DOCUMENT**

Title Page:


**Quality Assurance Manual
Approval Signatures**

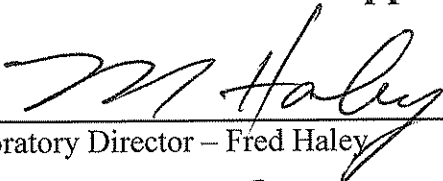

Laboratory Director – Fred Haley

11/16/09

Date



Operations Manager – Trevor Brenner

11/16/09


Date



Client Services Manager – Kathleen Robb

11/16/09

Date



Quality Manager – David Dawes

11/16/09

Date



Sample Control Manager – Maria Escalante

11/16/09

Date



Technical Director, **Semivolatiles** – Gerardo Muñoz

11/16/09

Date



Technical Director, **Volatiles** – Valerie Sierzchula

11/16/09


Date



Technical Director, **Metals** – Frank Rocha

11/16/09

Date



Technical Director, **Wet Chemistry** – Tung Nguyen

11/16/09


Date



Technical Director, **Organic Prep** – Logan Alvis

11-16-09

Date



Technical Director, **Microbiology** – Priyuni Patel

11-16-09

Date

SOPs AND POLICIES REFERENCED IN THE QA MANUAL

Corporate Documents

SOP/Policy Reference	Title
CA-Q-S-001	Solvent and Acid Lot Testing and Approval
CA-Q-S-002	Acceptable Manual Integration Practices
CA-Q-S-003	Management of Change Procedure
CA-Q-S-004	Method Compliance & Data Authenticity Audits
CA-Q-S-006	Detection Limits
CA-Q-S-005	Calibration Curves (General)
CW-Q-S-001	Corporate Document Control and Archiving
CW-Q-S-002	Writing a Standard Operating Procedure (SOPs)
CA-L-S-001	Internal Investigation of Potential Data Discrepancies and Determination for Data Recall
CA-L-S-002	Subcontracting Procedures
CA-L-P-001	Ethics Policy
CA-L-P-002	Contract Compliance Policy
CW-L-P-001	Record Retention
CW-F-P-002	Authorization Matrix
CA-C-S-001	Work Sharing Process
CA-T-P-001	Qualified Products List
CW-F-S-004	Controlled Purchases Policy

Local Laboratory Documents

SOP/Policy Reference	Title
IR-QA-DOC	Document Control and Review
CNTRLLIM.SOP	Control Charts and Statistical Process Control
IR-QA-LOTTEST	Container and Reagent Verification by Lot Testing
IR-QA-CAR	Corrective Actions
IR-QA-TRAINING	Training and Documentation
IR-SC-LOGIN	Sample Control
IR-QA-DATAREV	General Data Review
IR-PM-DATA	Project Management Data Reporting, Validation and Distribution
IR-QA-BAL	Balance Calibration, Verification and Documentation
IR-QA-THERMA	Thermometer Calibration/Temperature Monitoring and Documentation
IR-QA-STDCNTRL	Reagent and Standard Preparation, Control, and Documentation
IR-SC-FIELD	Field Sampling
IR-QA-SUBSAMP	Subsampling
IR-QA-REFBLANK	Refrigerator Storage Blank
IR-IT-COMPSECU	Computer Security
IR-QA-PIPET	Pipet Calibration
IR-QA-ARCHIVE	Record Archiving
IR-QA-MDL	Determination of Method Detection Limits
IR-QA-WATER	Laboratory Water Quality
IR-QA-LOGBOOK	Logbooks, Documentation, and Laboratory Communication

SOP/Policy Reference	Title
IR-QA-QAPP_REV	Review and Communication of Client QAPP Requirements

4.2.9 LIMS Administrator

LIMS administration is conducted at the corporate level. Requests for repairs and service are addressed using the Intranet (OASIS) HelpDesk request form.

Figure 4-1 Corporate Organizational Chart
(Attached)

5.3 QUALITY SYSTEM SUPPORTING DOCUMENTATION

- Quality Assurance Summary (QAS) – A concise summary of all client/QAPP specified requirements that affect laboratory operations

Table 16-1. Audit Types and Frequency

Internal Audits	Description	Performed by	Frequency
	Technical Data Audits	QA Department or Designee	- 100% of all methods over a two year period.
	Instrument	QA Department or Designee	100% of all organic instruments and any inorganic chromatography instruments over a two year period
	Department/ Systems	QA Department or Designee	- Annual for entire labs support departments & equipment (e.g., thermometers, balances), can be divided into sub-sections over the course of the year.
	Performance Audits (Double-Blind PTs)	Corporate QA, Laboratory QA Department or Designee	- As needed.
	Special	QA Department or Designee	- As Needed
External Audits	Description	Performed by	Frequency
	Program / Method Compliance	Regulatory Agencies, Clients, accreditation organizations	- As required by program and/or clients needs
	Performance Audits	Provided by a third party.	- As required by a client or regulatory agency. Generally provided semi-annually through the analysis of PT samples.

16.2.1.1 Technical Data Audits

This consists of authenticity audits performed on reports and raw data. Tracking of this metric will be based on methods however, analyst, instrument, mint miner and raw data reviews will be included in these evaluations. It is expected that 50% of the laboratory methods be audited during the year. An audit schedule is documented using the 'Technical Data-Method Audit' tab in the Monthly QA Metrics Report.

Figure 17-1 Example QA Monthly Report

<p><i>Name of preparer (QAM)</i> <i>Date report submitted to corporate</i> <i>GM, LD, additional staff as warranted</i></p>
<p><u>THREE KEY ISSUES FOR MONTH:</u> <i>Include a discussion of three key issues that were focused on this month.</i></p>
<p><u>METRICS CONCERNS</u> <i>For any quality metrics that fall in 'red' or yellow', describe actions or improvement activities underway.</i></p> <p>Revised reports Data Recall Audits Performance Testing Corrective Action</p> <p>SOPs</p>

HTVs

CORRECTIVE ACTIONS

Highlights: *Provide discussion of any major investigations or closures.*

Total NCRs:

'True CARs/PT CARs/Follow-ups/Internal Audits (Not closed):

CARs past due:

EE Oversight NCRs:

Missed HT NCRs:

Revised report CARs:

Revised Reports: *Describe the most frequent cause for report revisions and corrective/preventive action measures underway.*

Data Investigations/Recalls: *Provide a short summary or update of any events handled at the lab level as per Section 6.2.2 in the Investigation/Recall SOP. Include detailed explanation on the 'Data Recall' tab.*

Client Complaints: *Describe the most serious client complaints and associated corrective actions in progress. Include client company names.*

Client Compliments: *Describe any compliments received - include client company names.*

AUDITS

Total Findings:

Past due:

2008:

Internal Audits (QA Technical, Departmental Quality Systems and Lab Requested Investigations): *Discuss any outstanding issues or concerns (may attach summary).*

External Audits: *Discuss any outstanding issues or concerns (may attach summary). Include schedule for upcoming audits.*

PROFICIENCY TESTING STUDIES

PT Corrective Actions: *Include discussion of any outstanding issues.*

SOPs

SOPs: *Provide a discussion of any concerns. If SOPs are greater than 6 months overdue, provide a corrective action plan. Include an SOP Tracking Tab in your monthly report.*

SOPs added:

SOPs removed:

SOPs revised:

Change forms written:

Past due SOPs with QA:

Past due SOPs with LAB:

SOPs have not been developed for the following methods or processes (include list).

MDLs , TRAINING DOCUMENTATION AND CONTROL LIMITS

MDLs Due (or attach summary): *Include discussion of any concerns*

Control Limits Due (or attach summary): *Include discussion of any concerns*

Training Documentation: *Describe any concerns or system failures*

HOLD TIME VIOLATIONS

Describe major HT violation events and associated corrective actions in progress.

CERTIFICATIONS

Describe any issues, lapses or potential revocations:

Certification Packages Being Worked On (Include Due Date):

REGULATORY UPDATE

Include information on new state or federal regulations that may impact the laboratory – new methods that require new instrumentation, deletion of methods, changes in sampling requirements or frequencies, ...

MISCELLANEOUS

Include any issues that may impact quality within the laboratory.

Element Status Report

MDL synchronization:

Standards not reviewed:

Number of testcodes created/reviewed:

TRAINING or MEETINGS

Include information on participation in any industry or regulatory meetings or any training sessions being scheduled.

NEXT MONTH (Items planned for next month)

<p>LAB DIRECTOR COMMENTS AND PLANNED CORRECTIVE ACTIONS:</p> <p>Date:</p> <p>Comments:</p> <p>Signature (Name):</p>
--

Figure 17-2 Laboratory Metrics, Frequency and Evaluation Criteria

Category	Objective	Period	Metrics
Revised Reports		This month	# Reports for month
		This month	# Reports revised due to lab error
	<3%	This month	% Reports Revised due to lab error (1.0)
	Indicator	This month	# Reports Reviewed by QA
Data Recall	<1	Jan-to-date	# Data Recall Investigations Past Due (1.0) (check data recall tab)
	Indicator	Jan09-date	Cumulative # Days Data Recalls Open
Client	>3	This month	# Client Complaints (1.0)
	>3	This month	# Client Compliments
QA Technical Data Audits		Current	# of Technical Method Data Audits Planned
		Jan09 to Dec09	# of Technical Method Data Audits performed Jan09-Dec09
	4.55% per month	Jan09 to Dec09	% of Technical Method Data Audits Performed (2.0)
Audits		Currently	# of Planned Department Quality Systems Audits (cumulative)
		Jan-to-date	# of Planned Department Quality Systems Audits Complete
	activity per quarter	Jan-to-date	% Annual Internal Systems Audit Complete (1.0)
Audits - Corrective Actions		Jan-to-date	Total Number of Audit Findings (Int. & Ext.) (include summary tabs)
		Current	# Audit Findings Past Due (internal & external)
	Indicator	Opened in 2008	2008 Open Audit Findings
Proficiency Testing		Jan-to-date	# of PT analytes participated and received scores
		Jan-to-date	# of PT analytes not acceptable
	>97%	Jan - to date	% PT Cumulative Score (2.0)
	<6	Jan-to-date	# PT Repeat Analyte Failures Cumulative (1.0) (analyte failed more than once in 4 consecutive studies by PT Type)
Corrective Action		Jan-to-date	Total # Corrective Action Items (audits, PTs, lab invest)
		Current	# Corrective Action Items Past Due
	<15%	Current	% Corrective Action Items Past Due (1.0)
SOPs / Method Compliance		Current	# SOPs
		Current	# SOP with Procedure Compliance Review/Revision Past Due
		Current	# Methods or Administrative procedures without approved SOPs

Category	Objective	Period	Metric
	100%	Current	% SOP Complete (1.0)
Ethics Training		Current	Date of Last Comprehensive Ethics Training Session
	0	Current	# Staff >90 Days from Hire Date AND have not received Comprehensive Ethics Training (1.0)
Operations Method & Personnel	Good	Current	Total # MDLs/MDLVs Required
		Current	# MDLs/MDLVs Past Due
	100%	Current	% MDLs/MDLVs Complete (1.0)
	Good	Current	Training Documentation Records (Good>90%, Fair 70-90%, or Poor <70%)
30	2008 Average	This month	Hold Time Violations due to Lab Error
Accreditation	Good	Current	Total Access Update Status (Good, Fair, Poor)
	Good	Current	Total Access Certification pdfs current (Good, Fair, Poor)
	<5	Jan-to-date	Method certification Losses (performance or audit issues) (1.0)
Quality System Review		Current	Last NELAC Audit Date (Where applicable - informational)
		Current	QAM Effective Date
	<12 months	Current	Last Management QS Review Date (1.0)

20.7.10 Subsequent to the initial MDL determination, annual MDL verification standard is required. For methods performed on multiple instruments, a full MDL study (by the procedure in 40 CFR Part 136, Appendix B or alternatively by other technically acceptable practices) is required annual on at least one of the instruments.. See laboratory SOP IR-QA-MDL, "Determination of Method Detection Limits" for more details.

Table 20-1. Laboratory SOPs

DEPARTMENT	FILENAME	DESCRIPTION
Administrative	IR-ADM-POW	POWER OUTAGES
Administrative	IR-IT-COMPUSEC	COMPUTER SECURITY
Administrative	IR-ADMIN-SOFT	SOFTWARE MAINTENANCE
EXTRACTIONS	IR-WET-SETT	SETTLABLE MATTER (EPA METHOD 160.5 / SM2540F)
EXTRACTIONS	IR-PREP-ORP	STANDARD METHOD 2580B (OXIDATION REDUCTION POTENTIAL)
EXTRACTIONS	IR-WI-UPDRO	UPRR PORTOLA DRO STUDY
EXTRACTIONS	IR-WET-TURB	TURBIDITY, NEPHELOMETRIC (EPA METHOD 180.1 AND STANDARD METHOD 2130B)
EXTRACTIONS	IR-WET-ODOR	THRESHOLD ODOR (SM 2150B & EPA 140.1)
EXTRACTIONS	IR-EXT-3510_D	EPA METHOD 3510C (DIESEL EXTRACTION FOR WATER)
EXTRACTIONS	IR-WET-FE2	FERROUS IRON BY SM 3500Fe-D MODIFIED
EXTRACTIONS	IR-EXT-PFE_D	EPA METHOD 3545 (PRESSURIZED FLUID EXTRACTION [PFE], DIESEL EXTRACTION FOR SOIL)

DEPARTMENT	FILENAME	DESCRIPTION
EXTRACTIONS	IR-EXT-1664	GRAVIMETRIC DETERMINATION OF N-HEXANE EXTRACTABLE MATERIAL AND SILICA GEL TREATED N-HEXANE EXTRACTABLE MATERIAL IN WATER
EXTRACTIONS	IR-WET-PH	EPA METHOD 150.1/ 9040B/ 9045C (ELECTROMETRIC pH)
EXTRACTIONS	IR-EXT-9071	HEM and STG-HEM IN SOLID SAMPLES, EPA 9071B MOD/EPA 3550C MOD
EXTRACTIONS	IR-EXT-3510_P	EPA METHOD 3510C (ORGANOCHLORINE PESTICIDES AND PCBS EXTRACTION FOR WATER)
EXTRACTIONS	IR-EXT-3580A	EPA METHOD 3580A Waste Dilution
EXTRACTIONS	IR-EXT-3545_SV	EPA METHOD 3545 (PRESSURIZED FLUID EXTRACTION [PFE], SEMI-VOLATILE EXTRACTION FOR SOIL)
EXTRACTIONS	IR-EXT-IGNITE	IGNITABILITY IN SOIL
EXTRACTIONS	IR-EXT-3520C	EPA METHOD 3520C AND EPA METHOD 625 (CONTINUOUS LIQUID-LIQUID EXTRACTION)
EXTRACTIONS	IR-EXT-418_413	EPA METHOD 413.2 AND 418.1 (TOTAL RECOVERABLE PETROLEUM HYDROCARBONS, OIL AND GREASE FOR WATER AND SOIL)
EXTRACTIONS	IR-EXT-3545P	EPA METHOD 3545 (PRESSURIZED FLUID EXTRACTION [PFE], PESTICIDE AND PCB EXTRACTION FOR SOIL)
EXTRACTIONS	IR-WET-COLOR	EPA METHOD 110.2 & SM 2120B (COLOR, COLORIMETRIC-PLATINUM-COBALT)
EXTRACTIONS	IR-EXT-NA2SO4	PREPARATION OF SODIUM SULFATE FOR EXTRACTIONS
EXTRACTIONS	IR-EXT-CALUFT	DIESEL EXTRACTION FOR SOIL, CA LUFT METHOD
GC-BTEX	FIXGAS.SOP	ASTM 1946-92 (FIXED GASES)
GC-BTEX	IR-GCV-RSK	METHANE, ETHANE AND ETHYLENE BY GC HEADSPACE (RSK-175)
GC-BTEX	IR-GCV-8015_8021	GASOLINE RANGE ORGANICS (GRO) / BTEX AND MTBE/MINERAL SPIRITS
GC-BTEX	IR-GCV-AIR	EPA METHOD 8015/8020, MODIFIED FOR AIR AND CARB METHOD 410A (BTEX, MTBE AND FUEL HYDROCARBONS AS GASOLINE)
GCMS-SEMI	14DIOX_8270C.SOP	1,4-DIOXANE BY 8270C MODIFIED SCAN MODE
GCMS-SEMI	IR-MSS-NITROSA	NITROSAMINES BY GC/MS USING CHEMICAL IONIZATION (EPA 1625C MODIFIED)
GCMS-SEMI	IR-MSS-PAHSIM	PAHs COMPOUNDS BY EPA 8270C SELECTIVE ION MONITORING (SIM) MODE
GCMS-SEMI	IR-MSS-548_1	EPA METHOD 548.1(DETERMINATION OF ENDOTALL IN DRINKING WATER BY ION EXCHANGE EXTRACTION, ACIDIC METHANOL METHYLATION AND GCMS)

DEPARTMENT	FILENAME	DESCRIPTION
GCMS-SEMI	IR-MSS-525_2	EPA METHOD 525.2 (ORGANIC COMPOUNDS BY LIQUID-SOLID EXTRACTION AND GAS CHROMATOGRAPGY/MASS SPECTROMETRY)
GCMS-SEMI	IR-MSS-CHLOR	DICHLOROACETALDEHYDE AND TRICHLOROACETALDEHYDE BY EPA 8270C MOD, SELECTIVE ION MONITORING (SIM) MODE
GCMS-SEMI	IR-MSS-8270C_625	EPA METHOD 8270C (SEMI-VOLATILE ORGANIC COMPOUNDS)/EPA METHOD 625 (BASE/NEUTRALS AND ACIDS)
GCMS-VOL	IR-MSV-524	EPA METHOD 524.2 (PURGEABLE ORGANIC COMPOUNDS)
GCMS-VOL	IR-MSV-PREP	VOLATILE ORGANIC PREPARATION (EPA 5030B & 5035A)
GCMS-VOL	IR-MSV-TPH	TOTAL PETROLEUM HYDROCARBONS BY GCMS (TPH BY GCMS)
GCMS-VOL	IR-MSV-123TCP	1,2,3-Trichloropropane by GCMS SIM MODE, EPA 524.2
GCMS-VOL	IR-MSV-SIM	Volatile Organic Compounds by GCMS-SIM, (1,2,3-Trichloropropane and 1,4-Dioxane)
GCMS-VOL	IR-MSV-8260_624	EPA METHOD 8260B/624 (VOLATILE ORGANIC COMPOUNDS)
GC-SEMI	PCBs.SOP	EPA METHOD 8082/608 (POLYCHLORINATED BIPHENYLS (PCBS) BY GC)
GC-SEMI	IR-GCV-504	EPA METHOD 504.1 (EDB, DBCP, AND 123TCP IN WATER BY MICROEXTRACTION AND GAS CHROMATOGRAPHY)
GC-SEMI	IR-GCS-8015_D	EPA METHOD 8015B AND MODIFIED FOR DHS LUFT (TOTAL PETROLOLEUM HYDROCARBONS AS DIESEL)
GC-SEMI	IR-GCV-ALC	EPA METHOD 8015B MODIFIED (METHANOL AND ETHANOL BY GC)
GC-SEMI	IR-GCS-552_2	EPA METHOD 552.2 (DETERMINATION OF HALOACETIC ACIDS IN DW BY LIQUID-LIQUID EXTRACTION, DERIVATIZATIONS BY GC)
GC-SEMI	IR-GCS-8015_AZ	C10 -C32 HYDROCARBONS IN SOIL (ADHS METHOD 8015AZ R1)
GC-SEMI	IR-GCS-PEST	ORGANOCHLORINE PESTICIDES BY GC (EPA METHODS 608 & 8081A)
Health & Safety	IR-EHS-RESP	RESPIRATORY PROTECTION PLAN - VOLUNTARY
Health & Safety	IR-EHS-WASTE	HAZARDOUS WASTE DISPOSAL
HPLC-DW	IR-SV-531.1	EPA 531.1 (Measurement of Carbamates in Water by Direct Aqueous Injection HPLC with Post Column Derivatization)
INORGANIC PREP	3050B.SOP	ACID DIGESTION FOR TOTAL METALS BY GFAA AND ICP IN SOIL (EPA METHOD 3050B)
INORGANIC PREP	IR-PREP-WASH	GLASSWARE WASHING

DEPARTMENT	FILENAME	DESCRIPTION
INORGANIC PREP	IR-WI-PREP	SUMMARY OF SHORT HOLDING TIMES
INORGANIC PREP	IR-PREP-3005_200_2	EPA 200.2 and 3005A. (Acid Digestion of Water for Total Recoverable or Dissolved Metals by ICP and ICPMS)
INORGANIC PREP	IR-PREP-3010_20	ACID DIGESTION OF AQUEOUS SAMPLES AND EXTRACTS FOR TOTAL METALS BY ICP AND GCFAA (EPA METHOD 3010A & 3020A)
INORGANIC PREP	IR-PREP-1311-12-TI22	TCLP, SPLP (EPA METHOD 1311 & 1312) AND STLC/ WET EXTRACTION (TITLE 22, SECTION 66261.126, APPENDIX III)
INORGANIC PREP	IR-EXT-1010	EPA METHOD 1010 (PENSKEY-MARTENS CLOSED-CUP METHOD FOR DETERMINING IGNITABILITY)
INORGANIC PREP	IR-PREP-LFR_Leach	LFR Special Leachate Procedure
INORGANIC PREP	IR-WI-MET2	Modified Soil Digestion Procedure for OCSD
INORGANIC PREP	IR-WI-MET1	Aqua Regia Digestion for Metals Analysis of Soil Samples
METALS	IR-MET-CEC	EPA METHOD 9081A CATION-EXCHANGE CAPACITY OF SOILS (SODIUM ACETATE)
METALS	IR-MET-ICP	ICP METALS ANALYSES (EPA METHOD 6010B, EPA METHOD 200.7)
METALS	IR-MET-ICPMS	METALS BY ICP/MS (EPA METHOD 200.8 & EPA 6020)
METALS	IR-MET-HG	MERCURY, COLD-VAPOR ATOMIC ABSORPTION SPECTROMETRY (EPA METHODS 245.1/7470A/7471)
METALS	IR-WI-MET2	Modified Soil Digestion Procedure for OCSD
METALS	IR-MET-ORG-PB	ORGANIC LEAD BY GRAPHITE FURNACE AA (CA DTSC 939-M)
MICRO	IR-MICRO-9223B	TOTAL COLIFORM AND E. COLI PRESENCE/ABSENCE OR (Quanti-Tray) MPN BY COLILERT, COLILERT 18, OR COLISURE SM 9223B
MICRO	IR-MICRO-PURE_CULTURES	MICROBIOLOGICAL - PURE CULTURE PREPARATION AND MAINTENANCE
MICRO	IR-MICRO-QC_EQUIP-ENVIRONMENT	MICROBIOLOGICAL QUALITY CONTROL CHECKS FOR LABORATORY EQUIPMENTS AND LABORATORY ENVIRONMENT
MICRO	IR-MICRO-MRQS	MICROBIOLOGICAL MEDIA, REAGENTS AND QUANTITATION SUPPLIES - RECEIVING, PREPARATION AND QUALITY CONTROL CHECK
MICRO	IR-MICRO-GLP	MICROBIOLOGICAL GOOD LABORATORY PRACTICE (GLP)
PM	IR-PM-DOC	PROJECT MANAGEMENT--COMMUNICATION AND DOCUMENTATION
PM	IR-PM-CLIENT	PROJECT MANAGEMENT--CLIENT/PROJECT SET-UP

DEPARTMENT	FILENAME	DESCRIPTION
PM	IR-PM-DATA	PROJECT MANAGEMENT -- DATA REPORTING, VALIDATION AND DISTRIBUTION
PM	IR-PM-WIP	WELL INVESTIGATION PROGRAM (WIP) Package Generation
PM	IR-PM-EDF	EDF (ELECTRONIC DATA FORMAT)
PM	IR-PM-DATAPACK	DATA PACKAGE GENERATION
QA	Honeywell_QAS	Honeywell Waste Service Agreement (11/01/2007)
QA	IR-QA-ICOC	LEGAL CUSTODY PROCEDURES
QA	IR-QA-MDL	DETERMINATION OF METHOD DETECTION LIMITS
QA	IR-QA-QAPP_REV	REVIEW AND COMMUNICATION OF CLIENT QUALITY REQUIREMENTS
QA	IR-QA-LOGBOOK	LOGBOOKS, DOCUMENTATION, AND LABORATORY COMMUNICATION
QA	IR-QA-WIPES	WORK INSTRUCTION FOR WIPE SAMPLING
QA	IR-QA-SUBSAMP	SUBSAMPLING
QA	IR-QA-WATER	LABORATORY WATER QUALITY
QA	IR-QA-QAD	QUALITY ASSURANCE DEPARTMENT
QA	IR-QA-THERMA	THERMOMETER CALIBRATION, TEMPERATURE MONITORING, AND DOCUMENTATION
QA	IR-QA-PIPET	PIPET CALIBRATION
QA	IR-QA-CAR	CORRECTIVE ACTIONS
QA	IR-QA-CNTRLLIM	CONTROL CHARTS AND STATISTICAL PROCESS CONTROL
QA	IR-QA-REFRBLANK	REFRIGERATOR STORAGE BLANKS
QA	IR-QA-SIGFIG	SIGNIFICANT FIGURES
QA	IR-QA-STDCNTRL	REAGENT AND STANDARD CONTROL AND DOCUMENTATION
QA	IR-QA-REV	GENERAL DATA REVIEW
QA	IR-QA-ARCH	RECORD ARCHIVING
QA	IR-QA-TRAIN	TRAINING AND DOCUMENTATION
QA	IR-QA-LOTTEST	CONTAINER AND REAGENT VERIFICATION BY LOT TESTING
QA	IR-QA-DATAQUAL	USE OF DATA QUALIFIERS
QA	IR-QA-BPREQS	BP LaMP Technical Requirements
QA	IR-QA-DOC	DOCUMENT CONTROL
QA	IR-QA-BAL	BALANCE CALIBRATION VERIFICATION AND DOCUMENTATION
QA	IR-QA-ETEDW.SOP	EARTH TECH/EDWARDS AFB PROJECT REQUIREMENTS
Sample Control	FIELD.SOP	FIELD SAMPLING
Sample Control	IR-SC-MLOG	MANUAL ENTRY OF SAMPLES FOR SAMPLE CONTROL
Sample Control	IR-SC-COURIER	COURIER PROCEDURES
Sample Control	IR-SC-LOGIN	SAMPLE CONTROL

DEPARTMENT	FILENAME	DESCRIPTION
sample Control	IR-SC-OBLIT_LABELS	OBLITARATION OF CLIENT LABELS
Sample Control	IR-SC-BPRESER	BOTTLE PRESERVATION
WETCHEM	IR-WET-3001	EPA METHOD 300.1 (THE DETERMINATION OF INORGANIC ANIONS BY ION CHROMATOGRAPHY)
WETCHEM	IR-WET-ICMS	Determination of Perchlorate by Ion Chromatography/Mass Spectrometry, EPA 332.0
WETCHEM	IR-WET-TRC	EPA METHOD 330.5/SM 4500-Cl G (CHLORINE AND CHLORAMINES)
WETCHEM	IR-WET-TOC	EPA METHOD 415.1/SM 5310B OR EPA METHOD SW 9060 (TOTAL ORGANIC CARBON)
WETCHEM	IR-WET-TVS	EPA METHOD 160.4/SM2540E (FIXED AND VOLATILES RESIDUE IN WATERS)
WETCHEM	IR-WET-5310C	TOTAL AND DISSOLVED ORGANIC CARBON (STANDARD METHOD 5310C)
WETCHEM	IR-WET-TSS	EPA METHOD 160.2/SM 2540D (TOTAL SUSPENDED SOLIDS; NON-FILTERABLE RESIDUE)
WETCHEM	IR-WET-FLUOR	EPA METHOD 340.2/9214/SM 4500F (FLUORIDE BY POTENTIOMETRIC, ION SELECTIVE ELECTRODE)
WETCHEM	IR-WET-376	SULFIDE, COLORIMETRIC, METHYLENE BLUE (STANDARD METHOD 4500 S2-, EPA 376.2)
WETCHEM	IR-WET-COD	EPA METHOD 410.4/SM 5520D (CHEMICAL OXYGEN DEMAND)
WETCHEM	IR-WET-BOD	BIOCHEMICAL OXYGEN DEMAND / CARBONACEOUS BIOLOGICAL OXYGEN DEMAND (EPA METHOD 405.1/SM 5210B)
WETCHEM	IR-WET-420	EPA METHOD 420.1/9065 (PHENOLICS, TOTAL RECOVERABLE)
WETCHEM	IR-WET-MERCAP	MERCAPTANS, TOTALS (LACSD 258)
WETCHEM	IR-WET-7196	EPA METHOD 7196A/STANDARD METHODS 3500-CR D (HEXAVALENT CHROMIUM, COLORIMETRIC + ALKALINE DIGEST (EPA 3060A)
WETCHEM	IR-WET-TDS	TOTAL DISSOLVED SOLIDS, FILTERABLE RESIDUE (EPA METHOD 160.1/SM2540C)
WETCHEM	IR-WET-2540G	STANDARD METHOD 2540G (TOTAL FIXED AND VOLATILE SOLIDS IN SOLIDS AND SEMISOLIDS)
WETCHEM	IR-WET-PERM	Permanganate
WETCHEM	IR-WET-THIO	THIOSULFATE BY TITRATION (LACSD 253B)
WETCHEM	IR-WET-5560C	SM 5560C (VOLATILE ORGANIC ACIDS BY DISTILLATION)
WETCHEM	IR-WET-PCBSA	EPA 314.0 MOD. (DETERMINATION OF 4-CHLOROBENZENESULFONIC ACID (PCBSA) BY ION CHROMATOGRAPHY)
WETCHEM	IR-WET-CN_WAD	STANDARD METHODS 4500-CN, I - WEAK ACID DISSOCIABLE CYANIDE
WETCHEM	IR-WET-ACID	ACIDITY, TITRIMETRIC (EPA METHOD 305.1/SM 2310B)

DEPARTMENT	FILENAME	DESCRIPTION
WETCHEM	IR-WET-CRIC	Determination of Hexavalent Chromium by Ion Chromatography--EPA Methods 7199 and 218.6
WETCHEM	IR-WET-NH3ISE	AMMONIA POTENTIOMETRIC, ION SELECTIVE ELECTRODE (EPA METHOD 350.3/SM4500-NH3 D)
WETCHEM	IR-WET-COND	SPECIFIC ELECTRICAL CONDUCTANCE (EPA METHOD 120.1 / STANDARD METHOD 2510B)
WETCHEM	IR-WET-PAINT	PAINT FILTER LIQUIDS TEST, EPA 9095A
WETCHEM	IR-WET-TS	EPA METHOD 160.3 (TOTAL SOLIDS / PERCENT SOLIDS / PERCENT MOISTURE, GRAVIMETRIC, DRIED AT 103-105 C)
WETCHEM	IR-WET-OXY	EPA METHOD 360.1 / STANDARD METHOD 4500-O-G (DISSOLVED OXYGEN)
WETCHEM	IR-WET-CO2	STANDARD METHOD 4500-CO2 (TITRIMETRIC METHOD FOR FREE CARBON DIOXIDE)
WETCHEM	IR-WET-300	EPA METHOD 300.0 and EPA SW9056 (THE DETERMINATION OF INORGANIC ANIONS BY ION CHROMATOGRAPHY)
WETCHEM	IR-WET-TOTALCN	EPA 9010B, 9014 & SM 4500-CN~ -B,C,E (CYANIDES, TOTAL)
WETCHEM	IR-WET-MBAS	EPA METHOD 425.1 & SM 5540C (ANION SURFACTANTS AS METHYLENE BLUE ACTIVE SUBSTANCES)
WETCHEM	IR-WET-HARD	HARDNESS BY TITRATION EPA 130.2/SM2340C
WETCHEM	IR-WET-AMENCN	STANDARD METHOD 4500-CN-G/9010B (CYANIDES, AMENABLE TO CHLORINATION)
WETCHEM	IR-WET-ALK	ALKALINITY BY SM2320B, EPA METHOD 310.1
WETCHEM	IR-WET-314.0	Determination of Perchlorate by Ion Chromatography--EPA 314.0
WETCHEM	IR-WET-TKN	TOTAL KJELDAHL NITROGEN (EPA METHOD 351.3.2/SM 4500-Norg-C)
WETCHEM	IR-WET-TITR	NITROGEN AMMONIA (TITRIMETRIC) (EPA METHOD 350.2/SM4500-NH3-B, C)
WETCHEM	IR-WET-SULFIDE_TITR	EPA METHOD 9030/9034 / SM 4500S-F - ACID SOLUBLE/INSOLUBLE SULFIDES
WETCHEM	IR-WET-PHOSP	EPA METHOD 365.3 (PHOSPHORUS, ALL FORMS)
WETCHEM	IR-WET-3060A	ALKALINE DIGESTION PROCEDURE FOR HEXAVALENT CHROMIUM EPA 3060A (FOR METHOD EPA 7196 & EPA 7199)
WETCHEM	IR-WET-SPECGRAV	SPECIFIC GRAVITY BY MASS RATIO (SM2710F)
WETCHEM	IR-WET-INORG-CAL	Inorganic Calculations for Ion Balance, Langlier, Aggressive Index, Hardness, Unionized Sulfide, Larson-Skold Index, Sodium Absorption Ratio, Salinity

Table 21-1 Laboratory Equipment and Instrumentation

Department	Item	Manufacturer	Model	Serial Number	Installation
BTEX	3-door Refrigerator	True Manufacturing Co			1997
BTEX	3-door Refrigerator	True Manufacturing Co			1997
BTEX	Air Concentrator	Entech	2000	43	1993
BTEX	Auto Sampler	Varian	Archon	14169	2005
BTEX	Auto Sampler	Varian	Archon	14635	2005
BTEX	Auto Sampler (Archon)	Varian	Archon	14411	2006
BTEX	Auto Sampler (DPM)	Varian	Archon	14654	2005
BTEX	Auto Sampler (DPM)	O.I. Analytical	MPM16/DPM16	H308369/89049 B	1993
BTEX	Auto Sampler (DPM)	O.I. Analytical	MPM16/DPM16	105950257/329 240	1997
BTEX	Auto Sampler (DPM)	O.I. Analytical	MPM/DPM 16	91349/D122416 646	1993
BTEX	Auto Sampler (DPM)	O.I. Analytical	MPM16/DPM16	H303322/C4204 11196	1993
BTEX	Gas Chromatograph (FID)	Hewlett Packard	5890 Series II	S/N3126A36955	1997
BTEX	Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	S/N3133A37156	1992
BTEX	Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	S/N3203A40477	1993
BTEX	Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	S/N3203A41169	1993
BTEX	Gas Chromatograph (FID/PID)	Hewlett Packard	5890A	S/N2750A15898	1997
BTEX	Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	S/N3336A60066	1997
BTEX	Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	S/N3033A33301	1998
BTEX	Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	S/N3121A35567	1993
BTEX	Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	S/N3223A2733	1993
BTEX	Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	S/N3336A60064	1993
BTEX	Gas Chromatograph (FID/PID/ELCD)	Hewlett Packard	5890 Series II	S/N3203A40699	1993
BTEX	Purge & Trap Concentrator	O.I. Analytical	4460A	12584-1027	1992
BTEX	Purge & Trap Concentrator	O.I. Analytical	4460A	123811014	1993
BTEX	Purge & Trap Concentrator	O.I. Analytical	4560	H401460019	1993
BTEX	Purge & Trap Concentrator	O.I. Analytical	4460A	108061863	1997
BTEX	Purge & Trap Concentrator	O.I. Analytical	4560	N222460463	1998
BTEX	Purge & Trap Concentrator	O.I. Analytical	4560	N111460835	1993
BTEX	Purge & Trap Concentrator	O.I. Analytical	4560	A229100	1992
BTEX	Purge & Trap Concentrator	O.I. Analytical	4460A	M214048	1993
BTEX	Tall Freezer				
BTEX	Tall Freezer				
Drinking Water	3 Glass Door Refrigerator				2009
Drinking Water	Archon	O.I. Analytical	4552	14420	2009
Drinking Water	Concentrator	O.I. Analytical	4560	M012460798	2009
Drinking Water	Gas Chromatograph/Mass Spectrometer	Agilent	6890N / 5973	CN10521030 / US40620627	2009
Extractions	Accelerated Solvent Extractor	Dionex	ASE 200	00120362	2001

Department	Item	Manufacturer	Model	Serial Number	Installation
Extractions	Accelerated Solvent Extractor	Dionex	ASE 200	96040278	2000
Extractions	Accelerated Solvent Extractor	Dionex	ASE 200	97240463	2001
Extractions	Accelerated Solvent Extractor	Dionex	ASE 200	96090216	2001
Extractions	Accelerated Solvent Extractor	Dionex	ASE 200	07090745	2007
Extractions	Accelerated Solvent Extractor	Dionex	ASE 200E	07090746	2007
Extractions	Accelerated Solvent Extractor	Dionex	ASE 200	99120782	2002
Extractions	Automated Extractor	Horizon Technology	SPE-DEX 4790	03-0359	2003
Extractions	Automated Extractor	Horizon Technology	SPE-DEX 4790	03-0360	2003
Extractions	Drying Oven	Fisher		40200001	
Extractions	Drying Oven	Fisher	630G	800121	
Extractions	Fixed Wavelength Infrared Spectrophotometer	Foxboro	Miran1FF	2592	1997
Extractions	Flashpoint Tester	Koehler	K-162	10A/Y-2	1992
Extractions	Kiln	Cress Electric Klin	E2418	0503DD	2005
Extractions	Rapid Vap	Labconco	Rapidvap	266435	
Extractions	Rapid Vap	Labconco	Rapidvap	21098412F	2002
Extractions	Rapid Vap	Labconco	Rapidvap	705319	1999
Extractions	Rapid Vap	Labconco	Rapidvap	010194458E	2002
Extractions	Rapid Vap	Labconco	Rapidvap	040824527F	
Extractions	Rapid Vap	Labconco	Rapidvap	020196541F	2001
Extractions	Small Freezer				
Extractions	Small Refrigerator				
Extractions	SPE-Controller	Horizon Technology	SPE-DEX	020357	2003
Extractions	SpeedVapII	Horizon	SpeedVap 9000	00-248	2005
Extractions	SpeedVapII	Horizon	SpeedVap 9000	99-216	2007
Extractions	SpeedVapIII	Horizon	SpeedVap III	04-2019	2007
Extractions	Turbo Vap	Zymark	Turbovap II	04053	2002
Extractions	Turbo Vap II	Zymark	Turbovap II	04511	2002
Extractions	Turbo Vap II	Zymark	Turbovap II	4272	2002
Extractions	Turbo Vap II	Zymark	Turbovap II	TV0239N11193	2002
Extractions	Turbo Vap LV	Caliper LifeSciences	103200/2	TV0429N12434	2004
Extractions	Turbo Vap LV	Caliper LifeSciences	103200/2	TV0429N12435	
Extractions	TurboVap II	Zymark	TurboVap II	04429	2008
Extractions	TurboVap II	Zymark	TurboVap II	04427	2008
GCMS-Semi	Auto Sampler for GC	Hewlett Packard	7673B		1993
GCMS-Semi	Auto Sampler for GC	Hewlett Packard	7673B		1995
GCMS-Semi	Auto Sampler for GC	Hewlett Packard	7673B		1993
GCMS-Semi	Auto Sampler for GC	Agilent	G2614A	US12812101	2003
GCMS-Semi	Auto Sampler for GC	Agilent	G2614A	CN33826431	2005
GCMS-Semi	Auto Sampler for GC	Hewlett Packard	7673B		1993
GCMS-Semi	Auto Sampler for GC	Agilent	G2614A	CN63340749	2006
GCMS-Semi	Auto Sampler for GC	Hewlett Packard	18593B	3120A26939	1992

Department	Item	Manufacturer	Model	Serial Number	Installation
GCMS-Semi	Auto Sampler for GC	Agilent	G2614A	CN42629414	0
GCMS-Semi	Auto Sampler for GC	Hewlett Packard			2008
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890Ser.II/5971	3140A39653	1993
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890Ser.II/5972	3235A46723	1995
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890Ser.II/5971	3133A37717	1993
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890Ser.II	3033A32428	1987
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Agilent	6890/5973/G2589A	US10130035/U S10480674	2003
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973/G2578A	US10341048/U S33210028	2005
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890Ser.II/5971	3033A30488/31 33A37717	1993
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5975B/G3171A	CN10636107/U S62724086	2006
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890IIB/5971A	2921A24077/31 88A02848	1992
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Agilent	6890/5973/G2579A	CN10427051/U S41720775	2007
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973 Inert	CN10349032/U S33220240	2008
GCMS-Semi	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	6890Plus (G1530A)/5973 (G1098A)	US00032006/U S93122851	2008
GCMS-Semi	Small Freezer				
GCMS-Semi	Tall Freezer				
GCMS-Semi	Top/Bottom Freezer				
GCMS-Semi	Top/Bottom Freezer				
GCMS-Semi	Top/Bottom Freezer				
GCMS-Semi	Top/Bottom Freezer				
GCMS-Semi	Top/Bottom Refrigerator				
GCMS-Semi	Top/Bottom Refrigerator				
GCMS-Semi	Top/Bottom Refrigerator				
GCMS-Semi	Top/Bottom Refrigerator				
GCMS-Volatiles	3-door Refrigerator	True Manufacturing Co			1997
GCMS-Volatiles	3-door Refrigerator	True Manufacturing Co			1997
GCMS-Volatiles	3-door Refrigerator	True Manufacturing Co			1997
GCMS-	3-door Refrigerator	True Manufacturing Co			1997

Department	Item	Manufacturer	Model	Serial Number	Installation
Volatiles					
GCMS-Volatiles	Archon	O.I. Analytical	4552	12221	2009
GCMS-Volatiles	Auto Sampler	O.I. Analytical	4552	14418	2004
GCMS-Volatiles	Auto Sampler	O.I. Analytical	4552	14407	2006
GCMS-Volatiles	Auto Sampler	O.I. Analytical	4552	14417	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	13388	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	14636	2004
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	14633	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	14634	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	14662	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	13171	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	14638	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	14637	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	14418	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	13389	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	14639	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	14492	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon	14195	2006
GCMS-Volatiles	Auto Sampler (Archon)	Varian	Archon DY505220-16	12731	2001
GCMS-Volatiles	Auto Sampler (DPM)	O.I. Analytical	DPM 16	B704411427	2003
GCMS-Volatiles	Concentrator	O.I. Analytical	4560	N228460103	2009
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	6890/5973A	US00020097/U S72810389	1999
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	6890/5973A	US00022931/U S82311546	2000
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6850/5973N	US00001207/U S01140222	2001
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6850/5973	US00001206/U S01140215	2001
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6850/5973N	US0001947/US 10340261	2002
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6850/5973N	US00002140/U S10440793	2002

Department	Item	Manufacturer	Model	Serial Number	Installation
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6850/5973N	US00002860/U S21843317	2003
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6890/5973	US00034262/U S01112246	2004
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973	CN10318006/U S30945515	2004
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973	CN10318007/U S30945517	2004
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890II/5971A	3235A46434/30 40A01409	2000
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973	CN0523048/US 43146864	2006
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973	CN01521014/U S44647184	2005
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973	US00001682/U S92522712	2001
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973N	US10222064/U S10462085	2006
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973	US10206070/U S10462145	2006
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973 inert	CN10339005/U S35120285	2007
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890II/5972	3336A60514/35 24A02884	1997
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Agilent	6890N / 5973 Inert	CN10345035 / US33220184	2009
GCMS-Volatiles	Gas Chromatograph/Mass Spectrometer	Hewlett Packard	6890/5973A	US00007750/U S70810354	2000
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	K810460876	1999
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	J513460474	1997
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	K841460440	2001
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	M946460833	2001
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	K82946045	2002
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	J431460443	2002
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	N228460103	2003
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	K907460143	2004
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	J624460525	2004
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	J513460468	2004

Department	Item	Manufacturer	Model	Serial Number	Installation
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	L930460194	2000
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	A229108	2006
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	L924460239	2005
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	E324406	2001
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	E324406	2006
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	H351460339	2006
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	C301264	1997
GCMS-Volatiles	Purge & Trap Concentrator	O.I. Analytical	4560	K728460713	1999
GCMS-Volatiles	Tall Freezer				
GCMS-Volatiles	Tall Freezer				
GCMS-Volatiles	Tall Freezer				
GCMS-Volatiles	Top/Bottom Refrigerator				
GC-Semi	Auto Sampler for GC	Hewlett Packard	18596A	2718A09693	
GC-Semi	Auto Sampler for GC	Hewlett Packard	18596A	2718A08776	
GC-Semi	Auto Sampler for GC	Hewlett Packard	18596B	3202A27470	
GC-Semi	Auto Sampler for GC	Hewlett Packard	18596B	3445A17015	
GC-Semi	Auto Sampler for GC	LEAP			
GC-Semi	Auto Sampler for GC	Hewlett Packard	7673B		
GC-Semi	Auto Sampler for GC	Agilent	G2614A	US20914533	
GC-Semi	Auto Sampler for GC	Hewlett Packard	18596B	3206A27724	
GC-Semi	Auto Sampler for GC	Agilent	G2614A	CN24322262	
GC-Semi	Auto Sampler for GC	Hewlett Packard	7673		
GC-Semi	Auto Sampler for GC	Hewlett Packard	7673		
GC-Semi	Auto Sampler for GC	Agilent	G2614A	CN55237971	
GC-Semi	Auto Sampler for GC	Agilent	G2614A	CN55237964	2007
GC-Semi	Auto Sampler for GC	Agilent	18596B	3202A27470	2008
GC-Semi	Auto Sampler for HPLC	Agilent	G1316A	DE91614525	2008
GC-Semi	Gas Chromatograph	Agilent	6890N/1530N	CN10551059	2007
GC-Semi	Gas Chromatograph (Dual ECD)	Hewlett Packard	5890 Series II	3223A43015	
GC-Semi	Gas Chromatograph (Dual ECD)	Hewlett Packard	5890 Series II	336A51142	
GC-Semi	Gas Chromatograph (Dual ECD)	Hewlett Packard	5890A	2728A14467	
GC-Semi	Gas Chromatograph (Dual ECD)	Hewlett Packard	5890Series II	2750A15311	
GC-Semi	Gas Chromatograph (Dual ECD)	Agilent	6890N	US10215019	2002
GC-Semi	Gas Chromatograph (Dual ECD)	Agilent	6890N/G1530N	US10250081	

Department	Item	Manufacturer	Model	Serial Number	Installation
GC-Semi	Gas Chromatograph (Dual ECD)	Hewlett Packard	5890 Series II	3235A45184	
GC-Semi	Gas Chromatograph (Dual ECD)	Agilent	6890N/G1540N	US10423015	
GC-Semi	Gas Chromatograph (Dual ECD)	Agilent	6890N/G1540N	US10423014	
GC-Semi	Gas Chromatograph (Dual ECD)	Agilent	6890N/G1540N	CN10551052	
GC-Semi	Gas Chromatograph (Dual FID)	Hewlett Packard	5890 Series II	3126A36534	
GC-Semi	Gas Chromatograph (Dual FID)	Hewlett Packard	5890 Series II	3133A37568	
GC-Semi	Gas Chromatograph (Dual FID)	Hewlett Packard	5890II	3235A44731	
GC-Semi	Gas Chromatograph (Dual FID)	Hewlett Packard	5890 Series II	2950A26022	
GC-Semi	Gas Chromatograph (FID/PID)	Agilent	5890 Series II	S/N3133A37568	2008
GC-Semi	GC (Dual ECD)	Agilent	6890N/G1530N	US10322076	2007
GC-Semi	GC (Dual ECD)	Agilent	7890A/G3440A	CN10741034	2007
GC-Semi	GC (Dual FID)	Agilent	6890N/G1540N	US10546009	2007
GC-Semi	GC (Dual FID)	Agilent	6890N/G1540N	US10546010	2007
GC-Semi	HPLC	Hewlett Packard	Series 1050	2807G00138	2008
GC-Semi	Injector for GC	Agilent	7673 series (18593B)	3120A27934	2008
GC-Semi	Injector Tower	Hewlett Packard	18593B	3120A27153	
GC-Semi	Injector Tower	Agilent	G2913A	CN55130059	2007
GC-Semi	Vacuum Degasser for HPLC	Hewlett Packard	G1322A	JP63202862	2008
Inorganic Prep	Centrifuge	Precision	Durafuge 100	40317924	2003
Inorganic Prep	Hot Plate	??			0
Inorganic Prep	Hot Plate	??			0
Inorganic Prep	pH Meter	Mettler Toledo	SevenEasy	1227116127	
Inorganic Prep	Rotator	N/A			0
Inorganic Prep	SPE	Horizon	SPE-3000XL PLUS	1006	2008
Inorganic Prep	Turbidity Meter	Orbeco-Hellige	965-10A	5187	2009
Inorganic Prep	Turbidity Meter	HF Instruments	DRT-100B	24942	
Inorganic Prep	Turbidity Meter	Orbeco-Hellige	965-10A	4389	2007
Inorganic Prep	Turbidity Meter	HF Instruments	DRT-100	34238	
Inorganic Prep	Turbidity Meter	Orbeco-Hellige	965-10A	4389	2007
Inorganic Prep	Turbidity Meter	Orbeco-Hellige	965	5078	2007
Metals	10 Place TCLP Rotator	Environmental Express	NA	61501	
Metals	10 Place TCLP Rotator	Environmental Express	5K939C	V00212AY10	0
Metals	12 Place TCLP Rotator	Associated Design	3790-12BRE	NA	
Metals	12 Place TCLP Rotator	Environmental Express		GFMG060J1	2002
Metals	20 Place TCLP Rotator	Ed W. Smith Machine Works	NA	NA	1999

Department	Item	Manufacturer	Model	Serial Number	Installation
Metals	4 Place TCLP Rotator	Environmental Express	NA	304504460	2005
Metals	8 Place Rotator	Associated Design	3740-8BRE	NA	2003
Metals	8 Place Rotator	Environmental Express	F057	E512-TMP	2002
Metals	Auto Sampler for Hg	Perkin Elmer	AS 91	6060	1995
Metals	Auto Sampler for ICP	Perkin Elmer	AS 91	4044	2000
Metals	Auto Sampler for ICP	Perkin Elmer	AS 93 Plus	1075	2002
Metals	Auto Sampler for ICP	Perkin Elmer	AS 91	913S3040101	1997
Metals	Auto Sampler for ICPMS	Perkin Elmer	CETAC	060019ASX	2001
Metals	Auto Sampler for Mercury	Perkin Elmer	AS 90	3380	1995
Metals	Auto Sampler for Metals	Perkin Elmer	AS-72	1464	1995
Metals	Auto Sampler for Metals	Cetac	ASX-500	080002ADX	2004
Metals	Auto Sampler for Metals	Perkin Elmer	AS 93 Plus	3023	2006
Metals	Centrifuge IEC HN SII	Thermo Electron	IEC HN SII	235526998	
Metals	Chiller for ICP	Neslab	CFT-75	199070024	2000
Metals	Chiller for ICP	Polyscience	N0772026	G36430	2005
Metals	Chiller for ICP	VWR	1173PD	106800421	2006
Metals	Chiller for ICP	Polyscience	N0772026	106A00726	2006
Metals	Chiller for ICPMS	Neslab	CFT-75	199064010	1999
Metals	Chiller for ICPMS	Neslab	CFT-75	100255292	2002
Metals	GFAA	Perkin Elmer	SIMAA 6000	5016	1993
Metals	GFAA	Perkin Elmer	4100ZL	6034	2009
Metals	Hg FIAS	Perkin Elmer	FIMS 400	4109	1995
Metals	Hg FIAS Mercury Analyzer	Perkin Elmer	FIMS 400	4167	1995
Metals	High volume stir plate	VWR	986920	090915011	2009
Metals	High volume stir plate with heating	VWR	986663	090930001	2009
Metals	Hot Block 36 Place	Environmental Express	SC154		0
Metals	Hot Block 36 Place	Environmental Express	SC154		0
Metals	Hot Block 36 Place	Environmental Express	SC154	1763CEC1138	0
Metals	Hot Block 36 Place	Environmental Express	SC154	N/A	0
Metals	Hot Block 54 Place	Environmental Express	SC154	3098CEC1491	0
Metals	Hot Block 54 Place	Environmental Express	SC154	424CEC0641	0
Metals	Hot Block 54 Place	Environmental Express	SC154	4186CEC1997	0
Metals	Hot Block 54 Place	Environmental Express	SC154	4186CEC1998	0
Metals	Inductively Coupled Plasma Spectrophotometer	Perkin Elmer	Optima 3000XL	069N4092201	1997
Metals	Inductively Coupled Plasma Spectrophotometer	Perkin Elmer	Optima 4300 DV	077N1100901	2002
Metals	Inductively Coupled Plasma Spectrophotometer	Perkin Elmer	Optima 5300DV	077N5112802	2006
Metals	Inductively Coupled Plasma Spectrophotometer	Perkin Elmer	Optima 5300DV	069N9120901	1997

Department	Item	Manufacturer	Model	Serial Number	Installation
Metals	Inductively Coupled Plasma Spectrophotometer/MS	Perkin Elmer	ELAN 6100E	1650004	2001
Metals	Inductively Coupled Plasma Spectrophotometer/MS	Perkin Elmer	ELAN 6100E	G1970008	2004
Microbiology	Small Incubator				2009
Microbiology	Small Incubator				
Microbiology	Tall Refrigerator				2009
Microbiology	Water Bath				2009
Microbiology	Water Bath				
Mobile Lab	Auto Sampler	O.I. Analytical	4552	14217	2005
Mobile Lab	Auto Sampler	O.I. Analytical	MPM-16	NA	1997
Mobile Lab	Auto Sampler (DPM)	O.I. Analytical	MPM 16		
Mobile Lab	Centrifuge	IEC	--	3634P-14	
Mobile Lab	Concentrator	O.I. Analytical	4560	B232110	1997
Mobile Lab	Concentrator	O.I. Analytical	4460A	NA	1997
Mobile Lab	Fixed Wavelength Infrared Spectrophotometer	Foxboro	Miran1FF	2733	
Mobile Lab	Gas Chromatograph (FID)	Hewlett Packard	5890 Series II	2311A39633	
Mobile Lab	Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	2921A23920	
Mobile Lab	Gas Chromatograph/Mass Spectrometer	Hewlett Packard/O.I.	6890/5973	US00029799	
Mobile Lab	Injector	Hewlett Packard	7673	NA	1997
Mobile Lab	Orbital Shaker	Lab-Line	--		
Mobile Lab	Purge & Trap Concentrator	O.I. Analytical	4460A		
Mobile Lab	Turbo Vap	Zymark	--		
Organic Prep	Chiller	Thermoeslab	M75	102252059	2001
Organic Prep	Chiller	Thermoeslab	M75	101226011	1999
Organic Prep	Chiller	VWR	1177PD	G42546	2004
Organic Prep	Chiller	VWR	1177PD	106A00879	2005
Organic Prep	Chiller	VWR	1177PD	106A00748	2005
Sample Control	3 door Fridge (check sample)	TRUE	TRUE	790441	1997
Sample Control	3 door Fridge (extractables)	TRUE	TRUE	752937	1997
Sample Control	3 door Fridge (extractables)	TRUE	TRUE	818217	1997
Sample Control	3 door Fridge (hazardous)	TRUE	TRUE	790472	1997
Sample Control	3 door Fridge (ICOC-H2O)	TRUE	TRUE	765992	1997
Sample Control	3 door Fridge (ICOC-SOIL)	TRUE	TRUE	818222	1997
Sample Control	3 door Fridge (Receiving)	TRUE	TRUE		1997
Sample Control	3 door Fridge (TOC)	TRUE	TRUE	659811	1997
Sample Control	3-door Refrigerator	True Manufacturing Co	GDM-72	982041	1997
Sample Control	3-door Refrigerator	True Manufacturing Co	GDM-72F	1105095	1997
Sample Control	Glass Door Refrigerator				
Sample Control	Horizontal Freezer				

Department	Item	Manufacturer	Model	Serial Number	Installation
Sample Control	Ice Machine	Microban	XAC830	63K0426BL075	2004
Sample Control	Plastic Shredder	Prodeva	315-S	11090	2001
Sample Control	Small Refrigerator				
Sample Control	Tall Freezer				
Sample Control	Tall Freezer				
Sample Control	Walk-in Refrigerator				
Wetchem	Ammonia Probe	Orion	96-12		
Wetchem	Auto Sampler	Man Tech	PC-Titrate PC1000-102	MS-9K8-210	2009
Wetchem	Auto Sampler	Dionex	AS 40	98050117	2007
Wetchem	Auto Sampler for IC	Dionex	AS40	932811	
Wetchem	Auto Sampler for IC	Dionex	AS 50	01010295	2007
Wetchem	Auto Sampler for IC	Dionex	AS 40	03080145	
Wetchem	Auto Sampler for IC	Dionex	AS 40	98050116	
Wetchem	Auto Sampler for IC	Dionex	AS 40	04110044	
Wetchem	Auto Sampler for IC	Dionex	AS 40	97010434	
Wetchem	Auto Sampler for IC	Dionex	AS 50	03080453	2005
Wetchem	Auto Sampler for IC	Dionex	AS 40	06110242	2002
Wetchem	Auto Sampler for IC	Dionex	AS 50	00100242	0
Wetchem	Auto Sampler for IC14	Dionex	AS40	98050117	2008
Wetchem	Auto Sampler for ICMS	Metrohm	788	NS	2004
Wetchem	Auto Samplers	Dionex	AS 40	95030213	1997
Wetchem	Auto Samplers	Dionex	AS 100	1350188	1997
Wetchem	Auto Samplers	Dionex	AS 100	9950036	1997
Wetchem	Auto Samplers for IC	Dionex	AS 50	99010307	1997
Wetchem	Autotitration with autosampler	Mantek	Tetra Rinse/Autosampler	MS-9K9-108	2002
Wetchem	Block Digestor	Bioscience	163-466T		1997
Wetchem	Block Digestor	Bioscience	2091B1		1997
Wetchem	BOD	Accumet	25	C0021582	0
Wetchem	BOD	Orion Research	EA490	10593A	0
Wetchem	BOD auto-analyzer	Mantek	Tetra Rinse	MS-004-189	
Wetchem	BOD Incubator	VWR	2020	6003205	2002
Wetchem	BOD Incubator	Fisher	307C	00037-090-00	2002
Wetchem	BOD probe	Jenco			
Wetchem	Centrifuge	Fisher Scientific	AccuSpin 300	40327924	2003
Wetchem	Chiller	VWR	1173PD	106600242	2005
Wetchem	COD Reactor	Bioscience Inc.	2091B1	34613302	
Wetchem	COD Reactor	Bioscience Inc.	163-466T	COD-T349	
Wetchem	Conductivity Meter	VWR	21800-012	Q022545	2009
Wetchem	Conductivity Probe	Yellow Springs	32	COD0031	

Department	Item	Manufacturer	Model	Serial Number	Installation
Wetchem	Conductivity/Dissolved Oxygen Probe	Corning	M90	001253	
Wetchem	Cyanide Distillation	Andrew Glass Co	110-10-R	A780509	1999
Wetchem	Cyanide Distillation	Andrew Glass Co	110-10-R	A8X0309	1999
Wetchem	Cyanide Distillation	Andrew Glass Co	110-10-R		1999
Wetchem	Cyanide Distillation Unit	Andrew Glass Co	MIDI System	MCVA13908221	
Wetchem	Cyanide Distillation Unit	Andrew Glass Co	MIDI System	33212579	
Wetchem	Digestion Unit	Buchi	K-435	000-0032-294-00DMC	2000
Wetchem	Digestion Unit	Gerhardt	Kjeldatherm KB	4062216	2007
Wetchem	Distillation Unit	Buchi	K-324	411930090002	2000
Wetchem	Distillation Unit	Gerhardt	Vapodest30	4051679	2007
Wetchem	Drying Oven	Lab Line			
Wetchem	Drying Oven	Scientific Products	DX-61	194002	
Wetchem	Drying Oven	Fisher	630G	801N0001	
Wetchem	Fluoride Probe	Orion	96-09	9609BN	
Wetchem	IC Perchlorate with autosamplers	Dionex	CD 25/AS 50	04060626/04070015	1997
Wetchem	IC with autosamplers	Dionex	CD25A/AS 40	03070269/96060542	2007
Wetchem	Incubator	VWR	2020	1001802	2002
Wetchem	Incubator				
Wetchem	Ion Chromatograph	Dionex	DX-4500	892835	1989
Wetchem	Ion Chromatograph (with UV/VIS) Chromium	Dionex	AD 20	98020642	2000
Wetchem	Ion Chromatograph 300.0	Dionex	LC20	94010215	2007
Wetchem	Ion Chromatograph 300.0	Dionex	DX-100	94120366	1997
Wetchem	Ion Chromatograph 300.0	Dionex	ICS-1000	03110585	2002
Wetchem	Ion Chromatograph 300.0	Dionex	LC 30	97040546	2002
Wetchem	Ion Chromatograph 300.1	Dionex	LC 25	02050420	2005
Wetchem	Ion Chromatograph 314.0 with autosampler	Dionex	CD25/IP25	04060626/04060363	2008
Wetchem	Ion Chromatograph Chromium	Dionex	AD 20	95020077	2002
Wetchem	Ion Chromatograph Chromium	Dionex	AD 25	01070608	2007
Wetchem	Ion Chromatograph Perchlorate	Dionex	CD 20	98060923	1996
Wetchem	Ion Chromatograph Perchlorate	Dionex	CD 25	01090576	2002
Wetchem	Ion Chromatograph/Mass Spectrometer	Metrohm (IC) / Agilent (MS)	LC30-1/LC110/IC800	1820023004102 /US34800214	2005
Wetchem	Kone Lab	Lab Medics	Aquakem 250	E2319629	2004
Wetchem	pH Meter	Beckman	Phi - 40		
Wetchem	pH Meter	Beckman	Phi - 40		
Wetchem	pH Meter	Beckman	Phi - 32		
Wetchem	pH Meter for Ammonia	Pinnacles Series	M530P	05470998	0

Department	Item	Manufacturer	Model	Serial Number	Installation
Wetchem	pH Meter for Fluoride	Fisher Scientific Acc Research	AR15	AR81208052	0
Wetchem	pH Probe	Orion	91-56	9156000	
Wetchem	pH Probe	Orion	91-56		
Wetchem	pH/mV Meter for Alkalinity	Denver Instrument	UB-10 (Basic)	300728.1	2008
Wetchem	pH/mV Meter for BOD	Denver Instrument	Basic	13036	0
Wetchem	Small Refrigerator				
Wetchem	TOC	Dohrmann	DC-190	N5C636T	1987
Wetchem	TOC Analyzer	O.I. Analytical	Solids	C905776109	2009
Wetchem	TOC Analyzer	Shimadzu	5000A	33N01036A	1998
Wetchem	TOC Analyzer with Auto Sampler	Tekmar-Dohrmann	Phoenix 8000	US02106006	2002
Wetchem	TOC Autosampler	Shimadzu	ASI-500A-H-P	33212579	1998
Wetchem	TOC Soil Sampler Module	Shimadzu	SSM-5000A	34613302	1998
Wetchem	Top/Bottom Refrigerator	Maytag	MTB1955GR		2007
Wetchem	UV/VS Spectrometer	Thermo Spectronic	Genesys20	3SGG06B0117	2002
Wetchem	UV/VS Spectrometer (Diode Array Detector)	Hewlett Packard	8452A		

24.2.3 Project Receipt Checklist

All received samples are logged into LIMS in accordance with the Project Receipt Checklist.

Figure 24-5 Sample Acceptance Policy

(Attached)

Figure 24-6 Project Receipt Checklist


(Attached)


Appendix 2 Laboratory Org Chart


(Attached)

TestAmerica

THE LEADER IN ENVIRONMENTAL TESTING

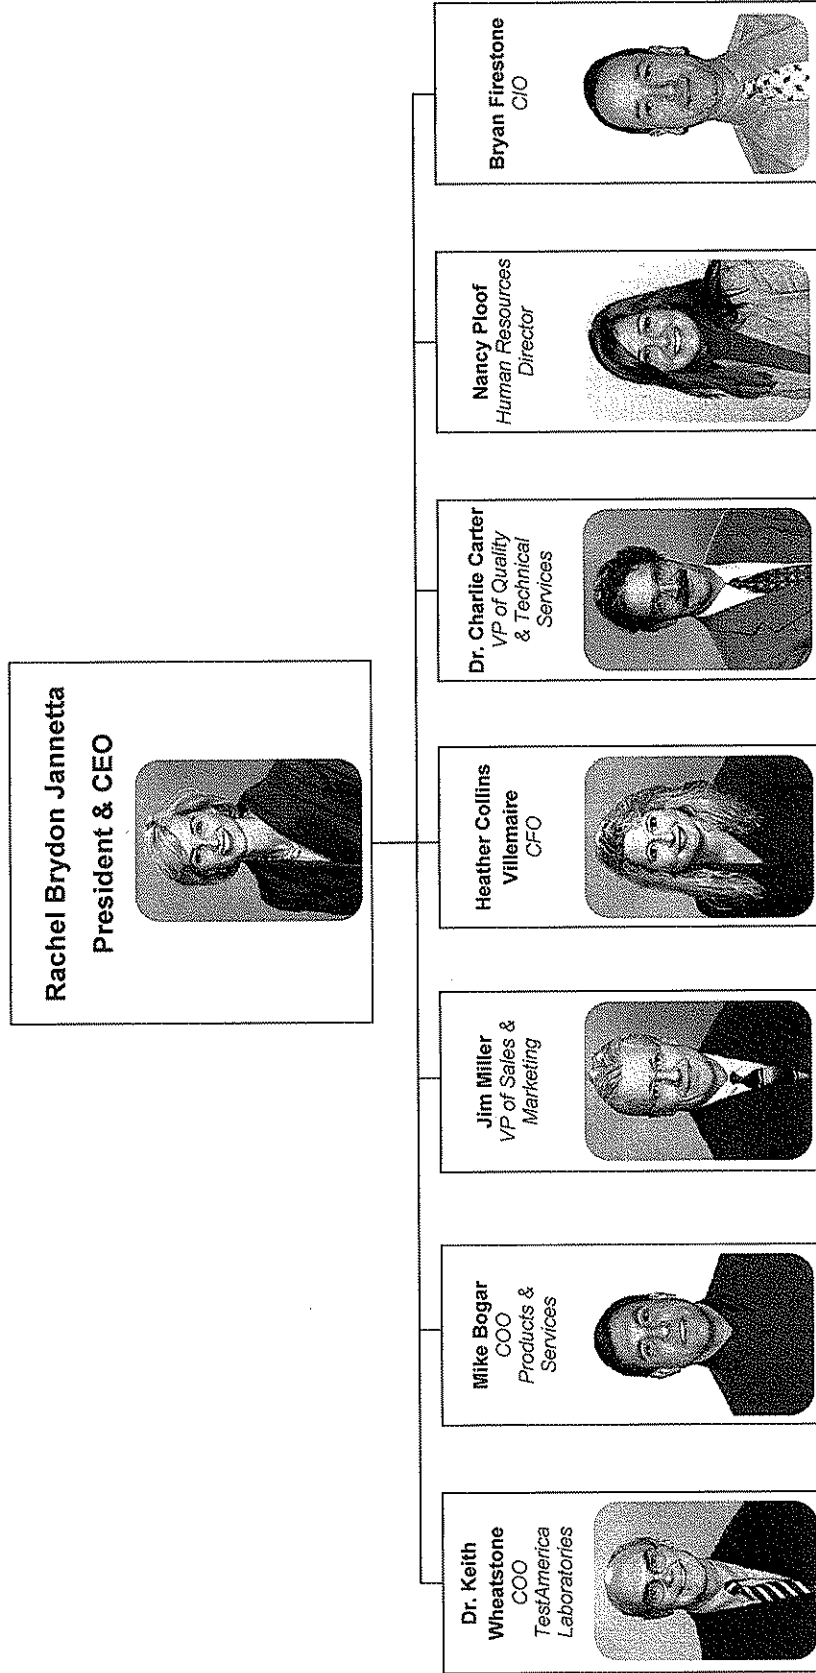

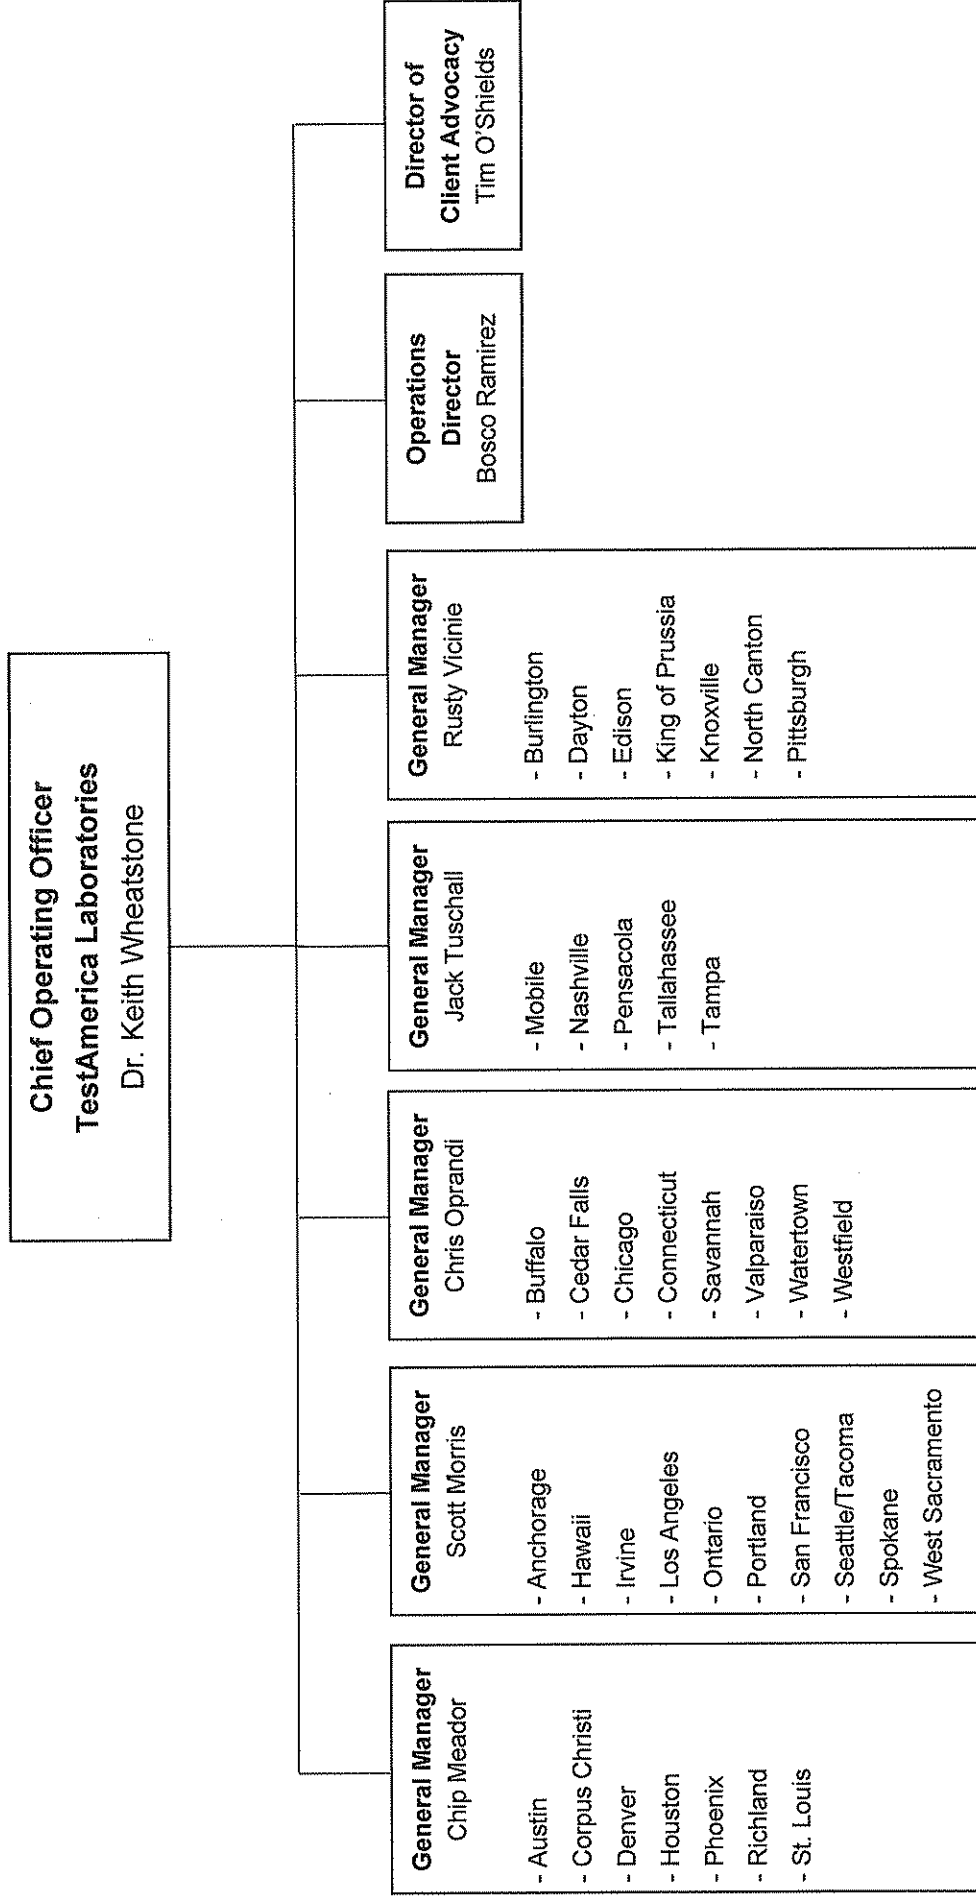

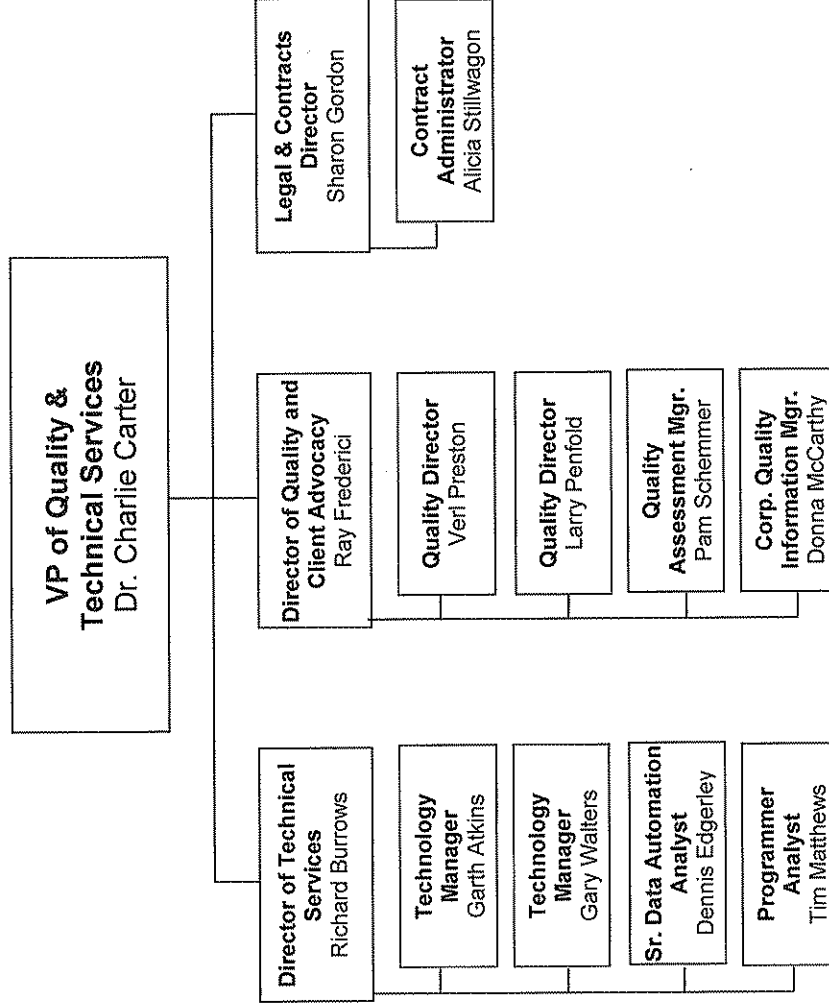

Note: QA Managers a dotted line reporting relationship to Corporate QA.

TestAmerica Sample Acceptance Policy

All incoming work will be evaluated against the criteria listed below. Where applicable, data from any samples that do not meet the criteria listed below will be noted on the laboratory report defining the nature and substance of the variation. In addition the client will be notified either by telephone, fax or e-mail ASAP after the receipt of the samples.

- 1) Samples must arrive with labels intact with a Chain of Custody filled out completely. The following information must be recorded.
 - Client name, address, phone number and fax number (if available)
 - Project name and/or number
 - The sample identification
 - Date, time and location of sampling
 - The collectors name
 - The matrix description
 - The container description
 - The total number of each type of container
 - Preservatives used
 - Analysis requested
 - Requested turnaround time (TAT)
 - Any special instructions
 - Purchase Order number or billing information (e.g. quote number) if available
 - The date and time that each person received or relinquished the sample(s), including their signed name.
 - The date and time of receipt must be recorded between the last person to relinquish the samples and the person who receives the samples in the lab, and they must be exactly the same.
 - **Information must be legible**
- 2) Samples must be properly labeled.
 - Use durable labels (labels provided by TestAmerica are preferred)
 - Include a unique identification number
 - Include sampling date and time & sampler ID
 - Include preservative used.
 - Use indelible ink
 - **Information must be legible**
- 3) Proper sample containers with adequate volume for the analysis and necessary QC are required for each analysis requested. See TA Sample Container Guide.
- 4) Samples must be preserved according to the requirements of the requested analytical method (See TA Sample Container Guide). Most analytical methods require chilling samples to 4° C (other than water samples for metals analysis). For these methods, the criteria are met if the samples are chilled to below 6° C and above freezing (0°C). For methods with other temperature criteria (e.g. some bacteriological methods require ≤ 10 °C), the samples must arrive within ± 2° C of the required temperature or within the method specified range. **Note:** Samples that are hand delivered to the laboratory immediately after collection may not have had time to cool sufficiently. In this case the samples will be considered acceptable as long as there is evidence that the chilling process has begun (arrival on ice).

Continued on other side.

- Chemical preservation (pH) will be verified prior to analysis and the project manager will be notified immediately if there is a discrepancy. If analyses will still be performed, all affected results will be flagged to indicate improper preservation.
- 5) Sample Holding Times
- TestAmerica will make every effort to analyze samples within the regulatory holding time. Samples must be received in the laboratory with enough time to perform the sample analysis. Except for short holding time samples (< 48hr HT) sample must be received with at least 48 hrs (working days) remaining on the holding time for us to ensure analysis.
 - Analyses that are designated as "field" analyses (Odor, pH, Dissolved Oxygen, Disinfectant Residual; a.k.a. Residual Chlorine, and Redox Potential) should be analyzed ASAP by the field sampler prior to delivering to the lab. However, if the analyses are to be performed in the laboratory, TestAmerica will make every effort to analyze the samples within 24 hours from receipt of the samples in the testing laboratory. Samples for "field" analyses received after 4:00 pm on Friday or on the weekend will be analyzed no later than the next business day after receipt (Monday unless a holiday). Samples will remain refrigerated and sealed until the time of analysis. The actual times of all "field" sample analyses are noted on the "Short Hold Time Detail Report" in the final report. Only samples analyzed outside of these criteria will be qualified on the final report with an 'H' to indicate holding time exceedance.
- 6) All samples submitted for Volatile Organic analyses must have a Trip Blank submitted at the same time. TestAmerica will supply a blank with the bottle order.
- 7) The project manager will be notified if any sample is received in damaged condition TestAmerica will request that a sample be resubmitted for analysis.
- 8) Recommendations for packing samples for shipment.
- Pack samples in Ice rather than "Blue" ice packs.
 - Soil samples should be placed in plastic zip-lock bags. The containers often have dirt around the top and do not seal very well and are prone to intrusion from the water from melted ice.
 - Water samples would be best if wrapped with bubble-wrap or paper (newspaper, or paper towels work) and then placed in plastic zip-lock bags.
 - Fill extra cooler space with bubble wrap.

G:\Depts\QUALITY\FORMS\SMPACPT7.DOC

Drinking Water Sample Acceptance Policy / Sampling Instructions

Sample Acceptance Policy

All incoming work will be evaluated against the criteria listed below. Where applicable, data from any samples that do not meet the criteria listed below will be noted on the laboratory report defining the nature and substance of the variation. The project manager will be notified if any sample is received in damaged condition. TestAmerica will request that a sample be resubmitted for analysis.

1) Samples must arrive with labels intact with a Chain of Custody filled out completely. The following information must be recorded and **must be legible**.

- *Client name, address, phone number and fax number (if available)*
- *Project name/number and/or P.O. number*
- *Public Water System ID (if applicable)*
- *Indicate whether lab data are for State compliance purposes and/or State's EDT requirements*
- *Date, time and location of sampling*
- *The collectors name and signature*
- *Confirmation of acid preservation in the field for methods 524.2, 525.2 and 508.1*
- *The matrix description*
- *The total number of containers for each sample ID*
- *Analysis requested*
- *Requested turnaround time (TAT)*
- *Any special instructions*
- *The date and time that each person received or relinquished the sample(s), including their signed name.*

2) **Proper sample containers with adequate volume for the analysis and necessary QC are required for each analysis requested. Insufficient samples to meet the method QC requirements will result in notation in the analytical reports to reflect the anomaly.**

3) **Sample Holding Times**

TestAmerica will make every effort to analyze samples within the regulatory holding time. Samples must be received in the laboratory with enough time to perform the sample analysis. Except for short holding time samples (< 48hr HT) sample must be received with at least 48 hrs (working days) remaining on the holding time for us to ensure analysis.

Analyses that are "field" analyses (e.g. pH, DO, residual chlorine) will be analyzed within 24 hours from receipt of the samples in the laboratory. Field analyses samples received after 4:00 pm on Friday or on the weekend will be analyzed no later than the next business day after receipt (Monday unless a holiday).

4) Pack samples in Ice rather than "Blue" ice packs. Water samples would be best if wrapped with bubble-wrap or paper (newspaper, or paper towels work) and then placed in plastic zip-lock bags. Fill extra cooler space with bubble wrap.

Drinking Water 500 Series Sampling Instructions

- 1) The following are general sampling instructions for collection and maintenance of sample integrity prior to chemical testing for various parameters in drinking waters. Be sure to consult your Regulator and/or Project Plan for any other specific sampling instructions.
- 2) **Do not rinse bottles that are pre-preserved.**
- 3) The presence or absence of residual chlorine should be verified in the field prior to sample collection.
- 4) **Fill the additional 1-L containers (labeled "QC") that are provided to meet the Quality Control requirements for the analytical methods (duplicate and/or matrix spikes). Duplicates are required for UCMR requirements.**
- 5) **Wear gloves whenever handling acids. Recap the acid containers tightly after they're used and return them to TestAmerica for proper disposal.**
- 6) **Do not open unused containers and return them to TestAmerica.**

Parameter	Methodology	Sampling Instructions
Volatile Organics(524.2) 1,2,3 TCP (524.2 SIM) Chlorinated sources	EPA 524.2 EPA 524.2 SIM	Fill 3 40 mL-VOA vials (preserved w/ascorbic acid) with sample without any headspace. Carefully and quickly add the supplied HCL(5 drops=0.25 mL) to pH <2. Keep unopened Trip Blank with samples. Store all samples at 4 °C or less.
Volatile Organics (524) 1,2,3, TCP (524.2 SIM) Non-Chlorinated Sources	CA DHS 524.2 SIM	Fill 3 40 mL-VOA with HCL. Keep unopened Trip Blank with samples. Store all samples at 4 °C or less.
Total Trihalomethanes	EPA 524.2	Fill 3 40 mL-VOA vials (preserved w/sodium thiosulfate) with sample without any headspace. Keep unopened Trip Blank with samples. Store all samples at 4 °C or less.
EDB/DBCP	EPA 504.1	Fill 3 40 mL-VOA vials (preserved w/sodium thiosulfate) with sample without any headspace. Keep unopened Trip Blank with samples. Store all samples at 4 °C or less.
Organohalide Pesticides/PCBs	EPA 505	Fill 3 40 mL-VOA vials (preserved w/sodium thiosulfate) with sample. Store all samples at 4 °C or less.
Chlorinated Acids	EPA 515.4	Fill 1-250 mL amber glass (preserved w/sodium sulfite) with sample. Store all samples at 4 °C or less.
Semivolatle Organics	EPA 525.2	Fill 2 1-Liter glass-amber containers (preserved w/sodium sulfite) with sample. Carefully and quickly add the supplied HCL (3 mL) to pH <2. Store all samples at 4 °C or less.
Semivolatle Organics Nonchlorinated Sources	EPA 525.2	Fill 2 1-Liter glass-amber containers with HCL. Store all samples at 4 °C or less.
Carbamates	EPA 531.1	Fill 3 60 mL-VOA vials (preserved w/sodium thiosulfate & monochloroacetic acid) with sample. Store all samples at 4 °C or less.
Glyphosate	EPA 547.1	Fill 3 amber 60 mL-VOA vials (preserved w/sodium thiosulfate) with sample. Store all samples at 4 °C or less.
Endothall	EPA 548.1	Fill 1-1-Liter glass-amber container (preserved w/sodium thiosulfate) with sample. Seal the container and shake vigorously for 1 minute. Store all samples at 4°C or less.
Diquat/Paraquat	EPA 549.2	Fill 1-1-Liter PVC-amber container (preserved w/sodium thiosulfate & sulfuric acid) with sample. Store all samples at 4 °C or less.

Parameter	Methodology	Sampling Instructions
Haloacetic acids	EPA 552.2	Fill 3 60 mL-amber-VOA vials (preserved w/ammonium chloride) with sample. Seal the vials and agitate by hand for 1 minute. Store all samples at 4 °C or less.
Bacteriology (Coliform & HPC)	EPA 9215/21/23	Fill sterile 125 mL bottle (preserved w/sodium thiosulfate) with sample. Store all samples at 4 °C or less.
General Physical: (Color, Odor, Turbidity)	SM2120B, SM2150B, EPA180.1	Fill 500 mL clear glass bottle (unpreserved) with sample. Store all samples at 4 °C or less.
General Mineral: (Ca, Mg, Na, K, Fe, Cu, Mn, Zn, Hardness, Alkalinity, SO ₄ , Cl, NO ₃ , F, pH, EC, TDS, MBAS) Others that can be included: NO ₂ , CLO ₄	EPA 150.1, 300.0, 200.7 SM4500F, SM2320B, SM2340B, SM2510B, SM2540C, SM5540C	Fill 1-Liter clear poly bottle (unpreserved) with sample. [for non-metals] Fill 500 mL poly bottle (preserved w/nitric acid) with sample. [for metals] Store all samples at 4 °C or less.
Inorganic Chemical Group: Al, Sb, As, Ba, Be, Cd, Cr, Cu, CN, F, Pb, Hg, Ni, NO ₃ , NO ₂ , Se, TI	EPA 200.8, 300.0, SM4500-CN-C,E	This group can be run from the "General Mineral" bottles plus "Cyanide" bottle [total of 3 bottles]
Cyanide	SM4500-CN-C,E	Fill 500 mL poly bottle (preserved w/sodium hydroxide) with sample. If sample is from a chlorinated source, it must first be de-chlorinated with ascorbic acid. Store all samples at 4 °C or less.
Lead & Copper Rule	EPA 200.8	Fill 1-Liter poly bottle (un-preserved) "first-draw" sample. Samples will be acidified upon receipt at the laboratory. Acidification must be performed within 14 days of sampling.
Metals	EPA 200.8, 200.7	Fill 500 mL poly bottle (preserved w/nitric acid) with sample. Cooling is not required..
Total Organic Carbon	SM5310B	Fill 3 40 mL-VOA vials (preserved w/hydrochloric acid) with sample without any headspace. Store all samples at 4 °C or less.
Perchlorate	EPA 314.0	Fill 500 mL poly bottle (unpreserved) with sample. Store all samples at 4 °C or less.
Radiochemistry – Gross Alpha	EPA 900.0	Fill 500 mL poly bottle (preserved w/nitric acid) with sample. Cooling is not required.
Radiochemistry – Gross Beta	EPA 900.0	Can be run from above bottle
Radiochemistry – Uranium	EPA 200.8	Fill 500 mL poly bottle (preserved w/nitric acid) with sample. Cooling is not required.
Radiochemistry – Uranium	ASTM D5174	Fill 500 mL poly bottle (preserved w/nitric acid) with sample. Cooling is not required.
Radiochemistry – Radium 226	EPA 903.1	Fill 1-Liter poly bottle (preserved w/nitric acid) with sample. Cooling is not required.
Radiochemistry – Radium 228	EPA 904.0	Fill 2 1-Liter poly bottle (preserved w/nitric acid) with sample. Cooling is not required.
Radiochemistry – Strontium 90	EPA 905.0	Fill 1-Liter poly bottle (preserved w/nitric acid) with sample. Cooling is not required.
Radiochemistry – Tritium	EPA 906.0	Fill 250 mL glass bottle (unpreserved) with sample. Cooling is not required.
Radiochemistry – Radon	ASTM D5072	Fill 2 40 mL-VOA vials (un-preserved) with sample without any headspace. Cooling is not required.
Asbestos	EPA 100.2	Fill 1-Liter poly bottle (un-preserved) with sample. Cooling is not required.
Dioxin (2,3,7,8-TCDD)	EPA 1613B	Fill 2 1-Liter glass-amber containers (un-preserved) with sample. Store all samples at 4 °C or less.

PROJECT RECEIPT CHECKLIST

Client: _____ Project: _____

Element ID : _____

Received by: _____ Date/Time Received: _____

Delivered by : Client TA-Courier DHL Fed Ex UPS Other _____

***** Initial / Date

Custody Seal Status Cooler: Intact Broken None _____

Custody Seal Status Samples: Intact Broken None _____

COC present Yes No _____

Sampler name on COC Yes No N/A..... _____

All signatures present on COC Yes No N/A..... _____

Number of coolers: _____

Cooler temperature(s) in °C: _____

Samples outside temperature criteria but received on ice: Yes N/A... _____

Short hold present? Yes No _____

Turn Around Time: SAME DAY RUSH-24HR RUSH-48HR

RUSH-72HR NORMAL..... _____

Anomalies: No Yes – See NOD _____


Number of containers in cooler(s): _____

Number of containers on chain of custody(s) _____

Did Chain of custody(s) agree with sample labels ID's: Yes No – See NOD _____

Labeled..... _____

Irvine Organizational Chart

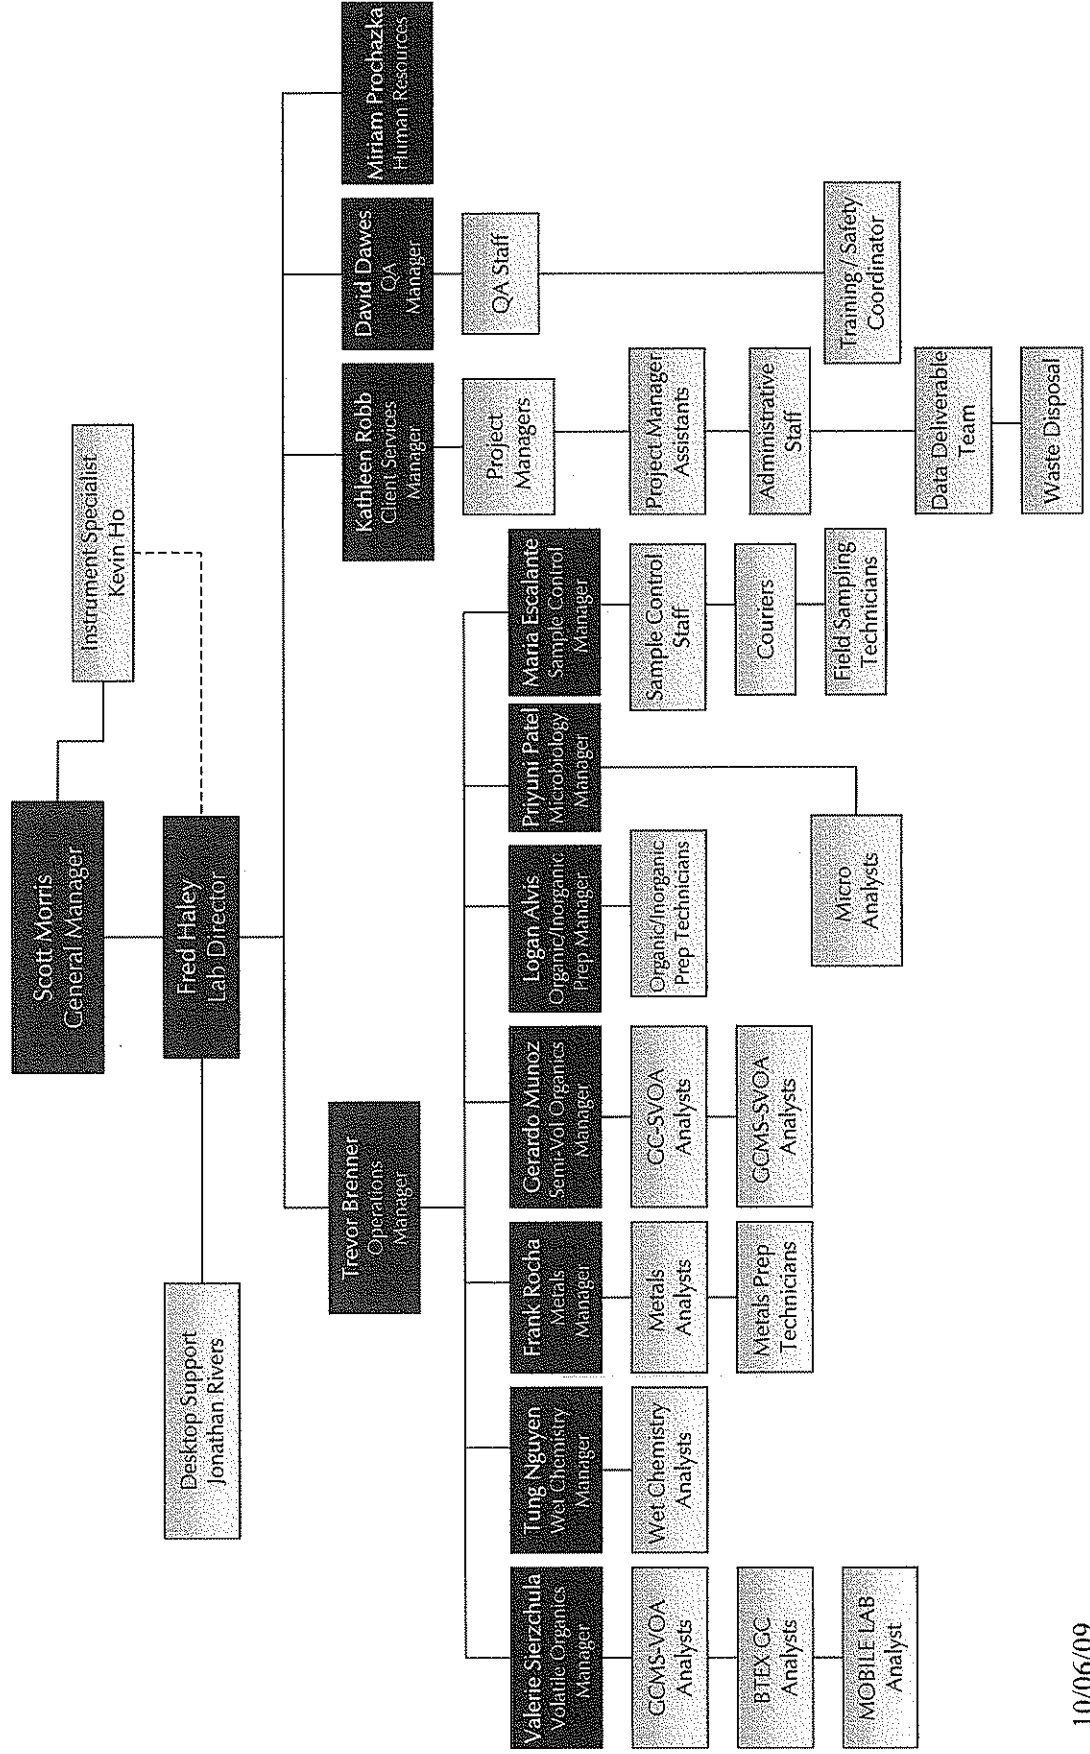

Cover Page:

Quality Assurance Manual

TestAmerica Irvine
17461 Derian Avenue, Suite 100
Irvine, CA 92614
Tel 949-261-1022
Fax 949-260-3299
www.testamericainc.com

Copyright Information:

This documentation has been prepared by TestAmerica Laboratories, Inc. and its affiliates ("TestAmerica"), solely for their own use and the use of their customers in evaluating their qualifications and capabilities in connection with a particular project. The user of this document agrees by its acceptance to return it to TestAmerica upon request and not to reproduce, copy, lend, or otherwise disclose its contents, directly or indirectly, and not to use it for any other purpose other than that for which it was specifically provided. The user also agrees that where consultants or other outside parties are involved in the evaluation process, access to these documents shall not be given to said parties unless those parties also specifically agree to these conditions.

THIS DOCUMENT CONTAINS VALUABLE CONFIDENTIAL AND PROPRIETARY INFORMATION. DISCLOSURE, USE OR REPRODUCTION OF THESE MATERIALS WITHOUT THE WRITTEN AUTHORIZATION OF TESTAMERICA IS STRICTLY PROHIBITED. THIS UNPUBLISHED WORK BY TESTAMERICA IS PROTECTED BY STATE AND FEDERAL LAW OF THE UNITED STATES. IF PUBLICATION OF THIS WORK SHOULD OCCUR THE FOLLOWING NOTICE SHALL APPLY:

















©COPYRIGHT 2007 TESTAMERICA INC. ALL RIGHTS RESERVED

Facility Distribution No. _____

Distributed To: _____

Title Page:

**Quality Assurance Manual
Approval Signatures**

 _____ Laboratory Director – Fred Haley	 _____ Date 1/30/08
 _____ Quality Manager - David Dawes	 _____ Date 1/30/08
 _____ Technical Director, Semivolatiles – Gerardo Muñoz	 _____ Date 1/30/08
 _____ Technical Director, Volatiles – Valerie Sierzchula	 _____ Date 1/30/08
 _____ Technical Director, Metals – Denny Tran	 _____ Date 1/30/08
 _____ Technical Director, Wet Chemistry – Tung Nguyen	 _____ Date 1/30/08
 _____ Technical Director, Inorganic Prep – Jim Blustein	 _____ Date 1/30/08
 _____ Technical Director, Organic Prep – Michelle Castro	 _____ Date 1/30/08

SECTION 2

TABLE OF CONTENTS

Section No.	Title	Page No.	Effective Date
-	COVER PAGE	COVER	01/31/2008
1.0	TITLE PAGE	1-1	01/31/2008
2.0	SECTION 2	2-1	01/31/2008
3.0	INTRODUCTION	3-1	01/31/2008
3.1	Introduction And Compliance References	3-1	01/31/2008
3.2	Terms And Definitions	3-1	01/31/2008
3.3	Scope / Fields Of Testing	3-1	01/31/2008
3.4	Management Of The Manual	3-2	01/31/2008
4.0	ORGANIZATION AND MANAGEMENT (NELAC 5.4.1)	4-1	01/31/2008
4.1	Overview	4-1	01/31/2008
4.2	Roles And Responsibilities	4-2	01/31/2008
4.3	Deputies	4-13	01/31/2008
5.0	QUALITY SYSTEM (NELAC 5.4.2)	5-1	01/31/2008
5.1	Quality Policy Statement	5-1	01/31/2008
5.2	Ethics And Data Integrity	5-1	01/31/2008
5.3	Quality System Supporting Documentation	5-2	01/31/2008
5.4	Qa/Qc Objectives For The Measurement Of Data	5-3	01/31/2008
5.5	Criteria For Quality Indicators	5-5	01/31/2008
5.6	Statistical Quality Control	5-5	01/31/2008
5.7	Quality System Metrics	5-6	01/31/2008
6.0	DOCUMENT CONTROL (NELAC 5.4.3)	6-1	01/31/2008
6.1	Overview	6-1	01/31/2008
6.2	Document Approval And Issue	6-1	01/31/2008
6.3	Procedures For Document Control Policy	6-2	01/31/2008
6.4	Obsolete Documents	6-3	01/31/2008
7.0	REVIEW OF WORK REQUEST	7-1	01/31/2008
7.1	Overview	7-1	01/31/2008
7.2	Review Sequence And Key Personnel	7-2	01/31/2008
7.3	Documentation	7-3	01/31/2008
8.0	SUBCONTRACTING OF TESTS (NELAC 5.4.5)	8-1	01/31/2008
8.1	Overview	8-1	01/31/2008
8.2	Qualifying And Monitoring Subcontractors	8-1	01/31/2008
8.3	Oversight And Reporting	8-4	01/31/2008
8.4	Contingency Planning	8-5	01/31/2008
9.0	PURCHASING SERVICES AND SUPPLIES (NELAC 5.4.6)	9-1	01/31/2008
9.1	Overview	9-1	01/31/2008
9.2	Glassware	9-1	01/31/2008
9.3	Reagents, Standards & Supplies	9-1	01/31/2008

Section No.	Title	Page No.	Effective Date
9.4	Purchase Of Equipment/Instruments/Software	9-3	01/31/2008
9.5	Services	9-4	01/31/2008
9.6	Suppliers	9-4	01/31/2008
10.0	SERVICE TO THE CLIENT (NELAC 5.4.7)	10-1	01/31/2008
10.1	Overview	10-1	01/31/2008
10.2	Special Services	10-1	01/31/2008
10.3	Client Communication	10-1	01/31/2008
10.4	Reporting	10-1	01/31/2008
10.5	Client Surveys	10-2	01/31/2008
11.0	COMPLAINTS (NELAC 5.4.8)	11-1	01/31/2008
11.1	Overview	11-1	01/31/2008
11.2	External Complaints	11-1	01/31/2008
11.3	Internal Complaints	11-2	01/31/2008
11.4	Management Review	11-2	01/31/2008
12.0	CONTROL OF NON-CONFORMING WORK (NELAC 5.4.9)	12-1	01/31/2008
12.1	Overview	12-1	01/31/2008
12.2	Responsibilities And Authorities	12-1	01/31/2008
12.3	Evaluation Of Significance And Actions Taken	12-2	01/31/2008
12.4	Prevention Of Nonconforming Work	12-2	01/31/2008
12.5	Method Suspension/Restriction (Stop Work Procedures)	12-2	01/31/2008
13.0	CORRECTIVE ACTION (NELAC 5.4.10)	13-1	01/31/2008
13.1	Overview	13-1	01/31/2008
13.2	Definitions	13-1	01/31/2008
13.3	General	13-1	01/31/2008
13.4	Closed Loop Corrective Action Process	13-2	01/31/2008
13.5	Technical Corrective Actions	13-3	01/31/2008
13.6	Basic Corrections	13-4	01/31/2008
14.0	PREVENTIVE ACTION (NELAC 5.4.11)	14-1	01/31/2008
14.1	Overview	14-1	01/31/2008
14.2	Management Of Change	14-2	01/31/2008
15.0	CONTROL OF RECORDS (NELAC 5.4.12)	15-1	01/31/2008
15.1	Overview	15-1	01/31/2008
15.2	Technical And Analytical Records	15-4	01/31/2008
15.3	Laboratory Support Activities	15-5	01/31/2008
15.4	Administrative Records	15-5	01/31/2008
15.5	Records Management, Storage And Disposal	15-6	01/31/2008
16.0	AUDITS (NELAC 5.4.13)	16-1	01/31/2008
16.1	Overview	16-1	01/31/2008
16.2	Technical And Analytical Records	16-1	01/31/2008
16.3	External Audits	16-3	01/31/2008
16.4	Audit Findings	16-5	01/31/2008
17.0	MANAGEMENT REVIEWS (NELAC 5.4.14)	17-1	01/31/2008
17.1	Quality Assurance Report	17-1	01/31/2008
17.2	Annual Management Review	17-2	01/31/2008

Section No.	Title	Page No.	Effective Date
17.3	Potential Integrity Related Managerial Reviews	17-3	01/31/2008
18.0	PERSONNEL (NELAC 5.5.2)	18-1	01/31/2008
18.1	Overview	18-1	01/31/2008
18.2	Education And Experience Requirements For Technical Personnel	18-1	01/31/2008
18.3	Training	18-3	01/31/2008
18.4	Data Integrity And Ethics Training Program	18-4	01/31/2008
19.0	ACCOMMODATIONS AND ENVIRONMENTAL CONDITIONS (NELAC 5.5.3)	19-1	01/31/2008
19.1	Overview	19-1	01/31/2008
19.2	Environment	19-1	01/31/2008
19.3	Work Areas	19-2	01/31/2008
19.4	Floor Plan	19-2	01/31/2008
19.5	Building Security	19-3	01/31/2008
20.0	01/31/2008 (NELAC 5.5.4)	20-1	01/31/2008
20.1	Overview	20-1	01/31/2008
20.2	STANDARD OPERATING PROCEDURES (Sops)	20-1	01/31/2008
20.3	Laboratory Methods Manual	20-1	01/31/2008
20.4	Selection Of Methods	20-2	01/31/2008
20.5	Laboratory Developed Methods And Non-Standard Methods	20-5	01/31/2008
20.6	Validation Of Methods	20-5	01/31/2008
20.7	Method Detection Limits (Mdl)/ Limits Of Detection (Lod)	20-7	01/31/2008
20.8	Instrument Detection Limits (Idl)	20-8	01/31/2008
20.9	Verification Of Detection And Reporting Limits	20-8	01/31/2008
20.10	Retention Time Windows	20-9	01/31/2008
20.11	Evaluation Of Selectivity	20-10	01/31/2008
20.12	Estimation Of Uncertainty Of Measurement	20-10	01/31/2008
20.13	Control Of Data	20-11	01/31/2008
21.0	EQUIPMENT (AND CALIBRATIONS) (NELAC 5.5.5)	21-1	01/31/2008
21.1	Overview	21-1	01/31/2008
21.2	Preventive Maintenance	21-1	01/31/2008
21.3	Support Equipment	21-3	01/31/2008
21.4	Instrument Calibrations	21-5	01/31/2008
21.5	Policy On Tentatively Identified Compounds (Tics) – Gc/Ms Analysis	21-13	01/31/2008
21.6	Policy On Gc/Ms Tuning	21-14	01/31/2008
22.0	MEASUREMENT TRACEABILITY (NELAC 5.5.6)	22-1	01/31/2008
22.1	Overview	22-1	01/31/2008
22.2	Nist-Traceable Weights And Thermometers	22-2	01/31/2008
22.3	Reference Standards / Materials	22-2	01/31/2008
22.4	Documentation And Labeling Of Standards, Reagents, And Reference Materials	22-2	01/31/2008
23.0	SAMPLING (NELAC 5.5.7)	23-1	01/31/2008
23.1	Overview	23-1	01/31/2008

Section No.	Title	Page No.	Effective Date
23.2	Sampling Containers	23-1	01/31/2008
23.3	Field Quality Control (Qc)	23-2	01/31/2008
23.4	Definition Of Holding Time	23-2	01/31/2008
23.5	Sampling Containers, Preservation Requirements, Holding Times	23-3	01/31/2008
23.6	Sample Aliquots / Subsampling	23-3	01/31/2008
24.0	HANDLING OF SAMPLES (NELAC 5.5.8)	24-1	01/31/2008
24.1	Chain Of Custody (Coc)	24-1	01/31/2008
24.2	Sample Receipt	24-2	01/31/2008
24.3	Sample Acceptance Policy	24-4	01/31/2008
24.4	Sample Storage	24-5	01/31/2008
24.5	Hazardous Samples And Foreign Soils	24-5	01/31/2008
24.6	Sample Shipping	24-6	01/31/2008
24.7	Sample Disposal	24-6	01/31/2008
25.0	ASSURING THE QUALITY OF TEST RESULTS (NELAC 5.5.9)	25-1	01/31/2008
25.1	Overview	25-1	01/31/2008
25.2	Controls	25-1	01/31/2008
25.3	Negative Controls	25-1	01/31/2008
25.4	Positive Controls	25-2	01/31/2008
25.5	Sample Matrix Controls	25-4	01/31/2008
25.6	Acceptance Criteria (Control Limits)	25-6	01/31/2008
25.7	METHOD DETECTION LIMITS (Mdl)	25-8	01/31/2008
25.8	Additional Procedures To Assure Quality Control	25-8	01/31/2008
26.0	REPORTING RESULTS (NELAC 5.5.10)	26-1	01/31/2008
26.1	Overview	26-1	01/31/2008
26.2	Test Reports	26-1	01/31/2008
26.3	Reporting Level Or Report Type	26-3	01/31/2008
26.4	Electronic Reporting And Signature Policy	26-4	01/31/2008
26.5	Supplemental Information For Test	26-5	01/31/2008
26.6	Environmental Testing Obtained From Subcontractors	26-7	01/31/2008
26.7	Client Confidentiality	26-7	01/31/2008
26.8	Format Of Reports	26-7	01/31/2008
26.9	Amendments To Test Reports	26-8	01/31/2008
26.10	Policies On Client Requests For Amendments	26-8	01/31/2008

LIST OF TABLES

Table No.	Title	Page	Effective Date
9-1	<u>Storage of Reagents and Chemicals</u>	9-7	01/31/2008
13-1	<u>Example - General Corrective Action Procedures</u>	13-7	01/31/2008
15-1	<u>Record Index</u>	15-1	01/31/2008
15-2	<u>Special Record Retention Requirements</u>	15-2	01/31/2008
16-1	<u>Audit Types and Frequency</u>	16-1	01/31/2008
20-1	<u>Laboratory SOPs by Department and Method</u>	20-19	01/31/2008
21-1	<u>Example - Laboratory Equipment & Instrumentation</u>	21-17	01/31/2008
21-2	<u>Example – Schedule of Routine Maintenance</u>	21-28	01/31/2008
21-3	<u>Example – Periodic Calibration</u>	21-30	01/31/2008
22-1	<u>Example – Standard Source & Preparation</u>	22-1	01/31/2008
23-1	<u>Holding Times, Preservation and Container Requirements - Drinking Water (SDWA)</u>	23-5	01/31/2008
23-2	<u>Holding Times, Preservation and Container Requirements - NPDES – Bacteria, Protozoa, Toxicity Tests</u>	23-8	01/31/2008
23-3	<u>Holding Times, Preservation and Container Requirements - NPDES – Inorganic</u>	23-9	01/31/2008
23-4	<u>Holding Times, Preservation and Container Requirements - NPDES – Organic</u>	23-12	01/31/2008
23-5	<u>Holding Times, Preservation and Container Requirements - NPDES - Radiological</u>	23-14	01/31/2008
23-6	<u>Holding Times, Preservation and Container Requirements - RCRA – Aqueous</u>	23-15	01/31/2008
23-7	<u>Holding Times, Preservation and Container Requirements - RCRA – Non-Aqueous</u>	23-17	01/31/2008
23-8	<u>Holding Times, Preservation and Container Requirements - Air Samples</u>	23-19	01/31/2008

LIST OF FIGURES

Figure No.	Title	Page	Effective Date
3-1	<u>Example - Format for a QA/QC Policy Memorandum</u>	3-4	01/31/2008
4-1	<u>Corporate Organizational Chart</u>	4-15	01/31/2008
8-1	<u>Example - Client-Approved Subcontractor Form</u>	8-7	01/31/2008
8-2	<u>Example - Subcontracting Laboratory Approval Form (Initial / Renewal)</u>	8-8	01/31/2008
8-3	<u>Example - Subcontracted Sample Form</u>	8-9	01/31/2008
9-1	<u>Materials Request Sheet</u>	9-6	01/31/2008
9-2	<u>Example - JD Edwards Vendor Add Request Form</u>	9-8	01/31/2008
9-3	<u>New Instrumentation Checklist</u>	9-9	01/31/2008
13-1a & b	<u>Example - Corrective Action Report</u>	13-5	01/31/2008
16-1	<u>Example - Internal Audit Workbook</u>	16-7	01/31/2008
16-2	<u>Example – Internal Audit System Checklist</u>	16-8	01/31/2008
16-3	<u>Example – External Audit Database—individual finding</u>	16-9	01/31/2008
17-1	<u>Example - QA Monthly Report to Management</u>	17-4	01/31/2008
17-2	<u>Example – Laboratory Metrics Categories</u>	17-6	01/31/2008
20-1	<u>Example – Demonstration of Capability Documentation</u>	20-24	01/31/2008
20-2	<u>Example – New Method / Additional Analyte Checklist</u>	20-25	01/31/2008
20-3	<u>Work Flow</u>	20-27	01/31/2008
24-1	<u>Example – Chain of Custody</u>	24-8	01/31/2008
24-2	<u>Example - Custody Seal</u>	24-9	01/31/2008
24-3	<u>Example – Internal Chain of Custody Form</u>	24-10	01/31/2008
24-4	<u>Example – Sample Disposal Record</u>	24-11	01/31/2008

Figure No.	Title	Page	Effective Date
24-5	<u>Example – Sample Acceptance Policy</u>	24-12	01/31/2008
24-6	<u>Example – Cooler Receipt Form</u>	24-13	01/31/2008
24-7	<u>Example – Notification of Discrepancy (NOD)</u>	25-14	01/31/2008
26-1	<u>Read and Understand Memo for: Electronic Reporting and Electronic Signatures Policy</u>	26-10	01/31/2008
26-2	<u>Agreement for Electronic Reports</u>	26-11	01/31/2008

LIST OF APPENDICES

Appendix No.	Title	Page	Effective Date
1	<u>TestAmerica Ethics Policy No. CA-L-P-001</u>	Appendix 1-1	01/31/2008
2	<u>Example - Laboratory Organization Chart</u>	Appendix 2-1	01/31/2008
3	<u>Laboratory Floor Plan</u>	Appendix 3-1	01/31/2008
4	<u>Summary of Calibration, QC Procedures and Corrective Action</u>	Appendix 4-1	01/31/2008
5	<u>Glossary / Acronyms</u>	Appendix 5-1	01/31/2008
6	<u>Laboratory Certifications, Accreditations, Validations</u>	Appendix 6-1	01/31/2008
7	<u>Data Qualifiers</u>	Appendix 7-1	01/31/2008

SOPs AND POLICIES REFERRED TO IN THE QA MANUAL

SOP/Policy Reference	Title
CA-Q-S-001	Solvent and Acid Lot Testing and Approval
CA-Q-S-002	Acceptable Manual Integration Practices
CA-Q-S-003	Management of Change Procedure
CA-Q-S-004	Method Compliance & Data Authenticity Audits
CA-Q-S-005	Calibration Curves (General)
CW-Q-S-001	Corporate Document Control and Archiving
CW-Q-S-002	Writing a Standard Operating Procedure (SOPs)
CA-L-S-001	Internal Investigation of Potential Data Discrepancies and Determination for Data Recall
CA-L-S-002	Subcontracting Procedures
CA-L-P-001	Ethics Policy
CA-L-P-002	Contract Compliance Policy
CW-L-P-001	Record Retention
CW-F-P-002	Authorization Matrix
CA-C-S-001	Work Sharing Process
CA-T-P-001	Qualified Products List
CW-F-S-004	Controlled Purchases Policy
IR-QA-DOC	Document Control and Review
CNTRLLIM.SOP	Control Charts and Statistical Process Control
LOTTEST.SOP	Container and Reagent Verification by Lot Testing
CAR.SOP	Corrective Actions
TRAINING.SOP	Training and Documentation

SOP/Policy Reference	Title
MDL.SOP	Determination of Method Detection Limits
LOGIN.SOP	Sample Control
DATAREV.SOP	General Data Review
PMDATA.SOP	Project Management Data Reporting, Validation and Distribution
BAL.SOP	Balance Calibration, Verification and Documentation
THERMA.SOP	Thermometer Calibration/Temperature Monitoring and Documentation
IR-QA-STD	Reagent and Standard Preparation, Control, and Documentation
FIELD.SOP	Field Sampling
LOTTEST.SOP	Container and Reagent Verification by Lot Testing
SUBSAMP.SOP	Subsampling
REFBLANK.SOP	Refrigerator Storage Blank
COMPSECU.SOP	Computer Security
PIP.SOP	Pipet Calibration
ARCHIV.SOP	Record Archiving

SECTION 3

INTRODUCTION (NELAC 5.1 - 5.3)

3.1 INTRODUCTION AND COMPLIANCE REFERENCES

Test America Irvine's Quality Assurance Manual (QAM) is a document prepared to define the overall policies, organization objectives and functional responsibilities for achieving TestAmerica's data quality goals. Each TestAmerica laboratory maintains a local perspective in its scope of services and client relations and maintains a national perspective in terms of quality.

The QAM has been prepared to assure compliance with the 2003 National Environmental Laboratory Accreditation Conference (NELAC) standards and ISO/IEC Guide 17025 (1999). In addition, the policies and procedures outlined in this manual are compliant with the various accreditation and certification programs listed in Appendix 6. The relevant NELAC section is included in the heading of each QAM section.

The QAM has been prepared to be consistent with the requirements of the following documents:

- EPA 600/4-88/039, *Methods for the Determination of Organic Compounds in Drinking Water*, EPA, Revised July 1991.
- EPA 600/R-95/131, *Methods for the Determination of Organic Compounds in Drinking Water*, Supplement III, EPA, August 1995.
- EPA 600/4-79-019, *Handbook for Analytical Quality Control in Water and Wastewater Laboratories*, EPA, March 1979.
- EPA SW-846, *Test Methods for the Evaluation of Solid Waste*, 3rd Edition, September 1986; Update I, July 1992; Update II, September 1994; and Update III, December 1996.
- Federal Register, 40 CFR Parts 136, 141, 172, 173, 178, 179 and 261.
- APHA, *Standard Methods for the Examination of Water and Wastewater*, 18th Edition, 19th, 20th and 21st Edition.

3.2 TERMS AND DEFINITIONS

A Quality Assurance Program is a company-wide system designed to ensure that data produced by TestAmerica Irvine conforms to the standards set by state and/or federal regulations. The program functions at the management level through company goals and management policies, and at the analytical level through Standard Operating Procedures (SOPs) and quality control. The TestAmerica program is designed to minimize systematic error, encourage constructive, documented problem solving, and provide a framework for continuous improvement within the organization.

Refer to Appendix 5 for the Glossary/Acronyms.

3.3 SCOPE / FIELDS OF TESTING

TestAmerica Irvine analyzes thousands of environmental and industrial samples every month. Sample matrices vary among air, drinking water, effluent water, groundwater, hazardous waste,

sludge and soils. The Quality Assurance Program contains specific procedures and methods to test samples of differing matrices for chemical, physical and biological parameters. The Program also contains guidelines on maintaining documentation of analytical process, reviewing results, servicing clients and tracking samples through the laboratory. The technical and service requirements of all requests to provide analyses are thoroughly evaluated before commitments are made to accept the work. Measurements are made using published reference methods or methods developed and validated by the laboratory.

The methods covered by this manual include the most frequently requested water, air, industrial waste, and soil methodologies needed to provide analytical services in the United States and its territories. The specific list of test methods used by the laboratory can be found in [Appendix 4](#). The approach of this manual is to define the minimum level of quality assurance and quality control necessary to meet requirements. All methods performed by TestAmerica Irvine shall meet these criteria as appropriate. In some instances, quality assurance project plans (QAPPs), project specific data quality objectives (DQOs) or local regulations may require criteria other than those contained in this manual. In these cases, the laboratory will abide by the requested criteria following review and acceptance of the requirements by the Laboratory Director and the Quality Assurance (QA) Manager. In some cases, QAPPs and DQOs may specify less stringent requirements. The Laboratory Director and the QA Manager must determine if it is in the lab's best interest to follow the less stringent requirements.

3.4 MANAGEMENT OF THE MANUAL

3.4.1 Review Process

The manual is reviewed annually by the QA Manager and laboratory personnel to assure that it reflects current practices and meets the requirements of TestAmerica Irvine's clients and regulators. Occasionally, the manual may need changes in order to meet new or changing regulations and operations. The QA Manager will review the changes in the normal course of business and incorporate changes into revised sections of the document. The updates will be reviewed by the QA Manager, Laboratory Director, Technical Director(s), relevant operational staff and Corporate Quality Assurance (if a change is made to the Corporate template) and then formally incorporated into the document in periodic updates. The QAM is based on a Corporate QAM Template that is prepared and approved by the Chief Operating Officers (COOs) and Corporate Quality Assurance. This template is reviewed annually by the COOs, Corporate Quality, and each laboratory. Necessary changes are coordinated by the Vice President of Quality and Environmental Health & Safety (EHS) and distributed to each laboratory for inclusion in the laboratory specific QA Manuals.

Policies in the QAM that require immediate attention may be addressed through the use of Corporate QA/QC Policy Memoranda. QA/QC Policy Memoranda are published from time to time to facilitate immediate changes to QA/QC Policy. QA/QC Policy Memoranda supersede the QAM and all other SOPs (refer to Section 5.3). All policy memoranda are dated, archived and distributed by their placement into the front of the QAM between the signature page and Section 2. At a minimum, each policy memorandum is approved by the same authorized signatories as shown on the cover page of the QA Manual. In addition, Corporate QA/QC Policy Memoranda are signed by the COOs and VP of Quality and EHS. The QA/QC Policy Memoranda are incorporated into the QAM during the periodic updates. Policy memorandum

may also include an expiration date if appropriate. An example format can be found in Figure 3-1. A similar procedure is followed for local laboratory changes.

Laboratory-specific QAM changes are approved and documented through the Management of Change process (Refer to SOP No. CA-Q-S-003, Management of Change Procedure).

3.4.2 Control

This manual is considered confidential within TestAmerica and may not be altered in any manner by other than a duly appointed representative from TestAmerica. If the document has been provided to external users or regulators, it is for the exclusive purpose of reviewing TestAmerica Irvine's quality systems and shall not be used in any other way without the written permission of an appointed representative of TestAmerica. [The procedure for control of distribution is incorporated by reference to the current revision of the laboratory's SOP, IR-QA-DOC \(Document Control and Review\).](#)

The order of precedence in the event of a conflict between policies is outlined in Section 5.3 of this Quality Assurance Manual.

Figure 3-1.

Example - Format for a QA/QC Policy Memorandum

Corporate (or Laboratory) QA/QC Policy Memorandum # _____

Effective Date: _____ Expiration Date: When Appropriate QAM Section is Revised

Corporate: <i>(Only needed for Corporate Memorandum – Delete if Laboratory)</i>			
COO - West	Date	Vice-President, QA and EHS	Date
COO - East	Date		
Local:			
Laboratory Director Approval	Date	Quality Assurance Approval	Date
Technical Director Approval	Date	Technical Director Approval	Date
Technical Director Approval	Date	Technical Director Approval	Date
Technical Director Approval	Date	Technical Director Approval	Date

1. **Purpose**

2. **Procedure**

3. **Attachments**

4. **References/Cross References**

SECTION 4

ORGANIZATION AND MANAGEMENT (NELAC 5.4.1)

4.1 OVERVIEW

TestAmerica Irvine is part of a national network of laboratories known as TestAmerica. This Quality Assurance Manual (QAM) is applicable to the TestAmerica Irvine laboratory only.

TestAmerica Irvine
17461 Derian Avenue, Suite 100
Irvine, CA 92614
Tel 949-261-1022
Fax 949-260-3299
EPA Lab ID CA01531

The Corporate organization chart can be found in Figure 4-1 and the laboratory's organization chart can be found in Appendix 2. The locations of other TestAmerica labs are as follows:

Aerotech Environmental Laboratories (AEL)
TestAmerica Anchorage
TestAmerica Austin
TestAmerica Buffalo
TestAmerica Buffalo Grove
TestAmerica Burlington
TestAmerica Cedar Falls
TestAmerica Chicago
TestAmerica Connecticut
TestAmerica Corpus Christi
TestAmerica Dayton
TestAmerica Denver
TestAmerica Edison
TestAmerica Honolulu
TestAmerica Houston
TestAmerica King of Prussia
TestAmerica Knoxville
TestAmerica Los Angeles
TestAmerica Mobile
TestAmerica Morgan Hill
TestAmerica Nashville
TestAmerica North Canton
TestAmerica Ontario
TestAmerica Orlando
TestAmerica Pensacola
TestAmerica Phoenix
TestAmerica Pittsburgh
TestAmerica Portland
TestAmerica Richland

TestAmerica San Francisco
TestAmerica Savannah
TestAmerica Seattle
TestAmerica Spokane
TestAmerica St. Louis
TestAmerica Tacoma
TestAmerica Tallahassee
TestAmerica Tampa
TestAmerica Valparaiso
TestAmerica Watertown
TestAmerica West Sacramento
TestAmerica Westfield

4.2 ROLES AND RESPONSIBILITIES

In order for the Quality Assurance Program to function properly, all members of the staff must clearly understand and meet their individual responsibilities as they relate to the quality program. The following descriptions define each role in its relationship to the Quality Assurance Program.

4.2.1 Quality Assurance Program

The responsibility for quality lies with every employee of TestAmerica Irvine. All employees have access to the QAM and are responsible for knowing the content of this manual and upholding the standards therein. Each person carries out his/her daily tasks in a manner consistent with the goals and in accordance with the procedures in this manual and the laboratory's SOPs.

4.2.2 President/Chief Executive Officer (CEO)

The President/CEO is a member of the Board of Directors and is ultimately responsible for the quality and performance of all TestAmerica facilities. The President/CEO establishes the overall quality standard and data integrity program for the Analytical Division, providing the necessary leadership and resources to assure that the standard and integrity program are met.

4.2.3 Chief Operating Officer (COO)

The COO serves as the ranking executive for all respective analytical laboratory operational functions and reports to the President/CEO of the Analytical Division. The COO is responsible for the daily management of all analytical laboratories, long-term planning and development of technical policies and management plans. The COO ensures the attainment of corporate objectives through the selection, development, motivation, and evaluation of top management personnel. The COO approves all operating budgets and capital expenditures. The COO signs-off on the final QAM template that contains company policies for implementing the Quality Program

4.2.4 General Manager (GM)

Each GM reports directly to the COO. Each GM has full responsibility for the overall administrative and operational management of their respective laboratories. The GM's responsibilities include allocation of personnel and resources, long-term planning, setting goals, and achieving the financial, business, and quality objectives of TestAmerica. The GM ensures timely compliance with corporate management directives, policies, and management systems reviews. The GM is also responsible for restricting any laboratory from performing analyses that cannot be consistently and successfully performed to meet the standards set forth in this manual.

4.2.5 Vice President of Client and Technical Services

The Vice President (VP) of Client and Technical Services reports directly to the President/CEO and is responsible for offerings to clients including quality assurance, environmental health and safety, risk management, technical assistance, legal compliance and contract administration. The VP of Client and Technical Services provides support and direction to the Executive Director and Directors of these areas, and supports the COO in decisions regarding long term planning, resource allocation and capital expenditures.

4.2.6 Executive Director of Quality and Environmental Health and Safety (QA/EHS)

The Executive Director of QA/EHS reports to the VP of Client and Technical Services. With the aid of the Senior Management Team, Laboratory Director/ Managers, Quality Directors, EHS Directors, QA Managers and EHS Coordinators, the Executive Director-QA/EHS has the responsibility for the establishment, general overview and Corporate maintenance of the Quality Assurance and Environmental, Health and Safety Program within TestAmerica. Additional responsibilities include:

- Review of QA/QC aspects of Corporate SOPs, national projects and expansions or changes in services.
- Coordination/preparation of the Corporate QAM Template that is used by each laboratory to prepare its own laboratory-specific QAM.
- Maintenance of Corporate Policies, Quality Memorandums and SOPs. Maintenance of data investigation records that are reported to Corporate Management.
- Working with various organizations outside of TestAmerica to further the development of quality standards and represent TestAmerica at various trade meetings.
- Preparation of a monthly report that includes quality metrics across the Analytical Division and a summary of any quality related initiatives and issues.
- With the assistance of the Corporate Senior Management Team and the EHS Directors, development and implementation of the TestAmerica Environmental, Health and Safety Program.

4.2.7 Quality Directors (Corporate)

The Quality Directors report to the Executive Director-QA/EHS. Together with the Executive Director-QA/EHS, the Quality Directors have the responsibility for the establishment, general

overview and maintenance of the Analytical Division's Quality Assurance Program within TestAmerica. The Quality Directors are responsible for:

- Oversight of the QA/QC programs within each laboratory. This includes a final review of each laboratory-specific QAM and receipt of each laboratory's QA monthly report.
- Working with management to develop a plan of correction when a laboratory's quality system is determined to be inadequate.
- Review of QA/QC aspects of national projects.
- Assistance with certification activities.
- Providing assistance as needed in the selection of Quality Assurance Managers and reviewing their effectiveness.

4.2.8 Ethics and Compliance Officers (ECOs)

TestAmerica has designated two senior members of the Corporate staff to fulfill the role of Ethics and Compliance Officer (ECO) – VP-Client and Technical Services and the Executive Director–QA/EHS. Each ECO acts as a back-up to the other ECO and both are involved when data investigations occur. Each ECO has a direct line of communication to the entire senior Corporate and lab management staff.

The ECOs ensure that the organization distributes the data integrity and ethical practices policies to all employees and ensures annual trainings and orientation of new hires to the ethics program and its policies. The ECO is responsible for establishing a mechanism to foster employee reporting of incidents of illegal, unethical, or improper practices in a safe and confidential environment.

The ECOs monitor and audit procedures to determine compliance with policies and to make recommendations for policy enhancements to the CEO, COO, Laboratory Director/Manager or other appropriate individuals within the laboratory. The ECO will assist the laboratory QA Manager in the coordination of internal auditing of ethical policy related activities and processes within the laboratory, in conjunction with the laboratories regular internal auditing function.

The ECOs will also participate in investigations of alleged violations of policies and work with the appropriate internal departments to investigate misconduct, remedy the situation, and prevent recurrence of any such activity.

4.2.9 Director of Technical Services

The Director of Technical Services is responsible for establishing, implementing and communicating TestAmerica's Technical Policies, SOPs, and Manuals. Other responsibilities include conducting technical assessments as required, acting as a technical resource in national contracts review, coordinating new technologies, establishing best practices, advising staff on technology advances, innovations, and applications.

4.2.10 Chief Information Officer (CIO)

The CIO is responsible for establishing, implementing and communicating TestAmerica's Information Technology (IT) Policies, SOPs and Manuals. Other responsibilities include coordinating new technologies, development of electronic communication tools such as TestAmerica's intranet and internet sites, ensuring data security and documentation of software, ensuring compliance with the NELAC standard, and assistance in establishing, updating, and maintaining Laboratory Information Management Systems (LIMS) at the various TestAmerica facilities.

4.2.11 Environmental Health and Safety Directors (EHSDs) (Corporate)

The EHSDs report directly to the Executive Director-QA/EHS. The EHSDs are responsible for the development and implementation of the TestAmerica Environmental, Health and Safety program. Responsibilities include:

- Consolidation and tracking all safety and health-related information and reports for the company, and managing compliance activities for TestAmerica locations.
- Coordination/preparation of the corporate Environmental, Health and Safety Manual Template that is used by each laboratory to prepare its own laboratory-specific Safety Manual/CHP.
- Development and execution of the company Environmental Health and Safety Internal Audit program.
- Preparation of information and training materials for laboratory EHS Coordinators.
- Assistance in the internal and external coordination of employee exposure and medical monitoring programs to insure compliance with applicable safety and health regulations.
- Serving as Department of Transportation (D.O.T.) focal point and providing technical assistance to location management.
- Serving as Hazardous Waste Management main contact and providing technical assistance to location management.

4.2.6 Laboratory Director

TestAmerica Irvine's Laboratory Director is responsible for the overall quality, safety, financial, technical, human resource and service performance of the whole laboratory and reports to their respective GM. The Laboratory Director provides the resources necessary to implement and maintain an effective and comprehensive Quality Assurance and Data Integrity Program.

Specific responsibilities include, but are not limited to:

- Provides one or more technical directors for the appropriate fields of testing. The name(s) of the Technical Director will be included in the national database. If the Technical Director is absent for a period of time exceeding 15 consecutive calendar days, the Laboratory Director must designate another full time staff member meeting the qualifications of the Technical Director to temporarily perform this function. If the absence exceeds 65 consecutive calendar days, the primary accrediting authority must be notified in writing.

- Ensures that all analysts and supervisors have the appropriate education and training to properly carry out the duties assigned to them and ensures that this training has been documented.
- Ensures that personnel are free from any commercial, financial and other undue pressures which might adversely affect the quality of their work.
- Ensures TestAmerica's human resource policies are adhered to and maintained.
- Ensures that sufficient numbers of qualified personnel are employed to supervise and perform the work of the laboratory.
- Ensures that appropriate corrective actions are taken to address analyses identified as requiring such actions by internal and external performance or procedural audits. Procedures that do not meet the standards set forth in the QAM or laboratory SOPs may be temporarily suspended by the Laboratory Director.
- Reviews and approves all SOPs prior to their implementation and ensures all approved SOPs are implemented and adhered to.
- Pursues and maintains appropriate laboratory certification and contract approvals. Supports ISO 17025 requirements.
- Ensures client specific reporting and quality control requirements are met.
- Captains the management team, consisting of the QA Manager, the Technical Director(s), and the Operations Manager as direct reports.

4.2.7 Quality Assurance (QA) Manager

The QA Manager has responsibility and authority to ensure the continuous implementation of the quality system based on ISO 17025.

The QA Manager reports directly to the Laboratory Director and has access to Corporate QA for advice and resources. This position is able to evaluate data objectively and perform assessments without outside (i.e., managerial) influence. Corporate QA may be used as a resource in dealing with regulatory requirements, certifications and other quality assurance related items. The QA Manager directs the activities of the QA officers to accomplish specific responsibilities, which include, but are not limited to:

- Having functions independent from laboratory operations for which he/she has quality assurance oversight.
- Maintaining and updating the QAM.
- Monitoring and evaluating laboratory certifications; scheduling proficiency testing samples.
- Monitoring and communicating regulatory changes that may affect the laboratory to management.
- Training and advising the laboratory staff on quality assurance/quality control procedures that are pertinent to their daily activities.
- Having a general knowledge of the analytical test methods for which data audit/review is performed (and/or having the means of getting this information when needed).
- Arranging for or conducting internal audits on quality systems and the technical operation.

- The laboratory QA Manager will maintain records of all ethics-related training, including the type and proof of attendance.
- Maintain, improve, and evaluate the corrective action database and the corrective and preventive action systems.
- Notifying laboratory management of deficiencies in the quality system and ensuring corrective action is taken. Procedures that do not meet the standards set forth in the QAM or laboratory SOPs are temporarily suspended following the procedures outlined in Section 13.
- Monitoring standards of performance in quality control and quality assurance.
- Coordinating of document control of SOPs, MDLs, control limits, and miscellaneous forms and information.
- Review a percentage of all final data reports for internal consistency. Review of Chain of Custody (COC), correspondence with the analytical request, batch QC status, completeness of any corrective action statements, 5% of calculations, format, holding time, sensibility and completeness of the project file contents.
- Review of external audit reports and data validation requests.
- Follow-up with audits to ensure client QAPP requirements are met.
- Establishment of reporting schedule and preparation of various quality reports for the Laboratory Director, clients and/or Corporate QA.
- Development of suggestions and recommendations to improve quality systems.
- Research of current state and federal requirements and guidelines.
- Captains the QA team to enable communication and to distribute duties and responsibilities.

4.2.8 Technical Director/Department Manager

Department Managers are also designated as Technical Directors provided they meet the requirements specified in section 4.1.1.1 of the NELAC Standard. The Technical Director(s) report(s) directly to the Laboratory Director. He/she is accountable for all analyses and analysts with respect to ISO 17025. The scope of responsibility ranges from the new-hire process and existing technology through the ongoing training and development programs for existing analysts and second- and third-generation instrumentation. Specific responsibilities include, but are not limited to:

- Coordinating, writing, and reviewing preparation of all test methods, i. e., SOPs, with regard to quality, integrity, regulatory and optimum and efficient production techniques, and subsequent analyst training and interpretation of the SOPs for implementation and unusual project samples. He/she insures that the SOPs are properly managed and adhered to at the bench. He/she develops standard costing of SOPs to include supplies, labor, overhead, and capacity (design vs. demonstrated versus first-run yield) utilization.
- Reviewing and approving, with input from the QA Manager, proposals from marketing, in accordance with an established procedure for the review of requests and contracts. This procedure addresses the adequate definition of methods to be used for analysis and any limitations, the laboratory's capability and resources, the client's expectations. Differences are resolved before the contract is signed and work begins. A system documenting any

significant changes is maintained, as well as pertinent discussions with the client regarding their requirements or the results of the analyses during the performance of the contract. All work subcontracted by the laboratory must be approved by the client. Any deviations from the contract must be disclosed to the client. Once the work has begun, any amendments to the contract must be discussed with the client and so documented.

- Monitoring the validity of the analyses performed and data generated in the laboratory. This activity begins with reviewing and supporting all new business contracts, insuring data quality, analyzing internal and external non-conformances to identify root cause issues and implementing the resulting corrective and preventive actions, facilitating the data review process (training, development, and accountability at the bench), and providing technical and troubleshooting expertise on routine and unusual or complex problems.
- Providing training and development programs to applicable laboratory staff as new hires and, subsequently, on a scheduled basis. Training includes instruction on calculations, instrumentation management to include troubleshooting and preventive maintenance.
- Enhancing efficiency and improving quality through technical advances and improved LIMS utilization. Capital forecasting and instrument life cycle planning for second generation methods and instruments as well as asset inventory management.
- Coordinating sample management from “cradle to grave,” insuring that no time is lost in locating samples.
- Scheduling all QA/QC-related requirements for compliance, e.g., MDLs, etc.
- Captains department supervisors to communicate quality, technical, personnel, and instrumental issues for a consistent team approach.
- Coordinates audit responses with supervisors and QA Manager.

4.2.9 LIMS Administrator

The LIMS Administrator reports directly to the Laboratory Director. In the pursuit of his/her duties, he/she:

- Establishes and maintains the laboratory information system (LIMS) for tracking all samples in the laboratory.
- Updates and enhances LIMS.
- Develops expertise in the requirements described in Good Automated Laboratory Practices (GALP)-EPA 2185, 1995 Edition, in order to ensure compliance.
- Programs and tests software modifications/changes.
- Coordinates testing to ensure that all LIMS software accurately performs its intended functions. Testing is performed and documented after installation or when modifications/changes are made.
- Maintains historical files of software, software operating procedures (manuals), software changes/modifications (Change Log) and software version numbers.
- Maintains log of repairs and service performed on LIMS hardware.
- Develops and verifies security practices to assure the integrity of LIMS data. Identifies threats, potential threats, and future threats.

- Maintains awareness of any environmental conditions of the facility housing the LIMS that may compromise LIMS raw data and informs management.
- LIMS database back-up once daily.

4.2.10 Operations Manager

The Operations Manager manages and directs the analytical production sections of the laboratory. He/She reports directly to the Laboratory Director. He/She assists the Technical Director in determining the most efficient instrument utilization. More specifically, he/she:

- Evaluates the level of internal/external non-conformances for all departments.
- Continuously evaluates production capacity and improves capacity utilization.
- Continuously evaluates turnaround time and addresses any problems that may hinder meeting the required and committed turnaround time from the various departments.
- Develops and improves the training of all analysts in cooperation with the Technical Director/QA Manager/Training Coordinator and in compliance with regulatory requirements.
- Is responsible for efficient utilization of supplies.
- Constantly monitors and modifies the processing of samples through the departments.

4.2.11 Client Services Manager

The Client Services Manager reports to the Laboratory Director and serves as the interface between the laboratory's technical departments and the laboratory's clients. The staff consists of the Project Management team. With the overall goal of total client satisfaction, the functions of this position are outlined below:

- Technical training and growth of the Project Management team.
- Technical liaison for the Project Management team.
- Human resource management of the Project Management team.
- Responsible to ensure that clients receive the proper sampling supplies.
- Accountable for response to client inquiries concerning sample status.
- Responsible for assistance to clients regarding the resolution of problems concerning COC.
- Ensuring that client specifications, when known, are met by communicating project and quality assurance requirements to the laboratory.
- Notifying the supervisors of incoming projects and sample delivery schedules.
- Accountable to clients for communicating sample progress in daily status meeting with agreed-upon due dates.
- Responsible for discussing with client any project-related problems, resolving service issues, and coordinating technical details with the laboratory staff.
- Responsible for staff familiarization with specific quotes, sample log-in review, and final report completeness.

- Monitor the status of all data package projects in-house to ensure timely and accurate delivery of reports.
- Inform clients of data package-related problems and resolve service issues.
- Coordinate requests for sample containers and other services (data packages).

4.2.12 Technical Manager

The Technical Manager is responsible for the development and implementation of new methods, maintenance and repair of all instruments and equipment, troubleshooting, the acquisition of new instruments, training new personnel and cross-training current employees to operate in other departments. The Technical Manager works closely with the Quality Assurance Director to ensure proper calibration and operation of all analytical equipment and directly with the Systems Administrator to help implement new computer analytical programs, maintain current system, and develop ideas for future improvements.

4.2.13 Project Manager

Project Managers are responsible for thoroughly coordinating client projects, maintaining clients' satisfaction and reviewing laboratory reports. All project status and technical questions generated by the client are directed to the Project Manager. Project Managers are responsible for reviewing potential work and incoming work with laboratory supervisors at daily operations meetings. The review is to ensure the lab has appropriate facilities and resources to perform the work and to disseminate client specific information.

4.2.14 Project Manager Assistant

The Project Manager (PM) Assistant provides clerical support to the project management staff in order to allow them to focus on client service and report review. The PM assistant performs faxing duties, prepares and sends electronic data deliverables (EDD) to clients, generates historical data as a cross reference for the laboratory, retrieves laboratory data, and tracks project reports

4.2.15 Sample Control Manager

The Sample Control Manager reports to the Laboratory Director. The responsibilities are outlined below:

- Direct the logging of incoming samples into the LIMS.
- Ensure the verification of data entry from login.
- Schedule and oversee all sample courier operations.
- Schedule and oversee all field sampling operations.
- Oversee the processing of bottle orders.
- Acts as a liason between the Project Managers and Analysts with respect to handling rush orders and resolving discrepancies with chain-of-custody forms and the routing of subcontracted analyses

4.2.16 Quality Assurance Scientist

The Quality Assurance (QA) Scientist performs several roles. The QA Scientist reports to the facility QA Manager and reviews data deliverable packages to ensure completeness and accuracy. As a statistician, the QA Scientist generates and reviews, in conjunction with the Quality Assurance Manager, Control Charts and Method Detection Limit (MDL) studies. The QA Scientist assists the QA Manager and lab staff with internal audits, corrective action review and overall implementation of the QA program and fills in as the “deputy” for QA Manager in their absence.

4.2.17 Training Coordinator

The Training Coordinator reports directly to the QA Manager. This person’s role is to oversee the entire regime of training in the laboratory and ensure that adequate procedures and documentation are in place to maintain a high and consistent laboratory performance. Duties are outlined below:

- Ensure both initial and on-going demonstrations of capability are performed and are current.
- Maintain all course and individual training records in an organized and up-to-date manner.
- Assist QA Manager in maintaining current SOPs.
- Conduct all initial orientation training for new hires covering QA, Ethics, and Health & Safety.
- Utilize the General Processes Audit to reinforce laboratory basics with new employees after they have worked in the laboratory for a few months.
- Perform or coordinate audits of new employees to assess their training and performance.
- Research and develop a training system for ongoing training in the department and/or for individual analyses.
- Develop personnel through the use of specialized trainings by coordinating experts from within the company or outside vendors to train on certain topics.
- Support laboratory personnel in special training needs that may arise.

4.2.18 Hazardous Waste Coordinator

The Hazardous Waste Coordinator reports directly to the Laboratory Director. The duties consist of:

- Staying current with the hazardous waste regulations.
- Continuing training on hazardous waste issues.
- Reviewing and updating annually the Hazardous Waste Contingency Plan in the Environmental Health & Safety Manual.
- Auditing the staff with regard to compliance with the Hazardous Waste Contingency Plan.

Contacting the hazardous waste subcontractors for review of procedures and opportunities for minimization of waste

4.2.19 Laboratory Analysts

Laboratory analysts are responsible for conducting analysis and performing all tasks assigned to them by the group leader or supervisor. The responsibilities of the analysts are listed below:

- Perform analyses by adhering to analytical and quality control protocols prescribed by current SOPs, this QA Manual, and project-specific plans honestly, accurately, timely, safely, and in the most cost-effective manner.
- Document standard and sample preparation, instrument calibration and maintenance, data calculations, sample matrix effects, and any observed non-conformance on worklists, benchsheets, lab notebooks and/or the Non-Conformance Database.
- Report all non-conformance situations, instrument problems, matrix problems and QC failures, which might affect the reliability of the data, to their supervisor, the Technical Director, and/or the QA Manager or member of QA staff.
- Perform 100% review of the data generated prior to entering and submitting for secondary level review.
- Suggest method improvements to their supervisor, the Technical Director, and the QA Manager. These improvements, if approved, will be incorporated. Ideas for the optimum performance of their assigned area, for example, through the proper cleaning and maintenance of the assigned instruments and equipment, are encouraged.
- Work cohesively as a team in their department to achieve the goals of accurate results, optimum turnaround time, cost effectiveness, cleanliness, complete documentation, and personal knowledge of environmental analysis.

4.2.20 Safety Officer

The Safety Officer reports to the Laboratory Director and ensures that systems are maintained for the safe operation of the laboratory. The Safety Officer is responsible to:

- Conduct ongoing, necessary safety training and conduct new employee safety orientation.
- Assist in developing and maintaining the Chemical Hygiene/Safety Manual.
- Administer dispersal of all Material Safety Data Sheet (MSDS) information.
- Perform regular chemical hygiene and housekeeping instruction.
- Give instruction on proper labeling and practice.
- Serve as chairman of the laboratory safety committee.
- Provide and train personnel on protective equipment.
- Oversee the inspection and maintenance of general safety equipment – fire extinguishers, safety showers, eyewash fountains, etc. and ensure prompt repairs as needed.
- Supervise and schedule fire drills and emergency evacuation drills.
- Determine what initial and subsequent exposure monitoring, if necessary to determine potential employee exposure to chemicals used in the laboratory.
- When determined necessary, conduct exposure monitoring assessments.
- Determine when a complaint of possible over-exposure is “reasonable” and should be referred for medical consultation.

- Assist in the internal and external coordination of the medical consultation/monitoring program conducted by TestAmerica's medical consultants

4.2.21 Data Package Coordinator

The Data Package Coordinator reports directly to the Technical Director. The person in this position manages the timely and thorough completion of data packages in accordance with project requirements

4.2.22 Data Package Assembler

The Data Package Assembler reports directly to the Data Package Coordinator as is responsible for the organization of data packages for final delivery. This includes insertion of dividers, creation of specialized summary forms, and the transcription of narrative comments.

4.2.23 Data Package Specialist

A Data Package Specialist is based in each analytical department and reports to that department's manager. The responsibilities include the retrieval and copying of all raw data required for the data package.

4.2.24 Couriers and Field Sampling Technicians

This group is responsible for general courier duties, water sampling by the grab method, and the proper installation of automatic ISCO 24-hour water sampling equipment.

4.2.25 Laboratory Technicians

Technicians prepare samples for analysis by weighing, extracting or digesting, filtering, or concentrating samples. Technicians prepare method specific QC Samples with each preparation batch. All personnel must adhere to all QC procedures specified in the analytical method and in accordance to laboratory procedures or policies and are responsible for the full documentation of these procedures.

4.2.26 Sample Control Technicians

Sample Control personnel report to the Sample Control Manager. These technicians are responsible for the receiving and logging-in of samples delivered to the laboratory. They record the condition of the samples and maintain chains of custody. They also ensure that samples have been preserved properly, have been delivered in the appropriate containers, have sufficient quantity for analysis, and are stored properly.

4.3 DEPUTIES


The following table defines who assumes the responsibilities of key personnel in their absence:

Key Personnel	Deputy
Laboratory Director	Client Services Manager
QA Manager	Senior QA Scientist

Key Personnel	Deputy
Department Manager/Technical Director	Department Group Leader
Client Services Manager	Department Group Leader
Safety Officer	Hazardous Waste Coordinator

Figure 4-1.

Corporate Organization Chart

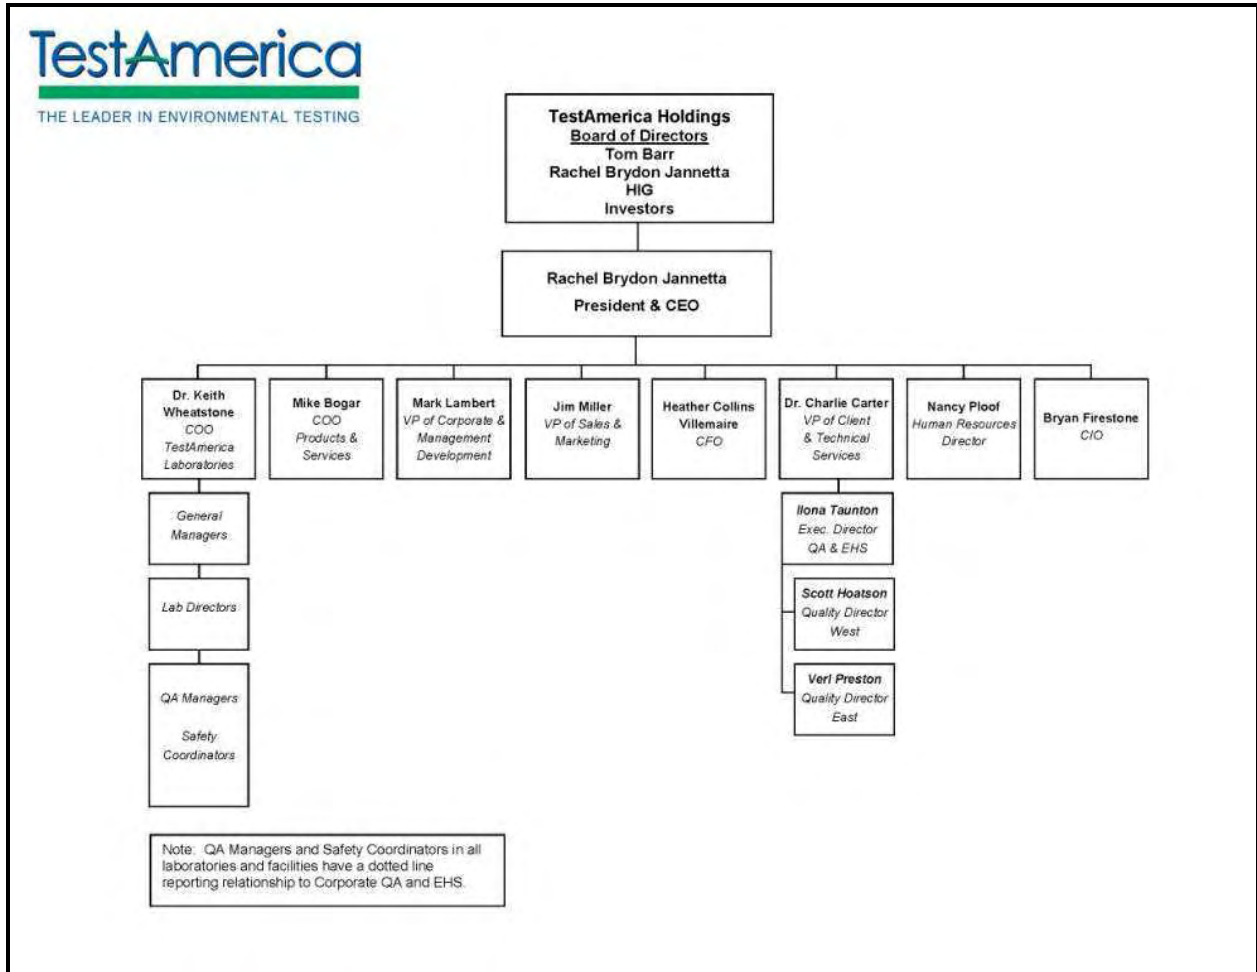

SECTION 5

QUALITY SYSTEM (NELAC 5.4.2)

5.1 QUALITY POLICY STATEMENT

The management of TestAmerica and TestAmerica Irvine are committed to providing data of known quality to its clients by adhering to approved methodologies, regulatory requirements and the QA/QC protocols described in this manual.

In all aspects of the laboratory and business operations, management is dedicated in maintaining the highest ethical standards. An Ethics Policy sign-off can be viewed in Appendix 1. Training on ethical and legal responsibilities is provided annually and each employee signs off annually on the policy as a condition of employment.

It is TestAmerica's Policy to continually improve systems and provide support to quality improvement efforts in laboratory, administrative and managerial activities. The company recognizes that the implementation of a quality assurance program requires management's commitment and support as well as the involvement of the entire staff.

TestAmerica Irvine strives to provide clients with the highest level of professionalism and the best service practices in the industry.

Every staff member at TestAmerica Irvine plays an integral part in quality assurance and is held responsible and accountable for the quality of their work. It is, therefore, required that all laboratory personnel are trained and agree to comply with applicable procedures and requirements established by this document.

5.2 ETHICS AND DATA INTEGRITY

TestAmerica is committed to ensuring the integrity of its data and meeting the quality needs of its clients. The 7 elements of TestAmerica's Ethics and Data Integrity Program include:

- An Ethics Policy (Policy No. CA-L-P-001) and employee ethics statements (Appendix 1).
- An Ethics and Compliance Officer (ECO).
- A training program.
- Self-governance through disciplinary action for violations.
- A confidential mechanism for anonymously reporting alleged misconduct and a means for conducting internal investigations of all alleged misconduct. (SOP No. CA-L-S-001)
- Procedures and guidance for recalling data if necessary (SOP No. CA-L-S-001).
- An effective external and internal monitoring system that includes procedures for internal audits (Section 16).

As an American Council of Independent Laboratories (ACIL) member, all TestAmerica laboratories adhere to the following ACIL Code of Ethics:

- Produce results, which are accurate and include QA/QC information that meets client pre-defined Data Quality Objectives (DQOs).
- Present services in a confidential, honest and forthright manner.
- Provide employees with guidelines and an understanding of the ethical and quality standards of our industry.
- Operate our facilities in a manner that protects the environment and the health and safety of employees and the public.
- Obey all pertinent federal, state and local laws and regulations and encourage other members of our industry to do the same.
- Educate clients as the extent and kinds of services available.
- Assert competency only for work for which adequate personnel and equipment are available and for which adequate preparation has been made.
- Promote the status of environmental laboratories, their employees, and the value of services rendered by them.

5.3 QUALITY SYSTEM SUPPORTING DOCUMENTATION

The laboratory's Quality System is communicated through a variety of documents prepared by the laboratory and company management:

- Quality Assurance Manual (QAM) Template
- Quality Assurance Manual – Each laboratory has a lab specific quality assurance manual.
- Corporate SOPs and Policies - Corporate SOPs and Policies are developed for use by all relevant laboratories. They are incorporated into the laboratory's normal SOP distribution, training and tracking system. Corporate SOPs may be general or technical.
- Work Instructions - A subset of procedural steps, tasks or forms associated with an operation of a management system (e.g., checklists, preformatted bench sheets, forms).
- Laboratory SOPs – General and Technical
- Corporate TestAmerica QA/QC Policy Memorandums (Refer to Section 3.4).
- Laboratory QA/QC Policy Memorandums (Refer to Section 3.4).

5.3.1 Order of Precedence

In the event of a conflict or discrepancy between policies, the order of precedence is as follows:

- TestAmerica QA/QC Policy Memorandum - Corporate
- Laboratory QA/QC Policy Memorandum
- Quality Assurance Manual
- Corporate SOPs and Policies
- Laboratory SOPs and Policies

- Other (Work Instructions (WI), memos, flow charts, etc.)

5.4 QA/QC OBJECTIVES FOR THE MEASUREMENT OF DATA

Quality Assurance (QA) and Quality Control (QC) are activities undertaken to achieve the goal of producing data that accurately characterize the sites or materials that have been sampled. Quality Assurance is generally understood to be more comprehensive than Quality Control. Quality Assurance can be defined as the integrated system of activities that ensures that a product or service meets defined standards.

Quality Control is generally understood to be limited to the analyses of samples and to be synonymous with the term "*analytical quality control*". QC refers to the routine application of statistically based procedures to evaluate and control the accuracy of results from analytical measurements. The QC program includes procedures for estimating and controlling precision and bias and for determining reporting limits.

Request for Proposals (RFPs) and Quality Assurance Project Plans (QAPP) provide a mechanism for the client and the laboratory to discuss the data quality objectives in order to ensure that analytical services closely correspond to client needs. The client is responsible for developing the QAPP. In order to ensure the ability of the laboratory to meet the Data Quality Objectives (DQOs) specified in the QAPP, clients are advised to allow time for the laboratory to review the QAPP before being finalized. Additionally, the laboratory will provide support to the client for developing the sections of the QAPP that concern laboratory activities.

Historically, laboratories have described their QC objectives in terms of precision, accuracy, representativeness, comparability, completeness, selectivity and sensitivity (PARCCSS).

5.4.1 Precision

The laboratory objective for precision is to meet the performance for precision demonstrated for the methods on similar samples and to meet data quality objectives of the EPA and/or other regulatory programs. Precision is defined as the degree of reproducibility of measurements under a given set of analytical conditions (exclusive of field sampling variability). Precision is documented on the basis of replicate analysis, usually duplicate or matrix spike (MS) duplicate samples. The calculation of precision is described in Section 25.

5.4.2 Accuracy

The laboratory objective for accuracy is to meet the performance for accuracy demonstrated for the methods on similar samples and to meet data quality objectives of the EPA and/or other regulatory programs. Accuracy is defined as the degree of bias in a measurement system. Accuracy may be documented through the use of laboratory control samples (LCS) and/or MS. A statement of accuracy is expressed as an interval of acceptance recovery about the mean recovery. The calculation of accuracy is described in Section 25.

5.4.3 Representativeness

The laboratory objective for representativeness is to provide data which is representative of the sampled medium. Representativeness is defined as the degree to which data represent a characteristic of a population or set of samples and is a measurement of both analytical and field sampling precision. The representativeness of the analytical data is a function of the procedures used in procuring and processing the samples. The representativeness can be documented by the relative percent difference between separately procured, but otherwise identical samples or sample aliquots.

The representativeness of the data from the sampling sites depends on both the sampling procedures and the analytical procedures. The laboratory may provide guidance to the client regarding proper sampling and handling methods in order to assure the integrity of the samples.

5.4.4 Comparability

The comparability objective is to provide analytical data for which the accuracy, precision, representativeness and reporting limit statistics are similar to these quality indicators generated by other laboratories for similar samples, and data generated by the laboratory over time.

The comparability objective is documented by inter-laboratory studies carried out by regulatory agencies or carried out for specific projects or contracts, by comparison of periodically generated statements of accuracy, precision and reporting limits with those of other laboratories, and by the degree to which approval from the US EPA or other pertinent regulatory agencies is obtained for any procedure for which significant modifications have been made.

5.4.5 Completeness

The completeness objective for data is 90% (or as specified by a particular project), expressed as the ratio of the valid data to the total data over the course of the project. Data will be considered valid if they are adequate for their intended use. Data usability will be defined in a QAPP, project scope or regulatory requirement. Data validation is the process for reviewing data to determine its usability and completeness. If the completeness objective is not met, actions will be taken internally and with the data user to improve performance. This may take the form of an audit to evaluate the methodology and procedures as possible sources for the difficulty or may result in a recommendation to use a different method.

5.4.6 Selectivity

Selectivity is defined as: The capability of a test method or instrument to respond to a target substance or constituent in the presence of non-target substances. Target analytes are separated from non-target constituents and subsequently identified/detected through one or more of the following, depending on the analytical method: extractions (separation), digestions (separation), interelement corrections (separation), use of matrix modifiers (separation), specific retention times (separation and identification), confirmations with different columns or detectors (separation and identification), specific wavelengths (identification), specific mass spectra (identification), specific electrodes (separation and identification), etc..

5.4.7 Sensitivity

Sensitivity refers to the amount of analyte necessary to produce a detector response that can be reliably detected (Method Detection Limit) or quantified (Reporting Limit).

5.5 CRITERIA FOR QUALITY INDICATORS

The laboratory prepares a [Quality Control Limit Summary that contains tables](#) that summarize the precision and accuracy acceptability limits for analyses performed at TestAmerica Irvine. This summary includes an effective date, is updated each time new limits are generated and is located on [the network server](#). Unless otherwise noted, limits within these tables are laboratory generated. Some acceptability limits are derived from US EPA methods when they are required. Where US EPA method limits are not required, TestAmerica Irvine has developed limits from evaluation of data from similar matrices. See laboratory SOP CNTRLLIM.SOP, Control Charts and Statistical Process Control. Additional criteria for development of control limits is contained in Section 25.

5.6 STATISTICAL QUALITY CONTROL

Statistically-derived precision and accuracy limits are required by selected methods (such as SW-846) and programs [such as the Ohio Voluntary Action Plan (VAP)]. TestAmerica Irvine routinely utilizes statistically-derived limits to evaluate method performance and determine when corrective action is appropriate. The analysts are instructed to use the current limits in the laboratory (dated and approved by the Technical Director and QA Manager) and entered into the Laboratory Information Management System (LIMS). The Quality Assurance department maintains an archive of all limits used within the laboratory. [The archive consists of the date range and number of points used in LIMS to generate the limits, thus allowing for recreation of the limits if necessary](#). If a method defines the QC limits, the method limits are used.

If a method requires the generation of historical limits, the lab develops such limits from recent data in the QC database of the LIMS following the guidelines described in Section 25. All calculations and limits are documented and dated when approved and effective. On occasion, a client requests contract-specified limits for a specific project.

Surrogate recoveries are determined for a specific time period as defined above. The resulting ranges are entered in LIMS.

Current QC limits are entered and maintained in the LIMS analyte database. As sample results and the related QC are entered into LIMS, the sample QC values are compared with the limits in LIMS to determine if they are within the acceptable range. The analyst then evaluates if the sample needs to be rerun or re-extracted/rerun or if a comment should be added to the report explaining the reason for the QC outlier.

5.6.1 QC Charts

As the QC limits are calculated, QC charts are generated showing warning and control limits for the purpose of evaluating trends. The QA Manager evaluates these periodically to determine if adjustments need to be made or for corrective actions to methods. All findings are documented and kept on file.

5.7 QUALITY SYSTEM METRICS

In addition to the QC parameters discussed above, the entire Quality System is evaluated on a monthly basis through the use of specific metrics (refer to Section 17). These metrics are used to drive continuous improvement in the laboratory's Quality System.

SECTION 6

DOCUMENT CONTROL (NELAC 5.4.3)

6.1 OVERVIEW

The QA Department is responsible for the control of documents used in the laboratory to ensure that approved, up-to-date documents are in circulation and out-of-date (obsolete) documents are archived or destroyed. The following documents, at a minimum, must be controlled at each laboratory Facility:

- Laboratory Quality Assurance Manual
- Laboratory Standard Operating Procedures (SOP)
- Laboratory Policies
- Work Instructions and Forms
- Corporate Policies and Procedures distributed outside the intranet

The Corporate staff posts Corporate Manuals, SOPs, Policies, Work Instructions, White Papers and Training Materials on the company intranet site. These are collectively termed “Official Documents” and encompass the Policies and Procedures that all facilities are required to employ. These official documents are only considered controlled when they are read on the company intranet site. Printed copies are considered uncontrolled unless the laboratory physically distributes them as controlled documents. A detailed description of the procedure for issuing, authorizing, controlling, distributing, and archiving official documents is found in Corporate SOP No. CW-Q-S-001, Corporate Document Control and Archiving [and the laboratory SOP IR-QA-DOC, Document Control and Review](#).

The laboratory QA Department also maintains access to various references and document sources integral to the operation of the laboratory. This includes reference methods and regulations. Instrument manuals (hard or electronic copies) are also maintained by the laboratory.

The laboratory maintains control of records for raw analytical data and supporting records such as [audit reports and responses](#), logbooks, standard logs, training files, MDL studies, Proficiency Testing (PT) studies, certifications and related correspondence, and non-conformance/corrective action reports. Raw analytical data consists of bound logbooks, instrument printouts, any other notes, magnetic media, electronic data and final reports. Discussion on records control is described in Section 15.

The maintenance of purchasing data is discussed in Section 9.

The maintenance of sales and marketing contracts is discussed in Section 7.

6.2 DOCUMENT APPROVAL AND ISSUE

The pertinent elements of a control system for each document include a unique name and number, the number of pages of the item, the effective date, revision number and the

laboratory's name. The QA Manager responsible for the maintenance of the system and maintains the items in the QA office and in the on-site long-term data storage area.

Controlled documents are authorized by the QA Department and other management. In order to develop a new document, a manager submits an electronic draft to the QA Department for suggestions and approval before use. Upon approval, QA personnel add the identifying version information to the document and retains the official document on file. The official document is provided as needed to those using it. Controlled documents shall be available at all locations where the operational activity described in the document is performed (may include electronic access). Controlled documents are identified as such and records of their distribution are kept by the QA Department. Document control may be achieved by either electronic or hardcopy distribution.

The QA Department maintains a list of the official versions of controlled documents.

Quality System Policies and Procedures will be reviewed at a minimum of every two years (annually for all drinking water program procedures) and will be revised as appropriate. Changes to documents occur when a procedural change warrants a revision of the document.

6.3 PROCEDURES FOR DOCUMENT CONTROL POLICY

For changes to the QA Manual, refer to *the Corporate Document Control SOP, CW-Q-S-001*. Uncontrolled copies must not be used within the laboratory. Previous revisions and back-up data are stored by the QA department. Electronic copies are stored on the Public server in the QA folder for the applicable revision.

For changes to SOPs, refer to SOP No. CW-Q-S-002, Writing a Standard Operating Procedure (SOP).

Forms, worksheets, work instructions and information are organized by department in the QA office. Electronic versions are kept on a hard drive in the QA department; hard copies are kept in QA files.

6.4 **OBSOLETE DOCUMENTS**

All invalid or obsolete documents are removed, or otherwise prevented from unintended use. The laboratory has specific procedures as described above to accomplish this. In general, obsolete documents are collected from employees according to distribution lists and are marked obsolete on the cover or destroyed. At least one copy of the obsolete document is archived as described in Section 15.

SECTION 7

REVIEW OF WORK REQUEST

7.1 OVERVIEW

TestAmerica Irvine has established procedures for the review of work requests and contracts, oral or written. The procedures include evaluation of the laboratory's capability and resources to meet the contract's requirements within the requested time period. All requirements, including the methods to be used, must be adequately defined, documented and understood. For many environmental sampling and analysis programs, testing design is site or program specific and does not necessarily "fit" into a standard laboratory service or product. It is TestAmerica's intent to provide both standard and customized environmental laboratory services to our clients.

A thorough review of technical and QC requirements contained in contracts is performed to ensure project success. The appropriateness of requested methods, and the lab's capability to perform them must be established. Projects, proposals and contracts are reviewed for adequately defined requirements and TestAmerica's capability to meet those requirements. Alternate test methods that are capable of meeting the clients' requirements may be proposed by the lab. A review of the lab's capability to analyze non-routine analytes is also part of this review process.

All projects, proposals and contracts are reviewed for the client's requirements in terms of compound lists, test methodology requested, sensitivity (detection and reporting levels), accuracy, and precision requirements (% Recovery and RPD). The reviewer ensures that the laboratory's test methods are suitable to achieve these regulatory and client requirements and that the laboratory holds the appropriate certifications and approvals to perform the work. The laboratory and any potential subcontract laboratories must be certified, as required, for all proposed tests.

The laboratory must determine if it has the necessary physical, personnel and information resources to meet the contract, and if the personnel have the expertise needed to perform the testing requested. Each proposal is checked for its impact on the capacity of the laboratory's equipment and personnel. As part of the review, the proposed turnaround time will be checked for feasibility.

Electronic or hard copy deliverable requirements are evaluated against the lab's capacity for production of the documentation.

If the laboratory cannot provide all services but intends to subcontract such services, whether to another TestAmerica facility or to an outside firm, this will be documented and discussed with the client prior to contract approval. (Refer to Section 8 for Subcontracting Procedures.)

The laboratory informs the client of the results of the review if it indicates any potential conflict, deficiency, lack of accreditation, or inability of the lab to complete the work satisfactorily. Any discrepancy between the client's requirements and TestAmerica's capability to meet those requirements is resolved in writing before acceptance of the contract. It is necessary that the contract be acceptable to both the laboratory and the client. Amendments initiated by the client and/or TestAmerica, are documented in writing.

All contracts, QAPPs, Sampling and Analysis Plans (SAPs), contract amendments, and documented communications become part of the project record.

The review process is repeated when there are amendments to the original contract by the client, and the participating personnel are informed of the changes.

7.2 REVIEW SEQUENCE AND KEY PERSONNEL

Appropriate personnel will review the work request at each stage of evaluation.

For routine projects and other simple tasks, a review by the Project Manager (PM) is considered adequate. The PM confirms that the laboratory has any required certifications, that it can meet the clients' data quality and reporting requirements and that the lab has the capacity to meet the clients turn around needs. It is recommended that, where there is a sales person assigned to the account, an attempt should be made to contact that sales person to inform them of the incoming samples.

For new, complex or large projects, the proposed contract is given to the National Account Director, who will decide which lab will receive the work based on the scope of work and other requirements, including certification, testing methodology, and available capacity to perform the work. The contract review process is outlined in SOP No. CA-L-P-002, Contract Compliance Policy.

This review encompasses all facets of the operation. The scope of work is distributed to the appropriate personnel, as needed based on scope of contract, to evaluate all of the requirements shown above (not necessarily in the order below):

- Legal & Contracts Director
- General Manager
- The Laboratory Project Management Director
- The Laboratory Operations Manager
- Laboratory and/or Corporate Technical Directors
- Laboratory and/or Corporate Information Technology Managers/Directors
- Regional and/or National Account representatives
- Laboratory and/or Corporate Quality
- Laboratory and/or Corporate Environmental Health and Safety Managers/Directors
- The Laboratory Director reviews the formal laboratory quote and makes final acceptance for their facility.

The National Account Director, Legal Contracts Director, or local account representative then submits the final proposal to the client.

In the event that one of the above personnel is not available to review the contract, his or her back-up will fulfill the review requirements.

The Legal & Contracts Director maintains copies of all signed contracts. The Client Services Manager and/or the Project Manager may also keep a copy of the contracts, as necessary.

7.3 DOCUMENTATION

Appropriate records are maintained for every contract or work request. All stages of the contract review process are documented and include records of any significant changes. All contract documentation is kept by Marketing and is archive in the same manner as all other laboratory documents.

The contract will be distributed to and maintained by the appropriate sales/marketing personnel and the Regional Account Manager. A copy of the contract and formal quote will be filed with the laboratory PM and/or the Lab Director.

Records are maintained of pertinent discussions with a client relating to the client's requirements or the results of the work during the period of execution of the contract. The PM keeps a phone log of conversations with the client.

7.3.1 Project-Specific Quality Planning

Communication of contract specific technical and QC criteria is an essential activity in ensuring the success of site specific testing programs. To achieve this goal, TestAmerica Irvine assigns a PM to each client. The PM is the first point of contact for the client. It is the PM's responsibility to ensure that project specific technical and QC requirements are effectively evaluated and communicated to the laboratory personnel before and during the project. QA department involvement may be needed to assist in the evaluation of custom QC requirements.

PM's are the direct client contact and they ensure resources are available to meet project requirements. Although PM's do not have direct reports or staff in production, they coordinate opportunities and work with laboratory management and supervisory staff to ensure available resources are sufficient to perform work for the client's project. Project management is positioned between the client and laboratory resources.

Prior to work on a new project, the dissemination of project information and/or project opening meetings may occur to discuss schedules and unique aspects of the project. Items to be discussed may include the project technical profile, turnaround times, holding times, methods, analyte lists, reporting limits, deliverables, sample hazards, or other special requirements. The PM introduces new projects to the laboratory staff through project kick-off meetings or to the supervisory staff during production meetings. These meetings provide direction to the laboratory staff in order to maximize production and client satisfaction, while maintaining quality. In addition, project notes may be associated with each sample batch as a reminder upon sample receipt and analytical processing.

During the project, any change that may occur within an active project is agreed upon between the client/regulatory agency and the PM/laboratory. These changes (e.g., use of a non-standard method or modification of a method) and approvals must be documented prior to implementation. Documentation pertains to any document, e.g., letter, e-mail, variance, contract addendum, which has been signed by both parties.

Such changes are also communicated to the laboratory during production meetings. Such changes are updated to the project notes and are introduced to the managers at these meetings. The laboratory staff is then introduced to the modified requirements via the PM or the individual laboratory Department Manager. After the modification is implemented into the laboratory process, documentation of the modification is made in the case narrative of the data report(s).

TestAmerica strongly encourages client visits to the laboratory and for formal/informal information sharing session with employees in order to effectively communicate ongoing client needs as well as project specific details for customized testing programs.

SECTION 8

SUBCONTRACTING OF TESTS (NELAC 5.4.5)

8.1 OVERVIEW

For the purpose of this quality manual, the phrase subcontract laboratory refers to a laboratory external to the corporate network. The phrase “work sharing” refers to internal transfers of samples between company laboratories. The term outsourcing refers to the act of subcontracting tests.

When contracting with our clients, the laboratory makes commitments regarding the services to be performed and the data quality for the results to be generated. When we must outsource testing for our clients because project scope, changes in laboratory capabilities, capacity or unforeseen circumstances, we must be assured that the subcontractors or work sharing laboratories understand the requirements and will meet the same commitments we have made to the client. Refer to the SOP on Subcontracting Procedures (CA-L-S-002) and the Work Sharing Process SOP (CA-C-S-001).

When outsourcing analytical services, the laboratory will assure, to the extent necessary, that the subcontract or work sharing laboratory maintains a program consistent with the requirements of this document, the requirements specified in NELAC/ISO 17025 and/or the client's Quality Assurance Project Plan (QAPP). All QC guidelines specific to the client's analytical program are transmitted to the subcontractor and agreed upon before sending the samples to the subcontract facility. Additionally, work requiring accreditation will be placed with an appropriately accredited laboratory. The laboratory performing the subcontracted work will be identified in the final report, as will non-NELAC accredited work where required.

8.2 QUALIFYING AND MONITORING SUBCONTRACTORS

Whenever a PM or Regional Account Executive (RAE) or Customer Service Manager (CSM) becomes aware of a client requirement or laboratory need where samples must be outsourced to another laboratory, the other laboratory(s) shall be selected based on the following:

- The first priority is to attempt to place the work in a qualified network laboratory;
- Firms specified by the client for the task (Documentation that a subcontractor was designated by the client must be maintained with the project file. This documentation can be as simple as placing a copy of an e-mail from the client in the project folder);
- Firms listed as pre-qualified and currently under a subcontract with the company ([in JD Edwards](#)): [A listing of all approved subcontracting laboratories and supporting documentation is available on the TestAmerica intranet site. Verify necessary accreditation for the requested tests prior to sending samples.](#);
- Firms identified in accordance with the company's Small Business Subcontracting program as small, women-owned, veteran-owned and/or minority-owned businesses;
- [NELAC or A2LA accredited laboratories](#);
- In addition, the firm must hold the appropriate certification to perform the work required.

All intra-company laboratories are pre-qualified for **work sharing** provided they hold the appropriate accreditations, can adhere to the project/program requirements, and the client approved sending samples to that laboratory. The client must provide acknowledgement that the samples can be sent to that facility (an e-mail is sufficient documentation or if acknowledgement is verbal, the date, time, and name of person providing acknowledgement must be documented). The originating laboratory is responsible for communicating all technical, quality, and deliverable requirements as well as other contract needs. Refer to SOP No. CA-C-S-001, Work Sharing Process.

When the potential sub-contract laboratory does not meet the above criteria, Account Executives or PMs may nominate a laboratory as a subcontractor based on need. The decision to nominate a laboratory must be approved by the Laboratory Director. The Laboratory Director requests that the QA Manager begin the process of approving the subcontract laboratory. The client must provide acknowledgement that the samples can be sent to that facility (an e-mail is sufficient documentation or if acknowledgement is verbal, the date, time, and name of person providing acknowledgement must be documented).

8.2.1 The QA Manager must ensure that the Subcontracting Approval Form (Figure 8-2) has been completed and have supporting documentation on file prior to initiation of any work. A letter or e-mail is sent to the lab requesting the following information:

8.2.1.1 If a lab is NELAC or A2LA accredited,

8.2.1.1.1 Copy of necessary certifications verifying that the required approvals are current. Ensure that all needed analytes are included; some may not be accredit-able (if so, document). Certificate and scope of International Standard accreditation are required, when applicable.

8.2.1.1.2 Insurance Certificate. This is required by TestAmerica's Chief Financial Officer

8.2.1.1.3 USDA soil permit if available**

8.2.1.2 For Laboratories accredited by other agencies with an auditing program:

8.2.1.2.1 Copy of necessary certifications verifying that the required approvals are current. Ensure that all needed analytes are included; some may not be accredit-able (if so, document). Certificate and scope of International Standard accreditation are required, when applicable.

8.2.1.2.2 Insurance Certificate. This is required by TestAmerica's Chief Financial Officer

8.2.1.2.3 USDA soil permit if available**

8.2.1.2.4 Description of Ethics and Data Integrity Plan.

8.2.1.2.5 The most recent 2 sets of full proficiency testing (PT) results relevant to the analyses of interest and any associated corrective action.

- 8.2.1.2.6** State Audit with Corrective Action Response
- 8.2.1.2.7** Example final report to confirm format is compliant and provides the necessary information. (minimally, it must be determined that Batch QC results are included in the laboratory reports and data is appropriately qualified.
- 8.2.1.2.8** A copy of raw data associated with the first project is requested for internal review. The raw data is reviewed by the QA Manager and the PM to ensure that the results meet the client's needs. If the QA manager is unfamiliar with the analysis being performed, notify Corporate QA for guidance on the review (it may need to be sent elsewhere for evaluation). This requirement can be skipped if an on-site visit of the laboratory is planned. (This requirement is effective as of the effective date of this section. Laboratories worked with previously [minimum of 6 months] are grandfathered in.)
- 8.2.1.2.9** DoD work includes additional requirements as described in Section 8.1 above.
- 8.2.1.3** For laboratories performing tests that are unaccredited or accredited by an agency without an audit program:
 - 8.2.1.3.1** A copy of their Quality Assurance Manual (controlled if possible). Ensure data quality limits for relevant methods are acceptable and that training procedures are adequate.
 - 8.2.1.3.2** Copy of necessary certifications (if available) verifying that the required approvals are current. Ensure that all needed analytes are included; some may not be accredit-able (if so, document). Certificate and scope of International Standard accreditation are required, when applicable.
 - 8.2.1.3.3** Insurance Certificate. This is required by TestAmerica's Chief Financial Officer.
 - 8.2.1.3.4** USDA soil permit if available**
 - 8.2.1.3.5** Evidence of a current SOP per method. A copy of the first page and signature page of the SOP is acceptable. A table of contents including effective dates may also be acceptable. The SOP can be examined if an on-site audit is performed.
 - 8.2.1.3.6** Description of Ethics and Data Integrity Plan.
 - 8.2.1.3.7** The most recent 2 sets of full proficiency testing (PT) results relevant to the analyses of interest and any associated corrective action.
 - 8.2.1.3.8** Example final report to confirm format is compliant and provides the necessary information. (minimally, it must be determined that Batch QC results are included in the laboratory reports and data is appropriately qualified.
 - 8.2.1.3.9** Statement of Qualification (SOQ) or summary list of Technical Staff and Qualifications – position, education and years of experience.

8.2.1.3.10 DoD work includes additional requirements as described in Section 8.1 above.

8.2.1.3.11 A copy of raw data associated with the first project is requested for internal review. The raw data is reviewed by the QA Manager and the PM to ensure that the results meet the client's needs. If the QA manager is unfamiliar with the analysis being performed, notify Corporate QA for guidance on the review (it may need to be sent elsewhere for evaluation). This requirement can be skipped if an on-site visit of the laboratory is planned. (This requirement is effective as of the effective date of this section. Laboratories worked with previously [minimum of 6 months] are grandfathered in.)

8.2.2 Once the information is received by the QA Manager, it is evaluated for acceptability and forwarded to Corporate Contracts for formal contracting with the laboratory. They will add the lab to the approved list on the intranet site along with the associate documentation and notify the finance group for JD Edwards.

**USDA permit is required if soils less than three feet deep from New York, North Carolina, South Carolina, Georgia, Florida, Tennessee, Alabama, Mississippi, Louisiana, Arkansas, Texas, Oklahoma, New Mexico, Arizona, California, Hawaii, or outside the continental U. S. are to be analyzed. These samples require special shipping measures; check with the EHS Department. It may be necessary to heat-treat the samples before shipping if the subcontract laboratory does not have a USDA permit; however, some analytes/tests may be irrelevant after heat treatment.

8.2.3 The client will assume responsibility for the quality of the data generated from the use of a subcontractor they have requested the lab to use. The qualified subcontractors on the intranet site are known to meet minimal standards. The company does not certify laboratories. The subcontractor is on our approved list and can only be recommended to the extent that we would use them.

8.2.4 The status and performance of qualified subcontractors will be monitored periodically by the Corporate Contract Department. Any problems identified will be brought to Corporate QA attention.

- Complaints shall be investigated. Documentation of the complaint, investigation and corrective action will be maintained in the subcontractor's file on the intranet site. Complaints must be posted using the Vendor Performance Report (Form No. CW-F-WI-009).
- Information must be updated on the intranet when new information is received from the subcontracted laboratories.
- Subcontractors in good standing will be retained on the intranet listing. The QA Manager will notify all network laboratories and Corporate QA and Corporate Contracts if any laboratory requires removal from the intranet site. This notification will be posted on the intranet site and e-mailed to all Lab Directors/Managers, QA Managers and Sales Directors.

8.3 OVERSIGHT AND REPORTING

The PM must request that the selected subcontractor be presented with a subcontract, if one is not already executed between the laboratory and the subcontractor. The subcontract must

include terms which flow down the requirements of our clients, either in the subcontract itself or through the mechanism of work orders relating to individual projects. A standard subcontract and the Lab Subcontractor Vendor Package (posted on the intranet) can be used to accomplish this, and the Legal & Contracts Director can tailor the document or assist with negotiations, if needed. The PM (or RAE or CSM) responsible for the project must advise and obtain client consent to the subcontract as appropriate, and provide the scope of work to ensure that the proper requirements are made a part of the subcontract and are made known to the subcontractor.

Prior to sending samples to the subcontracted laboratory, the PM confirms their certification status to determine if it's current and scope-inclusive. The information is documented on a Subcontracted Sample Form (Figure 8-3) and the form is retained in the project folder. For network laboratories, certifications can be viewed on the company website.

The Sample Control department is responsible for ensuring compliance with QA requirements and applicable shipping regulations when shipping samples to a subcontracted laboratory.

All subcontracted samples must be accompanied by a Chain of Custody (COC). A copy of the original COC sent by the client must be included with all samples subbed within the network.

The PM will communicate with the subcontracted laboratory to monitor the status of the analyses, facilitate successful execution of the work and ensure the timeliness and completeness of the analytical report.

Non-NELAC accredited work must be identified in the subcontractor's report as appropriate. If NELAC accreditation is not required, the report does not need to include this information.

Reports submitted from subcontractor laboratories are not altered and are included in their original form in the final project report. This clearly identifies the data as being produced by a subcontractor facility. If subcontract laboratory data is incorporated into the laboratories EDD (i.e., imported), the report must explicitly indicate which lab produced the data for which methods and samples.

Note: The results submitted by a network work sharing laboratory may be transferred electronically and the results reported by the network work sharing lab are identified on the final report. The report must explicitly indicate which lab produced the data for which methods and samples. The final report must include a copy of the completed COC for all work sharing reports.

8.4 CONTINGENCY PLANNING

The Laboratory Director may waive the full qualification of a subcontractor process temporarily to meet emergency needs. In the event this provision is utilized, Corporate QA must be informed, and the QA Manager will be required to verify adequacy of proficiency scores and certifications. The laboratory must also request a copy of the raw data to support the analytical results for the first project submitted to the subcontract laboratory unless the laboratory has NELAC accreditation. The raw data is reviewed by the QA Manager and the PM to ensure that the results meet the client's needs. The QA Manager will request full documentation and qualify

the subcontractor under the provisions above. The approval process should be completed within 30 calendar days of subcontracting.

Figure 8-1.

Example - Client-Approved Subcontractor Form

Client Information:

Client Name & Account Number: _____

Client Contact: _____

Client Address: _____

Project Information: (Please choose all applicable.)

❖ **Certification required:** **State** **NELAC** **A2LA** **Method**____
 Target compound_____ **Other**_____

❖ **Required Turn around time (method provisional)**_____

Subcontractor's Information:

Subcontractor's Name: _____

Subcontractor's Contact: _____

Subcontractor's Email: _____

Subcontractor's Address: _____

Subcontractor's Phone Number: _____

Analytical Test/Compound/Method to be subcontracted: _____

Certification Statement:

I hereby give **TestAmerica Irvine** permission to use the above noted subcontractor for the above noted testing procedures/methods. I realize that the above subcontractor will be held liable for the validity of the above mentioned testing procedures/methods. All subcontractors shall meet the requirements as spelled out in project information and will follow all analytical holding times and turn around times for analytical reports. The subcontract laboratory, and not TestAmerica, will be held liable for liquidated damages for delays in subcontracted analytical reports and/or electronic data deliverables.

Client Signature

Date

**Figure 8-2.
Example - Subcontracting Laboratory Approval Form (Initial / Renewal)**

SUBCONTRACTING LABORATORY APPROVAL

Reference: Section 8 – Quality Assurance Manual

Date: _____
Laboratory: _____
Address: _____

Contact and e-mail address: _____
Phone: Direct _____ Fax _____

Requested Item ³	Date Received	Reviewed/ Accepted	Date
1. QA Manual ³			
2. Copy of State Certification ¹			
3. State Audit with Corrective Action Response (or NELAC or A2LA Audit) ³			
4. Most Recent (and relevant) 2 Sets of WP/WS Reports with Corrective Action Response ^{1,3}			
5. SOQ or Summary list of Technical Staff and Qualifications ³			
6. SOPs for Methods to Be Loadshifted ^{2,3}			
7. USDA Soil Permit			
8. Insurance Certificate			
9. Sample Report ³			
10. For DoD Work: Statement that Lab quality system complies with QSM.			
11. For DoD Work: Approved by specific DoD Component laboratory approval process.			
11. Description of Ethics Program ³			

1 - Required when emergency procedures are implemented.
2 - Some labs may not submit copies due to internal policies. In these cases, a copy of the first page and signature page of the SOP is acceptable. This requirement may also be fulfilled by supplying a table of SOPs with effective dates.
3 - If the laboratory has NELAC accreditation, Item #s 4 through 10 are not required.

On Site Audit Planned: YES NO If yes, Date Completed: _____ By Whom: _____

Comments: _____

Lab Acceptable for Subcontracting Work: YES NO Limitations: _____

QA Manager: _____ Date: _____
(Printed Name)

Forwarded to Contract Coordinator, by: _____ Date: _____

Figure 8-3.

Example - Subcontracted Sample Form

Date/Time: _____

Subcontracted Laboratory Information:

- Subcontractor's Name: _____
- Subcontractor Point of Contact: _____
- Subcontractor's Address: _____
- Subcontractor's Phone: _____
- Analyte/Method: _____
- Certified for State of Origin: _____
- NELAC Certified: Yes _____ No _____
- A2LA (or ISO 17025) Certified: Yes _____ No _____
- CLP-like Required:
(Full doc required) Yes _____ No _____
- Requested Sample Due Date:
(Must be put on COC) _____

Project Manager: _____

Laboratory Sample # Range: _____
(Only of Subcontracted Samples)

Laboratory Project Number (Billing Control #): _____

All subcontracted samples are to be sent via bonded carrier and Priority Overnight. Please attach tracking number below and maintain these records in the project files.

PM Signature _____ **Date** _____

SECTION 9

PURCHASING SERVICES AND SUPPLIES (NELAC 5.4.6)

9.1 OVERVIEW

Evaluation and selection of suppliers and vendors is performed, in part, on the basis of the quality of their products, their ability to meet the demand for their products on a continuous and short term basis, the overall quality of their services, their past history, and competitive pricing. This is achieved through evaluation of objective evidence of quality furnished by the supplier, which can include certificates of analysis, recommendations, and proof of historical compliance with similar programs for other clients. To ensure that quality critical consumables and equipment conform to specified requirements, all purchases from specific vendors are approved by a member of the supervisory or management staff.

Capital expenditures are made in accordance with the Controlled Purchases Procedure, CW-F-S-004. Only one quote is required where the item being purchased is a sole source product, Examples of sole source capital expenditures are laboratory test equipment, client specified purchases and building leases. A minimum of two quotes is required where the opportunity exists to source from more than one vendor. All documentation related to the purchase of capital items will be maintained in the individual CapEx files located in Corporate Purchasing. Data will be held in accordance with the record retention policy.

TestAmerica will enter into formal contracts with vendors when it is advantageous to do so. Contracts will be signed in accordance with the Authorization Matrix Policy, CW-F-P-002. Examples of items that are purchased through vendor contracts are laboratory instruments, consumables, copiers and office supplies. Request for Proposals (RFP's) will be issued where more information is required from the potential vendors than just price. RFP's allow TestAmerica to determine if a vendor is capable of meeting requirements such as supplying all of the TestAmerica facilities, meeting required quality standards and adhering to necessary ethical and environmental standards. The RFP process also allows potential vendors to outline any additional capabilities they may offer.

Non-capital expenditure items are purchased through the requisition and approval process in JD Edwards or through other TestAmerica authorized methods (approved web-sites, purchasing cards). Labs have the ability to select from the approved vendors in JD Edwards.

9.2 GLASSWARE

Glassware used for volumetric measurements must be Class A or verified for accuracy according to laboratory procedure. Pyrex (or equivalent) glass should be used where possible. For safety purposes, thick-wall glassware should be used where available.

9.3 REAGENTS, STANDARDS & SUPPLIES

Chemical reagents, solvents, glassware, and general supplies are ordered as needed to maintain sufficient quantities on hand. Purchasing guidelines for equipment and reagents must meet with the requirements of the specific method and testing procedures for which they are

being purchased. Solvents and acids are pre-tested in accordance with Corporate SOP on Solvent & Acid Lot Testing & Approval, SOP No. CA-Q-S-001 and laboratory SOP on Container and Reagent Verification by Lot Testing, LOTTEST.SOP

9.3.1 Purchasing

The nature of the analytical laboratory demands that all material used in any of the procedures is of a known quality. The wide variety of materials and reagents available makes it advisable to specify recommendations for the name, brand, and grade of materials to be used in any determination. This information is contained in the method SOP. [The analyst should complete the Material Request Sheet \(Figure 9-1\) when requesting reagents, standards, or supplies.](#)

[All orders are initiated by analysts qualified for the method for which material is being ordered. Items ordered are based on Materials and Reagents specified in the laboratory's method SOP. If an item being ordered is not the exact item specified, approval must be obtained from the Technical Director prior to placing the order. The Operations Manager or Laboratory Director approves the order.](#)

9.3.2 Receiving

It is the responsibility of the purchasing receiver to receive the shipment. It is the responsibility of the analyst who ordered the materials to date the material when received. Once the ordered reagents or materials are received, the analyst compares the information on the label or packaging to the original order to ensure that the purchase meets the quality level specified. Material Safety Data Sheets (MSDSs) are kept in each department and online through the Company's intranet website. Anyone may review these for relevant information on the safe handling and emergency precautions of on-site chemicals.

9.3.3 Specifications

There are many different grades of analytical reagents available to the analyst. All methods in use in the laboratory specify the grade of reagent that must be used in the procedure. If the quality of the reagent is not specified, it may be assumed that it is not significant in that procedure and, therefore, any grade reagent may be used. It is the responsibility of the analyst to check the procedure carefully for the suitability of grade of reagent.

Chemicals must not be used past the manufacturer's expiration date and must not be used past the expiration time noted in a method SOP. If dates are not provided, the laboratory may contact the manufacturer to determine an expiration date.

The laboratory assumes a five year expiration date on inorganic dry chemicals unless noted otherwise by the manufacturer or by the reference source method.

- An expiration date can not be extended if the dry chemical is discolored or appears otherwise physically degraded, the dry chemical must be discarded.
- Expiration dates can be extended if the dry chemical is found to be satisfactory based on acceptable performance of quality control samples (Continuing Calibration Verification (CCV), Blanks, Laboratory Control Sample (LCS), etc.).

- If the dry chemical is used for the preparation of standards, the expiration dates can be extended 6 months if the dry chemical is compared to an unexpired independent source in performing the method and the performance of the dry chemical is found to be satisfactory. The comparison must show that the dry chemical meets CCV limits. The comparison studies are maintained in the QA office.

Wherever possible, standards must be traceable to national or international standards of measurement or to national or international reference materials. Records to that effect are available to the user.

Compressed gases in use are checked for pressure and secure positioning daily. The minimum total pressure must be 300 psig (at least 500 psig for overnight) or the tank must be replaced. The quality of the gases must meet method or manufacturer specification or be of a grade that does not cause any analytical interference.

Water used in the preparation of standards or reagents must have a conductivity of less than 1.0 $\mu\text{ohm-cm}$ at 25°C. The conductivity is checked and recorded daily. If the water's conductivity is less than the specified limit, the Technical Director, Operations Manager, Lab Director or QA Manager must be notified immediately in order to notify all departments, decide on cessation (based on intended use) of activities, and make arrangements for correction.

The laboratory may purchase reagent grade (or other similar quality) for use in the laboratory. This water must be certified "clean" by the supplier for all target analytes or otherwise verified by the laboratory prior to use. This verification is documented.

Standard lots are verified before first time use if the laboratory switches manufacturers or has historically had a problem with the type of standard.

Purchased VOA vials must be certified clean and the certificates must be maintained. If uncertified VOA vials are purchased, all lots must be verified clean prior to use. This verification must be maintained.

9.3.4 Storage

Reagent and chemical storage is important from the aspects of both integrity and safety. Light-sensitive reagents may be stored in brown-glass containers. Table 9-1 details specific storage instructions for reagents and chemicals. Section 22 discusses conditions for standard storage.

9.4 PURCHASE OF EQUIPMENT/INSTRUMENTS/SOFTWARE

When a new piece of equipment is needed, either for additional capacity or for replacing inoperable equipment, the analyst or supervisor makes a supply request to the Laboratory Director. If they agree with the request the procedures outlined in Policy No. CA-T-P-001, Qualified Products List, are followed. A decision is made as to which piece of equipment can best satisfy the requirements. The appropriate written requests are completed and purchasing places the order.

Upon receipt of a new or used piece of equipment, it is given a short name, such as GCMS77, and added to the QA-maintained equipment list described in Section. A New Instrumentation

Checklist is initiated (see figure 9-3) to ensure IT back-up, maintenance logbook creation, MDLs, etc are completed. The instrument's capability is assessed to determine if it is adequate or not for the specific application. For instruments, a calibration curve is generated, followed by MDLs, Demonstration of Capabilities (DOCs), and other relevant criteria (see Section 20). For software, its operation must be deemed reliable and evidence of instrument verification must be retained by the IT Department or QA Department as specified in the laboratory's procedure for software verification. Software certificates supplied by the vendors are filed with the LIMS Administrator. The manufacturer's operation manual is retained at the bench.

9.5 SERVICES

Service to analytical instruments (except analytical balances) is performed on an as needed basis. Routine preventative maintenance is discussed in Section 21. The need for service is determined by analysts and/or Department Managers. The service providers that perform the services are approved by the Department Managers.

9.6 SUPPLIERS

TestAmerica selects vendors through a competitive proposal / bid process, strategic business alliances or negotiated vendor partnerships (contracts). The level of control used in the selection process is dependent on the anticipated spend and the potential impact on TestAmerica business. Vendors that provide test and measuring equipment, solvents, standards, certified containers, instrument related service contracts or subcontract laboratory services shall be subject to more rigorous controls than vendors that provide off-the-shelf items of defined quality that meet the end use requirements. The JD Edwards purchasing system includes all suppliers /vendors that have been approved for use.

Evaluation of suppliers is accomplished by ensuring the supplier ships the product or material ordered and that the material is of the appropriate quality. This is documented by signing off on packing slips or other supply receipt documents. The purchasing documents contain the data that adequately describe the services and supplies ordered.

Any issues of vendor performance are to be reported immediately by the laboratory staff to the Corporate Purchasing Group by completing a Vendor Performance Report (CW-F-WI-009).

The Corporate Purchasing Group will work through the appropriate channels to gather the information required to clearly identify the problem and will contact the vendor to report the problem and to make any necessary arrangements for exchange, return authorization, credit, etc.

As deemed appropriate, the Vendor Performance Reports will be summarized and reviewed to determine corrective action necessary, or service improvements required by vendors

The laboratory has access to a listing of all approved suppliers of critical consumables, supplies and services. This information is provided through the JD Edwards purchasing system.

9.6.1 New Vendor Procedure

TestAmerica employees who wish to request the addition of a new vendor must complete a J.D. Edwards Vendor Add Request Form (CW-F-WI-007 – refer to Figure 9-2).

New vendors are evaluated based upon criteria appropriate to the products or services provided as well as their ability to provide those products and services at a competitive cost. Vendors are also evaluated to determine if there are ethical reasons or potential conflicts of interest with TestAmerica employees that would make it prohibitive to do business with them as well as their financial stability. The QA Department and/or the Technical Manager are consulted with vendor and product selection that have an impact on quality.

Figure 9-1.
Materials Request Sheet

The screenshot displays the 'General Requisition - Order Detail' window in a Microsoft Internet Explorer browser. The window title is 'General Requisition - Order Detail'. The application header shows 'JDE EDWARDS' and 'General Requisition - Order Detail'. Below the header is a menu bar with 'OK', 'Cancel', 'Form', 'Row', and 'Tools'. There are also icons for a checkmark, a red X, a printer, a grid, and a refresh button.

The main content area is divided into two tabs: 'Order Detail' (selected) and 'Line Defaults'. The 'Order Detail' tab contains a form with the following fields:

- Order Number: 409881 OR 00440
- Branch/Plant: 440260
- Supplier: 112521 VWR SCIENTIFIC PRODU... Order Revision: [empty]
- Address Number: 140 TesAmerica Irvine Order Date: 11/23/2007
- Hold Code: [empty] Blank - Hold Codes 42/HC
- Currency: USD Exchange Rate: [empty] Base: [empty] Foreign:

Below the form is a table with the following columns: Date Needed, Account Number, Vendor Part Number, Description 1, Quantity Ordered, Tr. UoM, Unit Cost, Extended Cost, Tax Y/N, Ln Ty, and Item Number. The table is currently empty, showing only the header row. A 'Records 1 - 1' indicator is visible above the table. A 'Customize Grid' button is located in the top right corner of the table area.

The Windows taskbar at the bottom shows the Start button and several open applications, including 'Inbox', '12 Remin...', 'ET-Edwa...', 'Adobe A...', 'QAM Te...', 'Element ...', 'Microsoft...', 'Microsoft...', 'PeopleSo...', and 'General ...'. The system clock shows '12:44 PM'.

Table 9-1.
Storage of Reagents and Chemicals

Chemical	Storage Requirements
Concentrated Acids and Bases	Stored in the original containers at room temperature. All organic acids must be stored separately from inorganic acids. Acids should not be stored with bases.
Bulk Dry Chemicals	Stored in the original containers at room temperature. All organic acids must be stored separately from inorganic acids. Acids should not be stored with bases.
Working Solutions containing Organic Compounds	Stored as per method recommendation/ requirement. They are generally stored refrigerated at $4^{\circ}\text{C} \pm 2^{\circ}\text{C}$.
Working Solutions containing only Inorganics	Stored at room temperature; refrigeration is optional.
Flammable Solvents	Stored in solvent cabinets at room temperature.
Non-Flammable Solvents	Stored separately from the flammable solvents in cabinets at room temperature.

Figure 9-2
Example – JD Edwards Vendor Add Request Form



JD Edwards Vendor Add Request Form

Vendor name:	Lab location <u>and</u> individual making request:
Vendor address (remit to):	Vendor phone:
Vendor address (remit to):	Vendor fax:
Contact name:	Product / service provided:

Reason for Vendor Addition: Check all reasons that apply

<input type="checkbox"/> Cost Reduction	Estimated Annual Savings \$
<input type="checkbox"/> Replace Current Vendor	Reason?
	Vendor being Replaced?
<input type="checkbox"/> New Product / Service	Describe:
<input type="checkbox"/> ISO Approved (Required for Aerotech / P&K only)	

Small Business:

Does this vendor help us to meet our small business objectives: _____
 If yes, which category: _____

Personal and Ethical Considerations:

Is there any personal conflict of interest with a TestAmerica employee and the vendor listed above? _____
 Have ethical considerations been taken into account in your evaluation of this vendor? _____

Can this product be sourced from another TestAmerica facility? _____

Please complete form and email to NCPurchasing@testamericainc.com or fax to (330) 966-9275.

I approve the addition of this vendor:

 Purchasing Manager - Patrick Eckman

 Corporate Controller - Leslie Bowers

Form No. CW-F-WI-007

Figure 9-3.
New Instrumentation Checklist

Instrumentation/Equipment Checklist

To be completed by the department:

Department:			
ID Number:			
Date Installed:			
Method(s) Performed:			

Type*:			
Manufacturer:			
Model Number:			
Serial Number:			

*IC, GC, Autosampler, Balance, ASE etc.

To be completed by QA:

Item	Applicable	Date/ Initials	Comments
Maintenance/monitoring logbook created	Yes <input type="checkbox"/> No <input type="checkbox"/>		
IT informed (so data backup process can be updated)	Yes <input type="checkbox"/> No <input type="checkbox"/>		
Instrument tagged with ID number	Yes <input type="checkbox"/> No <input type="checkbox"/>		
Instrument ID number entered into Element	Yes <input type="checkbox"/> No <input type="checkbox"/>		
Calibrated thermometer placed in unit	Yes <input type="checkbox"/> No <input type="checkbox"/>		
Passing calibration performed and documented	Yes <input type="checkbox"/> No <input type="checkbox"/>		
Passing MDLs performed for all relevant methods and matrices	Yes <input type="checkbox"/> No <input type="checkbox"/>		
Laboratory equipment list updated	Yes <input type="checkbox"/> No <input type="checkbox"/>		

G:\Depts\QUALITY\EQUIPMT\New Instrumentation Checklist_r1.doc
 Version 11/12/07

SECTION 10

SERVICE TO THE CLIENT (NELAC 5.4.7)

10.1 OVERVIEW

TestAmerica Irvine cooperates with clients and their representatives to monitor the laboratory's performance in relation to work performed for the client. It is the laboratory's goal to meet all client requirements in addition to statutory and regulatory requirements discussed in Section 5. The laboratory has procedures to ensure confidentiality to clients (Section 16 and 26).

Note: ISO 17025/NELAC 2003 states that a laboratory "shall afford clients or their representatives cooperation to clarify the client's request". This topic is discussed in Section 7.

10.2 SPECIAL SERVICES

The laboratory's standard procedures for reporting data are described in Section 26. When requested the following special services are provided:

- The laboratory will provide the client or the client's representative reasonable access to the relevant areas of the laboratory for the witnessing of tests performed for the client.
- The laboratory will work with client-specified third party data validators as specified in the client's contract.
- The laboratory will provide the client with all requested information pertaining to the analysis of their samples. An additional charge may apply for additional data/information that was not requested prior to the time of sample analysis or previously agreed upon.

10.3 CLIENT COMMUNICATION

Project managers are an important communication link to the clients. The lab shall inform its clients of any delays in project completion as well as any non-conformances in either sample receipt (refer to Section 24) or sample analysis. **Project management** will maintain ongoing client communication throughout the entire client project.

Technical Directors are available to discuss any technical questions or concerns that the client may have.

10.4 REPORTING

The laboratory will work with the client to produce any special communication reports required by the contract.

10.5 CLIENT SURVEYS

The laboratory assesses both positive and negative client feedback. The results are used to improve overall laboratory quality and client service.

TestAmerica Irvine participates in the American Council of Independent Laboratories (ACIL) Seal of Excellence program. This program includes the submission of a survey to laboratory clients. The clients send their responses directly to ACIL.

TestAmerica's Sales and Marketing teams periodically develops lab and client specific surveys to assess client satisfaction.

SECTION 11

COMPLAINTS (NELAC 5.4.8)

11.1 OVERVIEW

TestAmerica Irvine believes that effective client complaint handling processes have important business and strategic value. Listening to and documenting client concerns captures 'client knowledge' that helps to continually improve processes and improving client satisfaction. An effective client complaint handling process also provides assurance to the data user that the laboratory will stand behind its data, service obligations and products.

A client complaint is any expression of dissatisfaction with any aspect of our business services, communications, responsiveness, data, reports, invoicing and other functions expressed by any party, whether received verbally or in written form. Client inquiries, complaints or noted discrepancies are documented, communicated to management, and addressed promptly and thoroughly.

The laboratory has procedures for dealing with both external and internal complaints.

The nature of the complaint is identified, documented and investigated, and an appropriate action is determined and taken. In cases where a client complaint indicates that an established policy or procedure was not followed, the QA Department must evaluate whether a special audit must be conducted to assist in resolving the issue. A written confirmation or letter to the client, outlining the issue and response taken is recommended as part of the overall action taken.

The process of complaint resolution and documentation utilizes the procedures outlined in Section 13 (Corrective Actions) and is documented following [the laboratory's SOP for Corrective Actions, CAR.SOP](#). It is the laboratory's goal to provide a satisfactory resolution to complaints in a timely and professional manner.

11.2 EXTERNAL COMPLAINTS

An employee that receives a complaint initiates the complaint resolution process and the documentation of the complaint.

Complaints fall into two categories: correctable and non-correctable. An example of a correctable complaint would be one where a report re-issue would resolve the complaint. An example of a non-correctable complaint would be one where a client complains that their data was repeatedly late. Non-correctable complaints should be reviewed for preventive action measures to reduce the likely hood of future occurrence and mitigation of client impact.

The general steps in the complaint handling process are:

- Receiving Complaints
- Complaint Investigation and Service Recovery
- Process Improvement

The laboratory shall inform the initiator of the complaint of the results of the investigation and the corrective action taken, if any.

11.3 INTERNAL COMPLAINTS

Internal complaints include, but are not limited to: errors and non-conformances, training issues, internal audit findings, and deviations from methods. Corrective actions may be initiated by any staff member who observes a nonconformance and shall follow the procedures outlined in Section 13. In addition, Corporate management, Sales and Marketing and Information Technology (IT) may initiate a complaint by contacting the laboratory or through the corrective action system described in Section 13.

11.4 MANAGEMENT REVIEW

The number and nature of client complaints is reported by the QA Manager to the laboratory and QA Director in the QA Monthly report. Monitoring and addressing the overall level and nature of client complaints and the effectiveness of the solutions is part of the Annual Management Review (Section 17)

SECTION 12

CONTROL OF NON-CONFORMING WORK (NELAC 5.4.9)

12.1 OVERVIEW

When data discrepancies are discovered or deviations and departures from laboratory standard procedures, policies and/or client requests have occurred, corrective action is taken immediately. First, the laboratory evaluates the significance of the nonconforming work. Then, a corrective action plan is initiated based on the outcome of the evaluation. If it is determined that the nonconforming work is an isolated incident, the plan could be as simple as adding a qualifier to the final results and/or making a notation in the case narrative. If it is determined that the nonconforming work is a systematic or improper practices issue, the corrective action plan could include a more in depth investigation and a possible suspension of an analytical method. In all cases, the actions taken are documented using the laboratory's corrective action system (refer to Section 13).

Due to the frequently unique nature of environmental samples, sometimes departures from documented policies and procedures are needed. [When an analyst encounters such a situation, the problem is presented to the department manager or group leader for advice. The manager or group leader may elect to discuss it with the project manager or QA manager. If necessary, client may be contacted to decide on a logical course of action. Once an approach is agreed upon, the analyst documents it using the laboratories corrective action system described in Section 13. This information can then be supplied to the client in the form of a footnote or a case narrative with the report.](#)

[Project Management may encounter situations where a client may request that a special procedure be applied to a sample that is not standard lab practice. Based on a technical evaluation, the lab may accept or opt to reject the request based on technical or ethical merit. An example might be the need to report a compound that the lab does not normally report. The lab would not have validated the method for this compound following the procedures in Section 20. The client may request that the compound be reported based only on the calibration. Such a request would need to be approved by the Department Manager and QA Manager, documented and included in the project folder. Deviations **must** also be noted on the final report with a statement that the compound is not reported in compliance with NELAC \(or the analytical method\) requirements and the reason. Data being reported to a non-NELAC state would need to note the change made to how the method is normally run.](#)

12.2 RESPONSIBILITIES AND AUTHORITIES

SOP No. CA-L-S-001, Internal Investigation of Potential Data Discrepancies and Determination for Data Recall, outlines the general procedures for the reporting and investigation of data discrepancies and alleged incidents of misconduct or violations of the company's data integrity policies as well as the policies and procedures related to the determination of the potential need to recall data.

Under certain circumstances the [Laboratory Director, a Department Manager, or a member of the QA team](#) may exceptionally authorize departures from documented procedures or policies.

The departures may be a result of procedural changes due to the nature of the sample; a one-time procedure for a client; QC failures with insufficient sample to reanalyze, etc. In most cases, the client will be informed of the departure prior to the reporting of the data. Any departures must be well documented using the laboratory's corrective action procedures described in Section 13. [This information may also need to be documented in logbooks and/or data review checklists as appropriate.](#) Any impacted data must be referenced in a case narrative and/or flagged with an appropriate data qualifier.

Any misrepresentation or possible misrepresentation of analytical data discovered by any laboratory staff member must be reported to facility senior laboratory management within 24-hours. The Senior Management staff is comprised of the [Laboratory Director, the QA Manager, and the Department Managers](#). The reporting of issues involving alleged violations of the company's Data Integrity or Manual Integration procedures must be conveyed to an Ethics and Compliance Officer (ECO) and Quality Director within 24 hours.

Whether an inaccurate result was reported due to calculation or quantitation errors, data entry errors, improper practices, or failure to follow SOPs, the data must be evaluated to determine the possible effect.

The Laboratory Director, QA Manager, ECOs, COO's – East and West, General Managers and the Quality Directors – East and West have the authority and responsibility to halt work, withhold final reports, or suspend an analysis for due cause as well as authorize the resumption of work.

12.3 EVALUATION OF SIGNIFICANCE AND ACTIONS TAKEN

For each nonconforming issue reported, an evaluation of its significance and the level of management involvement needed is made. This includes reviewing its impact on the final data, whether or not it is an isolated or systematic issue, and how it relates to any special client requirements.

SOP No. CA-L-S-001 distinguishes between situations when it would be appropriate for the laboratory QA Manager and Laboratory Director (or his/her designee) to make the decision on the need for client notification (written or verbal) and data recall (report revision) and when the decision must be made with the assistance of the ECO's and Corporate Management. Laboratory level decisions are documented and approved using the laboratory's standard nonconformance/corrective action reporting (Section 13) in lieu of the data recall determination form contained in SOP No. CA-L-S-001.

12.4 PREVENTION OF NONCONFORMING WORK

If it is determined that the nonconforming work could recur, further corrective actions must be made following the laboratory's corrective action system (Section 13).

On a monthly basis, the QA Department evaluates non-conformances to determine if any nonconforming work has been repeated multiple times. If so, the laboratory's corrective action process may be followed.

12.5 METHOD SUSPENSION/RESTRICTION (STOP WORK PROCEDURES)

In some cases it may be necessary to suspend/restrict the use of a method or target compound which constitutes significant risk and/or liability to the laboratory. Suspension/restriction procedures can be initiated by any of the persons noted in Section 12.2, Paragraph 5 above.

Prior to suspension/restriction, confidentiality will be respected, and the problem and the required corrective and preventive action will be stated in writing and presented to the Laboratory Director.

The Laboratory Director shall arrange for the appropriate personnel to meet with the QA Manager as needed. This meeting shall be held to confirm that there is a problem, that suspension/restriction of the method is required and will be concluded with a discussion of the steps necessary to bring the method/target or test fully back on line. In some cases that may not be necessary if all appropriate personnel have already agreed there is a problem and there is agreement on the steps needed to bring the method, target or test fully back on line.

The QA Manager will also initiate a corrective action report as described in Section 13 if one has not already been started. A copy of any meeting notes and agreed upon steps should be faxed or e-mailed by the laboratory to the appropriate General Manager and member of Corporate QA. This fax/e-mail acts as notification of the incident.

After suspension/restriction, the lab will hold all reports to clients pending review. No faxing, mailing or distributing through electronic means may occur. The report must not be posted for viewing on the internet. It is the responsibility of the Laboratory Director to hold all reporting and to notify all relevant laboratory personnel regarding the suspension/restriction (i.e., Project Management, Log-in, etc...). Clients will NOT generally be notified at this time. Analysis may proceed in some instances depending on the non-conformance issue.

Within 72 hours, the QA Manager will determine if compliance is now met and reports can be released, OR determine the plan of action to bring work into compliance, and release work. A team, with all principals involved (Laboratory Director, [Department Manager](#), QA Manager) can devise a start-up plan to cover all steps from client notification through compliance and release of reports. [The Client Services Manager](#) and Sales and Marketing should be notified if clients must be notified or if the suspension/restriction affects the laboratory's ability to accept work. The QA Manager must approve start-up or elimination of any restrictions after all corrective action is complete. This approval is given by final signature on the completed corrective action report as described in Section 13.

SECTION 13

CORRECTIVE ACTION (NELAC 5.4.10)

13.1 OVERVIEW

A major component of TestAmerica's Quality Assurance (QA) Program is the problem investigation and feedback mechanism designed to keep the laboratory staff informed on quality related issues and to provide insight to problem resolution. When nonconforming work or departures from policies and procedures in the quality system or technical operations are identified, the corrective action procedure provides a systematic approach to assess the issues, restore the laboratory's system integrity, and prevent reoccurrence. Corrective actions are documented using [Non-Conformance Reports \(NCR\)](#) and [Corrective Action Reports \(CAR\)](#) (refer to Figure 13-1).

13.2 DEFINITIONS

- **Correction:** Actions necessary to correct or repair analysis specific non-conformances. The acceptance criteria for method specific QC and protocols as well as the associated corrective actions are contained in [the method specific SOPs](#). The analyst will most frequently be the one to identify the need for this action as a result of calibration checks and QC sample analysis. No significant action is taken to change behavior, process or procedure.
- **Corrective Action:** The action taken is not only a correction made to the immediate event, but a change in process, procedure or behavior that is required to eliminate the causes of an existing nonconformity, defect, or other undesirable situation in order to prevent recurrence.

13.3 GENERAL

Problems within the quality system or within analytical operations may be discovered in a variety of ways, such as QC sample failures, internal or external audits, proficiency testing (PT) performance, client complaints, staff observation, etc.

The purpose of a corrective action system is to:

- Identify non-conformance events and assign responsibility for investigation.
- Resolve non-conformance events and assign responsibility for any required corrective action.
- Identify Systematic Problems before they become serious.
- Identify and track Client complaints and provide resolution (see more on client complaints in Section 11).

13.3.1 Non-Conformance Report (NCR) - is used to document the following types of corrective actions:

- Deviations from an established procedure or SOP
- QC outside of limits (non matrix related)

- Isolated Reporting / Calculation Errors
- Client Complaints

13.3.2 Corrective Action Report (CAR) - is used to document the following types of corrective actions:

- Questionable trends that are found in the monthly review of NCRs.
- Issues found while reviewing NCRs that warrant further investigation.
- Failed or Unacceptable PT results.
- Corrective actions that cross multiple departments in the laboratory.
- Systematic Reporting / Calculation Errors
- Health and Safety Violations

13.4 CLOSED LOOP CORRECTIVE ACTION PROCESS

Any employee in the company can initiate a corrective action. There are four main components to a closed-loop corrective action process once an issue has been identified: Cause Analysis, Selection and Implementation of Corrective Actions (both short and long term), Monitoring of the Corrective Actions, and Follow-up.

13.4.1 Cause Analysis

- Upon discovery of a non-conformance event, the event must be defined and documented. An **NCR or CAR** must be initiated, someone is assigned to investigate the issue and the event is investigated for cause. Table 13-1 provides some general guidelines on determining responsibility for assessment.
- The cause analysis step is the key to the process as a long term corrective action cannot be determined until the cause is determined.
- If the cause is not readily obvious, the Department Manager, Lab Director, or QA Manager (or QA designee) is consulted.

13.4.2 Selection and Implementation of Corrective Actions

- Where corrective action is needed, the laboratory shall identify potential corrective actions. The action(s) most likely to eliminate the problem and prevent recurrence are selected and implemented. Responsibility for implementation is assigned.
- Corrective actions shall be to a degree appropriate to the magnitude of the problem identified through the cause analysis.
- Whatever corrective action is determined to be appropriate, the laboratory shall document and implement the changes. **The NCR or CAR** is used for this documentation.

13.4.3 Monitoring of the Corrective Actions

- The Department Manager and QA Manager is responsible to ensure that the corrective action taken was effective.

- Ineffective actions will be documented and re-evaluated until acceptable resolution is achieved. Department Managers are accountable to the Laboratory Director to ensure final acceptable resolution is achieved and documented appropriately.
- Each NCR and CAR is entered into a database for tracking purposes and a monthly summary of all corrective actions is printed out for review to aid in ensuring that the corrective actions have taken effect.
- The QA Manager reviews monthly NCRs and CARs for trends. Highlights are included in the QA monthly report (refer to Section 17). If a significant trend develops that adversely affects quality, an audit of the area is performed and corrective action implemented.
- Any out-of-control situations that are not addressed acceptably at the laboratory level may be reported to the Corporate Quality Director by the QA Manager, indicating the nature of the out-of-control situation and problems encountered in solving the situation.

13.4.4 Follow-up Audits

- Follow-up audits may be initiated by the QA Manager and shall be performed as soon as possible when the identification of a nonconformance casts doubt on the laboratory's compliance with its own policies and procedures, or on its compliance with state or federal requirements. (Section 16 includes additional information regarding internal audit procedures.)
- These audits often follow the implementation of the corrective actions to verify effectiveness. An additional audit would only be necessary when a critical issue or risk to business is discovered.

13.5 TECHNICAL CORRECTIVE ACTIONS

In addition to providing acceptance criteria and specific protocols for technical corrective actions in [the method SOPs and Appendix 4](#), the laboratory has general procedures to be followed to determine when departures from the documented policies and procedures and quality control have occurred (refer to Section 12 for information regarding the control of non-conforming work). The documentation of these procedures is through the use of an [NCR or CAR](#).

Table 13-1 includes examples of general technical corrective actions. For specific criteria and corrective actions refer to [specific method SOPs and Appendix 4](#).

Table 13-1 provides some general guidelines for identifying the individual(s) responsible for assessing each QC type and initiating corrective action. The table also provides general guidance on how a data set should be treated if associated QC measurements are unacceptable. Specific procedures are included in [Method SOPs](#), QAM Sections 20, 21 and Appendix 4, and SOP CA-L-S-001 (Internal Investigation of Potential Data Discrepancies and Determination for Data Recall). The QA Manager reviews all corrective actions, at a minimum, monthly and highlights are included in the QA monthly report.

To the extent possible, samples shall be reported only if all quality control measures are acceptable. If the deficiency does not impair the usability of the results, data will be reported with an appropriate data qualifier and/or the deficiency will be noted in the case narrative. Where

sample results may be impaired, the Project Manager is notified by a written NCR or CAR and appropriate corrective action (e.g., reanalysis) is taken and documented.

13.6 BASIC CORRECTIONS

When mistakes occur in records, each mistake shall be crossed-out, and not erased, deleted, made illegible, or otherwise obliterated (e.g. no white-out), and the correct value entered alongside. All such corrections shall be initialed (or signed) and dated by the person making the correction. In the case of records stored electronically, the original "uncorrected" file must be maintained intact and a second "corrected" file is created.

This same process applies to adding additional information to a record. All additions made later than the initial must also be initialed (or signed) and dated.

When corrections are due to reasons other than obvious transcription errors, the reason for the corrections (or additions) shall also be documented.

Figure 13-1a.
Example - Corrective Action Report (initial entry screen)

The screenshot shows a software window titled "Corrective Action Report - Leslie VanExel". The window has a menu bar with "Corrective Action", "Supervisor", "QA", "PM", "Print", and "Exit". Below the menu bar, there are several input fields: "CAR No." with a dropdown menu set to "<NEW>" and a search icon; "Status" with a dropdown menu set to "Open"; "Entered By" with a text box containing "Leslie VanExel"; "Date Entered" with a dropdown menu set to "10/28/2003"; and a "Client Complaint" checkbox which is unchecked. There are "Commit" and "Cancel" buttons. Below these fields are several tabs: "Issue", "Batch/Work Order Information", "Supervisor", "Quality Assurance", and "Project Management". The "Issue" tab is selected. Under "Issue Information", there are radio buttons for "Employee" (unselected) and "Department" (selected). The "Employee" dropdown is set to "None Specified" and the "Department" dropdown is set to "Administrators". There is also a "Date of Occurrence" dropdown set to "10/28/2003" and an "Instrument" dropdown. An "Additional Issue Notes" icon is present. Below this are four sections, each with a dropdown menu and a "Description" text area: "Issue", "Issue Cause", "Employee Oversight", and "Internal Corrective Action".

Figure 13-1b.
Example - Corrective Action Report (batch/workorder information)

Corrective Action Report - Leslie VanExel

Corrective Action Supervisor QA PM Print Exit

CAR No. 14 Status Open Client Complaint Enter

Entered By Michael Bracken Date Entered 10/17/2003 Cancel

Issue Batch/Work Order Information Supervisor Quality Assurance Project Management

Batch / Work Order Information

Batches / Work Orders Involved (Double Click to Modify)

Work Order	Sample	Matrix	Analysis	Analyte
------------	--------	--------	----------	---------

Client Information

Lab Number	Client	Project	Logged	Due
------------	--------	---------	--------	-----

Table 13-1.

Example – General Corrective Action Procedures

QC Activity (Individual Responsible for Initiation/Assessment)	Acceptance Criteria	Recommended Corrective Action
Initial Instrument Blank <i>(Analyst)</i>	- Instrument response < MDL or MRL.	- Prepare another blank. - If same response, determine cause of contamination: reagents, environment, instrument equipment failure, etc..
Initial Calibration Standards <i>(Analyst, Supervisor)</i>	- Correlation coefficient > 0.990 (organics) or >0.995 (inorganics) or RSD within Method SOP limits. - % Recovery within acceptance range documented in Method SOP, QAM section 21 and QAM Appendix 4	- Reanalyze standards. - If still unacceptable, remake standards and recalibrate instrument.
Independent Calibration Verification (Second Source) <i>(Analyst, Supervisor)</i>	% Recovery within control limits.	- Remake and reanalyze standard. - If still unacceptable, then remake calibration standards or use new primary standards and recalibrate instrument.
Continuing Calibration Standards <i>(Analyst, Data Reviewer)</i>	% Recovery within control limits.	- Reanalyze standard. - If still unacceptable, then recalibrate and rerun affected samples.
Matrix Spike / Matrix Spike Duplicate (MS/MSD) <i>(Analyst, Data Reviewer)</i>	- % Recovery within acceptance range documented in Method SOP, QAM section 21 and QAM Appendix 4	- If the acceptance criteria for duplicates or matrix spikes are not met because of matrix interferences, the acceptance of the analytical batch is determined by the validity of the LCS. - If the LCS is within acceptable limits the batch is acceptable. - The results of the duplicates, matrix spikes and the LCS are reported with the data set.
Laboratory Control Sample (LCS) <i>(Analyst, Data Reviewer)</i>	- % Recovery within acceptance range documented in Method SOP, QAM section 21 and QAM Appendix 4	- Batch must be re-prepared and re-analyzed. Note: If there is insufficient sample or the holding time cannot be met, contact client and report with flags.

QC Activity <i>(Individual Responsible for Initiation/Assessment)</i>	Acceptance Criteria	Recommended Corrective Action
Surrogates <i>(Analyst, Data Reviewer)</i>	- % Recovery within acceptance range documented in Method SOP, QAM section 21 and QAM Appendix 4.	- Individual sample must be repeated. - If associated analytes are ND, qualify data only
Method Blank (MB) <i>(Analyst, Data Reviewer)</i>	$< \text{MRL}^1$	- Reanalyze blank. - If still positive, determine source of contamination. If necessary, reprocess (i.e. digest or extract) entire sample batch. Report blank results. - If associated analytes are either ND or $>10x$ (inorganics) or $>20x$ (organics) data can be reported with qualifier
Proficiency Testing (PT) Samples <i>(QA Manager, Department Manager/Supervisor)</i>	- Criteria supplied by PT Supplier.	- Any failures or warnings must be investigated for cause. Failures may result in the need to repeat a PT sample to show the problem is corrected.
Reporting / Calculation Errors (Depends on issue – possible individuals include: Analysts, Data Reviewers, Project Managers, Department Manager/Supervisor, QA Manager, Corporate QA, Corporate Management)	- SOP CA-L-S-001, Internal Investigation of Potential Data Discrepancies and Determination for Data Recall.	- Corrective action is determined by type of error. Follow the procedures in SOP CA-L-S-001.
Client Complaints <i>(Project Managers, Lab Director, Sales and Marketing)</i>	- Not Applicable	- Corrective action is determined by the type of complaint. For example, a complaint regarding an incorrect address on a report will result in the report being corrected and then follow-up must be performed on the reasons the address was incorrect (e.g., database needs to be updated).
QA Monthly Report (Refer to Section 17 for an example) (QA Manager, Lab Director, Department Supervisors/Managers)	- QAM, SOPs.	- Corrective action is determined by the type of issue. For example, CARs for the month are reviewed and possible trends are investigated.

QC Activity (Individual Responsible for Initiation/Assessment)	Acceptance Criteria	Recommended Corrective Action
Health and Safety Violation (Safety Officer, Lab Director, Department Supervisor/Manager)	- Environmental Health and Safety (EHS) Manual.	- Non-conformance is investigated and corrected through CAR system.

Note:

1. Except as noted below for certain compounds, the method blank should be below the detection limit. Concentrations up to five times the reporting limit will be allowed for the ubiquitous laboratory and reagent contaminants: methylene chloride, toluene, acetone, 2-butanone and phthalates provided they appear in similar levels in the reagent blank and samples. This allowance presumes that the detection limit is significantly below any regulatory limit to which the data are to be compared and that blank subtraction will not occur. For benzene and ethylene dibromide (EDB) and other analytes for which regulatory limits are extremely close to the detection limit, the method blank must be below the method detection limit

SECTION 14.0

PREVENTIVE ACTION (NELAC 5.4.11)

14.1 OVERVIEW

The laboratory's preventive action programs improve, or eliminate potential causes of nonconforming product and/or nonconformance to the quality system. This preventive action process is a proactive continuous process improvement activity that can be initiated through feedback from clients, employees, business providers, and affiliates. The QA Department has the overall responsibility to ensure that the preventive action process is in place, and that relevant information on actions is submitted for management review.

Dedicating resources to an effective preventive action system emphasizes TestAmerica Irvine's commitment to its Quality Assurance (QA) program. It is beneficial to identify and address negative trends before they develop into complaints, problems and corrective actions. Additionally, customer service and satisfaction can be improved through continuous improvements to laboratory systems.

Opportunities for improvement may be discovered during management reviews, the QA Metrics Report, internal or external audits, proficiency testing performance, client complaints, staff observation, etc..

The monthly Quality Assurance Metrics Report shows performance indicators in all areas of the quality system. These areas include revised reports, corrective actions, audit findings, internal auditing and data authenticity audits, client complaints, PT samples, holding time violations, SOPs, ethics training, etc. These metrics are used to help evaluate quality system performance on an ongoing basis and provide a tool for identifying areas for improvement.

The laboratory's Corrective Action process (Section 13) is integral to implementation of preventive actions. A critical piece of the corrective action process is the implementation of actions to prevent further occurrence of a non-compliance event. Historical review of corrective action provides a valuable mechanism for identifying preventive action opportunities.

14.1.1 The following elements are part of a preventive action system:

- Identification of an opportunity for preventive action.
- Process for the preventive action.
- Define the measurements of the effectiveness of the process once undertaken.
- Execution of the preventive action.
- Evaluation of the plan using the defined measurements.
- Verification of the effectiveness of the preventive action. /=
- Close-Out by documenting any permanent changes to the Quality System as a result of the Preventive Action. Documentation of Preventive Action is incorporated into the monthly QA reports, corrective action process, management review, [and the Management of Change process \(see below\)](#).

Note: There may be varying levels of formality and documentation during the preventive action process due to the simplicity/complexity of the action taken.

14.1.2 Any Preventive Actions undertaken or attempted shall be taken into account during the Annual Management Review (Section 17). A highly detailed recap is not required; a simple recount of success and failure within the preventive action program will provide management a measure for evaluation.

14.2 MANAGEMENT OF CHANGE

The Management of Change process is designed to manage significant events and changes that occur within the laboratory. Through these procedures, the potential risks inherent with a new event or change are identified and evaluated. The risks are minimized or eliminated through pre-planning and the development of preventive measures. The types of changes covered under this system include: Facility Changes, Major Accreditation Changes, Addition or Deletion to Division's Capabilities or Instrumentation, Key Personnel Changes, Laboratory Information Management System (LIMS) changes. This process is discussed in further detail in SOP CA-Q-S-003, Management of Change.

SECTION 15.0

CONTROL OF RECORDS (NELAC 5.4.12)

TestAmerica Irvine maintains a record system appropriate to its needs and that complies with applicable standards or regulations as required. The system produces unequivocal, accurate records that document all laboratory activities. The laboratory retains all original observations, calculations and derived data, calibration records and a copy of the analytical report for a minimum of **five years** after it has been issued.

15.1 OVERVIEW

The laboratory has established procedures for identification, collection, indexing, access, filing, storage, maintenance and disposal of quality and technical records. A record index is listed in Table 15-1. Quality records are maintained by the Quality Assurance (QA) Manager **in a database, which is backed up as part of the regular network backup**. Records are of two types; either electronic or hard copy paper formats depending on whether the record is computer or hand generated (some records may be in both formats). Technical records are maintained by **the individual department managers**.

Table 15-1. Record Index¹

Technical Records	Official Documents	QA Records	Project Records	Administrative Records
Retention Period				
5 Years from analytical report issue*	5 Years from document retirement date*	5 Years from archival* Data Investigation: 7years or the life of the affected raw data storage whichever is greater (beyond 5 years if ongoing project or pending investigation)	5 Years from analytical report issue*	Personnel: 7 Years (HR Records must be maintained as per Policy CW-L-P-001) Finance: See Accounting and Control Procedures Manual
Specific Documents Covered				
Raw Data	Quality Assurance Manual (QAM)	Internal and External Audits/ Responses	Sample receipt and COC Documentation	Finance and Accounting
Logbooks ²	Work Instructions	Certifications	Contracts and Amendments	EH&S Manual, Permits, Disposal Records
Standards	SOPs	Corrective/Preventive Action	Correspondence	Employee Handbook
Certificates	Manuals	Management Reviews	QAPP	Personnel files, Employee Signature & Initials, Administrative Training Records (e.g., Ethics)
Analytical Records		Method & Software Validation, Verification data	SAP	
Lab Reports		Data Investigation	Telephone Logbooks	

	Policies		Lab Reports	Technical Training Records
--	----------	--	-------------	-------------------------------

¹ Record Types encompass hardcopy and electronic records.

² Examples of Logbook types: Maintenance, Instrument Run, Preparation (standard and samples), Standard and Reagent Receipt, Archiving, Balance Calibration, Temperature (hardcopy or electronic records).

* Exceptions listed in Table 15-2.

All records are legible and stored and retained in such a way that they are secure and readily retrievable at the laboratory facility or at Cor-O-Van, an off-site data storage facility. Retention of records are maintained on-site at the laboratory for approximately 1 year after their generation and moved offsite for the remainder of the required storage time. Records are maintained for a minimum of five years unless otherwise specified by a client or regulatory requirement.

For raw data and project records, record retention shall be calculated from the date the project report is issued. For other records, such as Controlled Documents, QA, or Administrative Records, the retention time is calculated from the date the record is formally retired. Records related to the programs listed in Table 15-2 have lengthier retention requirements and are subject to the requirements in Section 15.1.3. Policy CW-L-P-001 (Record Retention) provides additional information on record retention requirements.

15.1.1 Programs with Longer Retention Requirements

Some regulatory programs have longer record retention requirements than the standard record retention time. These are detailed in Table 15-3 with their retention requirements. In these cases, the longer retention requirement is enacted. If special instructions exist such that client data cannot be destroyed prior to notification of the client, the container or box containing that data is marked as to who to contact for authorization prior to destroying the data. For clients with specific retention requirements that exceed the laboratory defaults specified in Table 15-1, a complete data package is assembled and archived for the requisite period.

Table 15-2. Special Record Retention Requirements

Program	¹ Retention Requirement
Drinking Water – All States	10 years (project records)
Drinking Water Lead and Copper Rule	12 years (project records)
TSCA - 40 CFR Part 792	10 years after publication of final test rule or negotiated test agreement

¹Note: Extended retention requirements must be noted with the archive documents or addressed in facility-specific records retention procedures.

15.1.2 All records are held secure and in confidence. Records maintained at the laboratory are located either in the department that originally generated the data or on the data storage shelves adjacent to Sample Receiving. Records archived off-site are stored in a secure location where a record is maintained of any entry into the storage facility. Logs are maintained in each

storage box to note removal and return of records.

15.1.3 The laboratory has procedures to protect and back-up records stored electronically and to prevent unauthorized access to or amendment of these records. All analytical data is maintained as hard copy or in a secure readable electronic format. For analytical reports that are maintained as copies in PDF format, see section 20.12.1 'Computer and Electronic Data Related Requirements' for more information. See [COMPSECU.SOP \(Computer Security\)](#) for details on back-up and security procedures.

15.1.4 The record keeping system allows for historical reconstruction of all laboratory activities that produced the analytical data, as well as rapid recovery of historical data ([Records stored off site should be accessible within 2 days of a request for such records](#)). The history of the sample from when the laboratory took possession of the samples must be readily understood through the documentation. This shall include inter-laboratory transfers of samples and/or extracts.

- The records include the identity of personnel involved in sampling, sample receipt, preparation, or testing. All analytical work contains the initials (at least) of the personnel involved. [The laboratory's copy of the chain of custody is stored with the invoice and the work order sheet generated by the LIMS.](#) The chain of custody would indicate the name of the sampler. [If any sampling notes are provided with a work order, they are kept with this package.](#)
- All information relating to the laboratory facilities equipment, analytical test methods, and related laboratory activities, such as sample receipt, sample preparation, or data verification are documented.
- The record keeping system facilitates the retrieval of all working files and archived records for inspection and verification purposes (e.g., set format for naming electronic files, set format for what is included with a given analytical data set.) Instrument data is stored [sequentially by instrument.](#) [A given day's analyses are maintained in the order of the analysis.](#) Run logs are maintained for each [instrument or method;](#) [a copy of each day's run long or instrument sequence is stored with the data to aid in re-constructing an analytical sequence.](#) Where an analysis is performed without an instrument, [bound logbooks or bench sheets](#) are used to record and file data. Standard and reagent information is recorded in [logbooks or entered into the LIMS for each method as required.](#)
- Changes to hardcopy records shall follow the procedures outlined in Section 13 and 20. Changes to electronic records in LIMS or instrument data are recorded in audit trails.
- The reason for a signature or initials on a document is clearly indicated in the records such as "sampled by," "prepared by," "reviewed by", or "Analyzed by".
- All generated data except those that are generated by automated data collection systems, are recorded directly, promptly and legibly in permanent dark ink.
- Hard copy data may be scanned into PDF format for record storage as long as the scanning process can be verified in order to ensure that no data is lost and the data files and storage media must be tested to verify the laboratory's ability to retrieve the information prior to the

destruction of the hard copy that was scanned. [The procedure for this verification can be found in SOP ARCHIV.SOP.](#)

- Also refer to Section 20.13.1 'Computer and Electronic Data Related Requirements'.

15.2 TECHNICAL AND ANALYTICAL RECORDS

15.2.1 The laboratory retains records of original observations, derived data and sufficient information to establish an audit trail, calibration records, staff records and a copy of each analytical report issued, for a minimum of five years unless otherwise specified by a client or regulatory requirement (refer to Section 15.1). The records for each analysis shall contain sufficient information to enable the analysis to be repeated under conditions as close as possible to the original. The records shall include the identity of laboratory personnel responsible for [the sampling](#), performance of each analysis and checking of results.

15.2.2 Observations, data and calculations are recorded at the time they are made and are identifiable to the specific task.

15.2.3 Changes to hardcopy records shall follow the procedures outlined in Section 13 and 20. Changes to electronic records in LIMS or instrument data are recorded in audit trails. The essential information to be associated with analysis, such as strip charts, tabular printouts, computer data files, analytical notebooks, and run logs, include (previous discussions relate where most of this information is maintained – specifics may be added below):

- laboratory sample ID code;
- Date of analysis and time of analysis is required if the holding time is seventy-two (72) hours or less, or when time critical steps are included in the analysis (e.g., drying times, incubations, etc.); instrumental analyses have the date and time of analysis recorded as part of their general operations. [Where a time critical step exists in an analysis, location for such a time is included as part of the documentation in a specific logbook or on a benchsheet.](#)
- Instrumentation identification and instrument operating conditions/parameters. [Operating conditions/parameters are typically recorded in either the instrument maintenance logs where available or as part of the most recent calibration method file.](#)
- analysis type;
- all manual calculations and manual integrations;
- analyst's or operator's initials/signature;
- sample preparation including [cleanup, separation protocols, incubation periods or subculture, ID codes, volumes, weights, instrument printouts, meter readings, calculations, reagents;](#)
- test results;
- standard and reagent origin, receipt, preparation, and use;
- calibration criteria, frequency and acceptance criteria;
- data and statistical calculations, review, confirmation, interpretation, assessment and reporting conventions;

- quality control protocols and assessment;
- electronic data security, software documentation and verification, software and hardware audits, backups, and records of any changes to automated data entries; and
- Method performance criteria including expected quality control requirements. [These are indicated both in the LIMS and on specific analytical report formats.](#)

15.3 LABORATORY SUPPORT ACTIVITIES

In addition to documenting all the above-mentioned activities, the following are retained QA records and project records (previous discussions in this section relate where and how these data are stored):

- all original raw data, whether hard copy or electronic, for calibrations, samples and quality control measures, including analysts' work sheets and data output records (chromatograms, strip charts, and other instrument response readout records);
- a written description or reference to the specific test method used which includes a description of the specific computational steps used to translate parametric observations into a reportable analytical value;
- copies of final reports;
- archived SOPs;
- correspondence relating to laboratory activities for a specific project;
- all corrective action reports, audits and audit responses;
- proficiency test results and raw data; and
- results of data review, verification, and crosschecking procedures

15.3.1 Sample Handling Records

Sample handling and tracking is discussed in Section 24. Records of all procedures to which a sample is subjected while in the possession of the laboratory are maintained. These include but are not limited to records pertaining to:

- sample preservation including appropriateness of sample container and compliance with holding time requirement;
- sample identification, receipt, acceptance or rejection and login;
- sample storage and tracking including shipping receipts, sample transmittal / COC forms; and
- procedures for the receipt and retention of samples, including all provisions necessary to protect the integrity of samples.

15.4 ADMINISTRATIVE RECORDS

The laboratory also maintains the administrative records in either electronic or hard copy form. See Table 15-1.

15.5 RECORDS MANAGEMENT, STORAGE AND DISPOSAL

15.5.1 All records (including those pertaining to test equipment), certificates and reports are safely stored, held secure and in confidence to the client. Certification related records are available to the accrediting body upon request.

15.5.2 All information necessary for the historical reconstruction of data is maintained by the laboratory. Records that are stored only on electronic media must be supported by the hardware and software necessary for their retrieval.

15.5.3 Records that are stored or generated by computers or personal computers have hard copy, write-protected backup copies, or an electronic audit trail controlling access.

15.5.4 TestAmerica Irvine has a record management system for control of laboratory notebooks, instrument logbooks, standards logbooks, and records for data reduction, validation, storage and reporting. Laboratory notebooks are issued on a per analysis basis, and are numbered sequentially within a given analysis. No analysis has more than one active notebook at a time, so all data are recorded sequentially within a series of sequential notebooks. Bench sheets are filed sequentially. Standards are maintained in the LIMS; some departments may also keep logbooks for standards prepared frequently (e.g. daily).

15.5.5 Records are considered archived when moved off-site. Access to archived hard-copy information is documented with an access log and in/out records is used in archived boxes to note data that is removed and returned. All records shall be protected against fire, theft, loss, environmental deterioration, and vermin. In the case of electronic records, electronic or magnetic sources, storage media are protected from deterioration caused by magnetic fields and/or electronic deterioration. Access to the data is limited to laboratory and company employees.

15.5.6 In the event that the laboratory transfers ownership or goes out of business, TestAmerica Irvine shall ensure that the records are maintained or transferred according to client's instructions. Upon ownership transfer, record retention requirements shall be addressed in the ownership transfer agreement and the responsibility for maintaining archives is clearly established. In addition, in cases of bankruptcy, appropriate regulatory and state legal requirements concerning laboratory records must be followed. In the event of the closure of the laboratory, all records will revert to the control of the corporate headquarters. Should the entire company cease to exist, as much notice as possible will be given to clients and the accrediting bodies who have worked with the laboratory during the previous 5 years of such action.

15.5.7 Records Disposal

15.5.7.1 Records are removed from the archive and disposed after 5 years unless otherwise specified by a client or regulatory requirement. On a project specific or program basis, clients may need to be notified prior to record destruction. Records are destroyed in a manner that ensures their confidentiality such as shredding, mutilation or incineration.

- 15.5.7.2** Electronic copies of records must be destroyed by erasure or physically damaging off-line storage media so no records can be read.
- 15.5.7.3** If a third party records management company is hired to dispose of records, a “Certificate of Destruction” is required. [Refer to Policy No. CW-L-P-001 (Records Retention).]

SECTION 16

AUDITS (NELAC 5.4.13)

16.1 OVERVIEW

Audits measure laboratory performance and insure compliance with accreditation/certification and project requirements. Audits specifically provide management with an on-going assessment of the quality of results produced by the laboratory, including how well the policies and procedures of the QA system and the Ethics and Data Integrity Program are being executed. They are also instrumental in identifying areas where improvement in the QA system will increase the reliability of data. There are two principle types of audits: Internal and External. Internal audits are performed by laboratory or corporate personnel. External audits are conducted by regulators, clients or third-party auditing firms. In either case, the assessment to program requirements is the focus.

Table 16-1. Audit Types and Frequency

Internal Audits	Description	Performed by	Frequency
	Analyst & Method Compliance	QA Department or Designee	- 100% of all methods over a two year period. - 100% of all analysts annually.
	Instrument	QA Department or Designee	100% of all organic instruments and any inorganic chromatography instruments over a two year period
	Work Order/ Final Report	QA Department or Designee	- 1 complete report each month.
	Support Systems	QA Department or Designee	- Annual for entire labs support departments & equipment (e.g., thermometers, balances), can be divided into sub-sections over the course of the year.
	Performance Audits (Double-Blind PTs)	Corporate QA, Laboratory QA Department or Designee	- As needed.
	Special	QA Department or Designee	- As Needed
External Audits	Description	Performed by	Frequency
	Program / Method Compliance	Regulatory Agencies, Clients, accreditation organizations	- As required by program and/or clients needs
	Performance Audits	Provided by a third party.	- As required by a client or regulatory agency. Generally provided semi-annually through the analysis of PT samples.

16.2 INTERNAL AUDITS

Annually, the laboratory prepares a schedule of internal audits to be performed throughout the year. As previously stated, these audits verify and monitor that operations continue to comply with the requirements of the laboratory's QA Manual and the Corporate Ethics Program. A

schedule of the internal audits is maintained by the QA Manager in the *Internal Audit Workbook*. An example can be found in Attachment 1.

It is the responsibility of the QA Manager to plan and organize audits in consideration of the laboratory work load and the department personnel schedules so that all pertinent personnel and operations are thoroughly reviewed. When designees (other than QA department personnel & approved by the QA Manager), perform audits, the QA Manager shall insure that these persons do not audit their own activities except when it can be demonstrated that an effective audit will be carried out. In general, the auditor:

- is neither the person responsible for the process being audited nor the immediate supervisor of the person responsible for the project/process.
- Is free of any conflicts of interest.
- Is free from bias and influences that could affect objectivity.

Laboratory personnel (e.g., supervisors and analysts) may assist with both method and support system audits as long as the items listed in the above paragraph are observed. These audits are conducted according to defined criteria listed in the checklists of the *Internal Audit Workbook*. These personnel must be approved by the QA Manager; and must complete the audit checklists in their entirety. This process introduces analyst experience and insight into the laboratory's auditing program.

The auditor must review the previous audit report and identify all items for verification of corrective actions. A primary focus will be dedicated to the ability of the laboratory to correct root-cause deficiencies and that the corrective action has been implemented and sustained as documented.

16.2.1 Systems

An annual systems audit is required to ensure compliance to analytical methods and SOPs, the laboratory's Data Integrity and Ethics Policies, NELAC quality systems, client and State requirements. This audit is performed in portions throughout the year through method, analyst, instrument, work order/final report and support system audits. Audits are documented and reported to management within 1 week of their performance. Systems audits cover all departments of the facility, both operational and support. The multiple audits are compiled into one systems audit package at the end of the year (*Internal Audit Workbook*).

16.2.1.1 Method, Analyst, Instrument and Work Order/Final Report Audits

Procedures for the method compliance, analyst, instrument and work order/final report audits are incorporated by reference to SOP No. CA-Q-S-004, Method Compliance and Data Authenticity Audits. These audits are not mutually exclusive. For example, the performance of a method audit will also cover multiple analysts and instruments. The laboratory's goal is to annually review all analysts and instruments as described in SOP No. CA-Q-S-004. The laboratory will also audit all methods within a two year time period and audit a minimum of one Work Order/Final Report from receiving through reporting on a monthly basis.

16.2.1.2 Support Systems

Support system audits are performed to ensure that all departments & ancillary equipment are operating according to prescribed criteria. Support system audits include the review of both non-analytical and operational departments. Support equipment audits (e.g., metrology items) include the review of balance calibrations, weight calibrations; water quality testing, etc.. Non-analytical may include sample receiving and bottle preparation. These types of support audits ensure that the operations are being performed to support ethical data as well as ensuring the accuracy & precision of the utilized equipment.

These audits can be performed in portions throughout the year or in one scheduled session. However, the audit schedule must document that these aspects are reviewed annually. Many of the metrology systems are considered to be surveillance activities that can be monitored by QA personnel or delegated to specified department personnel. These surveillance activities are performed on a semi-annual basis unless issues warrant a greater frequency or previous audits continually showing no deficiencies allow the frequency to be reduced to once a year.

An example audit checklist can be found in Attachment 2. Instructions for reporting findings are included in the *Internal Audit Workbook*. In general, findings are reported to management within 1 week of the audit and a response is due from management within 30 days.

16.2.2 Performance Audits

Corporate QA may arrange for double blind PT studies to be performed in the laboratories. Results are given to Management and Corrective actions of any findings are coordinated at each facility by the QA Managers and Laboratory Directors/Managers. These studies are performed on an as needed basis. They may be performed when concerns are raised regarding the performance of a particular method in specific laboratories, periodically to evaluate methods that may not normally be covered in the external PT program or may be used in the process of developing best practices. The local QA Manager may also arrange for PT studies on an as needed basis. (Refer to Section 16.3.2 for additional information on Performance Audits.)

16.2.3 Special Audits

Special audits are conducted on an as needed basis, generally as a follow up to specific issues such as client complaints, corrective actions, PT results, data audits, system audits, validation comments, regulatory audits or suspected ethical improprieties. Special audits are focused on a specific issue, and report format, distribution, and timeframes are designed to address the nature of the issue.

16.3 EXTERNAL AUDITS

TestAmerica facilities are routinely audited by clients and external regulatory authorities. External audits are performed when certifying agencies or clients conduct on-site inspections or submit performance testing samples for analysis. It is TestAmerica's policy to cooperate fully with regulatory authorities and clients. The laboratory makes every effort to provide the auditors with access to personnel, documentation, and assistance. The department managers are responsible for providing corrective actions to the QA Manager who coordinates the response for any deficiencies discovered during an external audit. Audit responses are due in the time allotted by the client or agency performing the audit. This time frame is generally 30 days.

Be aware that NELAC requires that the audit response report be acceptable to the primary accrediting authority after the second submittal. The lab shall have accreditation revoked for all or any portion of its scope of a accreditation for any or all fields of testing, a method, or analyte within a field of testing if it is not corrected.

TestAmerica Irvine cooperates with clients and their representatives to monitor the laboratory's performance in relation to work performed for the client. The client may only view data and systems related directly to the client's work. All efforts are made to keep other client information confidential.

16.3.1 Confidential Business Information (CBI) Considerations

During on-site audits, on-site auditors may come into possession of information claimed as business confidential. A business confidentiality claim is defined as "a claim or allegation that business information is entitled to confidential treatment for reasons of business confidentiality or a request for a determination that such information is entitled to such treatment." When information is claimed as business confidential, the laboratory must place on (or attach to) the information at the time it is submitted to the auditor, a cover sheet, stamped or typed legend or other suitable form of notice, employing language such as "trade secret", "proprietary" or "company confidential". Confidential portions of documents otherwise non-confidential must be clearly identified. CBI may be purged of references to client identity by the responsible laboratory official at the time of removal from the laboratory. However, sample identifiers may not be obscured from the information. Additional information regarding CBI can be found in within the 2003 NELAC standards.

16.3.2 Performance Audits

The laboratory is involved in performance audits conducted **semi-annually** through the analysis of PT samples provided by a third party. The laboratory generally participates in the following types of PT studies: WS (drinking water), WP (waste water/RCRA), and SOIL (RCRA)

- It is TestAmerica's policy that PT samples be treated as typical samples in the production process. Further, where PT samples present special or unique problems in the regular production process they may need to be treated differently, as would any special or unique request submitted by any client. The QA Manager must be consulted and in agreement with any decisions made to treat a PT sample differently due to some special circumstance.
- PTs generally do not have holding times associated with them. In the absence of any holding time requirement, it is recommended that the holding time begin when the PT sample is prepared according to the manufacturers instructions. Holding times should apply to full volume PT samples only if the provider gives a meaningful "sampling date". If this is not provided, it is recommended that the date/time of opening of the full volume sample be considered the beginning of holding time.
- Login will obtain the COC information from the documentation provided with the PTs with review by QA or other designated staff.

- Vials will be prepared as required in the instruction set provided with the samples. After preparation to full volume the sample may be spiked, digested, concentrated, etc., as would be done for any normal sample requiring similar analysis.
- PT samples will not undergo multiple preps, multiple runs, multiple methods (unless being used to evaluate multiple methods), multiple dilutions, UNLESS this is what would be done to a normal client sample (e.g. if a client requests, as PT clients do, that we split VOA coeluters, then dual analysis IS normal practice).
- The type, composition, concentration and frequency of quality control samples analyzed with the PT samples shall be the same as with routine environmental samples.
- Instructions may be included in the laboratory's SOPs for how low level samples are analyzed, including concentration of the sample or adjustment of the normality of titrant. When a PT sample falls below the range of the routine analytical method, the low-level procedure may be used.
- No special reviews shall be performed by operation and QA, UNLESS this is what would be done to a normal client sample. To the degree that special report forms or login procedures are required by the PT supplier, it is reasonable that the laboratory WOULD apply special review procedures, as would be done for any client requesting unusual reporting or login processes.
- Written responses to unacceptable PT results are required. In some cases it may be necessary for blind QC samples to be submitted to the laboratory to show a return to control.

16.4 AUDIT FINDINGS

Internal audit findings are documented using the Internal Audit Workbook. External audit findings are documented using the Audit Database. The laboratory is expected to prepare a response to audit findings within 30 days of receipt of an audit report unless the report specifies a different time frame. The response may include action plans that could not be completed within the 30 day timeframe. In these instances, a completion date must set and agreed to by operations management and the QA Manager.

Responsibility for developing and implementing corrective actions to findings is the responsibility of the Department Manager where the finding originated. Findings that are not corrected by specified due dates are reported monthly to management in the QA monthly report.


If any audit finding casts doubt on the effectiveness of the operations or on the correctness or validity of the laboratory's test results, the laboratory shall take timely corrective action, and shall notify clients in writing if the investigations show that the laboratory results have been affected. Once corrective action is implemented, a follow-up audit is scheduled to ensure that the problem has been corrected.

The procedures must be in accordance to SOP No. CA-L-S-001, Internal Investigations of Data Discrepancies and Determination of Data Recall.

Clients must be notified promptly in writing, of any event such as the identification of defective measuring or test equipment that casts doubt on the validity of results given in any test report or amendment to a test report. The investigation must begin within 24-hours of discovery of the problem and all efforts are made to notify the client within two weeks after the completion of the investigation.

Figure 16-1.

Example - Internal Audit Workbook



THE LEADER IN ENVIRONMENTAL TESTING

Internal Audit Workbook
Summary Page

Laboratory: **TestAmerica IRVINE**
 Last Update: January 31, 2008
 Workbook Instruction No.: CA-Q-WI-011

Item No.	Area Audited	Audit Type	Audit Cycle	Scheduled	Assigned Auditor	Date Audited	Date Reported	Date Closed	Tab No.	Comments
1	Balances	Surveillance	1 month		Dave				1	
13	Temp Logs/ Thermometers-Sample Control	Surveillance	1 month		Thong				2	
25	Maintenance Logs-Volatiles	Surveillance	1 month		Lan				4	
37	Pipets/Dispensers-Metals & Inorg prep	Surveillance	1 month		Rima	1/14/2008	1/14/2008		23	
49	Sample Storage and Disposal	System	1 yr						3	
50	Holding Blanks for Volatiles	System	6 mo						5	
51	Lab Water Quality Testing	System	6 mo						6	
52	Sample Control (Log In)	System	1 yr						7	
53	Shipping Procedures	System	1 yr						8	
54	Computer Operations (LIMS)*	System	1 yr						9	
55	SOP Distribution System	System	1 yr						10	
56	Archiving of Paper Records*	System	1 yr						11	
57	Statistical Process Control	System	1 yr						12	
58	Electronic Archiving*	System	1 yr						13	
59	Data Review System	System	1 yr						14	
60	Final Report Generation	System	1 yr						15	
61	Standards/Reagents	System	6 mo						16	
62	Manual Interpolation	System	1 yr						17	
63	Corrective Action System	System	1 yr						18	
64	Training Records	System	6 mo						19	
65	MIS	System	1 yr						20	
66	SOPs - Prep/Review/Update Process	System	1 yr						21	
67	Purchasing/Procurement	System	1 yr						22	
68	Subcontract Lab Approval	System	1 yr						24	
69	Customer Complaint System	System	1 yr						25	
70	Extractions-ChloralHydrate 8270C2	Method	2 yr		Adriana				26	
75	INORGANIC PREP--150_1	Method	2 yr		Lan				26	
80	GC-BTEX--80T5AIR	Method	2 yr		Thong				26	
85	Extractions--3510_PRR	Method	2 yr		Rima	1/29/2008	1/31/2008		26	

*Checklist Pending

Figure 16-2.

Example – Internal Audit System Checklist: Corrective Actions


 THE LEADER IN ENVIRONMENTAL TESTING (Summary Page)		TestAmerica <Location>					
		INTERNAL AUDIT - Corrective Actions [Printed Name(s) or Date(s)]					
		Area Audited:	<input style="width: 100%;" type="text"/>				
		Auditor:	<input style="width: 100%;" type="text"/>				
		Date:	<input style="width: 100%;" type="text"/>				
		Persons Contacted During Audit:	<input style="width: 100%;" type="text"/>				
		Date Reported to Department Manager:	<input style="width: 100%;" type="text"/>				
		Reported To:	<input style="width: 100%;" type="text"/>				
		Date Reported to Lab Director/Manager:	<input style="width: 100%;" type="text"/>				
		Reported To:	<input style="width: 100%;" type="text"/>				
		Date Response Due:	<input style="width: 100%;" type="text"/>				
		Response Received and Accepted by QA Manager:	<input style="width: 100%;" type="text"/>				
		Associated Corrective Action Report Number(s):	<input style="width: 100%;" type="text"/>				
		Scheduled Follow-up:	<input style="width: 100%;" type="text"/>				
Item	Requirement	Ref.	Y	N	NA	Evidence/Comments	Follow Up
1	Does the laboratory have a corrective action program in place?	5.4.10.1					
2	Does the laboratory have a current corrective action SOP or is this information in the QA Manual?	5.4.10.1					
3	Do all laboratory personnel have documented training and access to initiate corrective actions?	5.4.10.1					
4	Are causes clearly identified by department, staff name, scope of issue (how many reports affected)?	5.4.10.6					
5	Is a root cause for the issue identified?	5.4.10.2					
6	Is a corrective action (plan) clearly described?						
7	Was the corrective action fully implemented?						
8	Is documentation (if applicable) completed as specified by the corrective action (training, revised SOP, etc)						
9	Has a follow-up assessment been conducted to verify the corrective action was successful?						
10	Are corrective actions reviewed on a regular basis by management?	5.4.10.6a 5					
11	Is there a defined distribution flow for corrective action notification, review, closure, and follow-up?	5.4.10.6a					
12	Are non-conformances reviewed on a regular basis and used, if necessary, to initiate root cause corrective actions?						
13	Does the lab have a documented procedure for QC corrective action (i.e., documented within each method / parameter SOP or in the QA Manual)?	4.10.1					
14	Verify Corrective Actions from previous systems audits. List Items:						
15							
16							
17							
Auditor Signature: _____ <p style="text-align: right; margin-right: 50px;"> <u>Primary Reference(s):</u> Corporate SOP CA-Q-S-002, Acceptable Manual Integration Practices NELAC Standard, June 2003 DoD Quality Systems Manual, Version 3, January 2006 EPA Manual for the Certification of Laboratories Analyzing Drinking Water </p>							

Figure 16-3.

Example – External Audit Database—individual finding

Audit Issue Detail

Audit Code: 72 Agency: ESI for BNSF Type: Client Audit Date: 4/19/2006

Audit Issue Lab Comments

Reference Number: 05A-14 Date Initiated: 5/5/2006 Type of Issue: Finding Due Date: 5/30/2006 1735
Issue category:

Issue:
The Audit Team observed a small bottle of methanol near the GC/MS instruments that was being utilized for rinsing pipettes. Any containers of solvent designated for pipette rinsing should be clearly labeled "for rinsing only" and clearly labeled as methanol.

Response:
A training memo will be completed that states: All container for rinsing in the GCMS area will labeled "for rinsing only".
Estimated date of completion: 06/30/06
Response category:

Department: GCMS-Volatiles Status: In Progress Documentation: Training memo pending

Assigned To: Valerie Sierzchula Follow-up Date: 6/30/2006 Date Resolved: SOP to update:

Record: 17 of 33

SECTION 17

MANAGEMENT REVIEWS (NELAC 5.4.14)

17.1 QUALITY ASSURANCE REPORT

A comprehensive QA Report shall be prepared each month by the laboratory's QA Department and forwarded to the Laboratory Director for review and comments. The final report shall be submitted to the [Technical Directors and Operation](#) as well as the appropriate Quality Director and General Manager. All aspects of the QA system are reviewed to evaluate the suitability of policies and procedures. At a minimum, the report content will contain the items listed below. During the course of the year, the Laboratory Director, General Manager or Corporate QA may request that additional information be added to the report.

The TestAmerica QA Report template is comprised of a discussion of three key QA issues facing the laboratory and ten specific sections (Figure 17-1):

- **Metrics:** Describe actions or improvement activities underway to address any outlying quality metrics that have been reported in the monthly Quality System Metrics Table.
- **SOPs:** Report SOPs that have been finalized and report status of any outstanding SOP reviews.
- **Corrective Actions:** Describe highlights and the most frequent cause for report revisions and corrective/preventive action measures underway. Include a discussion of any recalls handled at the lab level as per Section 6.2.2 in the Investigation/Recall SOP (SOP: CA-L-S-001). Include a section for client feedback and complaints. Include both positive and negative feedback. Describe the most serious client complaints and resolutions in progress.
- **MDLs and Control Limits:** Report which MDLs/ MDL verifications are due. Report the same for Control Limits.
- **Audits:** Report Internal and External Audits that were conducted. Include all relevant information such as which methods, by whom, corrective actions needed by when and discuss unresolved audit findings.
- **Performance Testing (PT) Samples:** Report the PT tests that are currently being tested with their due dates, report recent PT results by study, acceptable, total reported and the month and year.
- **Certifications:** Report on any certification programs being worked on by due date, packages completed. Describe any issues, lapses, or potential revocations.
- **Regulatory Updates:** Include information on new state or federal regulations that may impact the laboratory. Report new methods that require new instrumentation, deletion of methods, changes in sampling requirements and frequencies etc...
- **Miscellaneous:** Include any issues that may impact quality within the laboratory. [This section is also used to communicate the status on any Management of Change Request Forms \(CRFs\) that have missed targeted due dates.](#)
- **Next Month:** Report on plans for the upcoming month.

- **Lab Director Comments Section:** This section gives the Laboratory Director the opportunity to comment on issues discussed in the report and to document plans to resolve these issues. Unresolved issues that reappear in subsequent monthly reports must be commented on by the Laboratory Director.
- **Quality Systems Metrics Table:** The report also includes statistical results that are used to assess the effectiveness of the quality system. Effective quality systems are the responsibility of the entire laboratory staff. Each laboratory provides their results in a template provided by Corporate QA (Figure 17-2).

On a monthly basis, Corporate QA compiles information from all the monthly laboratory reports. The VP-QA/EHS prepares a report that includes a compilation of all metrics and notable information and concerns regarding the QA programs within the laboratories. The report also includes a listing of new regulations that may potentially impact the laboratories. This report is presented to the Analytical Division Senior Management Team and General Managers.

17.2 ANNUAL MANAGEMENT REVIEW

The senior lab management team ([Laboratory Director](#), [Technical Directors](#), [QA Manager](#)), conducts an annual review of its quality systems and LIMS to ensure its continuing suitability and effectiveness in meeting client and regulatory requirements and to introduce any necessary changes or improvements. Corporate Operations and Corporate QA personnel may be included in this meeting at the discretion of the Laboratory Director. The LIMS review consists of examining any audits, complaints or concerns that have been raised through the year that are related to the LIMS. The laboratory will summarize any critical findings that can not be solved by the lab and report them to Corporate IT.

This review uses information generated during the preceding year to assess the “big picture” by ensuring that routine quality actions taken and reviewed on a monthly basis are not components of larger systematic concerns. The monthly review (refer to Section 17.1) should keep the quality systems current and effective, therefore, the annual review is a formal senior management process to review specific existing documentation. Significant issues from the following documentation are compiled or summarized by the QA Manager prior to the review meeting:

- Matters arising from the previous annual review.
- Prior Monthly QA Reports issues.
- Laboratory QA Metrics.
- Review of report reissue requests.
- Review of client feedback and complaints.
- Issues arising from any prior management or staff meetings.
- Minutes from prior Senior Management team meetings. Issues that may be raised from these meetings include:
 - Adequacy of staff, equipment and facility resources.
 - Adequacy of policies and procedures.
 - Future plans for resources and testing capability and capacity.

- The annual internal double blind PT program sample performance (if performed),
- [Review of the ACIL seal of excellence program performance.](#)
- Compliance to the Ethics Policy and Data Integrity Plan. Including any evidence/incidents of inappropriate actions or vulnerabilities related to data Integrity.

The annual review includes the previous 12 months. Based on the annual review, a report is generated by the QA Manager and management. The report is distributed to the appropriate General Manager and the Quality Director. The report includes, but is not limited to:

- The date of the review and the names and titles of participants.
- A reference to the existing data quality related documents and topics that were reviewed.
- Quality system or operational changes or improvements that will be made as a result of the review [e.g., an implementation schedule including assigned responsibilities for the changes (Action Table)].

The QA Manual is also reviewed at this time and revised to reflect any significant changes made to the quality systems.

17.3 POTENTIAL INTEGRITY RELATED MANAGERIAL REVIEWS

Potential integrity issues (data or business related) must be handled and reviewed in a confidential manner until such time as a follow-up evaluation, full investigation, or other appropriate actions have been completed and issues clarified. The Corporate Data Investigation/ Recall SOP shall be followed (SOP No. CA-L-S-001). All investigations that result in finding of inappropriate activity are documented and include any disciplinary actions involved, corrective actions taken, and all appropriate notifications of clients.

The Chairman/CEO, President/CEO, COOs and Quality Directors receive a monthly report from the VP of Quality and EHS summarizing any current data integrity or data recall investigations as described in SOP No. CA-L-S-001. The General Manager's are also made aware of progress on these issues for their specific labs.

Figure 17-1.

Example - QA Monthly Report to Management

LABORATORY: x
PERIOD COVERED: Month/Year
PREPARED BY: x DATE: Month Day, Year
DISTRIBUTED TO: xx (Include LD, GM, QA Director, etc...)

THREE KEY ISSUES FOR MONTH:

Include a discussion of three key issues that were focused in on this month.

1. x
 2. x
 3. x
-

1. METRICS

Describe actions or improvement activities underway to address any outlying quality metrics.

2. SOPs

See Tab for SOP specifics.

The following SOPs were finalized (or reviewed for accuracy): (See Tab)

The following SOPs are due to QA: xx

In QA to complete: xx

3. CORRECTIVE ACTION

Highlights: xx

Revised Reports:

Describe the most frequent cause for report revisions and corrective/preventive action measures underway.

Data Investigations/Recalls (Corporate Data Investigation/Recall SOP) :

Include a discussion of any recalls handled at the lab level as Corp SOP.

Client Feedback and Complaints:

Include both positive and negative feedback.

Describe the most serious client complaints) and resolutions in progress.

4. MDLs AND CONTROL LIMITS

MDLs Due:

Control Limits Due:

5. AUDITS

INTERNAL AUDITS

Discuss Any Outstanding Issues (or Attach Summary):

EXTERNAL AUDITS

Discuss Any Outstanding Issues (or Attach Summary):

6. PT SAMPLES

The following PT samples are now in house (Due Dates):

xx

7. CERTIFICATIONS

Certification Packages Being Worked On (Include Due Date):

x

Describe any issues, lapses, or potential revocations.

8. REGULATORY UPDATE

Include information on new state or federal regulations that may impact the laboratory – new methods that require new instrumentation, deletion of methods, changes in sampling requirements or frequencies, ...

9. MISCELLANEOUS

Include any issues that may impact quality within the laboratory.

10. NEXT MONTH

Items planned for next month.

LAB DIRECTOR COMMENTS AND PLANNED CORRECTIVE ACTIONS:

LAB DIRECTOR REVIEW:

DATE:

Figure 17-2.

Example - Laboratory Metrics Categories

Reports for month
Reports revised due to lab error
% Revised Reports
of Data Recall Investigations
of Reports Actually Recalled
Corrective Action Reports
Corrective Action Reports still open
Total Number of Unresolved Open Corrective Action Reports
% of Unresolved Open Corrective Action Reports
Reports independent QA reviewed
% QA Data Review: Reports
Technical staff (Analysts/technicians, including Temps)
of Analyst work product reviewed year-to-date
of Analytical instruments w/electronic data file storage capability
of Analytical instruments reviewed for data authenticity year-to-date
% Analyst/Instrument Data Authenticity Audits
Client Complaints
Client Compliments
of planned internal audits
of planned internal method audits performed year-to-date
% Annual Internal Audits Complete
of Open Internal Audit Findings Past Due
Total Number of External Audit Findings
of Open External Audit Findings Past Due
% External Audit Findings Past Due
of PT analytes participated and received scores
of PT analytes not acceptable
% PT Cumulative Score
PT Repeat Analyte Failures Cumulative (analyte failed more than once in 4 consecutive studies by PT Type) (only applies to failed analytes)
SOPs

SOPs Reviewed/revise within 24 months
Methods or Administrative procedures without approved SOPs
SOP Status
Method certification Losses due to performance/audit issues
Hold Time Violations due to lab error
Date of Last Comprehensive Ethics Training Session
Staff that haven't Received Comprehensive Ethics Training (>30 Days From Employment Date)
MDL Status (Good, Fair, or Poor) >90%, >70%, <70%
Training Documentation Records (Good, Fair, or Poor)
LQM Revision/review Date
QAM Updated to New Integrated Template
Last Annual Internal Audit Date (Opened, Closed)
Last Management QS Review Date
#SOPs required for 12 month review cycle (DOD or drinking water)
#SOPs for 12 month cycle/revise within 12 months (Includes QS and Methods Listed in QSM)
12 month % SOP Status (Includes QS and Methods Listed in QSM)

SECTION 18

PERSONNEL (NELAC 5.5.2)

18.1 OVERVIEW

TestAmerica's management believes that its highly qualified and professional staff is the single most important aspect in assuring a high level of data quality and service. The staff consists of professionals and support personnel as outlined in the organization chart in Appendix 2.

All personnel must demonstrate competence in the areas where they have responsibility. Any staff that is undergoing training shall have appropriate supervision until they have demonstrated their ability to perform their job function on their own. Staff shall be qualified for their tasks based on appropriate education, training, experience and/or demonstrated skills as required.

The laboratory employs sufficient personnel with the necessary education, training, technical knowledge and experience for their assigned responsibilities.

All personnel are responsible for complying with all QA/QC requirements that pertain to the laboratory and their area of responsibility. Each staff member must have a combination of experience and education to adequately demonstrate a specific knowledge of their particular area of responsibility. Technical staff must also have a general knowledge of lab operations, test methods, QA/QC procedures and records management.

Laboratory management is responsible for formulating goals for lab staff with respect to education, training and skills and ensuring that the laboratory has a policy and procedures for identifying training needs and providing training of personnel. The training shall be relevant to the present and anticipated responsibilities of the lab staff.

The laboratory only uses personnel that are employed by or under contract to, the laboratory. Contracted personnel, when used, must meet competency standards of the laboratory and work in accordance to the laboratory's quality system.

18.2 EDUCATION AND EXPERIENCE REQUIREMENTS FOR TECHNICAL PERSONNEL

TestAmerica makes every effort to hire analytical staff that possess a college degree (AA, BA, BS) in an applied science with some chemistry in the curriculum. [Exceptions can be made based upon the individual's experience and ability to learn. There are competent analysts and technicians in the industry who have not earned a college degree.](#) Selection of qualified candidates for laboratory employment begins with documentation of minimum education, training, and experience prerequisites needed to perform the prescribed task. Minimum education and training requirements for TestAmerica employees are outlined in job descriptions and are generally summarized for analytical staff in the table below.

The laboratory maintains job descriptions for all personnel who manage, perform or verify work affecting the quality of the environmental testing the laboratory performs. [Job Descriptions are](#)

located on the TestAmerica intranet site's Human Resources web-page (Also see Section 4 for position descriptions/responsibilities).

Experience and specialized training are occasionally accepted in lieu of a college degree (basic lab skills such as using a balance, colony counting, aseptic or quantitation techniques, etc. are also considered).

As a general rule for analytical staff:

Specialty	Education	Experience
Extractions, Digestions, some electrode methods (pH, DO, Redox, etc.), or Titrimetric and Gravimetric Analyses	H.S. Diploma	On the job training (OJT)
GFAA, CVAA, FLAA, Single component or short list Chromatography (e.g., Fuels, BTEX-GC, IC	A college degree in an applied science or 2 years of college and at least 1 year of college chemistry	Or 2 years prior analytical experience is required
ICP, ICPMS, Long List or complex chromatography (e.g., Pesticides, PCB, Herbicides, HPLC, etc.), GCMS	A college degree in an applied science or 2 years of college chemistry	or 5 years of prior analytical experience
Spectra Interpretation	A college degree in an applied science or 2 years of college chemistry	And 2 years relevant experience Or 5 years of prior analytical experience
Technical Directors/Department Managers – General	Bachelors Degree in an applied science or engineering with 24 semester hours in chemistry An advanced (MS, PhD.) degree may substitute for one year of experience	And 2 years experience in environmental analysis of representative analytes for which they will oversee
Technical Director – Wet Chem only (no advanced instrumentation)	Associates degree in an applied science or engineering or 2 years of college with 16 semester hours in chemistry	And 2 years relevant experience

Specialty	Education	Experience
Technical Director - Microbiology	Bachelors degree in applied science with at least 16 semester hours in general microbiology and biology An advanced (MS, PhD.) degree may substitute for one year of experience	And 2 years of relevant experience

When an analyst does not meet these requirements, they can perform a task under the direct supervision of a qualified analyst, peer reviewer or [Department Manager](#), and are considered an analyst in training. The person supervising an analyst in training is accountable for the quality of the analytical data and must review and approve data and associated corrective actions.

18.3 TRAINING

TestAmerica is committed to furthering the professional and technical development of employees at all levels.

Orientation to the laboratory's policies and procedures, in-house method training, and employee attendance at outside training courses and conferences all contribute toward employee proficiency. [Below are examples of various areas of required employee training:](#)

Required Training	Time Frame*	Employee Type
Environmental Health & Safety	Refer to EH&S Manual	All
Ethics – New Hires	1 week of hire	All
Ethics - Comprehensive	90 days of hire	All
Data Integrity	30 days of hire	Technical and PMs
Quality Assurance	90 days of hire	All
Ethics – Comprehensive Refresher	Annually	All
Initial Demonstration of Capability (DOC)	Prior to unsupervised method performance	Technical

The laboratory maintains records of relevant authorization/competence, education, professional qualifications, training, skills and experience of technical personnel (including contracted personnel) as well as the date that approval/authorization was given. These records are kept on file at the laboratory. Also refer to "Demonstration of Capability" in Section 20.

The training of technical staff is kept up to date by:

- Each employee must have documentation in their training file that they have read, understood and agreed to follow the most recent version of the laboratory QA Manual and SOPs in their area of responsibility. This documentation is updated as SOPs are updated.
- Documentation from any training courses or workshops on specific equipment, analytical techniques or other relevant topics are maintained in their training file.
- Documentation of proficiency (refer to Section 20).
- An Ethics Agreement signed by each staff member (renewed each year) and evidence of annual ethics training.
- A Confidentiality Agreement signed by each staff member signed at the time of employment.
- Human Resources maintains documentation and attestation forms on employment status & records; benefit programs; timekeeping/payroll; and employee conduct (e.g., ethics). This information is maintained in the employee's secured personnel file.

Further details of the laboratory's training program are described in the laboratory's Training and Documentation SOP, IR-QA-TRAIN.

18.4 DATA INTEGRITY AND ETHICS TRAINING PROGRAM

Establishing and maintaining a high ethical standard is an important element of a Quality System. Ethics and data integrity training is integral to the success of TestAmerica and is provided for each employee at TestAmerica. It is a formal part of the initial employee orientation within 1 week of hire, comprehensive training within 90 days, and an annual refresher for all employees. Senior management at each facility performs the ethics training for their staff.

In order to ensure that all personnel understand the importance TestAmerica places on maintaining high ethical standards at all times; TestAmerica has established an Ethics Policy No. CA-L-P-001 and an Ethics Statement/Agreement (Appendix 1). All initial and annual training is documented by signature on the signed Ethics Policy and Code of Ethical Conduct demonstrating that the employee has participated in the training and understands their obligations related to ethical behavior and data integrity.

Violations of this Ethics Policy will not be tolerated. Employees who violate this policy will be subject to disciplinary actions up to and including termination. Criminal violations may also be referred to the Government for prosecution. In addition, such actions could jeopardize TestAmerica's ability to do work on Government contracts, and for that reason, TestAmerica has a Zero Tolerance approach to such violations.

Employees are trained as to the legal and environmental repercussions that result from data misrepresentation. Key topics covered in the presentation include:

- Organizational mission and its relationship to the critical need for honesty and full disclosure in all analytical reporting.
- Ethics Policy (Appendix 1)
- How and when to report ethical/data integrity issues. Confidential reporting.
- Record keeping.
- Discussion regarding data integrity procedures.

- Specific examples of breaches of ethical behavior (e.g. peak shaving, altering data or computer clocks, improper macros, etc., accepting/offering kickbacks, illegal accounting practices, unfair competition/collusion)
- Internal monitoring. Investigations and data recalls.
- Consequences for infractions including potential for immediate termination, debarment, or criminal prosecution.
- Importance of proper written narration / data qualification by the analyst and project manager with respect to those cases where the data may still be usable but are in one sense or another partially deficient.

Additionally, a data integrity hotline (1-800-736-9407) is maintained by TestAmerica and administered by the Corporate Quality Department.

SECTION 19

ACCOMMODATIONS AND ENVIRONMENTAL CONDITIONS (NELAC 5.5.3)

19.1 OVERVIEW

TestAmerica Irvine is a 45,000 ft² secure laboratory facility with controlled access and designed to accommodate an efficient workflow and to provide a safe and comfortable work environment for employees. All visitors sign in and are escorted by laboratory personnel. Access is controlled by various measures.

The laboratory is equipped with structural safety features. Each employee is familiar with the location, use, and capabilities of general and specialized safety features associated with their workplace. The laboratory provides and requires the use of protective equipment including safety glasses, protective clothing, gloves, etc. OSHA and other regulatory agency guidelines regarding required amounts of bench and fume hood space, lighting, ventilation (temperature and humidity controlled), access, and safety equipment are met or exceeded.

Traffic flow through sample preparation and analysis areas is minimized to reduce the likelihood of contamination. Adequate floor space and bench top area is provided to allow unencumbered sample preparation and analysis space. Sufficient space is also provided for storage of reagents and media, glassware, and portable equipment. Ample space is also provided for refrigerated sample storage before analysis and archival storage of samples after analysis. Laboratory HVAC and deionized water systems are designed to minimize potential trace contaminants.

The laboratory is separated into specific areas for [sample receiving](#), [sample preparation](#), [volatile organic sample analysis](#), [non-volatile organic sample analysis](#), [inorganic sample analysis](#), and [administrative functions](#).

19.2 ENVIRONMENT

Laboratory accommodation, test areas, energy sources, lighting are adequate to facilitate proper performance of tests. The facility is equipped with heating, ventilation, and air conditioning (HVAC) systems appropriate to the needs of environmental testing performed at this laboratory.

The environment in which these activities are undertaken does not invalidate the results or adversely affect the required accuracy of any measurements.

The laboratory provides for the effective monitoring, control and recording of environmental conditions that may effect the results of environmental tests as required by the relevant specifications, methods, and procedures. [Such environmental conditions include temperature and barometric pressure](#). [These are monitored in relevant testing areas during the testing period](#).

When any of the method or regulatory required environmental conditions change to a point where they may adversely affect test results, analytical testing will be discontinued until the environmental conditions are returned to the required levels (refer to Section 12).

Environmental conditions of the facility housing the computer network and LIMS are regulated to protect against raw data loss.

19.3 WORK AREAS

There is effective separation between neighboring areas when the activities therein are incompatible with each other. Examples include:

- Volatile organic analysis is performed in a separate room provided with positive air pressure.
- Volatile organic chemical handling areas, including sample preparation and waste disposal, and volatile organic chemical analysis areas.

Access to and use of all areas affecting the quality of analytical testing is defined and controlled by secure access to the laboratory building as described below in the Building Security section.

Adequate measures are taken to ensure good housekeeping in the laboratory and to ensure that any contamination does not adversely affect data quality. These measures include regular cleaning to control dirt and dust within the laboratory.

Work areas are available to ensure an unencumbered work area. Work areas include:

- Access and entryways to the laboratory.
- Sample receipt areas.
- Sample storage areas.
- Chemical and waste storage areas.
- Data handling and storage areas.
- Sample processing areas.
- Sample analysis areas.

19.4 FLOOR PLAN

A floor plan can be found in Appendix 3.

19.5 BUILDING SECURITY

Building electronic keys are distributed to employees as necessary.

Visitors to the laboratory sign in and out in a visitor's logbook. A visitor is defined as any person who visits the laboratory who is not an employee of TestAmerica Irvine. In addition to signing into the laboratory, the Environmental, Health and Safety Manual contains requirements for visitors and vendors. There are specific safety forms that must be reviewed and signed.

Visitors (with the exception of company employees) are escorted by laboratory personnel at all times, or the location of the visitor is noted in the visitor's logbook.

Signs are posted in the laboratory designating employee only areas - "Authorized employees beyond this point".

SECTION 20.0

TEST METHODS AND METHOD VALIDATION (NELAC 5.5.4)

20.1 OVERVIEW

TestAmerica Irvine uses methods that are appropriate to meet our clients' requirements and that are within the scope of the laboratory's capabilities. These include sampling, handling, transport, storage and preparation of samples, and, where appropriate, an estimation of the measurement of uncertainty as well as statistical techniques for analysis of environmental data.

Instructions are available in the laboratory for the operation of equipment as well as for the handling and preparation of samples. All instructions, Standard Operating Procedures (SOPs), reference methods and manuals relevant to the working of the laboratory are readily available to all staff. Deviations from published methods are documented (with justification) in the laboratory's approved SOPs. SOPs are submitted to clients for review at their request. Significant deviations from published methods require client approval and regulatory approval where applicable.

20.2 STANDARD OPERATING PROCEDURES (SOPs)

TestAmerica Irvine maintains SOPs that accurately reflect all phases of the laboratory such as assessing data integrity, corrective actions, handling customer complaints as well as all analytical methods and sampling procedures. The method SOPs are derived from the most recently promulgated/approved, published methods and are specifically adapted to the laboratory facility. Modifications or clarifications to published methods are clearly noted in the SOPs. All SOPs are controlled in the laboratory (refer to Section 6 on Document Control):

- All SOPs contain a revision number, effective date, and appropriate approval signatures. Controlled copies are available to all staff.
- Procedures for preparation, review, revision and control are incorporated by reference to SOPs: **CW-Q-S-002** (Writing a Standard Operating Procedure (SOP) and **SOP IR-QA-DOC** (Document Control and Review)
- SOPs are reviewed at a minimum of every 2 years (annually for Drinking Water and DoD SOPs), and where necessary, revised to ensure continuing suitability and compliance with applicable requirements.

20.3 LABORATORY METHODS MANUAL

For each test method, the laboratory shall have available the published referenced method as well as the laboratory developed SOP. Refer to the corporate SOP CW-Q-S-002 "Writing a Standard Operating Procedure" for content and requirements of technical and non-technical SOPs.

Note: If more stringent standards or requirements are included in a mandated test method or regulation than those specified in this manual, the laboratory shall demonstrate that such requirements are met. If it is not clear which requirements are more stringent, the standard from

the method or regulation is to be followed. Any exceptions or deviations from the referenced methods or regulations are noted in the specific analytical SOP.

20.4 SELECTION OF METHODS

Since numerous methods and analytical techniques are available, continued communication between the client and laboratory is imperative to assure the correct methods are utilized. Once client methodology requirements are established, this and other pertinent information is summarized by the Project Manager. These mechanisms ensure that the proper analytical methods are applied when the samples arrive for log-in. For non-routine analytical services (e.g., special matrices, non-routine compound lists, etc.), the method of choice is selected based on client needs and available technology. The methods selected should be capable of measuring the specific parameter of interest, in the concentration range of interest, and with the required precision and accuracy.

20.4.1 Sources of Methods

Routine analytical services are performed using standard EPA-approved methodology. In some cases, modification of standard approved methods may be necessary to provide accurate analyses of particularly complex matrices. When the use of specific methods for sample analysis is mandated through project or regulatory requirements, only those methods shall be used.

In general, TestAmerica Irvine follows procedures from the referenced methods shown below in 20.3.1.4.

When clients do not specify the method to be used or methods are not required, the methods used will be clearly validated and documented in an SOP and available to clients and/or the end user of the data.

20.4.1.1 The analytical methods used by the laboratory are those currently accepted and approved by the U. S. EPA and the state or territory from which the samples were collected. Reference methods include:

- [Method 1664, Revision A: N-Hexane Extractable Material \(HEM; Oil and Grease\) and Silica Gel Treated N-Hexane Extractable Material \(SGT-HEM\); Non-polar Material\) by Extraction and Gravimetry, EPA-821-R-98-002, February 1999](#)
- [Guidelines Establishing Test Procedures for the Analysis of Pollutants Under the Clean Water Act, and Appendix A-C; 40 CFR Part 136, USEPA Office of Water. Revised as of July 1, 1995. Appendix A to Part 136 - Methods for Organic Chemical Analysis of Municipal and Industrial Wastewater \(EPA 600 Series\)](#)
- [Methods for Chemical Analysis of Water and Wastes, EPA 600 \(4-79-020\), 1983.](#)
- [Methods for the Determination of Inorganic Substances in Environmental Samples, EPA-600/R-93/100, August 1993.](#)
- [Methods for the Determination of Metals in Environmental Samples, EPA/600/4-91/010, June 1991. Supplement I: EPA-600/R-94/111, May 1994.](#)

- [Methods for the Determination of Organic Compounds in Drinking Water, EPA-600/4-88-039, December 1988, Revised, July 1991, Supplement I, EPA-600-4-90-020, July 1990, Supplement II, EPA-600/R-92-129, August 1992. Supplement III EPA/600/R-95/131 - August 1995 \(EPA 500 Series\) \(EPA 500 Series methods\)](#)
- [Technical Notes on Drinking Water Methods, EPA-600/R94-173, October 1994](#)
- [Standard Methods for the Examination of Water and Wastewater, 18th/19th /20th edition; Eaton, A.D. Clesceri, L.S. Greenberg, A.E. Eds; American Water Works Association, Water Pollution Control Federation, American Public Health Association: Washington, D.C.](#)
- [Test Methods for Evaluating Solid Waste Physical/Chemical Methods \(SW846\), Third Edition, September 1986, Final Update I, July 1992, Final Update IIA, August 1993, Final Update II, September 1994; Final Update IIB, January 1995; Final Update III, December 1996.](#)
- [Annual Book of ASTM Standards, American Society for Testing & Materials \(ASTM\), Philadelphia, PA.](#)
- [Manual for the Certification of Laboratories Analyzing Drinking Water \(EPA 815-R-05-004, January 2005\)](#)
- [Code of Federal Regulations \(CFR\) 40, Parts 136, 141, 172, 173, 178, 179 and 261](#)

The laboratory reviews updated versions to all the aforementioned references for adaptation based upon capabilities, instrumentation, etc., and implements them as appropriate. As such, the laboratory strives to perform only the latest versions of each approved method as regulations allow or require.

Other reference procedures for non-routine analyses may include methods established by specific states (e.g., Underground Storage Tank methods), ASTM or equipment manufacturers. Sample type, source, and the governing regulatory agency requiring the analysis will determine the method utilized.

The laboratory shall inform the client when a method proposed by the client may be inappropriate or out of date. After the client has been informed, and they wish to proceed contrary to the laboratory's recommendation, it will be documented.

20.4.2 Demonstration of Capability

Before the laboratory may institute a new method and begin reporting results, the laboratory shall confirm that it can properly operate the method. In general, this demonstration does not test the performance of the method in real world samples, but in an applicable and available clean matrix sample. If the method is for the testing of analytes that are not conducive to spiking, demonstration of capability may be performed on quality control samples.

20.4.2.1 A demonstration of capability is performed whenever there is a change in instrument type, method or personnel.

20.4.2.2 The initial demonstration of capability must be thoroughly documented and approved by the [Technical Director](#) and QA Manager prior to independently analyzing client samples. All associated documentation must be retained in accordance with the laboratories archiving procedures (refer to Section 15, Control of Records).

20.4.2.3 The laboratory must have an approved SOP, demonstrate satisfactory performance, and conduct a method detection limit study (when applicable). There may be other requirements as stated within the published method or regulations (i.e., retention time window study).

Note: In some instances, a situation may arise where a client requests that an unusual analyte be reported using a method where this analyte is not normally reported. If the analyte is being reported for regulatory purposes, the method must meet all procedures outlined within this QA Manual (SOP, MDL, and Demonstration of Capability). If the client states that the information is not for regulatory purposes, the result may be reported as long as the following criteria are met:

- The instrument is calibrated for the analyte to be reported using the criteria for the method and ICV/CCV criteria are met (unless an ICV/CCV is not required by the method).
- The reporting limit is set at or above the first standard of the curve for the analyte.
- The client request is documented and the lab informs the client of its procedure for working with unusual compounds. The final report must be footnoted: *Reporting Limit based on the low standard of the calibration curve.*
- Refer to Section 12 (Control of Non-Conforming Work).

20.4.3 Initial Demonstration of Capability (IDOC) Procedures

The laboratory's SOP IR-QA-TRAIN (Training and Documentation) describes in detail the process by which IDOCs are prepared, performed, evaluated, and documented.

20.4.3.1 The following criteria are to be met for any IDOC:

- The spiking standard used must be prepared independently from those used in instrument calibration.
- The analyte(s) shall be diluted in a volume of clean matrix sufficient to prepare four aliquots at the concentration specified by a method or the laboratory SOP.
- At least four aliquots shall be prepared (including any applicable clean-up procedures) and analyzed according to the test method (either concurrently or over a period of days).
- Using all of the results, calculate the mean recovery in the appropriate reporting units and the standard deviations for each parameter of interest.
- When it is not possible to determine the mean and standard deviations, such as for presence, absence and logarithmic values, the laboratory will assess performance against criteria described in the Method SOP.
- Compare the information obtained above to the corresponding acceptance criteria for precision and accuracy in the test method (if applicable) or in laboratory generated

acceptance criteria (LCS or interim criteria) if there is no mandatory criteria established. If any one of the parameters do not meet the acceptance criteria, the performance is unacceptable for that parameter.

20.4.3.2 When one or more of the tested parameters fail at least one of the acceptance criteria, the analyst must proceed according to either option listed below:

- Locate and correct the source of the problem and repeat the test for all parameters of interest beginning with 20.4.3.3 above.
- Beginning with 20.4.3.3 above, repeat the test for all parameters that failed to meet criteria. Repeated failure, however, will confirm a general problem with the measurement system. If this occurs, locate and correct the source of the problem and repeat the test for all compounds of interest beginning with 20.4.3.1 above.

A certification statement (see Figure 20-1) shall be used to document the completion of each initial demonstration of capability. [A copy of the certification is archived in the analyst's training folder.](#)

20.5 LABORATORY DEVELOPED METHODS AND NON-STANDARD METHODS

Any new method developed by the laboratory must be fully defined in an SOP/Methods Manual (Section 20.2) and validated by qualified personnel with adequate resources to perform the method. Method specifications and the relation to client requirements must be clearly conveyed to the client if the method is a non-standard method (not a published or routinely accepted method). The client must also be in agreement to the use of the non-standard method. The information included in the checklist below (Figure 20-2) is needed before samples are accepted for analysis by a new method.

20.6 VALIDATION OF METHODS

Validation is the confirmation by examination and the provision of objective evidence that the particular requirements for a specific intended use are fulfilled. (From 2003 NELAC Standard)

All non-standard methods, laboratory designed/developed methods, standard methods used outside of their scope, and major modifications to published methods must be validated to confirm they are fit for their intended use. The validation will be as extensive as necessary to meet the needs of the given application. The results are documented with the validation procedure used and contain a statement as to the fitness for use.

20.6.1 Method Validation and Verification Activities for All New Methods

While method validation can take various courses, the following activities can be required as part of method validation. Method validation records are designated QC records and are archived accordingly.

20.6.1.1 Determination of Method Selectivity

Method selectivity is the demonstrated ability to discriminate the analyte(s) of interest from other compounds in the specific matrix or matrices from other analytes or interference. In some cases to achieve the required selectivity for an analyte, a confirmation analysis is required as part of the method.

20.6.1.2 Determination of Method Sensitivity

Sensitivity can be both estimated and demonstrated. Whether a study is required to estimate sensitivity depends on the level of method development required when applying a particular measurement system to a specific set of samples. Where estimations and/or demonstrations of sensitivity are required by regulation or client agreement, such as the procedure in 40 CFR Part 136 Appendix B, under the Clean Water Act, these shall be followed. The laboratory determinations of MDLs are described in Section 20.6.

20.6.1.3 Relationship of Limit of Detection (LOD) to the Quantitation Limit (QL)

An important characteristic of expression of sensitivity is the difference in the LOD and the QL. The LOD is the minimum level at which the presence of an analyte can be reliably concluded. The QL is the minimum level at which both the presence of an analyte and its concentration can be reliably determined. For most instrumental measurement systems, there is a region where semi-quantitative data is generated around the LOD (both above and below the estimated MDL or LOD) and below the QL. In this region, detection of an analyte may be confirmed but quantification of the analyte is unreliable within the accuracy and precision guidelines of the measurement system. When an analyte is detected below the QL, and the presence of the analyte is confirmed by meeting the qualitative identification criteria for the analyte, the analyte can be reliably reported, but the amount of the analyte can only be estimated. If data is to be reported in this region, it must be done so with a qualification that denotes the semi-quantitative nature of the result.

20.6.1.4 Determination of Interferences

A determination that the method is free from interferences in a blank matrix is performed.

20.6.1.5 Determination of Range

Where appropriate, a determination of the applicable range of the method may be performed. In most cases, range is determined and demonstrated by comparison of the response of an analyte in a curve to established or targeted criteria. The curve is used to establish the range of quantitation and the lower and upper values of the curve represent upper and lower quantitation limits. Curves are not limited to linear relationships.

20.6.1.6 Determination of Accuracy and Precision

Accuracy and precision studies are generally performed using replicate analyses, with a resulting percent recovery and measure of reproducibility (standard deviation, relative standard deviation) calculated and measured against a set of target criteria.

20.6.1.7 Documentation of Method

The method is formally documented in an SOP. If the method is a minor modification of a standard laboratory method that is already documented in an SOP, an SOP Attachment describing the specific differences in the new method is acceptable in place of a separate SOP.

20.6.1.8 Continued Demonstration of Method Performance

Continued demonstration of Method Performance is addressed in the SOP. Continued demonstration of method performance is generally accomplished by batch specific QC samples such as LCS, method blanks or PT samples.

20.7 METHOD DETECTION LIMITS (MDL)/ LIMITS OF DETECTION (LOD)

Method detection limits (MDL) are initially determined in accordance with 40 CFR Part 136, Appendix B or alternatively by other technically acceptable practices that have been accepted by regulators. MDL is also sometimes referred to as Limit of Detection (LOD). The MDL theoretically represents the concentration level for each analyte within a method at which the Analyst is 99% confident that the true value is not zero. The MDL is determined for each analyte initially during the method validation process and updated as required in the analytical methods, whenever there is a significant change in the procedure or equipment, or based on project specific requirements (refer to 20.7.10). The analyst prepares at least seven replicates of solution spiked at one to five times the estimated method detection limit (most often at the lowest standard in the calibration curve) into the applicable matrix with all the analytes of interest. Each of these aliquots is extracted (including any applicable clean-up procedures) and analyzed in the same manner as the samples. Where possible, the seven replicates should be analyzed over 2-4 days to provide a more realistic MDL.

20.7.1 MDL's are initially performed for each individual instrument and non-microbiological method analysis. Unless there are requirements to the contrary, the laboratory will use the highest calculated MDL for all instruments used for a given method as the MDL for reporting purposes. This MDL is not required for methods that are not readily spiked (e.g. pH, turbidity, etc.) or where the lab does not report values to the MDL. Titration and gravimetric methods where there is no additional preparation involved, the MDL is based on the lowest discernable unit of measure that can be observed.

20.7.2 MDL's must be run against acceptable instrument QC, including ICV's and Tunes. This is to insure that the instrument is in proper working condition and falsely high or low MDL's are not calculated.

20.7.3 Use only clean matrix which is free of target analytes (e.g.: Laboratory reagent water, Ottawa Sand) unless a project specific MDL is required in a field sample matrix.

20.7.4 The Reporting Limit (also may be referred to as Limit of Quantitation or LOQ) should generally be between 2 and 5 times the MDL. If the MDL is being performed during method development, use this guideline to determine the Reporting Limit for the analysis.

20.7.5 If a sample is diluted, the reported MDL is adjusted according to the dilution factor.

20.7.6 The calculated MDL cannot be greater than the spike amount.

20.7.7 If the most recent calculated MDL does not permit qualitative identification of the analyte then the laboratory may use technical judgment for establishing the MDL (e.g., calculate what level would give a qualitative ID, compare with IDL (20.7), spike at a level where qualitative ID is determined and assign that value as MDL, minimum sensitivity requirements, Standard deviation of method blanks over time, etc.). [These alternate verification procedures are documented in the laboratory's MDL.SOP \(Determination of Method Detection Limits\).](#)

20.7.8 Each of the [replicate](#) spikes must be qualitatively identifiable (e.g., appear in both columns for dual column methods, characteristic ions for GCMS mass spectra, etc). Manual integrations to force the baseline for detection are not allowed.

20.7.9 The initial MDL is calculated as follows:

$$\text{MDL} = t_{(n-1, 1-\alpha = 0.99)} \times (\text{Standard Deviation of replicates})$$

where $t_{(n-1, 1-\alpha = 0.99)} = 3.143$ for [seven replicates](#). ([2.998 for eight](#))

20.7.10 Subsequent to the initial MDL determination, periodic MDL verification, confirmation or determinations may be performed by the procedure in [40 CFR Part 136, Appendix B](#) or alternatively by other technically acceptable practices (e.g., method blanks over time, single standard spikes that have been subjected to applicable sample prep processes, etc.). [The procedures utilized is documented in the laboratory SOP MDL.SOP \(Determination of Method Detection Limits\).](#)

20.7.11 Because of the inherent variability in results outside of the calibration range, TestAmerica does not recommend the reporting of results below the lowest calibration point in a curve; however, it is recognized that some projects and agencies require the reporting of results below the RL. Any result that falls between the MDL and the Reporting limit, when reported, will be qualified as an estimated value.

20.7.12 Detections reported down to the MDL must be qualitatively identified.

20.7.13 MDLs and Reporting limits are adjusted in LIMs based on moisture content and sample aliquot size.

20.8 INSTRUMENT DETECTION LIMITS (IDL)

20.8.1 The IDL is sometimes used to assess the reasonableness of the MDLs or in some cases required by the analytical method or program requirements. IDLs are most used in metals analyses but may be useful in demonstration of instrument performance in other areas.

20.8.2 IDLs are calculated to determine an instrument's sensitivity independent of any preparation method. IDLs are calculated either using 7 replicate spike analyses, like MDL but without sample preparation, or by the analysis of 10 instrument blanks and calculating 3 x the absolute value of the standard deviation.

20.8.3 If IDL is > than the MDL, it may be used as the reported MDL.

20.9 VERIFICATION OF DETECTION AND REPORTING LIMITS

20.9.1 Once an MDL is established, it must be verified, on each instrument, by analyzing a quality control sample (prepared as a sample) at approximately 2-3 times the calculated MDL for single analyte analyses (e.g. most wet chemistry methods, Atomic Absorption, etc.) and 1-4 times the calculated MDL for multiple analyte methods (e.g. GC, GCMS, ICP, etc.). The analytes must be qualitatively identified or see section 20.6.7 for other options. This verification does not apply to methods that are not readily spiked (e.g. pH, turbidity, etc.) or where the lab does not report to the MDL. If the MDL does not verify, then the lab will not report to the MDL, or redevelop their MDL or use the level where qualitative identification is established (See 20.6.7). MDLs must be verified at least annually if an annual MDL study is not performed.

20.9.2 When a Reporting limit is established, it must be initially verified by the analysis of a low level standard or QC sample (LCS at 1-2 the reporting limit) and annually thereafter. Unless there are requirements to the contrary the acceptance criteria is $\pm 50\%$. The annual requirement is waived for methods that have an annually verified MDL.

20.10 RETENTION TIME WINDOWS

Most organic analyses and some inorganic analyses use chromatography techniques for qualitative and quantitative determinations. For every chromatography analysis each analyte will have a specific time of elution from the column to the detector. This is known as the analyte's retention time. The variance in the expected time of elution is defined as the retention time window. As the key to analyte identification in chromatography, retention time windows must be established on every column for every analyte used for that method. [These records are kept with the files associated with an instrument for later quantitation of the analytes.](#)

For GC, HPLC and IC methods, there must be sufficient separation between analyte peaks so as to not misidentify analytes. In the mid-level standard, the distance between the valley and peak height cannot be any less than 25% of the sum of the peak heights of the analytes. This also applies to GCMS in the case where the two compounds share the same quantitation ion.

Note: Some analytes do not separate sufficiently to be able to identify or quantitate them as separate analytes (e.g. m-xylene and p-xylene) and are quantitated and reported as a single analyte (e.g. m,p-xylenes).

Once the analyst has determined that the instrument is in optimum working condition through calibration and calibration verification procedures, he or she uses a mid-range calibration or calibration verification standard to establish the retention times for each of the individual analytes in a method. The analyst makes three injections of the same standard over a 72-hour (24 hr period for 300.0) period, tabulating the retention times for each analyte for each of the three injections. The width of retention time window is normally the average absolute retention time ± 3 Standard Deviations. A peak outside the retention time window will not be identified by the computer as a positive match of the analyte of interest.

It is possible for the statistically calculated RT window to be too tight and need to be adjusted based on analyst experience. In these instances method default retention time windows may be used (e.g., for 8000 series methods a default of 0.03 minutes may be used, and EPA CLP 0.05

minutes is used). The same concept is applied when any peak outside of that window will not be identified by the computer as a positive match.

The calibration verification standard at the beginning of a run may be used to adjust the RT for an analyte. This is essentially re-centering the window but the size of the window remains the same. The RTs are verified when all analytes are within their RT windows and are properly identified.

20.11 EVALUATION OF SELECTIVITY

The laboratory evaluates selectivity by following the checks within the applicable analytical methods, which include [mass spectral tuning](#), [second column confirmation](#), [ICP interelement interference checks](#), [chromatography retention time windows](#), [sample blanks](#) and [specific electrode response factors](#).

20.12 ESTIMATION OF UNCERTAINTY OF MEASUREMENT

20.12.1 Uncertainty is “a parameter associated with the result of a measurement, that characterizes the dispersion of the values that could reasonably be attributed to the measurand” (as defined by the International Vocabulary of Basic and General Terms in Metrology, ISO Geneva, 1993, ISBN 92-67-10175-1). Knowledge of the uncertainty of a measurement provides additional confidence in a result’s validity. Its value accounts for all the factors which could possibly affect the result, such as adequacy of analyte definition, sampling, matrix effects and interferences, climatic conditions, variances in weights, volumes, and standards, analytical procedure, and random variation. Some national accreditation organizations require the use of an “expanded uncertainty”: the range within which the value of the measurand is believed to lie within at least a 95% confidence level with the coverage factor $k=2$.

20.12.2 Uncertainty is not error. Error is a single value, the difference between the true result and the measured result. On environmental samples, the true result is never known. The measurement is the sum of the unknown true value and the unknown error. Unknown error is a combination of systematic error, or bias, and random error. Bias varies predictably, constantly, and independently from the number of measurements. Random error is unpredictable, assumed to be Gaussian in distribution, and reducible by increasing the number of measurements.

20.12.3 The uncertainty associated with results generated by the laboratory can be determined by using the Laboratory Control Sample (LCS) accuracy range for a given analyte. The LCS limits are used to assess the performance of the measurement system since they take into consideration all of the laboratory variables associated with a given test over time (except for variability associated with the sampling). The percent recovery of the LCS is compared either to the method-required LCS accuracy limits or to the statistical, historical, in-house LCS accuracy limits.

20.12.4 To calculate the uncertainty for the specific result reported, multiply the result by the decimal of the lower end of the LCS range percent value for the lower end of the uncertainty range, and multiply the result by the decimal of the upper end of the LCS range percent value for the upper end of the uncertainty range. These calculated values represent a 99%-certain range for the reported result. As an example, suppose that the result reported is 1.0 mg/l, and

the LCS percent recovery range is 50 to 150%. The uncertainty range would be 0.5 to 1.5 mg/l, which could also be written as 1.0 +/- 0.5 mg/l.

20.12.5 In the case where a well recognized test method specifies limits to the values of major sources of uncertainty of measurement (e.g. 524.2, 525, etc) and specifies the form of presentation of calculated results, no further discussion of uncertainty is required.

20.13 CONTROL OF DATA

The laboratory has policies and procedures in place to ensure the authenticity, integrity, and accuracy of the analytical data generated by the laboratory.

20.13.1 Computer and Electronic Data Related Requirements

The three basic objectives of our computer security procedures and policies are shown below. [More detail is outlined in SOP COMPSECU.SOP \(Computer Security\)](#). The laboratory is currently running the [Element](#) which is a 3rd party LIMS system that has been highly customized to meet the needs of [the laboratory](#). It is referred to as LIMS for the remainder of this section. The LIMS utilizes [SQL](#) which is an industry standard relational database platform. It is referred to as Database for the remainder of this section.

20.13.1.1 Maintain the Database Integrity

Assurance that data is reliable and accurate through data verification (review) procedures, password-protecting access, anti-virus protection, data change requirements, as well as an internal LIMS permissions procedure.

- LIMS Database Integrity is achieved through data input validation, internal user controls, and data change requirements.
- Spreadsheets and other software developed in-house must be verified with documentation through hand calculations prior to use.

Note: “Commercial off-the-shelf software in use within the designed application range is considered to be sufficiently validated.” *From NELAC 2003 Standard.* However, laboratory specific configurations or modifications are validated prior to use.

- In order to assure accuracy, all data entered or transferred into the LIMS data system goes through a minimum of two levels of review.
- The QA department performs random data audits to ensure the correct information has been reported.
- Changes to reports are documented [using the non-conformance/corrective action database](#). [Changed report files are named “revision_a”, “revision_b”, etc to clearly differentiate them from the originally reported file.](#)
- Analytical data file security is provided through three policies.
 - The first policy forbids unauthorized personnel from using laboratory data acquisition computers.
 - The second policy is the implementation of network passwords and login names that restrict directory access.

- The third layer is maintained through the LIMS and includes the use of username/password combinations to gain access to the LIMS system, the fact that all data in the LIMS is associated with the user to added/reviewed the data, and the restriction of review authority of data.
- All software installations will be in accordance with any relevant copyright licensing regulations.
- All software installed on any computer within the laboratory must be approved by the Information Technology Department regional support technician assigned to the laboratory Shrink-wrapped or otherwise sealed OEM software that is directly related to instrument usage does not need approval but the Information Technology department must be notified of the installation.
- Anti-virus software shall be installed on all servers and workstations. The anti-virus software shall be configured to check for virus signature file and program updates on a daily basis and these updates will be pushed to all servers and workstations. The anti-virus software will be configured to clean any virus-infected file if possible, otherwise the file will be deleted. Disks and CDs brought from any outside source that are not OEM software must be scanned for viruses before being accessed.
- **Interlab LIMS Permissions Policy**
 - PURPOSE - The purpose of this policy is to provide a mechanism for maintaining the integrity of information contained in each laboratory's LIMS while providing the necessary access for information sharing to staff at other laboratory facilities.
 - DEFINITIONS - Host Laboratory: The laboratory facility that 'owns' the LIMS system or 'hosts' a project/job.
 - POLICIES
 - (a) All permissions for the laboratory's LIMS system must only be granted by a representative of that laboratory.
 - If someone outside of the host lab needs permissions for Project Management or other uses, they must go through the Lab Director or his/her designated representative.
 - Permissions must never be granted without the knowledge of the host laboratory.
 - (b) Only laboratory analytical or QA staff from the home laboratory may have edit permissions for laboratory analysis data.
 - (c) Any changes made in laboratory's LIMS system:
 - Must be documented and traceable.
 - If made by staff of an affiliate lab, written permission from the home lab to make the changes (email approval is sufficient) is required.
 - No corrections may be made in another laboratories system without their knowledge.
 - (d) Data qualifiers in laboratory reports must only be corrected, edited, etc. by the staff at the host laboratory.
 - (e) Full analytical data "View" only permissions may be granted to outside Project Management and Sales staff. Query Search permissions may also be granted so status may be checked.
 - (f) All qualifiers must be approved by QA staff before adding to standard reference (static) tables.
 - (g) **Please contact Corporate QA or IT staff if you have any questions regarding implementation or interpretation of this policy.**

20.13.1.2 Ensure Information Availability: Protection against loss of information or service through scheduled back-ups, secure storage of media, line filter, Uninterruptible Power Supply (UPS), and maintaining older versions of software as revisions are implemented.

- Insured by timely backup procedures on reliable backup media, stable file server network architecture, and UPS protection
- **UPS Protection:**
 - Each fileserver is protected by an appropriate power protection/backup unit. In the event of a power outage, there is approximately 15-30 minutes of up-time for the servers prior to shutdown. This allows for proper shutdown procedures to be followed with the file servers.
- File Server Architecture
 - All files are maintained on multiple Windows 2000 or newer servers which are secured physically in the Information Technology office. Access to these servers is limited to members of the Information Technology staff.
 - All supporting software is maintained for at least 5 years from the last raw data generated using that software. [Length of time is dependent on local regulations or client requirements (e.g., OVAP requires 10 years).]
- System Back-up Overview and Procedures
 - Data from both servers and instrument attached PC's are backed up and purged in compliance with the corporate back-up policy.
 - A Maintenance Plan has been defined to create a daily archive of all data within the LIMS database to a backup location. This backup is initiated automatically by either the database or back-up system.
 - Backup tapes will be stored in compliance with the corporate Data Backup Policy. Backup verifications are carried out in accordance with the corporate Data Backup Policy.
 - Instrument data back-ups are verified on a periodic basis by the QA department when performing electronic data audits. The audit takes place on data that has been moved to a back-up location ensuring that it has been moved.

20.13.1.3 Maintain Confidentiality: Ensure data confidentiality through physical access controls, and encryption of when electronically transmitting data.

- All servers are located in a secure area of the IT department offices. Access to the servers is limited to IT staff (Desktop Support, Director of LIMS support, Database administrator) and Lab Director.
- The company website contains SSL (Secure Socket Layer) encryption for secure website sessions and data transfers.
- The reporting portion of the LIMS system requires a project manager to enter their unique password anytime they create a report that displays a signature on it (.PDF).
- Electronic documents such as PDF files and electronic data deliverables will be made available to clients via the secure web site. The logon page for this web site contains an agreement that the customer must accept before they will be logged on which states that the customer agrees not to alter any electronic data made available to them.

- If electronic documents are made available outside of the web site, the customer must sign an agreement in advance that states they will not alter the data in any way.

20.13.2 Data Reduction

The complexity of the data reduction depends on the analytical method and the number of discrete operations involved (e.g., extractions, dilutions, instrument readings and concentrations). The analyst calculates the final results from the raw data or uses appropriate computer programs to assist in the calculation of final reportable values.

For manual data entry, e.g., Wet Chemistry, the data is reduced by the analyst and then verified by the Department Manager or alternate analyst prior to entering the data in LIMS. The spreadsheets, or any other type of applicable documents, are signed by both the analyst and reviewer to confirm the accuracy of the manual entry(s).

Manual integration of peaks will be documented and reviewed and the raw data will be flagged in accordance with the TestAmerica Corporate SOP CA-Q-S-002, *Acceptable Manual Integration Practices*.

Analytical results are reduced to appropriate concentration units specified by the analytical method, taking into account factors such as dilution, sample weight or volume, etc. Blank correction will be applied only when required by the method or per manufacturer's indication; otherwise, it should not be performed. Calculations are independently verified by appropriate laboratory staff. Calculations and data reduction steps for various methods are summarized in the respective analytical SOPs or program requirements.

20.13.2.1 All raw data must be retained in the daily run sequence folder, computer file (if appropriate), and/or logbook. All criteria pertinent to the method must be recorded. The documentation is recorded at the time observations or calculations are made and must be signed or initialed/dated (month/day/year). It must be easily identifiable who performed which tasks if multiple people were involved.

20.13.2.2 In general, concentration results are reported in milligrams per liter (mg/l) or micrograms per liter ($\mu\text{g/l}$) for liquids and milligrams per kilogram (mg/kg) or micrograms per kilogram ($\mu\text{g/kg}$) for solids. The units "mg/l" and "mg/kg" are the same as "parts per million (ppm)". The units " $\mu\text{g/l}$ " and " $\mu\text{g/kg}$ " are the same as "parts per billion (ppb)." For values greater than 10,000 mg/l, results can be reported in percent, i.e., 10,000 mg/l = 1%.

- Several environmental methods, such as color, turbidity, conductivity, use very specific, non-concentration units to report results (e.g., NTU, umhos/cm etc).
- Occasionally, the client requests that results be reported in units which take into account the measured flow of water or air during the collection of the sample. When they provide this information, the calculations can be performed and reported.

20.13.2.3 In reporting, the analyst or the instrument output records the raw data result using values of known certainty plus one uncertain digit. If final calculations are performed external to LIMS, the results should be entered in LIMS with at least three significant

figures. In general, client sample results are reported to 2 significant figures and QC samples are reported to 3 significant figures on the final report.

20.13.2.4 For those methods that do not have an instrument printout or an instrumental output compatible with the LIMS System, the raw results and dilution factors are entered directly into LIMS by the analyst, and the software calculates the final result for the analytical report. LIMS has a defined significant figure criterion for each analyte.

20.13.2.5 The laboratory strives to import data directly from instruments or calculation spreadsheets to ensure that the reported data are free from transcription and calculation errors. For those analyses with an instrumental output compatible with the LIMS, the raw results and dilution factors are transferred into LIMS electronically after reviewing the quantitation report, and removing unrequested or poor spectrally-matched compounds. The analyst prints a copy of what has been entered to check for errors. This printout and the instrument's printout of calibrations, concentrations, retention times, chromatograms, and mass spectra, if applicable, are retained with the data file. The data file is stored in a monthly folder on the instrument computer; periodically, this file is transferred to the server and, eventually, to a tape file.

20.13.3 Logbook / Worksheet Use Guidelines

Logbooks and worksheets are filled out 'real time' and have enough information on them to trace the events of the applicable analysis/task. (e.g. calibrations, standards, analyst, sample ID, date, time on short holding time tests, temperatures when applicable, calculations are traceable, etc.)

- Corrections are made following the procedures outlined in Section 13.
- Logbooks are controlled by [the QA department](#). A record is maintained of all logbooks in the lab.
- Unused portions of pages must be "Z"ed out, signed and dated.
- Worksheets are created with the approval of the [Technical Director and QA Manager](#) at the facility. The [QA Manager](#) controls all worksheets following the procedures in Section 6.

20.13.4 Review / Verification Procedures

Review procedures are outlined in several SOPs (LOGIN.SOP [Sample Control], DATAREV.SOP [General Data Review], PMDATA.SOP [Project Management Data Reporting, Validation and Distribution]) to ensure that reported data are free from calculation and transcription errors, that QC parameters have been reviewed and evaluated before data is reported. The laboratory also has an SOP discussing Manual Integrations to ensure the authenticity of the data. (**CA-Q-S-002**, Acceptable Manual Integration Practices) The general review concepts are discussed below, more specific information can be found in the SOPs.

20.13.4.1 The data review process at TestAmerica Irvine starts at the Sample Control level. Sample Control personnel review chain-of-custody forms and input the sample information and required analyses into a computer LIMS. The Sample Control Supervisor reviews the transaction of the chain-of-custody forms and the inputted

information. The Project Managers perform final review of the chain-of-custody forms and inputted information.

20.13.4.2 The next level of data review occurs with the Analysts. As results are generated, analysts review their work to ensure that the results generated meet QC requirements and relevant EPA methodologies. The Analysts transfer the data into the LIMS and add data qualifiers if applicable (see Appendix 7 for list of common data qualifiers). To ensure data compliance, a different analyst performs a second level of review. Second level review is accomplished by checking reported results against raw data and evaluating the results for accuracy. During the second level review, blank runs, QA/QC check results, continuing calibration results, laboratory control samples, sample data, qualifiers and spike information are evaluated. Approximately 15% of all sample data from manual methods and from automated methods, all GC/MS spectra and all manual integrations are reviewed. Manual integrations are also electronically reviewed utilizing auditing software to help ensure compliance to ethics and manual integration policies. Issues that deem further review include the following:

- QC data are outside the specified control limits for accuracy and precision
- Reviewed sample data does not match with reported results
- Unusual detection limit changes are observed
- Samples having unusually high results
- Samples exceeding a known regulatory limit
- Raw data indicating some type of contamination or poor technique
- Inconsistent peak integration
- Transcription errors
- Results outside of calibration range

20.13.4.3 Unacceptable analytical results may require reanalysis of the samples. Any problems are brought to the attention of the Laboratory Director, Project Manager, Quality Assurance Manager, Department Manager for further investigation. Corrective action is initiated whenever necessary.

20.13.4.4 The results are then entered or directly transferred into the computer database and a hard copy (or .pdf) is printed for the client.

20.13.4.5 As a final review prior to the release of the report, the Project Manager reviews the results for appropriateness and completeness. This review and approval ensures that client requirements have been met and that the final report has been properly completed. The process includes, but is not limited to, verifying that chemical relationships are evaluated, COC is followed, cover letters/ narratives are present, flags are appropriate, and project specific requirements are met. The following are some examples of chemical relationships that are reviewed (if data is available):

- Total Results are \geq Dissolved results (e.g. metals)

- Total Solids (TS) \geq TDS or TSS
- TKN \geq Ammonia
- Total Phosphorus \geq Orthophosphate
- COD \geq TOC
- Total cyanide \geq Amenable Cyanide
- TDS \geq individual anions

20.13.4.6 Any project that requires a data package is subject to a tertiary data review for transcription errors and acceptable quality control requirements. The Project Manager then signs the final report. (*Also see section 26 on Reporting Results*). The accounting personnel also check the report for any clerical or invoicing errors. When complete, the report is sent out to the client.

20.13.4.7 A visual summary of the flow of samples and information through the laboratory, as well as data review and validation, is presented in Figure 20-3.

20.13.5 Manual Integrations

Computerized data systems provide the analyst with the ability to re-integrate raw instrument data in order to optimize the interpretation of the data. Though manual integration of data is an invaluable tool for resolving variations in instrument performance and some sample matrix problems, when used improperly, this technique would make unacceptable data appear to meet quality control acceptance limits. Improper re-integrations lead to legally indefensible data, a poor reputation, or possible laboratory decertification. Because guidelines for re-integration of data are not provided in the methods and most methods were written prior to widespread implementation of computerized data systems, the laboratory trains all analytical staff on proper manual integration techniques using SOP CA-Q-S-002 as the guidelines.

- 20.13.5.1** The analyst must adjust baseline or the area of a peak in some situations, for example when two compounds are not adequately resolved or when a peak shoulder needs to be separated from the peak of interest. The analyst must use professional judgment and common sense to determine when manual integrating is required. Analysts are encouraged to ask for assistance from a senior analyst or manager when in doubt.
- 20.13.5.2** Analysts shall not increase or decrease peak areas to for the sole purpose of achieving acceptable QC recoveries that would have otherwise been unacceptable. The intentional recording or reporting of incorrect information (or the intentional omission of correct information) is against company principals and policy and is grounds for immediate termination.
- 20.13.5.3** Client samples, performance evaluation samples, and quality control samples are all treated equally when determining whether or not a peak area or baseline should be manually adjusted.
- 20.13.5.4** All manual integrations receive a second level review. Manual integrations must be indicated on an expanded scale “after” chromatograms such that the integration performed can be easily evaluated during data review. Expanded scale “before” chromatograms are also required for all manual integrations on QC parameters (calibrations, calibration verifications, laboratory control samples, internal standards, surrogates, etc.) unless the laboratory has another documented corporate approved procedure in place that can demonstrate an active process for detection and deterrence of improper integration practices.

**Table 20-1
Laboratory Method SOPs by Department and Method Reference**

DEPARTMENT	Method	TITLE	FILENAME
Administrative	Computer Security	COMPUTER SECURITY	COMPSECU.SOP
Administrative	Power Outage	POWER OUTAGES	POWEROUT.SOP
Administrative	Software	SOFTWARE MAINTENANCE	SOFTWARE.SOP
Extractions	CADHS LUFT Diesel	DIESEL EXTRACTION FOR SOIL, CA LUFT METHOD	DHSDIESEL.SOP
Extractions	EPA 3510C/EPA 625	EPA METHOD 3510C (BNA EXTRACTION BY SEPARATORY FUNNEL)	3510C_BNA.SOP
Extractions	EPA 3510C Diesel	EPA METHOD 3510C (DIESEL EXTRACTION FOR WATER)	3510_D.SOP
Extractions	EPA 3510C Pest/PCB	EPA METHOD 3510C (ORGANOCHLORINE PESTICIDES AND PCBs EXTRACTION FOR WATER)	3510_PR9.SOP
Extractions	EPA 3520C/EPA 625	EPA METHOD 3520C AND EPA METHOD 625 (CONTINUOUS LIQUID-LIQUID EXTRACTION)	3520C.SOP
Extractions	EPA 3545 Pest/PCB	EPA METHOD 3545 (PRESSURIZED FLUID EXTRACTION [PFE], PESTICIDE AND PCB EXTRACTION FOR SOIL)	3545_P.SOP
Extractions	EPA 3545 Semi-volatiles	EPA METHOD 3545 (PRESSURIZED FLUID EXTRACTION [PFE],SEMI-VOLATILE EXTRACTION FOR SOIL	3545_SV.SOP
Extractions	Na2SO4	PREPARATION OF SODIUM SULFATE FOR EXTRACTIONS	NA2SO4.SOP
GC-BTEX	EPA 8015/8020/CARB 410A	EPA METHOD 8015/8020, MODIFIED FOR AIR AND CARB METHOD 410A (BTEX, MTBE AND FUEL HYDROCARBONS AS GASOLINE)	8015AIR.SOP
GC-BTEX	EPA 8015B/8021B	GASOLINE RANGE ORGANICS (GRO) / BTEX AND MTBE	8015G.SOP
GC-BTEX	Mineral Spirits	GRO/BTEX/MTBE BY GC, ADDENDUM FOR DETERMINATION OF MINERAL SPIRITS (C8-C14) (EPA METHOD 8015B MOD.)	8015minsprt.SOP
GC-SEMI	EPA 8015B Diesel	EPA METHOD 8015B AND MODIFIED FOR DHS LUFT (TOTAL PETROLOLEUM HYDROCARBONS AS DIESEL)	8015D.SOP
GC-SEMI	EPA 8082/608	EPA METHOD 8082/608 (POLYCHLORINATED BIPHENYLS (PCBS) BY GC)	PCBs.SOP
GC-SEMI	EPA 8081A/608	ORGANOCHLORINE PESTICIDES BY GC (EPA METHODS 608 & 8081A)	PESTICIDES.SOP
GC-SEMI	EPA 8081A/608	ORGANOCHLORINE PESTICIDES BY GC (EPA METHODS 608 & 8081A) - Change Form ID - CF1	PESTICIDES.SOP-CF1
GCMS-SEMI	EPA 8270C MOD	1,4-DIOXANE BY 8270C MODIFIED SCAN MODE	14DIOX_8270C.SOP
GCMS-SEMI	8270C MOD	ADDENDUM FOR THE DETERMINATION OF DDT, DDD, DDE AND CHLOROBENZENE IN WATER AND METHYLENE CHLORIDE SOIL EXTRACTS	8270_DDT.SOP
GCMS-SEMI	Chloroacetaldehydes by GCMS	CHLORAL HYDRATE BY EPA 8270C SELECTIVE ION MONITORING (SIM) MODE	ChloralHydrate_8270Cr2.SOP
GCMS-SEMI	EPA 8270C/625	EPA METHOD 8270C (SEMI-VOLATILE ORGANIC COMPOUNDS)/EPA METHOD 625 (BASE/NEUTRALS AND ACIDS)	GCMS-SVOA.SOP
GCMS-SEMI	EPA 1625C MOD	NITROSAMINES BY GC/MS USING CHEMICAL IONIZATION (EPA 1625C MODIFIED)	IR-MSS-NITROSA
GCMS-VOL	EPA 8260B SIM	1,2,3-TRICHLOROPROPANE BY GAS CHROMATOGRAPHY/MASS SPECTROMETRY (GC/MS) SIM (SRL 524M-TCP, EPA 8260B SIM)	123TCP_R1.SOP
GCMS-VOL	EPA 8260B	EPA METHOD 8260B/624 (VOLATILE ORGANIC COMPOUNDS)	GCMS_VOA.SOP
GCMS-VOL	TPH by GCMS	TPH BY GCMS	GCMSTPH.SOP
GCMS-VOL	EPA 8260B MOD	VOLATILE ORGANIC COMPOUNDS BY GAS CHROMATOGRAPHY/MASS SPECTROMETRY (GC/MS) ADDENDUM FOR DETERMINATION OF 1,4-DIOXANE BY EPA 8260B MODIFIED	14DIOX.SOP
GCMS-VOL	EPA 5030B & 5035A	VOLATILE ORGANIC PREPARATION (EPA 5030B & 5035A)	IR-MSV-PREP
Health & Safety	Glass crusher	Glass Crusher	GLASSCR.SOP

DEPARTMENT	Method	TITLE	FILENAME
Health & Safety	Plastic shredder	PLASTIC SHREDDER	PLASTSH.SOP
Health & Safety	Safety Manual	SAFETY MANUAL & CHEMICAL HYGIENE PLAN	SMCHP.DOC
INORGANIC PREP	EPA 3050B	ACID DIGESTION FOR TOTAL METALS BY GFAA AND ICP IN SOIL (EPA METHOD 3050B)	3050B.SOP
INORGANIC PREP	EPA 3020A	ACID DIGESTION OF AQUEOUS SAMPLES AND EXTRACTS FOR TOTAL METALS BY GFAA (EPA METHOD 3020A)	3020A.SOP
INORGANIC PREP	EPA 3010A	ACID DIGESTION OF AQUEOUS SAMPLES AND EXTRACTS FOR TOTAL METALS BY ICP (EPA METHOD 3010A)	3010A.SOP
INORGANIC PREP	EPA 200.2/3005A	Acid Digestion of Water for Total Recoverable or Dissolved Metals by ICP and ICPMS	METPREP-W.SOP
INORGANIC PREP	EPA 1010	EPA METHOD 1010 (PENSKY-MARTENS CLOSED-CUP METHOD FOR DETERMINING IGNITABILITY)	1010.SOP
INORGANIC PREP	EPA 150.1/9040/9045/SM 4500H,B	EPA METHOD 150.1/ 9040B/ 9045C (ELECTROMETRIC pH)	150_1.SOP
INORGANIC PREP	SM 2120B	EPA METHOD 2120B (COLOR, COLORIMETRIC- PLATINUM-COBALT)	2120B.SOP
INORGANIC PREP	EPA 413.1	EPA METHOD 413.1 (TOTAL RECOVERABLE OIL AND GREASE FOR WATER)	413_1.SOP
INORGANIC PREP	EPA 413.2	EPA METHOD 413.2 (TOTAL RECOVERABLE OIL AND GREASE FOR WATER)	413_2.SOP
INORGANIC PREP	EPA 418.1	EPA METHOD 418.1 (TOTAL RECOVERABLE PETROLEUM HYDROCARBONS)	418_1.SOP
INORGANIC PREP	SM 3500Fe-D	FERROUS IRON BY SM 3500Fe-D	3500Fe_D.SOP
INORGANIC PREP	Glass Washing	GLASSWARE CLEANING	GLASS_E.SOP
INORGANIC PREP	EPA 1664A	GRAVIMETRIC DETERMINATION OF N-HEXANE EXTRACTABLE MATERIAL AND SILICA GEL TREATED N-HEXANE EXTRACTABLE MATERIAL IN WATER	1664A.SOP
INORGANIC PREP	Ignitability	IGNITABILITY IN SOIL	IGNITE.SOP
INORGANIC PREP	EPA 160.5	SETTLABLE MATTER (EPA METHOD 160.5 / SM2540F)	IR-WET-SETT
INORGANIC PREP	SM 2710F	SPECIFIC GRAVITY BY MASS RATIO (SM2710F)	2710F.SOP
INORGANIC PREP	SM 2580B	STANDARD METHOD 2580B (OXIDATION REDUCTION POTENTIAL)	ORP.SOP
INORGANIC PREP	STLC TITLE 22, SECTION 66261.126, APPENDIX II)	STLC/WET EXTRACTION (TITLE 22, SECTION 66261.126, APPENDIX II)	STLC.SOP
INORGANIC PREP	EPA 1311/1312	TCLP & SPLP (EPA METHOD 1311 & 1312)	1311_1312.SOP
INORGANIC PREP	SM 2150B & EPA 140.1	THRESHOLD ODOR (SM 2150B & EPA 140.1)	IR-WET-ODOR
INORGANIC PREP	EPA 180.1	TURBIDITY, NEPHELOMETRIC (EPA METHOD 180.1 AND STANDARD METHOD 2130B)	180_1.SOP
METALS	EPA 200.9	DETERMINATION OF TRACE ELEMENTS BY STABILIZED TEMPERATURE GRAPHITE FURNACE AA (EPA METHOD 200.9 & STANDARD METHOD 3113)	200_9.SOP
METALS	EPA 9081A	EPA METHOD 9081A CATION-EXCHANGE CAPACITY OF SOILS (SODIUM ACETATE)	9081A.SOP
METALS	EPA 6010B/EPA 200.7	ICP METALS ANALYSES (EPA METHOD 6010B, EPA METHOD 200.7)	ICP.SOP
METALS	EPA 245.1/7470A/7471A	MERCURY, COLD-VAPOR ATOMIC ABSORPTION SPECTROMETRY (EPA METHODS 245.1/7470A/7471)	MERCURY.SOP
METALS	EPA 200.8	METALS BY ICP/MS (EPA METHOD 200.8)	200_8.SOP
METALS	EPA 6020	METALS BY ICP/MS (EPA METHOD 6020)	6020.SOP
METALS	CA DTSC 939-M	ORGANIC LEAD BY GRAPHITE FURNACE AA (CA DTSC 939-M)	ORG_PB_GFAA.SOP
PM	Data packages	DATA PACKAGE GENERATION	DATAPACK
PM	EDFs	EDF (ELECTRONIC DATA FORMAT)	EDF.SOP
PM	Client/Project set-up	PROJECT MANAGEMENT--CLIENT/PROJECT SET-UP	PMCLIENT.SOP
PM	Client communication	PROJECT MANAGEMENT--COMMUNICATION AND DOCUMENTATION	PMDOC.SOP

DEPARTMENT	Method	TITLE	FILENAME
PM	Data reporting	PROJECT MANAGEMENT--DATA REPORTING, VALIDATION AND DISTRIBUTION	PMDATA.SOP
PM	WIP packages	WELL INVESTIGATION PROGRAM (WIP) Package Generation	WIP.SOP
QA	Balances	BALANCE CALIBRATION VERIFICATION AND DOCUMENTATION	BAL.SOP
QA	BP GCLN	BP GCLN Technical Requirements	BPREQS.SOP
QA	Lot testing	CONTAINER AND REAGENT VERIFICATION BY LOT TESTING	LOTTEST.SOP
QA	Control Limits	CONTROL CHARTS AND STATISTICAL PROCESS CONTROL	CNTRLLIM.SOP
QA	Corrective Actions	CORRECTIVE ACTIONS	CAR.SOP
QA	Data Integrity	DATA INTEGRITY AND BUSINESS ETHICS PLAN	DIBEP.SOP
QA	Ethics Policy	DATA INTEGRITY AND ETHICAL PRACTICES POLICY AND PROCEDURE	DMA_ETHICS.SOP
QA	MDLs	DETERMINATION OF METHOD DETECTION LIMITS	MDL.SOP
QA	Documents	DOCUMENT CONTROL	DOCCNTRL.SOP
QA	ET Edwards	EARTH TECH/EDWARDS AFB PROJECT REQUIREMENTS	IR-QA-ETEDW.SOP
QA	Data Review	GENERAL DATA REVIEW	DATAREV.SOP
QA	ICOC	LEGAL CUSTODY PROCEDURES	LEGALCOC.SOP
QA	Logbooks	LOGBOOK DOCUMENTATION	LOGBOOK.SOP
QA	Manual Integration	MANUAL INTEGRATION AND DATA INTEGRITY	MANINT.SOP
QA	Pipets	PIPET CALIBRATION	PIP.SOP
QA	QA Manual	QUALITY ASSURANCE MANUAL	QAM
QA	QA Department	QUALITY ASSURANCE DEPARTMENT	QADR5.SOP
QA	Reagents and Standards	REAGENT AND STANDARD CONTROL AND DOCUMENTATION	STDCTRL.SOP
QA	Archiving	RECORD ARCHIVING	ARCHIV.SOP
QA	Storage Blanks	REFRIGERATOR STORAGE BLANKS	REFBLK.SOP
QA	Sig Figs	SIGNIFICANT FIGURES	SIGFIGS.SOP
QA	Subsampling	SUBSAMPLING	SUBSAMP.SOP
QA	Thermometers	THERMOMETER CALIBRATION, TEMPERATURE MONITORING, AND DOCUMENTATION	THERMA.SOP
QA	Training	TRAINING AND DOCUMENTATION	TRAINING.SOP
QA	Qualifiers	USE OF DATA QUALIFIERS	DATAQUAL.SOP
Sample Control	Bottle Prep	BOTTLE PRESERVATION	BTLPRP.SOP
Sample Control	Courier	COURIER	COURIER.SOP
Sample Control	Field Sampling	FIELD SAMPLING	FIELD.SOP
Sample Control	Manual Entry	MANUAL ENTRY OF SAMPLES FOR SAMPLE CONTROL	MANULOG.SOP
Sample Control	Sample Control	SAMPLE CONTROL	LOGIN.SOP
WETCHEM	EPA 305.1	ACIDITY, TITRIMETRIC (EPA METHOD 305.1)	305_1.SOP
WETCHEM	EPA 3060A	ALKALINE DIGESTION PROCEDURE FOR HEXAVALENT CHROMIUM IN SOILS	3060A.SOP
WETCHEM	EPA 310.1/SM 2320B	ALKALINITY BY SM2320B, EPA METHOD 310.1	2320B.SOP
WETCHEM	EPA 350.3/SM 4500 NH3	AMMONIA POTENTIOMETRIC, ION SELECTIVE ELECTRODE	350_3r6.SOP
WETCHEM	EPA 405.1/SM 5210B	BIOCHEMICAL OXYGEN DEMAND / CARBONACEOUS BIOLOGICAL OXYGEN DEMAND (EPA METHOD 405.1/SM 5210B)	405_1.SOP
WETCHEM	EPA 7199/218.6	Determination of Hexavalent Chromium by Ion Chromatography--EPA Methods 7199 and 218.6	Cr6IC.SOP
WETCHEM	EPA 314.0	Determination of Perchlorate by Ion Chromatography--EPA 314.0	314_0.SOP

DEPARTMENT	Method	TITLE	FILENAME
WETCHEM	EPA 314.0 Modified	EPA 314.0 MOD. (DETERMINATION OF 4-CHLOROBENZENESULFONIC ACID (PCBSA) BY ION CHROMATOGRAPHY)	PCBSA.SOP
WETCHEM	EPA 160.2/SM 2540D	EPA METHOD 160.2/SM 2540D (TOTAL SUSPENDED SOLIDS; NON-FILTERABLE RESIDUE)	160_2.SOP
WETCHEM	EPA 160.3/SM 2540B	EPA METHOD 160.3 (TOTAL SOLIDS / PERCENT SOLIDS / PERCENT MOISTURE, GRAVIMETRIC, DRIED AT 103-105 C)	160_3.SOP
WETCHEM	EPA 160.4/SM 2540E	EPA METHOD 160.4/SM2540E (FIXED AND VOLATILES RESIDUE IN WATERS)	IR-WET-TVS
WETCHEM	EPA 300.0/9056	EPA METHOD 300.0 and EPA SW9056 (THE DETERMINATION OF INORGANIC ANIONS BY ION CHROMATOGRAPHY)	300_0.SOP
WETCHEM	EPA 300.1	EPA METHOD 300.1 (THE DETERMINATION OF INORGANIC ANIONS BY ION CHROMATOGRAPHY)	300_1.SOP
WETCHEM	EPA 330.5	EPA METHOD 330.5 (RESIDUAL CHLORINE)	330_5.SOP
WETCHEM	EPA 340.2/SM 4500F	EPA METHOD 340.2/SM 4500F (FLUORIDE BY POTENTIOMETRIC, ION SELECTIVE ELECTRODE)	340_2.SOP
WETCHEM	EPA 360.1/SM 4500O-G	EPA METHOD 360.1 / STANDARD METHOD 4500-O-G (DISSOLVED OXYGEN)	4500_OG.SOP
WETCHEM	EPA 365.3	EPA METHOD 365.3 (TOTAL PHOSPHORUS)	365_3.SOP
WETCHEM	EPA 410.4	EPA METHOD 410.4 (CHEMICAL OXYGEN DEMAND)	410_4.SOP
WETCHEM	EPA 415.1/9060/SM 5310B	EPA METHOD 415.1/SM 5310B OR EPA METHOD SW 9060 (TOTAL ORGANIC CARBON)	IR-WET-TOC
WETCHEM	EPA 420.1/9065	EPA METHOD 420.1/9065 (PHENOLICS, TOTAL RECOVERABLE)	420_1.SOP
WETCHEM	SM 5540C	EPA METHOD 5540C (ANION SURFACTANTS AS METHYLENE BLUE ACTIVE SUBSTANCES)	5540C.SOP
WETCHEM	EPA 7196A/SM 3500CR-D/EPA 3060A	EPA METHOD 7196A/STANDARD METHODS 3500-CR D (HEXAVALENT CHROMIUM, COLORIMETRIC + ALKALINE DIGEST (EPA 3060A)	7196A.SOP
WETCHEM	EPA 9030/9034/SM 4500S-F	EPA METHOD 9030/9034 / SM 4500S-F - ACID SOLUBLE/INSOLUBLE SULFIDES	9030_34.SOP
WETCHEM	EPA 9010B/9014/335.2	EPA METHODS 9010B, 9014 AND EPA 335.2 (TOTAL CYANIDE IN SOIL AND WATER)	9010_14.SOP
WETCHEM	EPA 130.2/SM 2340C	HARDNESS BY TITRATION EPA 130.2/SM2340C	2340c.SOP
WETCHEM	Various	Inorganic Calculations for Ion Balance, Langlier, Aggressive Index, Hardness, Unionized Sulfide, Larson-Skold Index, Sodium Absorption Ratio, Salinity	INORG_CALC.SOP
WETCHEM	LACSD 258	MERCAPTANS, TOTALS (LACSD 258)	258.SOP
WETCHEM	EPA 350.2/SM4500NH3 E	NITROGEN AMMONIA (TITRIMETRIC) (EPA METHOD 350.2/SM4500-NH3-B,E)	350_2r2.SOP
WETCHEM	EPA 120.1/SM 2510B	SPECIFIC ELECTRICAL CONDUCTANCE (EPA METHOD 120.1 / STANDARD METHOD 2510B)	120_1.SOP
WETCHEM	SM 2540G	STANDARD METHOD 2540G (TOTAL FIXED AND VOLATILE SOLIDS IN SOLIDS AND SEMISOLIDS)	2540G.SOP
WETCHEM	SM 4500CN-G	STANDARD METHOD 4500-CN-G/EPA 335.1/9010B (CYANIDES, AMENABLE TO CHLORINATION)	4500_CNG.SOP
WETCHEM	SM 4500CN-B,C,E	STANDARD METHOD 4500-CN- -B,C,E (CYANIDES, TOTAL)	4500_CN.SOP
WETCHEM	SM 4500CO2	STANDARD METHOD 4500-CO2 (TITRIMETRIC METHOD FOR FREE CARBON DIOXIDE)	4500_CO2.SOP
WETCHEM	SM 4500CN-I	STANDARD METHODS 4500-CN, I - WEAK ACID DISSOCIABLE CYANIDE	4500_CNI.SOP
WETCHEM	EPA 376.2/SM 4500S2-	SULFIDE, COLORIMETRIC, METHYLENE BLUE (STANDARD METHOD 4500 S2-, EPA 376.2)	4500_S.SOP
WETCHEM	LACSD 253B	THIOSULFATE BY TITRATION (LACSD 253B)	S2O3.SOP
WETCHEM	SM5310C	TOTAL AND DISSOLVED ORGANIC CARBON (STANDARD METHOD 5310C)	5310C.SOP
WETCHEM	EPA 160.1/SM 2540C	TOTAL DISSOLVED SOLIDS, FILTERABLE RESIDUE (EPA METHOD 160.1/SM2540C)	IR-WET-TDS

DEPARTMENT	Method	TITLE	FILENAME
WETCHEM	SM4500-Norg-C	TOTAL KJELDAHL NITROGEN	4500NORG_C.SOP

Figure 20-1a.
Example - Demonstration of Capability Checklist

TestAmerica Irvine	
Demonstration of Capability Checklist	
Initial / Annual	
<small>(Circle one)</small>	
Employee: _____	Procedure(s): _____
Job Title: _____	Matrix: _____
Department: _____	SOP Name/Revision: _____
<u>Task</u>	<u>Initials / Date Completed</u>
<i>Initial DOC Only</i>	
1 Employee has read and understands the published procedure(s). (i.e. pH published methods: EPA 9040B, EPA 150.1 & SM 4500)	_____ / _____
2 Employee has read, understands and agrees to follow the applicable SOP(s) without deviation.	_____ / _____
3 Using the SOP as a <u>step-by-step</u> reference, the trainer has demonstrated the entire procedure to the Employee. <i>If any inaccuracies or contradictions in the SOP are discovered at this time, notify the area Supervisor and the QA Manager before proceeding further.</i>	_____ / _____
4 Employee has performed the procedure under the direct supervision of an experienced staff member. (including standard and reagent preparation and calibration where applicable)	_____ / _____
5 Employee has independently performed the procedure and results have been reviewed and confirmed by experienced staff member.	_____ / _____
<hr/> <i>QA only</i> (Note when the training took place.)	
6 Trainer has completed a DOC for this method.	_____ / _____
7 Trainer has read the Training SOP.	_____ / _____
8 Employee has been trained on the Manual Integration and Data Integrity SOP (MANINT.SOP). Analysts only	_____ / _____
7 Employee has been trained on Ethics and Data Integrity.	_____ / _____
8 Employee has demonstrated capability by generating acceptable results on: (4 LCS replicates, PT sample, Blind QC, etc.)	_____ / _____
<p>The employee named above has successfully demonstrated proficiency to perform the above mentioned procedure, maintain applicable QA/QC requirements, and report results on his or her own.</p>	
Employee Signature: _____	Date: _____
Trainer Signature (if applicable): _____	Date: _____
Supervisory Signature: _____	Date: _____
Lab Director/QA approval: _____	Date: _____
<small>G:\Depts\QUALITY\TRAINING\CHKLIST7.DOC rev.7, 10/17/07</small>	

Figure 20-1b.
Example - Demonstration of Capability Document

DEMONSTRATION OF CAPABILITY CERTIFICATION STATEMENT

Date:
Laboratory Name:
Laboratory Address:
Analyst(s) Name(s):

Page 25 of 284

Matrix:
SOP# and Rev#:
Parameter:

We, the undersigned, CERTIFY that:

1. The analysts identified above, using the cited test method(s), which is in use at this facility for the analyses of samples under the National Environmental Laboratory Accreditation Program, have met the Demonstration of Capability.
2. The test method(s) was performed by the analyst(s) identified on this certification.
3. A copy of the test method(s) and the laboratory-specific SOPs are available for all personnel on-site.
4. The data associated with the demonstration capability are true, accurate, complete, and self explanatory.¹
5. All raw data (including a copy of this certification form) necessary to reconstruct and validate these analyses have been retained at the facility, and that the associated information is well organized and available for review by authorized assessors.

Technical Director's Name and Title

Signature

Date

Quality Assurance Manager

Signature

Date

¹ True: Consistent with supporting data.

Accurate: Based on good laboratory practices consistent with sound scientific principles/practices.

Complete: Includes the results of all supporting performance testing.

Self-Explanatory: Data properly labeled and stored so that the results are clear and require no additional explanation.

Figure 20-2.

Example - New Method / Additional Analyte Checklist

New Method / Additional Analyte Checklist

The following items are **required** to be completed prior to the acceptance of client samples. Fill in any blanks that do not apply with "NA". Provide associated instrument QC when samples or QC samples are analyzed (includes run log).

New Method _____ Added Analytes _____


1. _____ Standard Operating Procedure
 - Note: For additional analytes, a **ROMD [or whatever an internal communication memo is named in your lab]** can be used to add the analytes, include RL and matrix.
 - _____ Analysis SOP
 - _____ Preparation SOP
 - _____ SOP for any other relevant process
 - _____ Pages from any applicable logbooks (instrument, standards, etc)
 2. _____ Evaluation of Selectivity. As applicable: e.g. Retention Time Window Study, second column confirmation, Interelement correction checks, spectral or fluorescence profiles, etc.
 3. _____ Initial Calibration Curve (Include Tune verification or similar (e.g. degradation checks) if applicable)
 4. _____ Method Detection Limit (MDL) Study (summary and raw data)
 - _____ Water
 - _____ Soil
 - _____ Other
 5. _____ Real Sample and MS, MSD (**CA ELAP Requirement**)
 - Tap Water for water only methods
 - Local Soil sample for SW-846 methods (if applying for soil or soil/water)
 - Local water sample may be used in lieu of tap water if it is a non- drinking water method
 - Does not have to contain the target analytes
 6. _____ Reporting Limit Verification standard
 - Spike a blank matrix at the RL and process through the entire method. MDL study should be able to be used if recovery is good. Note the spike level(s) and recovery(yies)
 7. _____ Demonstration of Capability (DOC) per analyst (Precision and Accuracy (P&A) verification)
 - 4 LCS for each matrix – most acceptance criteria are in the methods. The MDL study may be used if DOC criteria are met.
 - Non-Standard methods – 3 x (1 LCS at LOQ-25%, 50%, 75% of the calibration range + Blank) prepared each day. (see NELAC Chpt 5, appendix C.3.3 (b))
 8. _____ Acceptable PT sample(s) if available

Notes: PT sample required for all new methods
PT sample required for all new analytes under NELAP
- Submitted by _____ Date _____
9. _____ Certification/Approval from Regulatory Agency where available.

QA Review / Acceptance _____ **Date** _____

Figure 20-3.

Work Flow

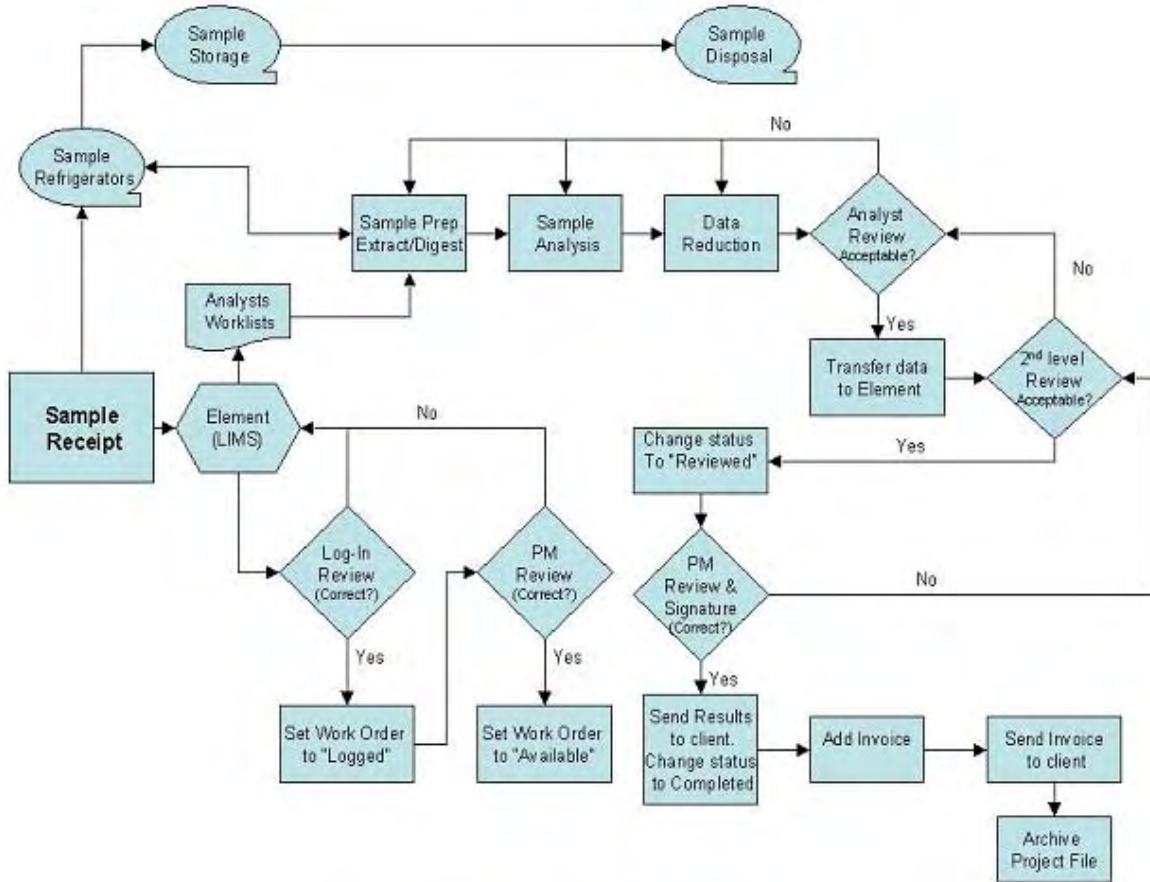

SECTION 21

EQUIPMENT (AND CALIBRATIONS) (NELAC 5.5.5)

21.1 OVERVIEW

TestAmerica purchases the most technically advanced analytical instrumentation for sample analyses. Instrumentation is purchased on the basis of accuracy, dependability, efficiency and sensitivity. Each laboratory is furnished with all items of sampling, preparation, analytical testing and measurement equipment necessary to correctly perform the tests for which the laboratory has capabilities. Each piece of equipment is capable of achieving the required accuracy and complies with specifications relevant to the method being performed. Before being placed into use, the equipment (including sampling equipment) is calibrated and checked to establish that it meets its intended specification. The calibration routines for analytical instruments establish the range of quantitation. Calibration procedures are specified in laboratory SOPs and are summarized in Appendix 4 of the QA manual. A list of laboratory equipment and instrumentation is presented in Table 21-1.

Equipment is only operated by authorized and trained personnel. Manufacturer instructions for equipment use are readily accessible to all appropriate laboratory personnel.

21.2 PREVENTIVE MAINTENANCE

21.2.1 TestAmerica Irvine follows a well-defined program to ensure proper equipment operation and to prevent the failure of laboratory equipment or instrumentation during use. This program of preventive maintenance helps to avoid delays due to instrument failure.

21.2.2 Routine preventive maintenance procedures and frequency, such as lubrication, cleaning, and replacements, should be performed according to the procedures outlined in the manufacturer's manual. Qualified personnel must also perform maintenance when there is evidence of degradation of peak resolution, a shift in the calibration curve, loss of sensitivity, or failure to continually meet one of the quality control criteria.

21.2.2.1 Calibrations, routine maintenance, and adjustments are part of the analysts' and Department Managers' responsibilities. However, service contracts may be in place for some instruments to cover any major repairs.

21.2.2.2 High purity gases, reagents, and spare parts are kept on hand to minimize repair time and optimize instrument performance.

21.2.3 Table 21-2 summarizes the schedule for routine maintenance. It is the responsibility of each Department Manager to ensure that instrument maintenance logs are kept for all equipment in his/her department. Preventative maintenance procedures may also be outlined in analytical SOPs or instrument manuals. (Note: for some equipment, the log used to monitor performance is also the maintenance log. Multiple pieces of equipment may share the same log as long as it is clear as to which instrument is associated with an entry.)

21.2.4 Instrument maintenance logs are controlled and are used to document instrument problems, instrument repair and maintenance activities. Maintenance logs shall be kept for all major pieces of equipment. [Instrument maintenance logs may also be used to specify instrument parameters.](#)

21.2.4.1 Documentation must include all major maintenance activities such as contracted preventive maintenance and service and in-house activities such as the replacement of electrical components, lamps, tubing, valves, columns, detectors, cleaning and adjustments.

21.2.4.2 Each entry in the instrument log includes the Analyst's initials, the date, a detailed description of the problem (or maintenance needed/scheduled), a detailed explanation of the solution or maintenance performed, and a verification that the equipment is functioning properly (state what was used to determine a return to control. e.g. CCV run on 'date' was acceptable, or instrument recalibrated on 'date' with acceptable verification, etc.).

21.2.4.3 When maintenance or repair is performed by an outside agency, service receipts detailing the service performed [can be affixed into the logbooks adjacent to pages describing the maintenance performed. This stapled-in page must be signed across the page entered and the logbook so that it is clear that a page is missing if only half a signature is found in the logbook.](#)

21.2.5 In addition, the maintenance records contain:

- The identification of the instrument/equipment (instrument's Serial Number and Model Number)
- The date the instrument/equipment was put into use.
- If available, the condition when the instrument was received (e.g. new, used, reconditioned).
- [Routine maintenance procedures and frequency or a reference to their location in the method SOP\(s\).](#)

21.2.6 If an instrument requires repair (subjected to overloading or mishandling, gives suspect results, or otherwise has shown to be defective or outside of specified limits) it shall be taken out of operation and tagged as out of service or otherwise isolated until such a time as the repairs have been made and the instrument can be demonstrated as operational by calibration and/or verification or other test to demonstrate acceptable performance. The laboratory shall examine the effect of this defect on previous analyses (refer to Sections 12 and 13).

21.2.7 In the event of equipment malfunction that cannot be resolved, service shall be obtained from the instrument vendor manufacturer, or qualified service technician, if such a service can be tendered. If on-site service is unavailable, arrangements shall be made to have the instrument shipped back to the manufacturer for repair. Back up instruments, which have been approved, for the analysis shall perform the analysis normally carried out by the malfunctioning instrument. If the back up is not available and the analysis cannot be carried out within the needed timeframe, the samples shall be subcontracted using the procedures outlined in Section 8.

If an instrument is sent out for service or transferred to another facility, it must be recalibrated and verified (including new initial MDL study) prior to return to lab operations.

21.3 SUPPORT EQUIPMENT

This section applies to all devices that may not be the actual test instrument, but are necessary to support laboratory operations. These include but are not limited to: [balances](#), [ovens](#), [refrigerators](#), [freezers](#), [incubators](#), [water baths](#), [field sampling devices](#), [temperature measuring devices](#), [thermal/pressure sample preparation devices](#) and [volumetric dispensing devices](#) if [quantitative results are dependent on their accuracy, as in standard preparation and dispensing or dilution into a specified volume](#). All raw data records associated with the support equipment are retained to document instrument performance.

21.3.1 Weights and Balances

The accuracy of the balances used in the laboratory is checked every working day, before use. All balances are placed on stable counter tops.

Each balance is checked prior to use with at least two certified ASTM type 1 weights spanning its range of use (weights that have been calibrated to ASTM type 1 weights may also be used for daily verification). ASTM type 1 weights used only for calibration of other weights (and no other purpose) are inspected for corrosion, damage or nicks at least annually and if no damage is observed, they are calibrated at least every 5 years by an outside calibration laboratory. Any weights (including ASTM Type 1) used for daily balance checks or other purposes are recalibrated/recertified annually to NIST standards (this may be done internally if laboratory maintains "calibration only" ASTM type 1 weights).

All balances are serviced annually by a qualified service representative, who supplies the laboratory with a certificate that identifies traceability of the calibration to the NIST standards.

All of this information is recorded in logs, and the recalibration/recertification certificates are kept on file. [The laboratory SOP BAL.SOP \(Balance Calibration, Verification and Documentation\) covers these procedures in greater detail.](#)

21.3.2 pH, Conductivity, and Turbidity Meters

The pH meters used in the laboratory are accurate to ± 0.1 pH units, and have a scale readability of at least 0.05 pH units. The meters automatically compensate for the temperature, and are calibrated with at least two working range buffer solutions before each use.

Conductivity meters are also calibrated before each use with a known standard to demonstrate the meters do not exceed an error of 1% or one umhos/cm.

Turbidity meters are also calibrated before each use. All of this information is documented in logs.

Consult pH and Conductivity, and Turbidity SOPs for further information.

21.3.3 Thermometers

All thermometers are calibrated on an annual basis with a NIST-traceable thermometer. IR thermometers, digital probes and thermocouples are calibrated quarterly.

The NIST thermometer is recalibrated every [five years](#) (unless thermometer has been exposed to temperature extremes or apparent separation of internal liquid) by an approved outside service and the provided certificate of traceability is kept on file. The NIST thermometer has increments of 0.2 °C, and has a range applicable to all method and certification requirements. The NIST traceable thermometer is used for no other purpose than to calibrate other thermometers.

[All of this information is documented in logbooks. Monitoring method-specific temperatures, including incubators, heating blocks, water baths, and ovens, is documented in method-specific logbooks. More information on this subject can be found in the laboratory's SOP THERMA.SOP \(Thermometer Calibration/Temperature Monitoring and Documentation\).](#)

21.3.4 Refrigerators/Freezer Units, Waterbaths, Ovens and Incubators

The temperatures of all refrigerator units and freezers used for sample and standard storage are monitored each working day.

Ovens, waterbaths and incubators are monitored on days of use.

All of this equipment has a unique identification number, and is assigned a unique thermometer for monitoring.

Sample storage refrigerator temperatures are kept between $> 0^{\circ}\text{C}$ and $\leq 6^{\circ}\text{C}$.

Specific temperature settings/ranges for other refrigerators, ovens waterbaths, and incubators can be found in method specific SOPs.

[All of this information is documented in Daily Temperature Logbooks and method-specific logbooks.](#)

21.3.5 Autopipettors, Dilutors, and Syringes

Mechanical volumetric dispensing devices including burettes (except Class A Glassware) are checked for accuracy at least quarterly. [Glass micro-syringes with volumes of 500 \$\mu\text{L}\$ or greater are checked for accuracy every six months.](#)

The laboratory maintains a sufficient inventory of autopipettors, and dilutors of differing capacities that fulfill all method requirements.

These devices are given unique identification numbers, and the delivery volumes are verified gravimetrically, at a minimum, on a quarterly basis ([every six months for applicable syringes](#)).

[For those dispensers that are not used for analytical measurements, a label is applied to the device stating that it is not calibrated.](#) Any device not regularly verified can not be used for any

quantitative measurements. See PIP.SOP (Pipet Calibration) for more details on pipettor, syringe, and dispenser calibration procedures.

Micro-syringes are purchased from Hamilton Company. Each syringe is traceable to NIST. The laboratory keeps on file an "Accuracy and Precision Statement of Conformance" from Hamilton attesting established accuracy.

21.3.6 Field Sampling Devices (Isco Auto Samplers)

Each Auto Sampler (ISCO) is assigned a unique identification number in order to keep track of the calibration. This number is also recorded on the sampling documentation.

The Auto Sampler is calibrated monthly by setting the sample volume to 100ml and recording the volume received. The results are filed in a logbook/binder. The Auto Sampler is programmed to run three (3) cycles and each of the three cycles is measured into a graduated cylinder to verify 100ml are received.

If the RSD (Relative Standard Deviation) between the 3 cycles is greater than 10%, the procedure is repeated and if the result is still greater than 10%, then the Auto Sampler is taken out of service until it is repaired and calibration verification criteria can be met. The results of this check are kept in a logbook/binder.

21.4 INSTRUMENT CALIBRATIONS

Calibration of analytical instrumentation is essential to the production of quality data. Strict calibration procedures are followed for each method. These procedures are designed to determine and document the method detection limits, the working range of the analytical instrumentation and any fluctuations that may occur from day to day.

Sufficient raw data records are retained to allow an outside party to reconstruct all facets of the initial calibration. Records contain, but are not limited to, the following: calibration date, method, instrument, analyst(s) initials or signatures, analysis date, analytes, concentration, response, type of calibration (Avg RF, curve, or other calculations that may be used to reduce instrument responses to concentration.)

Sample results must be quantitated from the initial calibration and may not be quantitated from any continuing instrument calibration verification unless otherwise required by regulation, method or program.

If the initial calibration results are outside of the acceptance criteria, corrective action is performed and any affected samples are reanalyzed if possible. If the reanalysis is not possible, any data associated with an unacceptable initial calibration will be reported with appropriate data qualifiers (refer to Section 13).

Note: Instruments are calibrated initially and as needed after that and at least annually.

21.4.1 CALIBRATION STANDARDS

Calibration standards are prepared using the procedures indicated in the Reagents and Standards section of the determinative method SOP. However, the general procedures are described below.

- 21.4.1.1** For each analyte and surrogate (if applicable) of interest, prepare calibration standards at the minimum number of concentrations as stated in the analytical methods. If a reference or mandated method does not specify the number of calibration standards, the minimum number is three, not including blanks or a zero standard. All of the standard solutions are prepared using Class A volumetric glassware, calibrated pipettes, and/or microsyringes and appropriate laboratory quality solvents and stock standards.
- 21.4.1.2** Standards for instrument calibration are obtained from a variety of sources. All standards are traceable to NIST whenever possible. Dilution standards are prepared from stock standards purchased from commercial suppliers. [The laboratory uses its LIMS to document the following standard information:](#) department, concentration, date of receipt, date of standard preparation, [expiration date](#), any dilutions made, lot number, supplier, type of solvent and a unique code number to identify the standard.
- 21.4.1.3** The lowest concentration calibration standard that is analyzed during an initial calibration must be at or below the stated reporting limit for the method based on the final volume of extract (or sample).
- 21.4.1.4** The other concentrations define the working range of the instrument/method or correspond to the expected range of concentrations found in actual samples that are also within the working range of the instrument/method. Results of samples not bracketed by initial instrument calibration standards (within calibration range to 3 significant figures) must be reported as having less certainty, e.g., defined qualifiers or flags (additional information may be included in the case narrative). The lowest calibration standard must be at or below the reporting limit. [The exception to these rules is ICP methods or other methods where the referenced method does not specify two or more standards.](#)
- 21.4.1.5** Given the number of target compounds addressed by some of the organic methods, it may be necessary to prepare several sets of calibration standards, each set consisting of the appropriate number of solutions at different concentrations. The initial calibration will then involve the analysis of each of these sets of the appropriate number of standards.
- 21.4.1.6** All initial calibrations are verified with a standard obtained from a second source and traceable to a national standard, when available (or vendor certified different lot if a second source is not available). [For unique situations, such as air analysis where no other source or lot is available, a standard made by a different analyst would be considered a second source.](#) This verification occurs immediately after the calibration curve has been analyzed, and before the analysis of any samples.

21.4.2 CALIBRATION FOR ORGANIC METHODS (GC, HPLC, GC/MS)

- 21.4.2.1** Many of the organic analytical methods utilize an internal standard calibration (GCMS and some GC). Because of the complex nature of the multiplex chromatograms produced by the method, some instruments necessitate the use of external standard calibration (most GC and HPLC). Surrogate compounds are included in the calibration processes for all appropriate organic analyses. For more details on the calibration types listed below, refer to SOP No. CA-Q-S-005, Calibration Curves.
- 21.4.2.2** Once the operating parameters have been established according to the method, each instrument is calibrated for the appropriate method. The analyst prepares five or more standard solutions at various concentrations containing all of the analytes of interest, internal standards, and surrogates that are appropriate for the method. Note: There are a several EPA methods that have different requirements and are exceptions (e.g. EPA 547) where a minimum of 3 calibration standards are prepared and analyzed.
- 21.4.2.3** The standard solutions are introduced into the instrument in the same manner as samples are; whether it be by direct injection, by headspace analysis, or by purge and trap. The calibration factor (CF) for methods that use external standards, and the response factor (RF) for methods that use internal standards are calculated for the five standards.
- External standard calibration involves comparison of instrument responses from the sample to the responses from the target compounds in the calibration standards. Sample peak areas (or peak heights) are compared to peak areas (or heights) of the standards. The ratio of the response to the amount of analyte in the calibration standard is defined as the Calibration factor (CF).
 - Internal standard calibration involves the comparison of instrument responses from the target compounds in the sample to the responses of specific standards added to the sample or sample extract prior to injection. The ratio of the peak area (or height) of the target compound in the sample or sample extract to the peak area (or height) of the internal standard in the sample or sample extract is compared to a similar ratio derived for each calibration standard. The ratio is termed the response factor (RF), and may also be known as a relative response factor in other methods.

In many cases, internal standards are recommended. These recommended internal standards are often brominated, fluorinated, or stable isotopically labeled analogs of specific target compounds, or are closely related compounds whose presence in environmental samples is highly unlikely. The use of specific internal standards is available in the method SOP.

Whichever internal standards are employed, the analyst needs to demonstrate that the measurement of the internal standard is not affected by method analytes and surrogates or by matrix interferences. In general, internal standard calibration is not as useful for GC and HPLC methods with non-MS detectors because of the inability to chromatographically resolve many internal standards from the target compounds. The use of MS detectors makes internal standard calibration practical because the masses of the internal standards can be resolved from those of the target compounds even when chromatographic resolution cannot be achieved.

When preparing calibration standards for use with internal standard calibration, add the same amount of the internal standard solution to each calibration standard, such that the concentration of each internal standard is constant across all of the calibration standards, whereas the concentrations of the target analytes will vary. The internal standard solution will contain one or more internal standards and the concentration of the individual internal standards may differ within the spiking solution (e.g., not all internal standards need to be at the same concentration in this solution). The mass of each internal standard added to each sample extract immediately prior to injection into the instrument or to each sample prior to purging must be the same as the mass of the internal standard in each calibration standard. The volume of the solution spiked into sample extracts should be such that minimal dilution of the extract occurs (e.g., 10 uL of solution added to a 1 mL final extract results in only a negligible 1% change in the final extract volume which can be ignored in the calculations).

An ideal internal standard concentration would yield a response factor of 1 for each analyte. However, this is not practical when dealing with more than a few target analytes. Therefore, as a general rule, the amount of internal standard should produce an instrument response (e.g., area counts) that is no more than 100 times that produced by the lowest concentration of the least responsive target analyte associated with the internal standard. This should result in a minimum response factor of approximately 0.01 for the least responsive target compound. Refer to SOP No. CA-Q-S-005, Calibration Curves, for specific calculations.

21.4.2.4 Policies regarding the use of calibration standard results for creating the calibration curve are as follows:

- A low calibration standard may be excluded from the calibration if the signal-to-noise ratio or spectral criteria are not suitable. The reporting level must be elevated to be the lowest calibration standard used for calibration.
- The upper calibration standard may be excluded if it saturates the detector or is obviously becoming non-linear. Any sample exceeding the upper standard used in the calibration must be diluted and re-analyzed.
- Mid-calibration standards may not be excluded unless an obvious reason is found, i.e., cracked vial, incorrectly made, etc. The failed standard should be re-run immediately and inserted into the initial calibration. If not useful, recalibration is required.

21.4.2.5 Percent RSD Corrective Action

Given the potentially large numbers of analytes that may be analyzed in some methods, it is likely that some analytes may exceed the acceptance limit for the RSD for a given calibration. In those instances, the following steps are recommended, but not required.

21.4.2.5.1 The first step is generally to check the instrument operating conditions. This option will apply in those instances where a linear instrument response is expected. It may involve some trade-offs to optimize performance across all target analytes. For instance, changes to the operating conditions necessary to achieve linearity for problem compounds may cause the RSD for other compounds to increase, but as long as all analytes meet the RSD limits for linearity, the calibration is acceptable.

21.4.2.5.2 If the RSD for any analyte is greater than the applicable acceptance criteria in the applicable [analytical method \(see also Appendix 4\)](#), the analyst may wish to review the results (area counts, calibration or response factors, and RSD) for those analytes to ensure that the problem is not associated with just one of the initial calibration standards. If the problem appears to be associated with a single standard, that one standard may be reanalyzed and the RSD recalculated. Replacing the standard may be necessary in some cases.

21.4.2.5.3 A third alternative is to narrow the calibration range by replacing one or more of the calibration standards with standards that cover a narrower range. If linearity can be achieved using a narrower calibration range, document the calibration linearity, and proceed with analyses. The changes to the upper end of the calibration range will affect the need to dilute samples above the range, while changes to the lower end will affect the overall sensitivity of the method. Consider the regulatory limits or action levels associated with the target analytes when adjusting the lower end of the range.

Note: When the purpose of the analysis is to demonstrate compliance with a specific regulatory limit or action level, the laboratory must ensure that the method quantitation limit is at least as low as the regulatory limit or action level.

21.4.2.6 Alternatively, the least squares regression may be used to determine linearity. A five point line must result in a correlation coefficient (r) of 0.990 or better using the least squares method to be considered acceptable. [In many cases it may be preferred that the curves be forced through zero \(not to be confused with including the origin as an additional data point, which is not allowed\).](#) **Note:** EPA method 8000B does not allow forcing through zero however the agency has reevaluated this position and has since changed this stance to allow forcing through zero. In addition, from EPA Method 8000C: "However, the use of a linear regression or forcing the regression through zero may NOT be used as a rationale for reporting results below the calibration range demonstrated by the analysis of the standards.").

21.4.2.7 Instead of a linear curve model (either Average RF or least squares regression), a second order curve (Quadratic) may be used (and preferred) as long as it contains at least six data points. As a rule of thumb, if there is a consistent trend in RFs (or CFs) in the calibration curve, either up or down, then quadratic curve fit may be indicated as the preferred calibration routine for that analyte. The coefficient of determination (COD or r^2) for the quadratic curve must be at least 0.99 for it to be considered acceptable. For more details on the calculations see Calibration Curve SOP CA-Q-S-005. Some limitations on the use of Quadratic Curve fits:

21.4.2.7.1 Care **MUST** be exercised to assure that the results from this equation are real, positive, and fit the range of the initial calibration.

21.4.2.7.2 They **may not** be used to mask instrument problems that can be corrected by maintenance. (Not to be used where the analyte is normally found to be linear in a properly maintained instrument).

- 21.4.2.7.3** They **may not** be used to compensate for detector saturation. If it is suspected that the detector is being saturated at the high end of the curve, remove the higher concentration standards from the curve and try a 1st order fit or average RF.

21.4.3 Calibration for Inorganic Analyses

EPA Method 7000 from EPA SW-846 is a general introduction to the quality control requirements for metals analysis. For inorganic methods, quality control measures set out in the individual methods and in the *Standard Methods for the Examination of Water and Wastewater* (20th Edition) may also be included. [Standard Operating Procedures for the analysis and the quality control documentation measures](#) are kept in each department's SOP binder.

In general, inorganic instrumentation is calibrated with external standards. Some exceptions would be [Inductively Coupled Plasma \(ICP\)](#), [Inductively Coupled Plasma Mass Spec \(ICPMS\)](#), and [Ion Chromatography Mass Spec \(ICMS\)](#). These analyses may use an internal standard to compensate for viscosity or other matrix effects. While the calibration procedures are much the same for inorganics as they are for organics, CF's or RF's are not used. The calibration model in 21.4.2.6 is generally used for most methods, however in some instances the model from section 21.4.2.7 may be used. A correlation coefficient (r) of 0.995 or greater must be used to accept a calibration curve generated for an inorganic procedure. Correlation coefficients are determined by hand-held scientific calculators or by computer programs [state what your lab uses] and documented as part of the calibration raw data. Coefficients of calibration curves used for quantitation must be documented as part of the raw data. Curves are not allowed to be stored in calculator memories and must be written on the raw data for the purposes of data validation.

- 21.4.3.1** "Calibrations" for titrimetric analyses are performed by standardizing the titrants against a primary standard solution. See specific methods in *Standard Methods for the Examination of Water and Wastewater* (20th Edition) for more information.
- 21.4.3.2** Spreadsheets that are used for general chemistry calculations must have all cells containing calculations locked to prevent accidental changes to the calculations.
- 21.4.3.3** [Instrument technologies \(e.g. ICP\) with validated techniques from the instrument manufacturer or other methods using a zero point and single point calibration](#) require the following:
- 21.4.3.3.1** [The instrument is calibrated using a zero point and a single point calibration standard.](#)
 - 21.4.3.3.2** [The linear range is established by analyzing a series of standards, one at the reporting limit \(RL\).](#)
 - 21.4.3.3.3** [Sample results within the established linear range do not need to be qualified.](#)
 - 21.4.3.3.4** [The zero point and single standard is run daily with each analytical batch.](#)
 - 21.4.3.3.5** [A standard at the RL is analyzed daily with each analytical batch and must meet established acceptance criteria.](#)

21.4.3.3.6 The linearity is verified at a frequency established by the manufacturer or method.

21.4.4 Calibration Verification

The calibration relationship established during the initial calibration must be verified at periodic intervals as specified in the laboratory method SOPs in accordance with the referenced analytical methods and [NELAC \(2003\) standard, Section 5.5.5.10](#). The process of calibration verification applies to both external standard and internal standard calibration techniques, as well as to linear and non-linear calibration models.

Note: The process of calibration verification referred to is fundamentally different from the approach called "calibration" in some methods. As described in those methods, the calibration factors or response factors calculated during calibration are used to update the calibration factors or response factors used for sample quantitation. This approach, while employed in other EPA programs, amounts to a daily single-point calibration, and is not appropriate nor permitted in SW-846 chromatographic procedures for trace environmental analyses.

21.4.4.1 Generally, the initial calibrations must be verified at the beginning of each 12-hour analytical shift during which samples are analyzed. (Some methods may specify more or less frequent verifications). The 12-hour analytical shift begins with the injection of the calibration verification standard (or the MS tuning standard in MS methods). The shift ends after the completion of the analysis of the last sample or standard that can be injected within 12 hours of the beginning of the shift.

21.4.4.2 A continuing instrument calibration verification (CCV) must be repeated at the beginning and, for methods that have quantitation by external calibration models, at the end of each analytical batch. Some methods have more frequent CCV requirements see specific SOPs. Most Inorganic methods require the CCV to be analyzed after every 10 samples.

21.4.4.3 The acceptance limits for calibration verifications can be found in each method SOP. As a rule of thumb: GCMS \pm 20%, GC and HPLC \pm 15%, Inorganics: \pm 10 or 15%. Actual methods may have wider or tighter limits; see [the method SOP for specifics](#).

21.4.4.4 If the response (or calculated concentration) for an analyte is within the acceptance limits of the response obtained during the initial calibration, then the initial calibration is considered still valid, and the analyst may continue to use the CF, RF or % drift values from the initial calibration to quantitate sample results.

21.4.4.5 If the response (or calculated concentration) for any analyte varies from the mean response obtained during the initial calibration by more than the acceptance criteria, then the initial calibration relationship may no longer be valid. If routine corrective action procedures fail to produce a second consecutive (immediate) calibration verification within acceptance criteria, then either the laboratory has to demonstrate performance after corrective action with two consecutive successful calibration verifications, or a new initial instrument calibration must be performed. However, sample data associated with an unacceptable calibration verification may be reported as qualified data under the following special conditions:

21.4.4.5.1 When the acceptance criteria for the calibration verification are exceeded high, i.e., high bias, and there are associated samples that are non-detects, then those non-detects may be reported. Otherwise, the samples affected by the unacceptable calibration verification shall be reanalyzed after a new calibration curve has been established, evaluated and accepted.

21.4.4.5.2 When the acceptance criteria for the calibration verification are exceeded low, i.e., low bias, those sample results may be reported if they exceed a maximum regulatory limit/decision level. Otherwise, the samples affected by the unacceptable verification shall be reanalyzed after a new calibration curve has been established, evaluated and accepted. **Alternatively, a reporting limit standard may be analyzed to demonstrate that the laboratory can still support non-detects at their reporting limit.**

21.4.4.6 Verification of Linear Calibrations

Calibration verification for linear calibrations involves the calculation of the percent drift or the percent difference of the instrument response between the initial calibration and each subsequent analysis of the verification standard. Use the equations below to calculate % Drift or % Difference, depending on the procedure specified in the method SOP. Verification standards are evaluated based on the % Difference from the average CF or RF of the initial calibration or based on % Drift or % Recovery if a linear or quadratic curve is used.

The Percent Difference is calculated as follows:

$$\% \text{ Difference} = \frac{(\text{CF}(v) \text{ or } \text{RF}(v)) - (\text{Avg. CF or RF})}{(\text{Avg. CF or RF})} \times 100$$

Where: CF(v) or RF(v) = CF or RF from verification standard
Avg. CF or RF = Average CF or RF from Initial Calibration.

The Percent Drift is calculated as follows:

$$\% \text{ Drift} = \frac{\text{Result} - \text{True Value}}{\text{True Value}} \times 100$$

The Percent Recovery is calculated as follows:

$$\% \text{ Recovery} = \frac{\text{Result}}{\text{True Value}} \times 100$$

21.4.4.7 Verification of a Non-Linear Calibration

Calibration verification of a non-linear calibration is performed using the percent drift or percent recovery calculations described in 21.4.4.6 above.

Regardless of whether a linear or non-linear calibration model is used, if initial verification criterion is not met, then no sample analyses may take place until the calibration has been verified or a new initial calibration is performed that meets the specifications listed in the method SOPs. If the calibration cannot be verified after the analysis of a single verification standard, then adjust the instrument operating conditions and/or perform instrument maintenance, and analyze another aliquot of the verification standard. If the calibration cannot be verified with the second standard, then a new initial calibration is performed.

All target analytes and surrogates, including those reported as non-detects, must be included in periodic calibration verifications for purposes of retention time confirmation and to demonstrate that calibration verification criteria are being met.

All samples must be bracketed by periodic analyses of standards that meet the QC acceptance criteria (e.g., calibration and retention time). [The frequency is found in the laboratory's SOP for the specific method.](#)

Note: If an internal standard calibration is being used (basically GCMS) then bracketing standards are not required, only daily verifications are needed. The results from these verification standards must meet the calibration verification criteria and the retention time criteria (if applicable).

21.5 POLICY ON TENTATIVELY IDENTIFIED COMPOUNDS (TICS) – GC/MS ANALYSIS

For samples containing components not associated with the calibration standards, a library search may be made for the purpose of tentative identification. The necessity to perform this type of identification will be determined by the purpose of the analyses being conducted. Data system library search routines should not use normalization routines that would misrepresent the library or unknown spectra when compared to each other.

Note: If the TIC compound is not part of the client target analyte list but is calibrated by the laboratory and is both qualitatively and/or quantitatively identifiable, it will not be reported as a TIC. If the compound is reported on the same form as true TICs, it must be qualified and/or narrated that the reported compound is qualitatively and quantitatively (if verification in control) reported compared to a known standard that is in control (where applicable).

For example, the RCRA permit or waste delisting requirements may require the reporting of non-target analytes. Only after visual comparison of sample spectra with the nearest library searches may the analyst assign a tentative identification. [See SOPs IR-MSV-8260 and IR-MSS-8270 for guidelines on making tentative identifications](#)

21.5.1 The following guidelines for making tentative identifications are taken from EPA SW846 III edition, method 8260B.

21.5.1.1.1 Relative intensities of major ions in the reference spectrum (ions greater than 10% of the most abundant ion) should be present in the sample spectrum.

- 21.5.1.1.2** The relative intensities of the major ions should agree within $\pm 20\%$. (Example: For an ion with an abundance of 50% in the standard spectrum, the corresponding sample ion abundance must be between 30 and 70%).
- 21.5.1.1.3** Molecular ions present in the reference spectrum should be present in the sample spectrum.
- 21.5.1.1.4** Ions present in the sample spectrum but not in the reference spectrum should be reviewed for possible background contamination or presence of coeluting compounds.
- 21.5.1.1.5** Ions present in the reference spectrum but not in the sample spectrum should be reviewed for possible subtraction from the sample spectrum because of background contamination or coeluting peaks. Data system library reduction programs can sometimes create these discrepancies.
- 21.5.1.1.6** The concentration of any non-target analytes identified in the sample (see above) should be estimated. The same formulae as calibrated analytes should be used with the following modifications: The areas A_x and A_{is} should be from the total ion chromatograms, and the RF for the compound should be assumed to be 1.
- 21.5.1.1.7** The resulting concentration should be reported indicating: (1) that the value is an estimate, and (2) which internal standard was used to determine concentration. Use the nearest internal standard free of interferences.
- 21.5.1.2** For general reporting if TICs are requested, the ten (10), largest non-target analyte peaks whose area count exceeds 10% of the nearest internal standard will be termed "Tentatively Identified Compounds" (TICs). More or fewer TICs may be identified based on client requirements.

21.5.1.3 TIC Reporting Limits

In general Reporting limits cannot be specified because of the unknown nature of the TIC. Any reporting limit that is reported can only be evaluated as an estimate as the quantitation is based on the assumption that the TIC responds exactly as the IS responds which is most likely not the case. In general, it is not recommended to set a Reporting limit at too low of a concentration as it gives a false impression.

TICs that meet the above identification criteria (Section 21.5.1) at 10% area of the IS: The RL would be 10% of the concentration of the internal standard used for quantitation. (e.g. 2.5 ug/L for 8260B, 4.0 ug/L for 8270C). In general, if the 10% area criteria is not met, the TIC RLs should be set at a level approximately 5x the level of the poorest performer in the analysis.

If a compound meets the TIC criteria, the reporting limit will reflect the ratio between the TIC and the IS or 5x the level of the poorest performer whichever is lower.

21.6 POLICY ON GC/MS TUNING

Prior to any GCMS analytical sequence, including calibration, the instrument parameters for the tune and subsequent sample analyses within that sequence must be set.

Prior to tuning/auto-tuning the mass spec, the parameters may be adjusted within the specifications set by the manufacturer or the analytical method. These generally don't need any adjustment but it may be required based on the current instrument performance. If the tune verification does not pass it may be necessary to clean the source or perform additional maintenance. Any maintenance is documented in the maintenance log.

21.6.1 The concentration of the BFB or DFTPP must be at or below the concentrations that are referenced in the analytical methods. Part of the purpose of the tune is to demonstrate sensitivity and analyzing solutions at higher concentrations does not support this purpose. Tune failures may be due to saturation and a lower BFB/DFTPP concentration may be warranted.

21.6.2 Tune evaluations usually utilize the "Autofind" function and are set up to look at the apex +/- 1 scan and average the three scans. Background correction is required prior to the start of the peak but no more than 20 scans before. Background correction cannot include any part of the target peak.

21.6.3 Other Options or if Auto Tune Fails:

21.6.3.1 Sometimes the instrument does not always correctly identify the apex on some peaks when the peak is not perfectly shaped. In this case, manually identify and average the apex peak +/- 1 scan and background correct as in 21.6.4 above. This is consistent with EPA 8260 and 8270.

21.6.3.2 Or the scan across the peak at one half peak height may be averaged and background corrected. This is consistent with Standard Methods 6200, EPA 624 and EPA 625.

21.6.3.3 Adjustments such as adjustments to the repeller and ion focus lenses, adjusting the EM Voltage, etc. may be made prior to tune verification as long as all of the subsequent injections in the 12 hour tune cycle are analyzed under the same MS tune settings and it is documented in the run sequence log and/or maintenance log that an adjustment was made. Excessive adjusting (more than 2 tries) without clear documentation is not allowed. Necessary maintenance is performed and documented in instrument log.

21.6.3.4 A single scan at the Apex (only) may also be used for the evaluation of the tune. For SW 846 and EPA 600 series methods, background correction is still required.

21.6.3.5 Cleaning the source or other maintenance may be performed and then follow steps for tune evaluation above. Note: If significant maintenance was performed, see methods 8000B or 8000C then the instrument may require recalibration prior to proceeding.

21.6.4 Tune evaluation printouts must include the chromatogram and spectra as well as the Tune evaluation information. In addition, the verifications must be sent directly to the printer or pdf file (no screen prints for DFTPP or BFB tunes). This ability should be built into the instrument software.

21.6.5 Since the limits are expressed in whole percentages, the results may be rounded to whole percentage before comparing to criteria when assessing the tune verification against the tune requirements. However, the comparison to the criteria is usually done automatically by the software and if the printout says "Fail" then there would have to be documentation of the hand calculation on the raw data and comparison to the criteria if the lab intends to still accept the tune. In most cases the analyst is better off performing an adjustment and rerunning the tune standard.

21.6.6 All MS tune settings must remain constant between running the tune check and all other samples. It is recommended that a separate tune method not be used, however a separate method may be used as long as the MS conditions between the methods are the same as the sample analysis method and tracked so any changes that are made to the analysis method are also made to the tune method.

Table 21-1. Laboratory Equipment and Instrumentation

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Accelerated Solvent Extractor	Dionex	ASE 200	96040278	2000	NEW
Accelerated Solvent Extractor	Dionex	ASE 200	120362	2001	NEW
Accelerated Solvent Extractor	Dionex	ASE 200	97040463	2001	NEW
Accelerated Solvent Extractor	Dionex	ASE 200	96090216	2001	NEW
Accelerated Solvent Extractor	Dionex	ASE 200	99120782	2002	NEW
Accelerated Solvent Extractor	Dionex	ASE 200E	07090745	2007	NEW
Accelerated Solvent Extractor	Dionex	ASE 200E	07090746	2007	NEW
Air Concentrator	Entech	2000		1993	NEW
Ammonia Probe	Orion	96-12			Footnote 1
Atomic Absorption Spectrophotometer	Perkin Elmer	SIMAA 6000	5016	1995	NEW
Auto sampler	Dionex	AS40	98050117	2007	NEW
Auto Sampler (Archon)	O.I. Analytical	4552	12243	2001	NEW
Auto Sampler (Archon)	Varian	Archon	14636	2006	NEW
Auto Sampler (Archon)	Varian	Archon	14633	2006	NEW
Auto Sampler (Archon)	Varian	Archon	14634	2006	NEW
Auto Sampler (Archon)	Varian	Archon	14632	2006	NEW
Auto Sampler (Archon)	Varian	Archon	13171	2006	NEW
Auto Sampler (Archon)	Varian	Archon	14638	2006	NEW
Auto Sampler (Archon)	O.I. Analytical	4552	14418	2004	NEW
Auto Sampler (Archon)	Varian	Archon	14407	2006	NEW
Auto Sampler (Archon)	O.I. Analytical	4552	14417	2006	NEW
Auto Sampler (Archon)	Varian	Archon	14418	2006	NEW
Auto Sampler (Archon)	Varian	Archon	14195	2006	NEW
Auto Sampler (Archon)	Varian	Archon	13388	2006	NEW

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Auto Sampler (Archon)	Archon		14411	2006	NEW
Auto Sampler (Archon)	Varian	Archon	14492	2006	NEW
Auto Sampler (Archon)	Varian	Archon	14637	2006	NEW
Auto Sampler (Archon)	Varian	Archon	14639	2006	NEW
Auto Sampler (Archon)	Varian	Archon	13389	2006	NEW
Auto Sampler (DPM)	O.I. Analytical	MPM 16		1993	NEW
Auto Sampler (DPM)	O.I. Analytical	MPM 16		1997	NEW
Auto Sampler (DPM)	O.I. Analytical	MPM/DPM 16		1993	NEW
Auto Sampler (DPM)	O.I. Analytical	MPM 16		1992	NEW
Auto Sampler (DPM)	O.I. Analytical	MPM-16		1993	NEW
Auto Sampler (DPM)	O.I. Analytical	DPM 16		2003	NEW
Auto Sampler (DPM)	O.I. Analytical	MPM 16			Footnote 1
Auto Sampler for GC	Hewlett Packard	7673A			Footnote 1
Auto Sampler for GC	Hewlett Packard	7673B			Footnote 1
Auto Sampler for GC	Hewlett Packard	7673B			Footnote 1
Auto Sampler for GC	Hewlett Packard	7673A			Footnote 1
Auto Sampler for GC	LEAP				
Auto Sampler for GC	Hewlett Packard	7673B			Footnote 1
Auto Sampler for GC	Agilent	7683			Footnote 1
Auto Sampler for GC	Hewlett Packard	18596M			Footnote 1
Auto Sampler for GC	Agilent	7683			Footnote 1
Auto Sampler for GC	Hewlett Packard	7673			Footnote 1
Auto Sampler for GC	Hewlett Packard	7673			Footnote 1
Auto Sampler for GC	Hewlett Packard	7673B		1993	NEW
Auto Sampler for GC	Hewlett Packard	7673B		1995	NEW

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Auto Sampler for GC	Hewlett Packard	7673B		1993	NEW
Auto Sampler for GC	Agilent	7683		2003	NEW
Auto Sampler for GC	Agilent	7683		2005	NEW
Auto Sampler for GC	Hewlett Packard	7673B		1993	NEW
Auto Sampler for GC	Agilent	7683B	CN63340749	2006	NEW
Auto Sampler for GC	Hewlett Packard	18593B	3120A26939	1992	NEW
Auto Sampler for GC	Agilent	7683	CN42637490		Footnote 1
Auto Sampler for GC	Agilent	G2614A	CN55237971		Footnote 1
Auto Sampler for IC	Dionex	AS			Footnote 1
Auto Sampler for IC	Dionex	AS	96060542		Footnote 1
Auto Sampler for IC	Dionex	AS	3080145		Footnote 1
Auto Sampler for IC	Dionex	AS	3080145		Footnote 1
Auto Sampler for IC	Dionex	AS50	0411004Y	2002	NEW
Auto Sampler for IC	Dionex	AS50	99010302	2005	NEW
Auto Sampler for IC	Dionex	AS40	932811		Footnote 1
Auto Sampler for IC	Dionex	AS40	06110242	2007	NEW
Auto Sampler for IC	Dionex	AS50	00100242		Footnote 1
Auto Sampler for Metals	Perkin Elmer	AS-72	1464	1995	NEW
Auto Sampler for Metals	Perkin Elmer	CETAC	060019ASX	2001	NEW
Auto Sampler for Metals	Perkin Elmer	AS 91	913S3040101	1997	NEW
Auto Sampler for Metals	Perkin Elmer	AS 93	1075	2002	NEW
Auto Sampler for Metals	Perkin Elmer	AS 90	3380	1995	NEW
Auto Sampler for Metals	Perkin Elmer	CETAC	080002ADX	2004	NEW
Auto Sampler for Metals	Perkin Elmer	AS 91	6060	1995	NEW
Auto Sampler for Metals	Perkin Elmer	AS 91	3023	2006	NEW

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Autosampler	Agilent	G2614A	CN55237964	2007	NEW
Block Digestor	Bioscience	163-466T		1997	NEW
Block Digestor	Bioscience	2091B1		1997	NEW
BOD auto-analyzer	ManTech	BODAssayPlus			Footnote 1
BOD Incubator	Fisher		00037-090-00		Footnote 1
BOD Incubator	??				Footnote 1
BOD probe	Jenco				Footnote 1
Centrifuge	IEC	--	3634P-14		Footnote 1
Centrifuge	Fisher Scientific	AccuSpin 300	603101639	2003	NEW
Centrifuge	Precision	Durafuge 100	40317924	2003	NEW
Centrifuge	International Centrifuge Co.	HN	98323M-1		Footnote 1
COD Reactor	Bioscience Inc.	2091B1	34613302		Footnote 1
COD Reactor	Bioscience Inc.	163-466T	COD-T349		Footnote 1
Concentrator	O.I. Analytical	4560		1999	NEW
Conductivity Probe	Yellow Springs	32	COD0031		Footnote 1
Conductivity/Dissolved Oxygen Probe	Corning	M90	001253		Footnote 1
Cyanide Distillation Unit	Andrews Glass	MIDI System	MCVA13908221		Footnote 1
Cyanide Distillation Unit	Andrews Glass	MIDI System	33212579		Footnote 1
Digestion Unit	Gerhardt	Kjeldatherm KB	4062216	2007	NEW
Distillation Unit	Gerhardt	Vapodist30	VAP005617	2007	NEW
Drying Oven	Fisher		40200001		Footnote 1
Drying Oven	Fisher	630G	800121		Footnote 1
Drying Oven	Lab Line				Footnote 1
Drying Oven	Scientific Products	DX-61	194002		Footnote 1
Drying Oven	Fisher	630G	801N0001		Footnote 1
Fixed Wavelength Infrared Spectrophotometer	Foxboro	Miran1FF	2592	1997	NEW
Fixed Wavelength Infrared Spectrophotometer	Foxboro	Miran1FF	2733		Footnote 1

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Flashpoint Tester	Koehler	K-162		1992	NEW
Fluoride Probe	Orion	96-09	9609BN		Footnote 1
Gas Chromatograph	Agilent	6890N	US10423014		Footnote 1
Gas Chromatograph	Agilent	6890N	CN10551059	2007	NEW
Gas Chromatograph (Dual ECD)	Hewlett Packard	5890 Series II	3223A43015		Footnote 1
Gas Chromatograph (Dual ECD)	Hewlett Packard	5890 Series II	336A51142		Footnote 1
Gas Chromatograph (Dual ECD)	Hewlett Packard	5890Series II	2750A15311		Footnote 1
Gas Chromatograph (Dual ECD)	Agilent	6890	US10215019		Footnote 1
Gas Chromatograph (Dual ECD)	Agilent	6890N	US10250081		Footnote 1
Gas Chromatograph (Dual ECD)	Hewlett Packard	5890 Series II	3235A45184		Footnote 1
Gas Chromatograph (Dual ECD)	Agilent	6890N	CN10551052		Footnote 1
Gas Chromatograph (Dual FID)	Hewlett Packard	5890 Series II	3126A36534		Footnote 1
Gas Chromatograph (Dual FID)	Hewlett Packard	5890 Series II	3133A37568		Footnote 1
Gas Chromatograph (Dual FID)	Hewlett Packard	5890II	3235A44731		Footnote 1
Gas Chromatograph (Dual FID)	Hewlett Packard	5890 Series II	2950A26022		Footnote 1
Gas Chromatograph (ECD)	Hewlett Packard	5890 Series II	3203A40480		Footnote 1
Gas Chromatograph (FID)	Hewlett Packard	5890 Series II	3126A36955	1997	NEW
Gas Chromatograph (FID)	Hewlett Packard	5890 Series II			Footnote 1

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	3203A40477	1993	NEW
Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	3203A41169	1993	NEW
Gas Chromatograph (FID/PID)	Hewlett Packard	5890A	2750A15898	1997	NEW
Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	3223A42733	1993	NEW
Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	3223A60064	1993	NEW
Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	3336A60064	1993	NEW
Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	3033A33301	1998	NEW
Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II	3336A60066	1997	NEW
Gas Chromatograph (FID/PID)	Hewlett Packard	5890 Series II			Footnote 1
Gas Chromatograph (FID/PID/ELCD)	Hewlett Packard	5890 Series II	3203A40699	1993	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	6890/5973A	US00007750	2001	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	6890/5973A	US00022931	2000	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	6850/5973N	US00001207	2001	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	6850/5973	US00001206	2001	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	6850/5973N	US01874908	2002	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	6850/5973N	US10440793	2002	NEW

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Gas Chromatograph/Mass Spectrometer	Agilent	6850/5973N	US00002860	2003	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973	US00034262	2004	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973	CN10318006	2004	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973	CN10318007	2004	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	6890N/5973		2006	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	6890N/5973		2005	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890II/5972		1997	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	6890N/5973		2000	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	6890/5973A	US00020097	1999	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890Ser.II/5971	3140A39653	1993	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890Ser.II/5972	3235A46723	1995	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890Ser.II/5971	3133A37717	1993	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	6890/5973	US10130035	2003	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973	US10341048	2005	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890Ser.II/5971	3033A30488	1993	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890Ser.II	3033A32428	1987	NEW

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Gas Chromatograph/Mass Spectrometer	Hewlett Packard				Footnote 1
Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973	US10206070/A12019	2006	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	6890N/5973N	US10222064/A13016	2006	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	5975B/6890N	US62724086/CN10636107	2006	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	6890N/5973		2001	NEW
Gas Chromatograph/Mass Spectrometer	Hewlett Packard	5890IIB/5971A	2921A24077/3188A02848	1992	NEW
Gas Chromatograph/Mass Spectrometer	Agilent	6890/5973	CN10427051/US41720775	2007	NEW
Hot Block	Environmental Express				Footnote 1
Hot Block	Environmental Express				Footnote 1
Hot Block	Environmental Express				Footnote 1
Hot Block	Environmental Express				Footnote 1
Hot Block	Environmental Express				Footnote 1
Hot Block	Environmental Express				Footnote 1
Hot Plate	??				Footnote 1
Hot Plate	??				Footnote 1
Inductively Coupled Plasma Spectrophotometer/MS	Perkin Elmer	ELAN6100E	1650004	2001	NEW
Inductively Coupled Plasma Spectrophotometer/MS	Perkin Elmer	ELAN6100E	G1970008	2004	NEW
Inductively Coupled Plasma Spectrophotometer	Perkin Elmer	Optima 3000	069N4092201	1997	NEW

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Inductively Coupled Plasma Spectropho tometer	Perkin Elmer	Optima 4300	077N1100901	2002	NEW
Inductively Coupled Plasma Spectropho tometer	Perkin Elmer	Optima 5300DV	077N5112802	2006	NEW
Injector	Agilent	7683 series	CN55130059	2007	NEW
Injector Tower	Hewlett Packard	7673			Footnote 1
Ion Chromatograph	Dionex	DX 500	98060923	1996	NEW
Ion Chromatograph	Dionex	DX 100	40452	1997	NEW
Ion Chromatograph	Dionex	DX 600	139082221	2002	NEW
Ion Chromatograph	Dionex	ICS-1000	03110585	2002	NEW
Ion Chromatograph	Dionex	CD25A	01060463	2005	NEW
Ion Chromatograph	Dionex	AD25	01050864	2007	NEW
Ion Chromatograph	Dionex	CD25-1	00070432	2002	NEW
Ion Chromatograph	Dionex	LC20	94010215	2007	NEW
Ion Chromatograph (with UV/VIS)	Dionex	DX 500	94120366	2000	NEW
Ion Chromatograph/M ass spectrometer	Metrohm/Agilent /	LC30- 1/LC110/IC800		2005	NEW
Kiln	Cress	E2418	0503DD	2005	NEW
Mercury Analyzer	Perkin Elmer	FIMS 400	4109	1995	NEW
Mercury Analyzer	Perkin Elmer	FIMS 400	4167	1995	NEW
Orbital shaker	Lab-Line	--			Footnote 1
pH Meter	Beckman	Phi - 40			Footnote 1
pH Meter	Beckman	Phi - 40			Footnote 1
pH Meter	Beckman	Phi - 32			Footnote 1
pH Meter	Mettler Toledo	SevenEasy	1227116127		
pH Probe	Orion	91-56	9156000		Footnote 1
pH Probe	Orion	91-56			Footnote 1

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Purge & Trap Concentrator	O.I. Analytical	4460A		1992	NEW
Purge & Trap Concentrator	O.I. Analytical	4460A		1993	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		1993	NEW
Purge & Trap Concentrator	O.I. Analytical	4460A		1997	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		1993	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		1992	NEW
Purge & Trap Concentrator	O.I. Analytical	4460A		1993	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		1998	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2001	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2000	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2001	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2001	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2002	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2002	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2003	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2004	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2004	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2004	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2006	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2005	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2000	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		1997	NEW
Purge & Trap Concentrator	O.I. Analytical	4460A			Footnote 1
Purge & Trap Concentrator	O.I. Analytical	4560	H351460339	2006	NEW
Purge & Trap Concentrator	O.I. Analytical				Footnote 1

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Purge & Trap Concentrator	O.I. Analytical	4560	E324406	2006	NEW
Purge & Trap Concentrator	O.I. Analytical	4560		2001	NEW
Purge and Trap Water/Soil AutoSampler	O.I. Analytical	4552		1993	NEW
Purge and Trap Water/Soil AutoSampler	EST	8100		2006	NEW
Rapid Vap	Labconco		266435		Footnote 1
Rapid Vap	Labconco		705319		Footnote 1
Rapid Vap	Labconco		21098412F		Footnote 1
Rapid Vap	Labconco		010194458E		Footnote 1
Rapid Vap	Labconco	7910000	040824527		Footnote 1
Rotator	N/A				Footnote 1
Rotator	N/A				Footnote 1
Rotator	N/A				Footnote 1
Rotator	N/A				Footnote 1
SPE-Controller	Horizon Technology	SPE-DEX	020357		Footnote 1
SPE-Extractor	Horizon Technology	SPE-DEX 4790	030359		Footnote 1
SPE-Extractor	Horizon Technology	SPE-DEX 4790	030360		Footnote 1
TOC Analyzer	Shimadzu	TOC-5000A	33N01036A	1998	NEW
TOC Analyzer w/AS	Tekmar-Dohrmann	Phoenix 8000	US02106006	2002	NEW
TOC Autosampler	Shimadzu	ASI-500A-H-P	33212579	1998	NEW
TOC Soil Sampler Module	Shimadzu	SSM-5000A	34613302	1998	NEW
Turbidity Meter	HF Instruments	DRT-100B	24942		Footnote 1
Turbidity Meter	Orbeco-Hellige	965-10A	4389	2007	NEW
Turbidity Meter	Orbeco-Hellige	965	5078	2007	NEW
Turbo Vap	Zymark		04053		Footnote 1
Turbo Vap	Zymark	--			Footnote 1
Turbo Vap II	Zymark		04516		Footnote 1

Instrument/ Equipment	Manufacturer	Model Number	Serial Number	Year Put into Service	Condition When Received
Turbo Vap II	Zymark		04272		Footnote 1
Turbo Vap II	Zymark		TV0239N11193		Footnote 1
Turbo Vap LV	Caliper LifeSciences	103200/2	TV0429N12434		Footnote 1
Turbo Vap LV	Caliper LifeSciences	103200/2	TV0429N12435		Footnote 1
UV/VS Spectrometer	Thermospectron ic	Genesys20		2002	NEW

¹Although equipment is operational and calibration maintained, this information is not available.

Table 21-2. Schedule of Routine Maintenance

Instrument	Procedure	Frequency
Graphite Furnace (GFAA)	Inspect graphite tube Inspect contact rings Clean windows Align lamp	Daily Daily Daily Daily
Mercury Analyzer	Check tubing for wear Fill rinse tank with 10% HCl Fill reductant bottle with 10% Stannous Chloride	Daily Daily Daily
ICP	Check/replace pump tubing Check liquid argon supply Check fluid level in waste container Check/clean/replace filters Check torch Clean torch and nebulizer	Daily/as needed Daily Daily Daily/as needed Daily As needed
ICP MS	Check/replace pump tubing Inspect torch and injector cones Clean/replace ion lens Replace torch o-rings Check/replace gas filters Change rough pump oil Check chiller water level	Daily/as needed Daily As needed As needed As needed As needed Weekly
UV-Vis Spectrophotometer	Clean sample holder Precision check/alignment of flow cell Wavelength verification check	As required As required Semi-annually
Gas Chromatograph/Mass Spectrometer (GCMS)	Bake trap (VOC only) Clean source Check/change vacuum pump oil Clean injectors; replace liners (SVOC only) Replace column Clean cooling fan grills	Daily As needed Annually, as needed Daily As needed Semiannually

Instrument	Procedure	Frequency
Gas Chromatograph (GC)	Change septum Check gases Replace or clip column Clean injectors; replace liners Clean cooling fan grills	As needed Daily As needed As needed Semiannually
Electron Capture Detector (ECD)	Detector wipe test (Ni-63) Detector cleaning	Semi-annually Sent out, as needed
Flame Ionization Detector (FID)	Detector cleaning	As required
Flame Photoionization Detector (FPD)	Clean and/or Replace Lamp	As required
Photoionization Detector (PID)	Change O-rings Clean lamp window	As required As required
Ion Chromatograph (IC)	Replace column disks Change guard columns Check pump seals Replace tubing Replace suppressor Check fluid level in waste container Clean cooling fan grills	As required As required As required As required As required Daily Semiannually
Balances	Class "S" traceable weight check Clean pan and check if level Outside calibration service	Daily, when used Daily At least Annually
Conductivity Meter	0.01 M KCl calibration Conductivity cell cleaning	Daily As required
Turbidimeter	Check light bulb Clean sample holder	Daily, when used Daily, when used
Deionized/Distilled Water	Daily conductivity check Check deionizer light Monitor for VOA's System cleaning Replace cartridge & large mixed bed resins	Daily Daily As required As required As required
Drying Ovens	Temperature monitoring Temperature adjustments	When used As required
Refrigerators/ Freezers	Temperature monitoring Temperature adjustment Defrosting/cleaning	Daily As required As required
pH/Specific Ion Meter	Calibration/check slope Clean electrode	Daily As required
BOD Incubator	Temperature monitoring Incubator cleaning	Daily As required
Centrifuge	Check brushes and bearings	As needed
Water baths	Temperature monitoring Water replaced	Daily Monthly or as needed
Automated Solvent Extraction units (ASE)	Check solvent reservoirs Check tubing	Daily Daily

Instrument	Procedure	Frequency
TurboVaps	Check gas lines Check water level Calibrate temperature	Daily Daily Annually
Total Organic Carbon Analyzer	Check gas flow Check reagent reservoir levels Replace o-rings Check autosampler needle Replace scrubbers Replace catalyst	Daily Daily As needed Daily Annually As needed
Automated Analyzer	Clean sampler Check all tubing Clean detector Clean optics and cells	Daily Daily Daily Daily
Infrared Spectrophotometer (IR)	Clean lens/optimize	As needed
Flashpoint Apparatus	Check gas line for leaks Check stirrer speed	Daily Annually
Rotators	Verify rotation speed	Annually

Table 21-3. Periodic Calibration

Instrument	Type of Calibration/ Number of Standards	Frequency	Acceptance Limits	Corrective Action
Analytical Balance	Accuracy determined using weights calibrated against ASTM Class 1 NIST-traceable weights. Minimum of 2 standards bracketing the weight of interest. Inspected and calibrated by an accredited vendor annually.	Daily	± 3 digits at smallest (rightmost) display	Clean, check level, insure lack of drafts, and that unit is warmed up, recheck. If fails, call service.
Top Loading Balance	Accuracy determined using weights calibrated against ASTM Class 1 NIST-traceable weights. Minimum of 2 standards bracketing the weight of interest. Inspected and calibrated by an accredited vendor.	Daily	± 3 digits at smallest (rightmost) display	Clean, check level, insure lack of drafts, and that unit is warmed up, recheck. If fails, call service.
Reference ASTM Class 1 NIST-traceable Weights	Accuracy determined by accredited weights and measurement laboratory.	1 year	As per ASTM Class 1 specifications	Replace.

Instrument	Type of Calibration/ Number of Standards	Frequency	Acceptance Limits	Corrective Action
Daily laboratory weights	Verified against laboratory's ASTM Class 1 reference set	1 year	±0.1mg of expected or less than lowest weight the balance can read	Replace
NIST-Traceable Thermometer	Accuracy determined by accredited measurement laboratory.	5 years	As per certificate.	Replace.
Thermometer, glass	Against NIST-traceable thermometer	Yearly at appropriate temperature range for intended use	Correction factor of ± 2°C	Replace
Thermometer, digital	Against NIST-traceable thermometer	Quarterly at appropriate temperature range for intended use.	Correction factor of ± 2°C	Replace
InfraRed Temperature Guns	Against NIST-traceable thermometer	Quarterly at appropriate temperature range for intended use.	Correction factor of ± 2°C	Repair/replace
Refrigerator	Temperature checked using NIST-traceable thermometer.	Daily. If out of range, check again a few hours later and document	>0 to 6°C	Adjust. Repair. While waiting for repair, seal door, attach "Out of Service" sign, move items to functional unit. Notify supervisor.
Freezer	Temperature checked using NIST-traceable thermometer	range, check again a few hours later and document	-10 to -20°C	Adjust. Repair. While waiting for repair, seal door, attach "Out of Service" sign, move items to functional unit. Notify supervisor.
Oven	Temperature checked using NIST-traceable thermometer.	When in use.	104 ± 1°C (drying) 180 ± 2°C (TDS)	Adjust. Replace.
Incubator	Temperature checked using NIST-traceable thermometer.	When in use.	BOD: 20 ± 1.0°C	Adjust. Replace.
Water Bath	Temperature checked using NIST-traceable thermometer.	When in use.	± 2°C	Adjust. Replace.

Instrument	Type of Calibration/ Number of Standards	Frequency	Acceptance Limits	Corrective Action
Volumetric Dispensing Devices (Eppendorf® pipette, automatic dilutor or dispensing devices)	One delivery by weight. Using DI water, dispense into tared vessel. Record weight with device ID number.	Monthly	± 2% Calculate accuracy by dividing weight by stated volume times 100 for percent.	Adjust. Replace.
Glass Microliter Syringes	None	Accuracy must be initially demonstrated if syringe was not received with a certificate attesting to established accuracy.	± 1%	Not applicable.
Conductivity Meter	Cell impedance calibrated with two KCl standards.	Each use.	2 nd source verified within vendor-specified limits	Recalibrate.
Deionized Water	Check in-line conductivity meter on system with conductivity meter in Inorganics Department.	Weekly	<1 µmhos/cm ²	Record on log. Report discrepancies to QA Director.

Table 21-4. Preventive Maintenance Procedures For Field Equipment

Instrument/ Equipment Type	Activity	Frequency	Maintenance
Automatic Sampler – ISCO 3710/3910	Check tubing and connections through pump head	Before and after use	Replace tubing when necessary
	Check battery power and program	Before and after use	Replace battery when necessary
	Clean tubing in pump head	After each use	Replace pump head tubing when necessary
	Clean tubing for sample collection	After each use	---
	Check functionality – manual sample; program sample	Prior to use	---
	Check sample container for breakage, etc.	Prior to use	Replace if needed
YSI 3000 – Depth Meter, Temperature, and Conductivity	Check battery	Before and after use	Replace batteries when necessary
	Check cable	Before and after use	Send for repair
	Check probe	Before and after use	Send for repair
	Check LCD	Before and after use	Send for repair
Bailers – Miscellaneous sizes	Check ball valve for overall condition	Prior to use	Clean/replace accordingly

Instrument/ Equipment Type	Activity	Frequency	Maintenance
	Check rope	Before, during and after use	Retie or replace as necessary
	Clean inside and out	Before and after use	---
Residual Chlorine – HACH Kit	Check battery	Before and after use	Replace batteries when necessary
	Inspect glass cells	Before and after use	Replace as necessary
	Clean glass cells	Prior to use	---
Residual Chlorine – HACH Kit	Inspect cell holder	Before and after use	Remove obstructions, if present
	Check expiration dates of reagents	Prior to use	Remove and reorder as necessary
	Inspect ampules for cracks	Before and after use	Replace as necessary
Dissolved Oxygen – HACH Kit	Check battery	Before and after use	Replace batteries when necessary
	Inspect cell holder	Before and after use	Remove obstructions, if present
	Inspect rubber ampule cover	Before and after use	Replace as necessary

SECTION 22

MEASUREMENT TRACEABILITY (NELAC 5.5.6)

22.1 OVERVIEW

Traceability of measurements shall be assured using a system of documentation, calibration, and analysis of reference standards. Laboratory equipment that are peripheral to analysis and whose calibration is not necessarily documented in a test method analysis or by analysis of a reference standard shall be subject to ongoing certifications of accuracy. At a minimum, these must include procedures for checking specifications of ancillary equipment: balances, thermometers, temperature, Deionized (DI) and Reverse Osmosis (RO) water systems, automatic pipettes and other volumetric measuring devices. With the exception of Class A Glassware (including glass microliter syringes that have a certificate of accuracy), quarterly accuracy checks are performed for all mechanical volumetric devices. Wherever possible, subsidiary or peripheral equipment is checked against standard equipment or standards that are traceable to national or international standards. The following definitions are provided by the American Association for Laboratory Accreditation (A2LA):

“Traceability is the property of a measurement result whereby it can be related to stated references, usually national or international standards, through an unbroken chain of comparisons, each step in the chain having stated uncertainties.” There are six essential elements:

- An unbroken chain of comparison
- A calculated measurement uncertainty for each step in the chain to allow for an overall uncertainty calculation
- Documentation of each step in each calibration report
- All steps in the chain are performed by individuals with evidence of technical competence and accredited by a recognized accreditation body
- Reference to International Standard (SI) units
- Recalibration at appropriate intervals to preserve traceability

Calibration is defined as “determining and documenting the deviation of the indication of a measuring instrument (or the stated value of a material measure) from the conventional ‘true’ value of the measurand.”

Uncertainty is defined as “a parameter associated with the result of a measurement that characterizes the dispersion of the value that could reasonably be attributed to the measurand.” Measurement of Uncertainty is discussed in Section 20 of this QA Manual.

22.2 NIST-TRACEABLE WEIGHTS AND THERMOMETERS

Reference standards of measurement shall be used for calibration only and for no other purpose, unless it can be shown that their performance as reference standards would not be invalidated.

For NIST-traceable weights and thermometers, the laboratory requires that all calibrations be conducted by a calibration laboratory accredited by A2LA, NVLAP (National Voluntary Laboratory Accreditation Program), APLAC (Asia-Pacific Laboratory Accreditation Cooperation), or EA (European Cooperation for Accreditation). A certificate and scope of accreditation is kept on file at the laboratory. Refer to Section 21 for calibration of weights and thermometers.

22.3 REFERENCE STANDARDS / MATERIALS

Reference standards/materials, where commercially available, are traceable to certified reference materials. Commercially prepared standard materials are purchased from vendors accredited by A2LA, NVLAP, with an accompanying Certificate of Analysis that documents the standard purity. If a standard cannot be purchased from a vendor that supplies a Certificate of Analysis, the purity of the standard is documented by analysis. (Refer to Section 9 for additional information on purchasing). The receipt of all reference standards must be documented. Reference standards are labeled with a unique [Standard Identification Number](#) and expiration date. All documentation received with the reference standard is retained as a QC record and references the [Standard Identification Number](#).

All reference, primary and working standards/materials, whether commercially purchased or laboratory prepared, must be checked regularly to ensure that the variability of the standard or material from the 'true' value does not exceed method requirements. The accuracy of calibration standards is checked by comparison with a standard from a second source. In cases where a second standard manufacturer is not available, a vendor certified different lot is acceptable for use as a second source. [For unique situations, such as air analysis where no other source or lot is available, a standard made by a different analyst would be considered a second source.](#) The appropriate Quality Control (QC) criteria for specific standards are defined in laboratory SOPs. In most cases, the analysis of an Initial Calibration Verification (ICV) or LCS (where there is no sample preparation) is used as the second source confirmation. These checks are generally performed as an integral part of the analysis method (e.g. calibration checks, laboratory control samples).

All standards and materials must be stored and handled according to method or manufacturer's requirements in order to prevent contamination or deterioration. Refer to Table 9-1 in Section 9 for general storage requirements and Table 22-1 for additional storage information. [Please refer to method SOPs "Standards and Reagents" section for additional details.](#) For safety requirements, please refer to method SOPs and the laboratory Environmental Health and Safety Manual.

22.4 DOCUMENTATION AND LABELING OF STANDARDS, REAGENTS, AND REFERENCE MATERIALS

Reagents must be at a minimum the purity required in the test method. The date of reagent receipt and the expiration date are documented. [The lots for most of the common solvents and](#)

acids are tested for acceptability prior to company wide purchase. Refer to SOP No. CA-Q-S-001, Solvent and Acid Lot Testing and Approval.

All manufacturer or vendor supplied Certificate of Analysis or Purity must be retained, stored appropriately, and readily available for use and inspection. These records are maintained by each laboratory department. Records must be kept of the date of receipt and date of expiration of standards, reagents and reference materials. In addition, records of preparation of laboratory standards, reagents, and reference materials must be retained, stored appropriately, and be readily available for use and inspection. For detailed information on documentation and labeling, please refer to the laboratory's SOP IR-QA-STD (Reagent and Standard Preparation, Control, and Documentation) as well as method specific SOPs.

Commercial materials purchased for preparation of calibration solutions, spike solutions, etc., are usually accompanied with an assay certificate or the purity is noted on the label. If the assay purity is 96% or better, the weight provided by the vendor may be used without correction. If the assay purity is less than 96% a correction will be made to concentrations applied to solutions prepared from the stock commercial material.

22.4.1 All standards, reagents, and reference materials must be labeled in an unambiguous manner. Standards are logged into the laboratory's LIMS system, and are assigned a unique identification number. The following information is typically recorded in the electronic database within the LIMS:

- Standard ID
- Description of Standard
- Department
- Preparer's name
- Final volume and number of vials prepared
- Solvent type and lot number
- Preparation Date
- Expiration Date
- Standard source type (stock or daughter)
- Standard type (spike, surrogate, other)
- Parent standard ID (if applicable)
- Parent Standard Analyte Concentration (if applicable)
- Parent Standard Amount used (if applicable)
- Component Analytes
- Final concentration of each analyte
- Comment box (text field)

Records are maintained electronically (with the exception of metals working standards which are prepared daily and documented in a controlled logbook) for standard and reference material

preparation. These records show the traceability to purchased stocks or neat compounds. These records also include method of preparation, date of preparation, expiration date and preparer's name or initials. Preparation procedures are provided in the Method SOPs.

22.4.2 All standards, reagents, and reference materials must be clearly labeled with a minimum of the following information:

- Expiration Date
- Standard ID Code (from LIMS or logbook)
- Special Health/Safety warnings if applicable

22.4.3 In addition, the following information may be helpful:

- Date of receipt for commercially purchased items or date of preparation for laboratory prepared items
- Date opened (for multi-use containers, if applicable)
- Description of standard (if different from manufacturer's label or if standard was prepared in the laboratory)
- Concentration (if applicable)
- Initials of analyst preparing standard or opening container

All containers of prepared reagents must include a preparation date, expiration date and an ID number to trace back to preparation.

Procedures for preparation of reagents can be found in the Method SOPs.

Standard ID numbers must be traceable through associated logbooks, worksheets and raw data.

All reagents and standards must be stored in accordance to the following priority: 1) with the manufacturer's recommendations; 2) with requirements in the specific analytical methods; and 3) according to Table 22-1.

Table 22-1.
Standard Sources and Preparation

Method Group	Source*	How Received	Stock Storage	Preparation	Intermediate & Working Standard Storage	Frequency
Metals	SPEX; Environmental Express	1000 ppm Solutions	Room Temperature	Working standards from stock	Room Temperature	Daily
Wet Chemistry	Ricca; Spectrum:ERA	Solutions	Refrigerate	As received	Refrigerate	Various
Volatile Organics	Absolute; Restek	Ampoule/ Solutions	Freezer (-10°C)	Working standards from stock	Refrigerate	Monthly; Gas, weekly
Semi-Volatile Organics	Absolute; Restek	Ampoule/ Solutions	Refrigerate or Room temp.	Working standards from stock	Refrigerate	Monthly
Infrared Spec- trophotometry	Aldrich; Sigma	Pure Reagent	Room Temperature	Working standards from stock	Refrigerate	Six months

*Or equivalent

SECTION 23.0

SAMPLING (NELAC 5.5.7)

23.1 OVERVIEW

TestAmerica Irvine provides sampling services. Sampling procedures are described in the SOP FIELD.SOP (Field Sampling).

23.2 SAMPLING CONTAINERS

The laboratory offers clean sampling containers for use by clients. These containers are obtained from reputable container manufacturers and meet EPA specifications as required. Any certificates of cleanliness that are provided by the supplier are maintained at the laboratory. Additionally, TestAmerica Irvine lot tests all 40-milliliter VOA vials for volatile organics by GCMS and all polyethylene bottles for common anions and trace-level metals.

23.2.1 Preservatives

Upon request, preservatives are provided to the client in pre-cleaned sampling containers. In some cases containers may be purchased pre-preserved from the container supplier. Whether prepared by the laboratory or bought pre-preserved, the grades of the preservatives are at a minimum:

- Hydrochloric Acid – Reagent ACS (Certified VOA Free) or equivalent
- Methanol – Purge and Trap grade
- Nitric Acid – Intra-Analyzed or equivalent
- Sodium Bisulfate – ACS Grade or equivalent
- Sodium Hydroxide – Intra-Analyzed or equivalent
- Sulfuric Acid – Intra-Analyzed or equivalent
- Sodium Thiosulfate – ACS Grade or equivalent

23.2.2 Preparing Container Orders

When new containers arrive at the laboratory, the lot numbers for VOA vials are checked against the list of laboratory-approved lots. For polyethylene bottles, the date of receipt is recorded on the box(es) and randomly selected bottles of each unpreserved size and each nitric-preserved size are submitted for metals and anion analysis. Upon request, the containers are then sent to clients for use in collecting samples. The shipping date, type and number of containers are maintained on file by the lab. Shipping personnel insure that container stock is rotated so that “first in” is “first out.” When a client requests containers, a client services representative creates a container request in LIMS; it is then stored permanently in LIMS with a unique container order number. Copies of the container request are printed for the shipping department. One copy goes to the client with the containers; one copy is filed in the shipping department. See the laboratory’s SOP LOGIN.SOP (Sample Control) and LOTTEST.SOP (Container and Reagent Verification by Lot Testing) for more details.

The laboratory also provides EnCore, TerraCore or other soil sampling devices when requested.

If containers are provided directly to the client from the manufacturer or from other sources, the laboratory will not be responsible for any of the above records.

23.3 FIELD QUALITY CONTROL (QC)

Common field quality control samples are defined in the following paragraphs. The frequency of field quality control samples should be specified in the site specific Quality Assurance Project Plan (QAPP) or by the client. TestAmerica provides trip blanks for VOC analysis with the sample containers for all volatile organic analyses. Blanks generated in the field will be analyzed along with the field samples (exception soil samples where the blank is aqueous).

23.3.1 Equipment Blank / Rinsate Blank - The equipment blank, sometimes referred to as a rinsate blank, is a sample of the water used to decontaminate sampling equipment. The source water should be as free of target analytes as possible. An aliquot of this water is poured over or through the sample collection device after decontamination, collected in a sample container, preserved with appropriate reagents, and returned to the laboratory. This serves as a check on sampling device cleanliness, and will also be affected by the site and sample handling conditions evaluated by the other types of blanks. The sampling time for the equipment blank should begin when the equipment is rinsed and the water is collected.

23.3.2 Field Blank - The field blank is water that is as free of target analytes as possible and from the same source as the equipment blank. The water is poured into a sampling container at the sampling site, preserved with the appropriate reagents, and returned to the laboratory. This serves as a check on reagent and environmental contamination. The sampling time for the field blank should be when the blank is prepared in the field.

23.3.3 Trip Blank - The trip blank pertains to volatile analysis only. This serves as a check on sample contamination originating from sample transport, sample container contamination, shipping and storage, or from certain site conditions. Trip blanks are often referred to as travel blanks. They are prepared using pre-cleaned sample containers. They are filled with organic-free water (the source of the organic free water is the same source of water used to prepare volatile standards, method blanks, LCS and sample dilutions), sealed and taken into the field with the empty containers which will be used for sampling. The recommended frequency is one trip blank per cooler (in duplicate or triplicate), per volatiles method. Unless otherwise specified, the sampling time for the trip blank is the time of receipt at the laboratory (When the "Trip" ends).

23.3.4 Field Duplicates - Field duplicates are replicate samples collected from the same sampling point or location during a field collection event. This control sample is used to demonstrate the ability of both the sampling and analytical process to generate data of acceptable precision.

23.4 DEFINITION OF HOLDING TIME

The date and time of sampling documented on the chain-of-custody (COC) form establishes the day and time zero. As a general rule, when the maximum allowable holding time is expressed in "days" (e.g 14 days, 28 days), the holding time is based on calendar day measured. Holding

times expressed in "hours" (e.g. 6 hours, 24 hours, etc.) are measured from date and time zero. The first day of holding time ends twenty-four hours after sampling. Holding times for analysis include any necessary reanalysis.

23.4.1 Semi-Volatile - Holding times for sample preparation for semi-volatile organics are measured from the sampling date until the day solvent contacts the sample. Holding times for analysis are measured from the date of initiation of extraction to the time of injection into the gas chromatograph.

23.4.2 Volatiles - Holding times for volatile organics are measured from the date (and time where applicable) of sampling to the date and time of injection into the gas chromatograph. The time of initiation of purging is considered the injection time, but data systems record the start of the chromatographic run rather than the start of purging. Hence, if a sample is so near expiration that the start-of-purging time rather than the chromatographic run time is needed to document the integrity of the sample; the analyst must observe and record the start-of-purging time in the instrument log. Extractions, e.g. for high level soils, must be completed in time to allow for analysis to be initiated within the maximum allowable holding time.

23.4.3 Inorganics - For inorganic and metals analysis, the preparation/digestion/distillation must be started within the maximum holding time as measured from the sampling date (and time where applicable).

23.5 SAMPLING CONTAINERS, PRESERVATION REQUIREMENTS, HOLDING TIMES

The preservation and holding time criteria specified in the following tables are derived from the source documents for the methods. If method required holding times (refer to Tables 23-1 to 23-7) or preservation requirements are not met, the reports will be qualified using a flag, footnote or case narrative. As soon as possible or "ASAP" is an EPA designation for tests for which rapid analysis is advised, but for which neither EPA nor the laboratory have a basis for a holding time.

23.6 SAMPLE ALIQUOTS / SUBSAMPLING

Taking a representative sub-sample from a container is necessary to ensure that the analytical results are representative of the sample collected in the field. The size of the sample container, the quantity of sample fitted within the container, and the homogeneity of the sample need consideration when sub-sampling for sample preparation. It is the laboratory's responsibility to take a representative subsample or aliquot of the sample provided for analysis. In that regard the following guidelines apply to analysts:

Analysts should handle each sample as if it is potentially dangerous. At a minimum, safety glasses, gloves, and lab coats must be worn when preparing aliquots for analysis.

23.6.1 For water samples, before taking each aliquot for analysis, invert the sample container end-over-end three times and immediately pour off the aliquot. Especially when suspended solids are present, adequate mixing of the sample is extremely important.

23.6.2 For solid samples, when volatile organics are not requested, if the solid can be mixed, stir before removing the aliquot. Mix more than is needed for the analysis to be performed (e.g. if 30 g are needed, mix 50-100 g, if 1 g is needed, mix 20 g, etc...).

- If the solid cannot be easily mixed: After thoroughly mixing the sample within the sample container or, for non-organic methods, the sample can be transferred to a wip bag (or other suitable plastic bag) for manual mixing, a sub-sample from various quadrants and depths of the sample are taken to acquire the required sample weight.
- For soil samples, avoid debris in the subsample aliquot as much as possible (e.g. gravel, sticks, roots and grass); note this information in the sample preparation record.
- If the solid is extremely heterogeneous, and the client has given no instructions, utilize the following technique: separate the like materials into groups on a clean surface and take portions of masses from each group, proportional to their contribution to the original sample, to make a composite. Record in detail exactly how the composite was created. For very unusual samples, consult with the QA department or Department Manager.

NOTE: Subsampling is addressed in greater detail in SUBSAMP.SOP (Subsampling).

23.6.3 For solid samples, when volatile organics analysis is requested, the sample should be manipulated as little as possible. In most cases, the sample will arrive already preserved or in an EnCore™ sampler of the correct mass (requiring quick preservation of the entire amount). If the client requests volatiles on a solid sample which has been collected in a jar and is in a common container from which aliquots for other test methods must be taken, login should deliver the container to the volatiles department for preparing a proper aliquot prior to any other aliquots being taken out.

23.6.4 For multiphasic samples, the client should instruct the laboratory as to the intent of the testing and how to handle the sample. If the entire sample is to be accounted for, and the phases do not mix easily with inversion/stirring, such that a representative aliquot can be taken, the analyst should record the percent by volume of each phase. The analysis must be conducted on each phase separately; the final results are combined mathematically, weighting the individual phase results by volume. One exception to this procedure is the situation addressed in the TCLP and SPLP methods for wastes containing free liquids. However, if the leachate and final filtrate are not miscible, it is necessary to combine mathematically the concentrations of the two (or more) solutions by volume.

Tables 23-1 to 23-7 detail holding times, preservation and container requirements, and sample volumes for SDWA and NPDES methods. **Please note:** *the holding times are program specific and different programs may have different holding times for equivalent methods (e.g., there are difference in Holding times for many Organic analytes between SDWA and NPDES. RCRA methods may also be different.)*

**Table 23-1.
Holding Times, Preservation and Container Requirements: Drinking Water (SDWA)**

PARAMETER	CONTAINER	PRESERVATION ^{1,2}		HOLDING TIME ³	SAMPLE VOLUME
		Temp. ²³	Chemical		
Asbestos	Plastic/Glass	4°C	None	48 hours ⁵	1 L
Coliforms (Total and Fecal)	Plastic/Glass ²⁰	10°C	Na ₂ S ₂ O ₃	30 hours ²¹	120 mL
Cyanide	Plastic/Glass	4°C	NaOH to pH >12	14 days	500 mL
Fluoride	Plastic/Glass	None	None	None	250 mL
Heterotrophic Plate Count	Plastic/Glass ²⁰	10°C	Na ₂ S ₂ O ₃	8 hours (24 hours ²²)	120 mL
Mercury	Plastic/Glass	None	HNO ₃ to pH<2	28 days	250 mL
Metals ⁴	Plastic/Glass	None	HNO ₃ to pH<2	6 months	250 mL
Nitrate	Plastic/Glass	4°C	None	48 hours ⁶	250 mL
Nitrate-Nitrite	Plastic/Glass	None	H ₂ SO ₄ to pH<2	28 days	250 mL
Nitrite	Plastic/Glass	4°C	None	48 hours	250 mL
THMs Only	Glass ⁸	4°C	Na ₂ S ₂ O ₃	14 days	3 X 40 mL
Volatile Organic Compounds	Glass ⁸	4°C	HCl to pH <2 Na ₂ S ₂ O ₃ or Ascorbic acid ⁹	14 days	3 X 40 mL
EDB, DBCP, 1,2,3-TCP (EPA 504.1)	Glass ⁸	4°C	Na ₂ S ₂ O ₃	14 days	3 X 40 mL
Organochlorine Pesticides/PCBs (EPA 505) ¹⁰	Glass ⁸	4°C	Na ₂ S ₂ O ₃	14 days ¹¹	3 X 40 mL
Nitrogen and Phos. Pesticides (EPA 507)	Glass-Amber ⁸	4°C	Na ₂ S ₂ O ₃	14 days ¹²	1 L
Total PCBs (EPA 508A)	Glass-Amber ⁸	4°C	None	14 days ¹³	1 L
Pesticides and PCBs (EPA 508.1) ¹⁴	Glass-Amber ⁸	4°C	HCl to pH <2 Na ₂ S ₂ O ₃ ⁹	14 days ¹³	1 L
Chlorinated Acids (EPA 515.1)	Glass-Amber ⁸	4°C	Na ₂ S ₂ O ₃	14 days ¹²	1 L
Semivolatiles (EPA 525.2)	Glass-Amber ⁸	4°C	HCl to pH <2 Na ₂ S ₂ O ₃ ⁹	14 days ¹³	1 L

PARAMETER	CONTAINER	PRESERVATION ^{1,2}		HOLDING TIME ³	SAMPLE VOLUME
		Temp. ²³	Chemical		
N-Methylcarbamoyloxamines and N-Methcarbamates (EPA 531.1)	Glass ⁸	4°C	Na ₂ S ₂ O ₃ , Monochloroacetic Acid buffer to pH<3	28 days	3 X 60 mL
Glyphosate (EPA 547)	Glass ⁸	4°C	Na ₂ S ₂ O ₃	14 days	3 X 60 mL
Endothall (EPA 548)	Na ₂ S ₂ O ₃	4°C	None	7 days ¹⁵	1 L
Diquat/Parquat (EPA 549.1)	Glass-Amber ⁸ (Silanized or PVC amber)	4°C	H ₂ SO ₄ to PH <2 Na ₂ S ₂ O ₃ ⁹	7 days ¹⁶	1 L
Chlorinated Disinfection Byproducts, Chlorinated Solvents, and Halogenated Pesticides/Herbicides (EPA 551)	Glass ⁸	4°C	Phosphate Buffer and Ammonium Chloride ¹⁹	14 days ¹⁷	3 X 60 mL
Haloacetic Acids (EPA 552.1)	Glass-Amber ⁸	4°C	Ammonium Chloride	28 days ¹⁸	250 mL

Key to Table

1. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at 4°C until compositing and sample splitting is completed.
2. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Hydrochloric acid, (HCl) in water, solutions at concentrations of 0.04% by weight or less (pH about 1.96 or greater); Nitric acid (HNO₃) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater); Sulfuric acid (H₂SO₄) in water solutions at concentrations of 0.35% by weight or less pH about 1.15 or greater; and Sodium hydroxide (NaOH) in water solutions at concentrations of 0.080% by weight or less (pH about 12.30 or less).
3. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
4. All metals except Hg.
5. Instructions for containers, preservation procedures and holding times as specified in Method 100.2 must be adhered to for all compliance analysis including those conducted with Method 100.1.
6. If the sample is chlorinated, the holding time for an un-acidified sample kept at 4°C is extended to 14 days.
7. Nitrate-Nitrite refers to a measurement of total nitrite.
8. With Teflon lined septum.
9. If chlorinated add Na₂S₂O₃ prior to acidification.
10. Heptaclor has a 7 day hold time
11. 14 days until extraction. 24 hours after extraction.
12. 14 days until extraction. 28 days after extraction.
13. 14 days until extraction. 30 days after extraction.
14. For cyanazine, cool to 4°C only.

Key to Table

15. 7 days until derivitation. 1 day after derivatation.
16. 7 days until extraction. 21 days after extraction.
17. 14 days until extraction. 14 days after extraction.
18. 28 days until extraction. 48 hours after extraction.
19. Sodium Sulfite may be used as a dechlorinating agent in some instances. Verify with laboratory prior to sampling.
20. Sterilized. Plastic must be Polypropylene.
21. 40 CFR part 141.74 regulations to avoid filtration or disinfection state 8 hours (DW compliance testing).
Most facilities are using either disinfection or filtration so the 8 would not apply in most cases.
22. 40 CFR part 141.74 regulations for Disinfection By-Product rule state 8 hours (DW compliance testing)
where SM 9215 allows up to 24 hours if sample is stored between > 0 and $\leq 4^{\circ}$ C
23. For samples with a temperature requirement of 4° C, a sample temperature of just above the water freezing temperature to $\leq 6^{\circ}$ C is acceptable.

Table 23-2
Holding Times, Preservation and Container Requirements: NPDES – Bacteria, Protozoa, Toxicity Tests

PARAMETER	CONTAINER ¹	PRESERVATION ^{2,3}		HOLDING TIME ⁴	SAMPLE VOLUME
		Temp.	Chemical		
Total, Fecal, and E.coli Coliforms	Plastic/Glass	10°C	0.0008 % Na ₂ S ₂ O ₃ ⁵	6 hours	100 mL
Fecal Streptococci	Plastic/Glass	10°C	0.0008 % Na ₂ S ₂ O ₃ ⁵	6 hours	100 mL
Enterococci	Plastic/Glass	10°C	0.0008 % Na ₂ S ₂ O ₃ ⁵	6 hours	100 mL
Cryptosporidium	LPDE Plastic	0-8°C	None	96 Hours	500 mL
Giardia	LPDE Plastic	0-8°C	None	96 Hours	500 mL
Toxicity – Acute/Chronic	Plastic/Glass	≤ 6°C ⁵	None	36 Hours	2 L

Key to Table

1. Plastic should be Polypropylene or other sterilizable plastic.
2. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at 4°C until compositing and sample splitting is completed.
3. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Hydrochloric acid, (HCl) in water, solutions at concentrations of 0.04% by weight or less (pH about 1.96 or greater); Nitric acid (HNO₃) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater); Sulfuric acid (H₂SO₄) in water solutions at concentrations of 0.35% by weight or less pH about 1.15 or greater); and Sodium hydroxide (NaOH) in water solutions at concentrations of 0.080% by weight or less (pH about 12.30 or less).
4. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
5. Samples must not be frozen. Sufficient ice should be placed with the samples in the shipping container to ensure that ice is still present when the samples arrive at the laboratory. However, even if ice is present, when samples arrive, it is necessary to measure the temperature of the samples and confirm that the ≤ 6°C temperature has not been exceeded.
6. Should only be used in the presence of residual chlorine.

Table 23-3
Holding Times, Preservation and Container Requirements: NPDES - Inorganic

PARAMETER	CONTAINER ¹	PRESERVATION ^{2,3}		HOLDING TIME ⁴	SAMPLE VOLUME
		Temp ¹⁴	Chemical		
Acidity	Plastic/Glass	≤ 6°C	None	14 days	100 mL
Alkalinity	Plastic/Glass	≤ 6°C	None	14 days	100 mL
Ammonia	Plastic/Glass	≤ 6°C	H ₂ SO ₄ to pH<2	28 days	400 mL
BOD 5 Day	Plastic/Glass	≤ 6°C	None	48 hours	1000 mL
Boron	Plastic ⁵	None	HNO ₃ to pH<2	6 months	200 mL
Bromide	Plastic/Glass	None	None	28 days	100 mL
CBOD 5 Day	Plastic/Glass	≤ 6°C	None	48 hours	1000 mL
COD	Plastic/Glass	≤ 6°C	H ₂ SO ₄ to pH<2	28 days	100 mL
Chloride	Plastic/Glass	None	None	28 days	50 mL
Chlorine, Residual	Plastic/Glass	None	None	15 min. ⁶	200 mL
Color	Plastic/Glass	≤ 6°C	None	48 hours	50 mL
Cyanide -Total	Plastic/Glass	≤ 6°C	NaOH to pH >12, 0.6 g ascorbic Acid ⁷	14 days	100 mL
Cyanide -Amenable	Plastic/Glass	≤ 6°C	NaOH to pH >12, 0.6 g ascorbic Acid ⁷	14 days	100 mL
Fluoride	Plastic	None	None	28 days	300 mL
Hardness	Plastic/Glass	None	HNO ₃ to pH<2 ⁸	6 months	100 mL
Hexavalent, Chromium	Plastic/Glass	≤ 6°C	Ammonium sulfate buffer pH = 9.3 - 9.7	28 dys / 24 hrs ¹⁵	200 mL
Hydrogen Ion (pH)	Plastic/Glass	None	None	15 min. ⁶	200 mL
Kjeldahl and organic Nitrogen	Plastic/Glass	≤ 6°C	H ₂ SO ₄ to pH <2	28 days	500 mL
Mercury ¹¹	Plastic/Glass	None	HNO ₃ to pH<2	28 days	200 mL
Metals ^{9,10}	Plastic/Glass	None	HNO ₃ to pH<2	6 months	200 mL
Nitrate	Plastic/Glass	≤ 6°C	None	48 hours	100 mL
Nitrate-Nitrite	Plastic/Glass	≤ 6°C	H ₂ SO ₄ to pH <2	28 days	100 mL
Nitrite	Plastic/Glass	≤ 6°C	None	48 hours	100 mL
Oil and Grease	Glass	≤ 6°C	H ₂ SO ₄ or HCl to pH <2	28 days	1 L

PARAMETER	CONTAINER ¹	PRESERVATION ^{2,3}		HOLDING TIME ⁴	SAMPLE VOLUME
		Temp ¹⁴	Chemical		
Organic Carbon (TOC)	Plastic/Glass	≤ 6°C	H ₂ SO ₄ or HCl to pH <2 ¹²	28 days	250 mL
Orthophosphate	Plastic/Glass	≤ 6°C	Filter within 15 min.	48 hours	250 mL
Oxygen, Dissolved Probe	Glass ¹³	None	None	15 min. ⁶	200 mL
Oxygen, Winkler	Glass ¹³	None	Fix on site and store in dark.	8 hours	300 mL
Phenols	Glass	≤ 6°C	H ₂ SO ₄ to pH <2	28 days	500 mL
Phosphorus, Elemental	Glass	≤ 6°C	None	48 hours	250 mL
Phosphorus, Total	Plastic/Glass	≤ 6°C	H ₂ SO ₄ to pH <2	28 days	250 mL
Residue, Total	Plastic/Glass	≤ 6°C	None	7 days	1 L
Residue, Filterable	Plastic/Glass	≤ 6°C	None	7 days	1 L
Residue, Non-Filterable	Plastic/Glass	≤ 6°C	None	7 days	1 L
Residue, Settleable	Plastic/Glass	≤ 6°C	None	48 hours	1 L
Residue, Volatile	Plastic/Glass	≤ 6°C	None	7 days	1 L
Silica	Plastic ⁵	≤ 6°C	None	28 days	250 mL
Specific Conductance	Plastic/Glass	≤ 6°C	None	28 days	250 mL
Sulfate	Plastic/Glass	≤ 6°C	None	28 days	250 mL
Sulfide	Plastic/Glass	≤ 6°C	Zinc acetate plus NaOH to pH>9	7 days	500 mL
Sulfite	Plastic/Glass	None	None	15 min. ⁶	200 mL
Surfactants	Plastic/Glass	≤ 6°C	None	48 hours	1 L
Temperature	Plastic/Glass	None	None	N/A	100 mL
Turbidity	Plastic/Glass	≤ 6°C	None	48 hours	1 L

Key to Table

1. Plastic should be Polyethylene.
2. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at ≤ 6°C until compositing and sample splitting is completed.

Key to Table

3. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Hydrochloric acid, (HCl) in water, solutions at concentrations of 0.04% by weight or less (pH about 1.96 or greater); Nitric acid (HNO₃) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater); Sulfuric acid (H₂SO₄) in water solutions at concentrations of 0.35% by weight or less (pH about 1.15 or greater); and Sodium hydroxide (NaOH) in water solutions at concentrations of 0.080% by weight or less (pH about 12.30 or less).
4. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
5. May also be collected in quartz or PTFE Plastic.
6. For compliance testing, the analysis must be performed in the field at the time of analysis. If transported to the laboratory for analysis, the analysis will be performed as soon as practical and reported qualified.
7. Should only be used in the presence of residual chlorine.
8. H₂SO₄ to a pH <2 is also acceptable.
9. Except Mercury and Hexavalent Chromium.
10. Samples should be filtered on site before adding HNO₃ preservative for dissolved metals.
11. Samples collected for determination of trace level mercury (100 ng/L) using EPA 1631 must be collected in tightly capped fluoropolymer or glad bottles and preserved with BrCl or HCl solution within 48 hours of sample collection. The time to preservation may be extended to 28 days if a sample is oxidized in the sample bottle. Samples collected for dissolved trace level mercury should be filtered in the laboratory. However, if circumstances prevent overnight shipping, samples should be filtered in a designated clean area in the field in accordance with procedures given in Method 1669. Samples that been collected for determination of total or dissolved trace level mercury must be analyzed within 90 days of sample collection.
12. Phosphoric acid (H₃PO₄) may also be used.
13. Should have glass lid or top.
14. Aqueous samples must be preserved at ≤6 °C unless otherwise indicated, and should not be frozen unless data demonstrating that sample freezing does not adversely impact sample integrity is maintained on file and accepted as valid by the regulatory authority. Also, for purposes of NPDES monitoring, the specification of "≤ °C" is used in place of the "4 °C" and "<4 °C" sample temperature requirements listed in some methods. It is not necessary to measure the sample temperature to three significant figures (1/100th of 1 degree); rather, three significant figures are specified so that rounding down to 6 °C may not be used to meet the ≤6 °C requirement. The preservation temperature does not apply to samples that are analyzed immediately (less than 15 minutes).
15. Holding time is 24 hours if pH adjustment is not performed.

Table 23-4
Holding Times, Preservation and Container Requirements: NPDES - Organic

PARAMETER	CONTAINER	PRESERVATION ^{1,2}		HOLDING TIME ³	SAMPLE VOLUME
		Temp. ¹⁵	Chemical		
Purgeable Halocarbons	Glass ⁴	≤ 6°C	0.0008 % Na ₂ S ₂ O ₃ ⁵	14 days	40 mL
Purgeable Aromatic Hydrocarbons	Glass ⁴	≤ 6°C	0.0008 % Na ₂ S ₂ O ₃ ⁵ , HCl to pH<2	14 days ⁶	40 mL
Acrolein and Acrylonitrile	Glass ⁴	≤ 6°C	0.0008 % Na ₂ S ₂ O ₃ ⁵ , adjust pH to 4-5 ⁷	14 days	40 mL
Phenols ⁹	Glass ⁴	≤ 6°C	0.0008 % Na ₂ S ₂ O ₃ ⁵	7 days ⁸	1 L
Benzidines ⁹	Glass ⁴	≤ 6°C	0.0008 % Na ₂ S ₂ O ₃ ⁵	7 days ^{8, 11}	1 L
Phthalate esters ⁹	Glass ⁴	≤ 6°C	None	7 days ⁸	1 L
Nitosamines ^{9,12}	Glass ⁴	≤ 6°C	0.0008 % Na ₂ S ₂ O ₃ ^{5,13}	7 days ⁸	1 L
PCBs ⁹	Glass ⁴	≤ 6°C	None	1 year ⁸	1 L
Nitroaromatics and Isophorone ⁹	Glass ⁴	≤ 6°C	0.0008 % Na ₂ S ₂ O ₃ ^{5,13}	7 days ⁸	1 L
Polynuclear Aromatic Hydrocarbons ⁹	Glass ⁴	≤ 6°C	0.0008 % Na ₂ S ₂ O ₃ ^{5,13}	7 days ⁸	1 L
Haloethers ⁹	Glass ⁴	≤ 6°C	0.0008 % Na ₂ S ₂ O ₃ ⁵	7 days ⁸	1 L
Chlorinated Hydrocarbons ⁹	Glass ⁴	≤ 6°C	None	7 days ⁸	1 L
CDD/CDFs ⁹ – Aqueous: Field/Lab Preservation	Glass	≤ 6°C	pH <9, 0.0008 % Na ₂ S ₂ O ₃ ⁵	1 year	1 L
CDD/CDFs ⁹ – Solids/Mixed Phase/ - Field Preservation	Glass	≤ 6°C	None	7 days	1 L
CDD/CDFs ⁹ – Tissue – Field Preservation	Glass	≤ 6°C	None	24 hours	
CDD/CDFs ⁹ – Solids/Mixed Phase/Tissue - Lab Preservation	Glass	< -10°C	None	1 year	1 L
Pesticides ⁹	Glass	≤ 6°C	pH 5-9 ¹⁴	7 days ⁸	1 L

Key to Table

1. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at $\leq 6^{\circ}\text{C}$ until compositing and sample splitting is completed.
2. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Hydrochloric acid, (HCl) in water, solutions at concentrations of 0.04% by weight or less (pH about 1.96 or greater); Nitric acid (HNO_3) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater); Sulfuric acid (H_2SO_4) in water solutions at concentrations of 0.35% by weight or less pH about 1.15 or greater); and Sodium hydroxide (NaOH) in water solutions at concentrations of 0.080% by weight or less (pH about 12.30 or less).
3. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
4. With Teflon lined septum.
5. Should only be used in the presence of residual chlorine.
6. Samples receiving no pH adjustments must be analyzed within 7 days. If 2-chlorovinylethylether is a target analyte, the sample should not be acidified.
7. The pH adjustment is not required if acrolein is not being measured. Samples for acrolein receiving no pH adjustment must be analyze within three days of sampling.
8. 7 days until extraction, 40 days after extraction. (PCB only – 1 year after extraction)
9. When the extractable analytes of concern fall within a single chemical category, the specified preservative and maximum holding times should be observed for optimum safeguard of sample integrity. When the analytes of concern fall within two or more categories, the sample may be preserved by cooling to $\leq 6^{\circ}\text{C}$ reducing residual chlorine with 0.0008 % sodium thiosulfate, storing in the dark, and adjusting the pH to 6-9. Samples preserved in this manner may be held for 7 days before extraction and for 40 days after extraction. Exceptions to this optional preservation and holding time procedure are noted in footnote 5 (re the requirement for thiosulfate reduction of residual chlorine) and footnotes 10 and 11(re the analysis of Benzidine).
10. If 1,2-diphenylhydrazine is likely to be present, adjust pH to of the sample to 4.0 ± 0.2 to prevent rearrangement to benzidine.
11. Extracts may be stored up to 30 days before analysis if storage temperature is $< 0^{\circ}\text{C}$.
12. For the analysis of diphenylnitrosamine, add 0.008 % $\text{Na}_2\text{S}_2\text{O}_3$ and ajust pH to 7-10 with NaOH within 24 hours of sampling.
13. Store in dark.
14. The pH adjustment may be performed upon receipt in the laboratory and may be omitted if the samples are extracted within 72 hours of collection. For the analysis of aldrin , add 0.0008 % $\text{Na}_2\text{S}_2\text{O}_3$.
15. Aqueous samples must be preserved at $\leq 6^{\circ}\text{C}$ unless otherwise indicated, and should not be frozen unless data demonstrating that sample freezing does not adversely impact sample integrity is maintained on file and accepted as valid by the regulatory authority. Also, for purposes of NPDES monitoring, the specification of " $\leq^{\circ}\text{C}$ " is used in place of the " 4°C " and " $<4^{\circ}\text{C}$ " sample temperature requirements listed in some methods. It is not necessary to measure the sample temperature to three significant figures (1/100th of 1 degree); rather, three significant figures are specified so that rounding down to 6°C may not be used to meet the $\leq 6^{\circ}\text{C}$ requirement. The preservation temperature does not apply to samples that are analyzed immediately (less than 15 minutes).

**Table 23-5.
 Holding Times, Preservation and Container Requirements: NPDES - Radiological**

PARAMETER	CONTAINER	PRESERVATION ^{1,2}		HOLDING TIME ³	SAMPLE VOLUME
		Temp.	Chemical		
Alpha, Beta, Radium	Plastic/Glass	None	HNO ₃ to pH<2	6 months	1 L

Key to Table

1. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at 4°C until compositing and sample splitting is completed.
2. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Nitric acid (HNO₃) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater).
3. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.

**Table 23-6.
Holding Times, Preservation and Container Requirements: RCRA - Aqueous**

PARAMETER	CONTAINER ¹	PRESERVATION ^{2,3}		HOLDING TIME ⁴	SAMPLE VOLUME
		Temp. ¹²	Chemical		
Chloride	Plastic/Glass	4°C	None	28 days	100 mL
Cyanide -Total	Plastic/Glass	4°C	NaOH to pH >12 ⁵	14 days	250 mL
Cyanide -Amenable	Plastic/Glass	4°C	NaOH to pH >12 ⁵	14 days	250 mL
Hydrogen Ion (pH)	Plastic/Glass	4°C	None	24 hours ¹¹	100 mL
Nitrate	Plastic/Glass	4°C	None	48 hours	28 days
Oil and Grease	Glass	4°C	HCl	28 days	1 L
Organic carbon (TOC)	Plastic/Glass	4°C	pH to <2 ⁶ Store in dark	28 days	28 days
Sulfate	Plastic/Glass	4°C	None	28 days	400 mL
Sulfide	Plastic/Glass	4°C	Add Zn Acetate	7 days	400 mL
Chromium VI	Plastic/Glass	4°C	None	24 hours	250 mL
Mercury	Plastic/Glass	None	HNO ₃ to pH<2	28 days	250 mL
Other Metals	Plastic/Glass	None	HNO ₃ to pH<2	6 months	250 mL
Acrolein and Acrylonitrile	Glass ¹⁰	4°C	0.0008 % Na ₂ S ₂ O ₃ ⁷ , Adjust pH to 4-5 ¹³	14 days	1 L
Benzidines	Glass ¹⁰	4°C	0.0008 % Na ₂ S ₂ O ₃ ⁷	7 days ⁸	1 L
Chlorinated Hydrocarbons	Glass ¹⁰	4°C	0.0008 % Na ₂ S ₂ O ₃ ⁷	7 days ⁸	1 L
Dioxins and Furans	Glass ¹⁰	4°C	0.0008 % Na ₂ S ₂ O ₃ ⁷	7 days ⁸	1 L
Haloethers	Glass ¹⁰	4°C	0.0008 % Na ₂ S ₂ O ₃ ⁷	7 days ⁸	1 L
Nitroaromatics and cyclic ketones	Glass ¹⁰	4°C	0.0008 % Na ₂ S ₂ O ₃ ⁷ , store in dark	7 days ⁸	1 L
Nitrosamines	Glass ¹⁰	4°C	0.0008 % Na ₂ S ₂ O ₃ ⁷ , store in dark	7 days ⁸	1 L
Organochlorine Pesticides	Glass ¹⁰	4°C	None	7 days ⁸	1 L
Organophosphorus Pesticides	Glass ¹⁰	4°C	Adjust pH ⁹	7 days ⁸	1 L
PCBs	Glass ¹⁰	4°C	None	7 days ⁸	1 L
Phenols	Glass ¹⁰	4°C	0.0008 % Na ₂ S ₂ O ₃ ⁷	7 days ⁸	1 L

PARAMETER	CONTAINER ¹	PRESERVATION ^{2,3}		HOLDING TIME ⁴	SAMPLE VOLUME
		Temp. ¹²	Chemical		
Phthalate Esters	Glass ¹⁰	4°C	None	7 days ⁸	1 L
Polynuclear Aromatic Hydrocarbons	Glass ¹⁰	4°C	0.0008 % Na ₂ S ₂ O ₃ ⁷ , store in dark	7 days ⁸	1 L
Purgeable Hydrocarbons	Glass ¹⁰	4°C	0.0008 % Na ₂ S ₂ O ₃ ⁷ Adjust pH <2 ²	14 days	40 mL
Purgeable Halocarbons	Glass ¹⁰	4°C	0.0008 % Na ₂ S ₂ O ₃ ⁷	14 days	40 mL
Total Organic Halides (TOX)	Glass ¹⁰	4°C	Adjust pH to <2 with H ₂ SO ₄	28 days	1 L
Radiological Tests (Alpha, Beta, Radium)	Plastic/Glass	None	HNO ₃ to pH<2	6 months	250 mL

Key to Table

1. Plastic should be Polyethylene.
2. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at 4°C until compositing and sample splitting is completed.
3. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Hydrochloric acid, (HCl) in water, solutions at concentrations of 0.04% by weight or less (pH about 1.96 or greater); Nitric acid (HNO₃) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater); Sulfuric acid (H₂SO₄) in water solutions at concentrations of 0.35% by weight or less pH about 1.15 or greater); and Sodium hydroxide (NaOH) in water solutions at concentrations of 0.080% by weight or less (pH about 12.30 or less).
4. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
5. If oxidizing agents are present, add 5 mL 0.1 N NaAsO₂ or 0.06 g of ascorbic acid per L. See Cyanide SOP for additional information about other interferences.
6. Adjust pH to <2 with H₂SO₄, HCl, or solid NaHSO₄. Free Chlorine must be removed prior to adjustment.
7. Free Chlorine must be removed by the appropriate addition of Na₂S₂O₃.
8. 7 days until extraction. 40 days after extraction.
9. Adjust pH to 5-8 using NaOH or H₂SO₄.
10. With Teflon lined septum.
11. Holding Time is listed as "As Soon as Possible" in SW 846. Per EPA MICE, the recommended maximum holding time for pH in water is 24 hours and pH in soil is 7 days. There are no mandated regulatory requirements.
12. For samples with a temperature requirement of 4°C, a sample temperature of just above the water freezing temperature to ≤ 6°C is acceptable.
13. Based on guidance from EPA MICE, if samples are received without pH adjustment, the holding time is 7 days.

**Table 23-7.
Holding Times, Preservation and Container Requirements: RCRA – Non-Aqueous**

PARAMETER	CONTAINER ¹	PRESERVATION		HOLDING TIME ²	SAMPLE WEIGHT
		Temp. ⁷	Chemical		
Chloride	Glass	4°C	None	28 days	50 g
Cyanide -Total	Glass	4°C	None	14 days	50 g
Cyanide -Amenable	Glass	4°C	None	14 days	50 g
Hydrogen Ion (pH)	Glass	4°C	None	7 days ⁶	50 g
Nitrate	Glass	4°C	None	N/A	50 g
Oil and Grease	Glass	4°C	None	28 days	50 g
Sulfide	Glass	4°C	Add Zn Acetate, zero headspace	7 days	50 g
Chromium VI	Glass	4°C	None	24 hours	50 g
Mercury	Plastic/Glass	None	None	28 days	50 g
Other Metals	Plastic/Glass	None	None	6 months	50 g
Acrolein and Acrylonitrile	Glass ⁴	4°C	None	14 days	50 g
Benzidines	Glass ⁴	4°C	None	14 days ³	50 g
Chlorinated Hydrocarbons	Glass ⁴	4°C	None	14 days ³	50 g
Dioxins and Furans	Glass ⁴	4°C	None	14 days ³	50 g
Haloethers	Glass ⁴	4°C	None	14 days ³	50 g
Nitroaromatics and cyclic ketones	Glass ⁴	4°C	None	14 days ³	50 g
Nitrosamines	Glass ⁴	4°C	None	14 days ³	50 g
Organochlorine Pesticides	Glass ⁴	4°C	None	14 days ³	50 g
Organophosphorus Pesticides	Glass ⁴	4°C	None	14 days ³	50 g
PCBs	Glass ⁴	4°C	None	14 days ³	50 g
Phenols	Glass ⁴	4°C	None	14 days ³	50 g
Phthalate Esters	Glass ⁴	4°C	None	14 days ³	50 g
Polynuclear Aromatic Hydrocarbons	Glass ⁴	4°C	None	14 days ³	50 g

PARAMETER	CONTAINER ¹	PRESERVATION		HOLDING TIME ²	SAMPLE WEIGHT
		Temp. ⁷	Chemical		
Purgeable Hydrocarbons	Glass ⁴	4°C	None	14 days ⁵	50 g
Purgeable Halocarbons	Glass ⁴	4°C	None	14 days ⁵	50 g
Total Organic Halides (TOX)	Glass ⁴	4°C	None	28 days	50 g

Key to Table

1. Plastic should be Polyethylene.
2. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
3. 14 days until extraction. 40 days after extraction.
4. With Teflon Lined Septum
5. See Volatile SOP for more detailed preservation requirements.
6. Holding Time is listed as "As Soon as Possible" in SW 846. Per EPA MICE, the recommended maximum holding time for pH in water is 24 hours and pH in soil is 7 days. There are no mandated regulatory requirements.
7. For samples with a temperature requirement of 4°C, a sample temperature of just above the water freezing temperature to ≤ 6°C is acceptable.

**Table 23-8.
 Holding Times, Preservation and Container Requirements: Air Samples**

PARAMETER	CONTAINER ¹	PRESERVATION		HOLDING TIME ²	SAMPLE WEIGHT
		Temp.	Chemical		
Volatile Organics	Summa Cannister	None	None	30 days	6L or 1L
Volatile Organics	Tedlar Bag	None	None	72 hrs ^{3,4}	1 L

Key to Table

1. Plastic should be Polyethylene.
2. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
3. Holding Time is based on SW 846 Method 0040 "SAMPLING OF PRINCIPAL ORGANIC HAZARDOUS CONSTITUENTS FROM COMBUSTION SOURCES USING TEDLAR® BAGS". Some states specifically enforce this holding time (e.g. Florida, New Jersey) and others have not specified this information in their regulatory requirements.
4. The holding time is 72 hours unless the laboratory has a documented validation study that indicates a longer HT is acceptable for the analytes of interest.

SECTION 24

HANDLING OF SAMPLES (NELAC 5.5.8)

Sample management procedures at [TestAmerica Irvine](#) ensure that sample integrity and custody are maintained and documented from sampling/receipt through disposal.

24.1 CHAIN OF CUSTODY (COC)

The COC form is the written documented history of any sample and can be initiated [when bottles are sent to the field](#), or at the time of sampling. This form is completed by the sampling personnel and accompanies the samples to the laboratory where it is received and stored under the laboratory's custody. The purpose of the COC form is to provide a legal written record of the handling of samples from the time of collection until they are received at the laboratory. It also serves as the primary written request for analyses from the client to the laboratory. The COC form acts as a purchase order for analytical services when no other contractual agreement is in effect. An example of a COC form may be found in Figure 24-1.

24.1.1 Field Documentation

The information the sampler needs to provide at the time of sampling on the container label is:

- Sample identification
- Date and time
- Preservative

During the sampling process, the COC form is completed and must be legible (see Figure 24-1). This form includes information such as:

- [Client name, address, phone number and fax number \(if available\)](#)
- [Project name and/or number](#)
- [The sample identification](#)
- [Date, time and location of sampling](#)
- [Sample collectors name](#)
- [The matrix description](#)
- [The container description](#)
- [The total number of each type of container](#)
- [Preservatives used](#)
- [Analysis requested](#)
- [Requested turnaround time \(TAT\)](#)
- [Any special instructions](#)
- [Purchase Order number or billing information \(e.g. quote number\) if available](#)
- [The date and time that each person received or relinquished the sample\(s\), including their signed name.](#)

The samples are stored in a cooler with ice, as applicable, and remain solely in the possession of the client's field technician until the samples are delivered to the laboratory. The sample collector must assure that each container is in his/her physical possession or in his/her view at all times, or stored in such a place and manner to preclude tampering. The field technician relinquishes the samples in writing on the COC form to the sample control personnel at the laboratory or to a TestAmerica courier. Samples are only considered to be received by lab when personnel at the laboratory have physical contact with the samples.

Note: Independent couriers (e.g. FedEx) are not required to sign the COC form. The COC is usually kept in the sealed sample cooler. The receipt from the courier is attached to the COC and kept with the entire project file.

24.1.2 Legal / Evidentiary Chain-of-Custody

If samples are identified for legal/evidentiary purposes on the COC, login will complete the custody seal (Figure 24-2), retain the shipping record with the COC, and initiate an internal COC (Figure 24-3) for laboratory use by analysts and a sample disposal record (Figure 24-4).

24.2 SAMPLE RECEIPT

Samples are received at the laboratory by designated sample receiving personnel and a unique laboratory project identification number is assigned. Each sample container shall be assigned a unique sample identification number that is cross-referenced to the client identification number such that traceability of test samples is unambiguous and documented. Each sample container is affixed with a durable sample identification label. Sample acceptance, receipt, tracking and storage procedures are summarized in the following sections.

24.2.1 Laboratory Receipt

(See LOGIN.SOP (Sample Control) for more details on sample receipt procedures)

When samples arrive at the laboratory, sample receiving personnel inspect the coolers and samples. On a client-specific basis, a Project Receipt Checklist may be filled out to document custody seals, cooler temperatures, preservation, and notifications of discrepancy. See Figure 24-6. The integrity of each sample must be determined by comparing sample labels or tags with the COC and by visual checks of the container for possible damage. Any non-conformance, irregularity, or compromised sample receipt must be documented on a Notification of Discrepancy Form (NOD). See Figure 24-7. Discrepancies are forwarded to the Project Manager and are brought to the immediate attention of the client. The COC, shipping documents, documentation of any non-conformance, irregularity, or compromised sample receipt, record of client contact, and resulting instructions become part of the project record.

24.2.1.1 Inspection of samples include a check for:

- Complete documentation to include sample identification, location, date and time of collection, collector's name, preservation type, sample type and any additional comments concerning the samples.
- Complete sample labels to include unique identification in indelible ink.
- Use of appropriate sample containers (see Section 23)

- Adherence to holding times as specified in the test method and/or summarized in Section 23.
 - Adequate sample volume for required analyses (see Section 23).
 - Damage or signs of contamination to sample container. Volatile vials are also inspected for headspace
- 24.2.1.2** Check and record the temperature of the samples, temperature blanks, that require thermal preservation.
- Samples shall be deemed acceptable if arrival temperature is just above freezing and less than or equal to 6.0° C. Samples that are hand-delivered immediately after collection may not be at the required temperatures; however, if there is evidence that the chilling process has begun, such as the arrival on ice, the samples shall be considered acceptable. This will be documented on the COC .
 - If the samples were shipped in ice and solid ice is still present and in direct contact with samples, report the samples as "received on ice." Direct contact means samples must be surrounded by ice cubes or crushed ice. Ice present in a plastic bottle or other container does not constitute direct contact. Samples shipped with only "blue ice" may not be reported as "received on ice".
- 24.2.1.3** Verify sample preservation as specified in the test method by inspection of the preservation listed on the container. Actual pH is verified by the laboratory at the time of analysis and documented on a benchsheet or runlog. Chlorine is checked at the time of analysis on samples requiring extractable organics, BOD, TOX, cyanide, fluoride, ammonia, TKN, CBOD and Nitrate; presence or absence is recorded.
- 24.2.1.4** After inspecting the samples, the sample receiving personnel sign and date the COC form, make any necessary notes of the samples' conditions and store them in appropriate refrigerators or storage locations.
- 24.2.1.5** If samples are received without a COC, TestAmerica will provide a generic COC form to be completed by the client when the samples are brought to the laboratory. The client is always provided with a copy of the completed COC form for their records.
- 24.2.1.6** If analyses with short holding times are requested, the dates and times are inspected to ensure that holding times have not already expired.
- 24.2.1.7** Samples received after normal working hours are left in their coolers and placed in the walk-in refrigerator. The person receiving the samples must record the date and time received, the presence or absence of ice and custody seals, the temperature of samples, presence and type of packing material, and initials.
- 24.2.1.8** Any deviations from the checks described in Section 24.2.1 that question the suitability of the sample for analysis, or incomplete documentation as to the tests required will be resolved by consultation with the client. If the sample acceptance criteria (Section 24.3) are not met, the laboratory shall either:

- Retain all correspondence and/or records of communications with the client regarding the disposition of rejected samples , or
- Fully document any decision to proceed with sample analysis that does not meet sample acceptance criteria.

24.2.2 Sample Log-in

All samples that are received by the laboratory are logged into the LIMS to allow the laboratory to track and evaluate sample progress. Each group of samples that are logged in together (typically one project from a given client/sampling event) is assigned a unique job number. Within each job, each sampling point (or sample) receives a unique number. Sample numbers are generated sequentially over time, and are not re-assigned. A sample may be composed of more than one bottle since different preservatives may be required to perform all analyses requested. Even if multiple containers are received for a single sample, each container is uniquely identified with an alphabetic letter added to the sample number. The LIMS generates sample labels that are attached to each bottle for a given sample.

Each job/set of samples is logged into LIMS with a minimum of the following information:

- Client Name, Project Name, Address, Phone, Fax, Report to information, invoice to information (most of this information is “default information” that is stored in the LIMS).
- Date and time sampled;
- Date and time received;
- Job and/or project description, sample description;
- Sample matrix, special sample remarks;
- Reporting requirements (i.e., QC level, report format, invoicing format);
- Turn-around-time requirements;
- Parameters (methods and reporting limits or MDLs are default information for a given parameter)

24.3 SAMPLE ACCEPTANCE POLICY

The laboratory has a written sample acceptance policy (Figure 24-5) that clearly outlines the circumstances under which samples shall be accepted or rejected. These include:

- a COC filled out completely;
- samples must be properly labeled;
- proper sample containers with adequate volume for the analysis and necessary QC;
- samples must be preserved according to the requirements of the requested analytical method;
- sample holding times must be adhered to;
- all samples submitted for water/solid Volatile Organic analyses must have a Trip Blank submitted at the same time;
- the project manager will be notified if any sample is received in damaged condition.

Data from samples which do not meet these criteria are flagged and the nature of the variation from policy is defined. A copy of the sample acceptance policy is provided to each client prior to shipment of samples.

24.4 SAMPLE STORAGE

In order to avoid deterioration, contamination or damage to a sample during storage and handling, from the time of receipt until all analyses are complete, samples are stored in refrigerators suitable for the sample matrix. (Exception: preserved metals samples are stored at room temperature.) Samples to be analyzed for volatile organic parameters are stored in separate refrigerators designated for volatile organic parameters only. Samples are never to be stored with reagents, standards or materials that may create contamination.

To ensure the integrity of the samples during storage, refrigerator blanks are maintained in the volatile sample refrigerators and analyzed every two weeks. See REFBLANK.SOP (Refrigerator Storage Blank) for more details.

Analysts and technicians retrieve the sample container allocated to their analysis from the designated refrigerator and place them on carts, analyze the sample, and return the remaining sample or empty container to the refrigerator from which it originally came. All unused portions of samples, including empty sample containers, are returned to the secure sample control area. All samples are kept in the refrigerators for three weeks after analysis, which meets or exceeds most sample holding times. After two to four weeks the samples are moved to dry room temperature, sample archive area where they are stored for an additional three weeks before they are disposed of. This six week holding period allows samples to be checked if a discrepancy or question arises. Special arrangements may be made to store samples for longer periods of time. This extended holding period allows additional metal analyses to be performed on the archived sample and assists clients in dealing with legal matters or regulatory issues.

Access to the laboratory is controlled such that sample storage need not be locked at all times unless a project specifically demands it. Samples are accessible to laboratory personnel only. Visitors to the laboratory are prohibited from entering the refrigerator and laboratory areas unless accompanied by an employee of TestAmerica.

24.5 HAZARDOUS SAMPLES AND FOREIGN SOILS

To minimize exposure to personnel and to avoid potential accidents, hazardous and foreign soil samples are stored in an isolated area designated for hazardous waste only. For any sample that is known to be hazardous at the time of receipt or, if after completion of analysis the result exceeds the acceptable regulatory levels, a Hazardous Sample Notice must be completed by the analyst. This form may be completed by Sample Control, Project Managers, or analysts and must be attached to the report. The sample itself is clearly marked with a red stamp, stamped on the sample label reading "HAZARDOUS" or "FOREIGN SOIL" and placed in a colored and/or marked bag to easily identify the sample. The date, log number, lab sample number, and the result or brief description of the hazard are all written on the Hazardous & Foreign Soil Sample Notice. A copy of the form must be included with the original COC and Work Order and the original must be given to the Sample Control Custodian. Analysts will notify Sample Control of any sample determined to be hazardous after completion of analysis by completing a

Hazardous Sample Notice. All hazardous samples are either returned to the client or disposed of appropriately through a hazardous waste disposal firm that lab-packs all hazardous samples and removes them from the laboratory. Foreign soil samples are sent out for incineration by a USDA-approved waste disposal facility.

24.6 SAMPLE SHIPPING

In the event that the laboratory needs to ship samples, the samples are placed in a cooler with enough ice to ensure the samples remain just **above freezing and at or below 6.0°C** during transit. The samples are carefully surrounded by packing material to avoid breakage (yet maintain appropriate temperature). For sample shipments which include water/solid volatile organic analyses, a trip blank is enclosed when required by method specifications or state or regulatory programs. **The chain-of-custody form is signed by the sample control technician and attached to the shipping paperwork.** Samples are generally shipped overnight express or hand-delivered by a TestAmerica courier to maintain sample integrity. All personnel involved with shipping and receiving samples must be trained to maintain the proper chain-of-custody documentation and to keep the samples intact and on ice. The Environmental, Health and Safety Manual contains additional shipping requirements.

24.7 SAMPLE DISPOSAL

Samples should be retained for a minimum of **30** days after the project report is sent, however, provisions may be made for earlier disposal of samples once the holding time is exceeded. Some samples are required to be held for longer periods based on regulatory or client requirements (e.g., 60 days after project report is sent). The laboratory must follow the longer sample retention requirements where required by regulation or client agreement. Several possibilities for sample disposal exist: the sample may be consumed completely during analysis, the sample may be returned to the customer or location of sampling for disposal, or the sample may be disposed of in accordance with the laboratory's waste disposal procedures **as documented in the laboratory's Chemical Hygiene Plan.** All procedures in the laboratory Environmental, Health and Safety Manual are followed during disposal. Samples are normally maintained in the laboratory no longer than **six weeks** from receipt unless otherwise requested. Unused portions of samples found or suspected to be hazardous according to state or federal guidelines may be returned to the client upon completion of the analytical work.

If a sample is part of a known litigation, the affected legal authority, sample data user, and/or submitter of the sample must participate in the decision about the sample's disposal. All documentation and correspondence concerning the disposal decision process must be kept on file. Pertinent information includes the date of disposal, nature of disposal (such as sample depletion, hazardous waste facility disposal, return to client), names of individuals who conducted the arrangements and physically completed the task. The laboratory will remove or deface sample labels prior to disposal unless this is accomplished through the disposal method (e.g., samples are incinerated). A Waste Disposal Record (Figure 24-4) should be completed.

Figure 24-1.

Example: Chain of Custody (COC)

17461 Denham Av., Suite 120, Irvine, CA 92614 (949) 261-1022 FAX (949) 260-3297
 1014 E. Casley Dr., Suite A, Colton, CA 92534 (909) 370-4667 FAX (909) 370-1046
 8630 South 51st St., Suite B-120, Phoenix, AZ 85044 (480) 795-0043 FAX (480) 795-0851
 2520 E. Sunset Rd. #3, Las Vegas, NV 89120 (702) 798-3020 FAX (702) 798-3621

CHAIN OF CUSTODY FORM Page _____ of _____

Client Name/Address:			Project/PO Number:			Analysis Requested										
Project Manager:			Phone Number:													
Sampler:			Fax Number:													
Sample Description	Sample Matrix	Container Type	# of Cont.	Sampling Date	Sampling Time	Preservatives	Special Instructions									
Relinquished By: _____			Date/Time: _____			Received by: _____			Date/Time: _____			Turnaround Time: (Check)				
Relinquished By: _____			Date/Time: _____			Received by: _____			Date/Time: _____			same day _____ 72 hours _____				
Relinquished By: _____			Date/Time: _____			Received in Lab by: _____			Date/Time: _____			24 hours _____ 5 days _____				
												48 hours _____ normal _____				
												Sample integrity: (Check)				
												intact _____ on ice _____				

Note: By relinquishing samples to Del Mar Analytical, client agrees to pay for the services requested on this chain of custody form and any additional analyses performed on this project. Payment for services is due within 30 days from the date of invoice. Sample(s) will be disposed of after 30 days.

Figure 24-2.

Example: Custody Seal



Figure 24-3.

Example: Internal Chain of Custody (COC)

TestAmerica

ANALYTICAL TESTING CORPORATION

17461 Derian Avenue, Suite 100 Irvine, CA 92614 (949) 261-1022 fax: (949) 260-3297

WORK ORDER

IPL2715

Client:

Client Code:

Project Manager:

Project Name:

Project Number:

Printed:

Internal Sample Custody

Refrigerator ID:

Sample	In	Out	In	Out	In	Out	In	Out	Archived	Disposed
IPL2715-01G										
IPL2715-01H										
IPL2715-01I										
IPL2715-01L										
IPL2715-01M										
IPL2715-01P										
IPL2715-01Q										
IPL2715-01R										
IPL2715-01S										
IPL2715-01T										

Reviewed By _____


Date _____

Time _____

12/28/2006 10:08:48AM
Page 13 of 16

Figure 24-5a.

Example: Sample Acceptance Policy, page 1



TestAmerica Sample Acceptance Policy

All incoming work will be evaluated against the criteria listed below. Where applicable, data from any samples that do not meet the criteria listed below will be noted on the laboratory report defining the nature and substance of the variation. In addition the client will be notified either by telephone, fax or e-mail ASAP after the receipt of the samples.

- 1) Samples must arrive with labels intact with a Chain of Custody filled out completely. The following information must be recorded.
 - Client name, address, phone number and fax number (if available)
 - Project name and/or number
 - The sample identification
 - Date, time and location of sampling
 - The collectors name
 - The matrix description
 - The container description
 - The total number of each type of container
 - Preservatives used
 - Analysis requested
 - Requested turnaround time (TAT)
 - Any special instructions
 - Purchase Order number or billing information (e.g. quote number) if available
 - The date and time that each person received or relinquished the sample(s), including their signed name.
 - The date and time of receipt must be recorded between the last person to relinquish the samples and the person who receives the samples in the lab, and they must be exactly the same.
 - **Information must be legible**
- 2) Samples must be properly labeled.
 - Use durable labels (labels provided by TestAmerica are preferred)
 - Include a unique identification number
 - Include sampling date and time & sampler ID
 - Include preservative used.
 - Use indelible ink
 - **Information must be legible**
- 3) Proper sample containers with adequate volume for the analysis and necessary QC are required for each analysis requested. See TA Sample Container Guide.
- 4) Samples must be preserved according to the requirements of the requested analytical method (See TA Sample Container Guide). Most analytical methods require chilling samples to 4° C (other than water samples for metals analysis). For these methods, the criteria are met if the samples are chilled to below 6° C and above freezing (0° C). For methods with other temperature criteria (e.g. some bacteriological methods require ≤ 10 °C), the samples must arrive within ± 2° C of the required temperature or within the method specified range. **Note:** Samples that are hand delivered to the laboratory immediately after collection may not have had time to cool sufficiently. In this case the samples will be considered acceptable as long as there is evidence that the chilling process has begun (arrival on ice).

Continued on other side.

17461 Derian Ave., Suite 100, Irvine, CA 92606 (949) 261-1022 FAX (949) 261-1228

Figure 24-5b.

Example: Sample Acceptance Policy, page 2


- Chemical preservation (pH) will be verified prior to analysis and the project manager will be notified immediately if there is a discrepancy. If analyses will still be performed, all affected results will be flagged to indicate improper preservation.
- For Volatile Organic analyses in drinking water (Methods 502.2 or 524.2). Residual chlorine must be neutralized prior to preservation. If there is prior knowledge that the samples are not chlorinated, state it on the COC and use the VOA vials pre-preserved with HCl. The following are other options for a sampler and laboratory where the presence of chlorine is not known:
 - 1. Test for residual chlorine in the field prior to sampling.
 - If no chlorine is present, the samples are to be preserved using HCl as usual.
 - If chlorine is present, add either ascorbic acid or sodium thiosulfate prior to adding HCl.
 - 2. Use VOA vials pre-preserved with sodium thiosulfate or ascorbic acid and add HCl after filling the VOA vial with the sample.
- 5) Sample Holding Times
 - TestAmerica will make every effort to analyze samples within the regulatory holding time. Samples must be received in the laboratory with enough time to perform the sample analysis. Except for short holding time samples (< 48hr HT) sample must be received with at least 48 hrs (working days) remaining on the holding time for us to ensure analysis.
 - Analyses that are designated as "field" analyses (Odor, pH, Dissolved Oxygen, Disinfectant Residual; a.k.a. Residual Chlorine, and Redox Potential) should be analyzed ASAP by the field sampler prior to delivering to the lab. However, if the analyses are to be performed in the laboratory, TestAmerica will make every effort to analyze the samples within 24 hours from receipt of the samples in the testing laboratory. Samples for "field" analyses received after 4:00 pm on Friday or on the weekend will be analyzed no later than the next business day after receipt (Monday unless a holiday). Samples will remain refrigerated and sealed until the time of analysis. The actual times of all "field" sample analyses are noted on the "Short Hold Time Detail Report" in the final report. Only samples analyzed outside of these criteria will be qualified on the final report with an 'H' to indicate holding time exceedance.
- 6) All samples submitted for Volatile Organic analyses must have a Trip Blank submitted at the same time. TestAmerica will supply a blank with the bottle order.
- 7) The project manager will be notified if any sample is received in damaged condition TestAmerica will request that a sample be resubmitted for analysis.
- 8) Recommendations for packing samples for shipment.
 - Pack samples in Ice rather than "Blue" ice packs.
 - Soil samples should be placed in plastic zip-lock bags. The containers often have dirt around the top and do not seal very well and are prone to intrusion from the water from melted ice.
 - Water samples would be best if wrapped with bubble-wrap or paper (newspaper, or paper towels work) and then placed in plastic zip-lock bags.
 - Fill extra cooler space with bubble wrap.

G:\Depts\QUALITY\FORMS\SMFACT6.DOC

Updated January 31, 2008

Figure 24-6.

Example: Cooler Receipt Form



**Project Receipt Checklist
(Single Cooler)**

Client Name: _____ Project: _____

Received by: _____ Date/Time Received: _____

Delivered by : Client TA DHL Fed Ex UPS Other _____

Custody Seal and Temperature	Initial / Date
Custody Seal Status Cooler: <input type="checkbox"/> Intact <input type="checkbox"/> Broken <input type="checkbox"/> None	_____
Custody Seal Status Samples: <input type="checkbox"/> Intact <input type="checkbox"/> Broken <input type="checkbox"/> None	_____
Custody Seal #(s): _____ <input type="checkbox"/> No Seal #.....	_____
Sampler Signature on COC <input type="checkbox"/> Yes <input type="checkbox"/> No <input type="checkbox"/> N/A.....	_____
Therm # _____ Correction Factor _____ °C	_____
Temperature - BLANK _____ °C _____ CF = _____ °C.....	_____
Cooler #1 ID _____	_____
Samples outside temperature criteria but received within 6 hours of final sampling <input type="checkbox"/> Yes <input type="checkbox"/> N/A...	_____

Sample Fraction Listing and Preservation Check

Completed: Yes N/A _____

See attached Summary

Notification of Discrepancy (NOD) form


Anomalies: Yes N/A _____

If, YES, see attached NOD form

G:\Dept\QUALITY\FORMS\Trime PRC_r0.doc
09/18/07

Figure 24-7.

Example: Notification of Discrepancy Form (NOD)



THE LEADER IN ENVIRONMENTAL TESTING

NOTIFICATION OF DISCREPANCY

DATE: _____ TIME: _____ PM: _____ SC INITIALS: _____	
CLIENT/PROJECT NAME: _____	
Rush/Short Hold? <input type="checkbox"/> Yes <input type="checkbox"/> No	WORK ORDER #: _____

Project Not Set Up in Element New Client COC Received ON HOLD
 Analysis Requested on COC – Not Listed for Project in Element
 PM To Add Analysis: _____
 Clarification of Analysis: _____
 Hold Time Expired: (Analysis) _____
 Turnaround Time Not Checked: _____
 Did Not Receive Sample(s) Listed on COC: _____
 Received Extra Sample(s) Not Listed on COC: _____
 Sample Collector's name missing on COC: _____
 Sample Description(s) or Date/Time Sampled Do Not Match COC: _____

 Improper Preservative: _____
 VOAs have headspace (bubble>6mm): _____
 Sample Received Broken: _____
 Improper Temperature (_____ °) (Comments): _____
 Insufficient Sample Volume: _____
 Other: _____

PROJECT MANAGER RESOLUTION:	(Date & Time when returned to SC)

Approval By: _____	Date: _____	Time: _____
--------------------	-------------	-------------

G:\D:\ept\QUALITY\FORMS\NOD\FORM06.doc

SECTION 25.0

ASSURING THE QUALITY OF TEST RESULTS (NELAC 5.5.9)

25.1 OVERVIEW

In order to assure our clients of the validity of their data, the laboratory continuously evaluates the quality of the analytical process. The analytical process is controlled not only by instrument calibration as discussed in Section 21, but also by routine process quality control measurements (e.g. Blanks, Laboratory Control Samples (LCS), Matrix Spikes (MS), duplicates (DUP), surrogates, Internal Standards (IS)). These quality control checks are performed as required by the method or regulations to assess precision and accuracy. In addition to the routine process quality control samples, Proficiency Testing (PT) Samples (concentrations unknown to laboratory) are analyzed to help ensure laboratory performance.

25.2 CONTROLS

Sample preparation or pre-treatment is commonly required before analysis. Typical preparation steps include [homogenization](#), [grinding](#), [solvent extraction](#), [sonication](#), [acid digestion](#), [distillation](#), [reflux](#), [evaporation](#), [drying and ashing](#). During these pre-treatment steps, samples are arranged into discreet manageable groups referred to as preparation (prep) batches. Prep batches provide a means to control variability in sample treatment. Control samples are added to each prep batch to monitor method performance and are processed through the entire analytical procedure with investigative/field samples.

25.3 NEGATIVE CONTROLS

25.3.1 Method Blanks are used to assess preparation and analysis for possible contamination during the preparation and processing steps.

25.3.1.1 The method blank is prepared from a clean matrix similar to that of the associated samples that is free from target analytes (e.g., Reagent water, Ottawa sand, glass beads, etc.) and is processed along with and under the same conditions as the associated samples.

25.3.1.2 The method blank goes through all of the steps of the process (including as necessary: filtration, clean-ups, etc.).

25.3.1.3 The specific frequency of use for method blanks during the analytical sequence is defined in the specific standard operating procedure for each analysis. Generally it is 1 for each batch of samples; not to exceed 20 environmental samples.

25.3.1.4 Evaluation criteria and corrective action for method blanks is defined in the specific standard operating procedure for each analysis. [Generally, corrective action is taken if the concentration of a target analyte in the blank is at or above the reporting limit as established by the method or regulation:](#)

- The source of contamination is investigated

- Measures are taken to minimize or eliminate the source of the contamination
- Affected samples are reprocessed or the results are qualified on the final report.

25.3.2 Calibration Blanks are prepared and analyzed along with calibration standards where applicable. They are prepared using the same reagents that are used to prepare the standards. In some analyses the calibration blank may be included in the calibration curve.

25.3.3 Instrument Blanks are blank reagents or reagent water that may be processed during an analytical sequence in order to assess contamination in the analytical system. In general, instrument blanks are used to differentiate between contamination caused by the analytical system and that caused by the sample handling or sample prep process. Instrument blanks may also be inserted throughout the analytical sequence to minimize the effect of carryover from samples with high analyte content.

25.3.4 Trip Blanks are required to be submitted by the client with each shipment of samples requiring aqueous and solid volatiles analyses. A trip blank is prepared by the laboratory by filling a clean container with pure deionized water that has been purged to remove any volatile compounds. Appropriate preservatives are also added to the container. The trip blank is sent with the bottle order and is intended to reflect the environment that the containers are subjected to throughout shipping and handling and help identify possible sources if contamination is found. The field sampler returns the trip blank in the cooler with the field samples. Trip Blanks are also sometimes referred to as Travel Blanks.

25.3.5 Field Blanks are sometimes used for specific projects by the field samplers. A field blank prepared in the field by filling a clean container with pure reagent water and appropriate preservative, if any, for the specific sampling activity being undertaken. (EPA OSWER)

25.3.6 Equipment Blanks are also sometimes created in the field for specific projects. An equipment blank is a sample of analyte-free media which has been used to rinse common sampling equipment to check effectiveness of decontamination procedures. (NELAC)

25.3.7 Holding Blanks, also referred to as refrigerator or freezer blanks, are used to monitor the sample storage units for volatile organic compounds during the storage of VOA samples in the laboratory ([refer to section 24.](#))

25.3.8 Field blanks, equipment blank and trip blanks, when received, are analyzed in the same manner as other field samples. When known, blanks should not be selected for matrix QC, as it does not provide information on the behavior of the target compounds in the field samples. Usually, the client sample ID will provide information to identify the field blanks with labels such as "FB", "EB", or "TB".

25.4 POSITIVE CONTROLS

Control samples (e.g., QC indicators) are analyzed with each batch of samples to evaluate data based upon (1) Method Performance (Laboratory Control Sample (LCS) or Blank Spike (BS)), which entails both the preparation and measurement steps; and (2) Matrix Effects (Matrix Spike (MS) ([Matrix spikes are not applicable to air](#)) or Sample Duplicate (MD, DUP), which evaluates field sampling accuracy, precision, representativeness, interferences, and the effect of the matrix on the method performed. Each regulatory program and each method within those programs specify the control samples that are prepared and/or analyzed with a specific batch

Note that frequency of control samples vary with specific regulatory, methodology and project specific criteria. Complete details on method control samples are as listed in each analytical SOP [and in Appendix 4 for select methods](#).

25.4.1 Method Performance Control - Laboratory Control Sample (LCS)

25.4.1.1 The LCS measures the accuracy of the method in a blank matrix and assesses method performance independent of potential field sample matrix affects in a laboratory batch.

25.4.1.2 The LCS is prepared from a clean matrix similar to that of the associated samples that is free from target analytes (for example: Reagent water, Ottawa sand, glass beads, etc.) and is processed along with and under the same conditions as the associated samples. The LCS is spiked with verified known amounts of analytes or is made of a material containing known and verified amounts of analytes, taken through all preparation and analysis steps along with the field samples. Where there is no preparation taken for an analysis (such as in aqueous volatiles), or when all samples and standards undergo the same preparation and analysis process (such as Phosphorus), a calibration verification standard is reported as the LCS. [In some instances where there is no practical clean solid matrix available, aqueous LCS's may be processed for solid matrices; final results may be calculated as mg/kg or ug/kg, assuming 100% solids and a weight equivalent to the aliquot used for the corresponding field samples, to facilitate comparison with the field samples.](#)

25.4.1.3 [Certified pre-made reference material purchased from a NIST/A2LA accredited vendor may also be used for the LCS when the material represents the sample matrix or the analyte is not easily spiked \(e.g. solid matrix LCS for metals, TDS, etc.\).](#)

25.4.1.4 As stated in the opening of this section, the LCS goes through all of the steps of the process (including as necessary: filtration, clean-ups, etc.).

25.4.1.5 The specific frequency of use for LCS during the analytical sequence is defined in the specific standard operating procedure for each analysis ([see Appendix 4](#)). It is generally 1 for each batch of samples; not to exceed 20 environmental samples.

25.4.1.6 If the mandated or requested test method, or project requirements, do not specify the spiking components, the laboratory shall spike all reportable components to be reported in the Laboratory Control Sample (and Matrix Spike) where applicable (e.g.

no spike of pH). However, in cases where the components interfere with accurate assessment (such as simultaneously spiking chlordane, toxaphene and PCBs in Method 608), the test method has an extremely long list of components or components are incompatible, at a minimum, a representative number of the listed components (see below) shall be used to control the test method. The selected components of each spiking mix shall represent all chemistries, elution patterns and masses, permit specified analytes and other client requested components. However, the laboratory shall ensure that all reported components are used in the spike mixture within a two-year time period.

25.4.1.6.1 For methods that have 1-10 target analytes, spike all components.

25.4.1.6.2 For methods that include 11-20 target analytes, spike at least 10 or 80%, whichever is greater.

25.4.1.6.3 For methods with more than 20 target analytes, spike at least 16 components.

25.4.1.6.4 Exception: Due to analyte incompatibility in pesticides, Toxaphene and Chlordane are only spiked at client request based on specific project needs.

25.4.1.6.5 Exception: Due to analyte incompatibility between the various PCB aroclors, aroclors 1016 and 1260 are used for spiking as they cover the range of all of the aroclors. Specific aroclors may be used by request on a project specific basis.

25.4.1.7 **Accuracy Calculation:** Percent Recovery (%R) Calculation (applies to LCS, CCV, Surrogates, and Matrix Spikes.

$$\%R = \frac{AV}{TV} \times 100$$

Where: AV = Analyzed Value
TV = True Value

25.5 **SAMPLE MATRIX CONTROLS**

25.5.1 **Matrix Spikes (MS)**

25.5.1.1 The Matrix spike is used to assess the effect sample matrix of the spiked sample has on the precision and accuracy of the results generated by the method used.

25.5.1.2 An MS is essentially a sample fortified with a known amount of the test analyte(s). At a minimum, with each matrix-specific batch of samples processed, an MS is carried through the complete analytical procedure. Unless specified by the client, samples used for spiking are randomly selected and rotated between different client projects.

25.5.1.3 If the mandated or requested test method does not specify the spiking components, the laboratory shall spike all reportable components to be reported in the Laboratory Control Sample and Matrix Spike. However, in cases where the components interfere with accurate assessment (such as simultaneously spiking chlordane,

toxaphene and PCBs in Method 608), the test method has an extremely long list of components or components are incompatible, a representative number of the listed components (see LCS analytes 25.4.1.6 above) may be used to control the test method. The selected components of each spiking mix shall represent all chemistries, elution patterns and masses, permit-specified analytes and other client requested components. However, the laboratory shall ensure that all reported components are used in the spike mixture within a two-year time period.

- 25.5.1.4** The percent recovery calculation for matrix spikes is essentially the same as the calculation shown in 25.2.1.7 except that:

$$AV = Sp - Sa$$

Where: Sp = Spike result
Sa = Sample result

25.5.2 Surrogate Spikes

- 25.5.2.1** Surrogate Spikes are similar to matrix spikes except the analytes are compounds with properties that mimic the analyte of interest and are unlikely to be found in environment samples.

- 25.5.2.2** Surrogate compounds are added to all samples, standards, and blanks, for all organic chromatography methods except when the matrix precludes its use or when a surrogate is not available. The recovery of the surrogates is compared to the acceptance limits for the specific method (also refer to Section 25.5). Poor surrogate recovery may indicate a problem with sample composition and shall be reported, with data qualifiers, to the client whose sample produced poor recovery.

25.5.3 Duplicates

- 25.5.3.1** For a measure of analytical precision, with each matrix-specific batch of samples processed, a matrix duplicate (MD or DUP) sample, matrix spike duplicate (MSD), or LCS duplicate (LCSD) is carried through the complete analytical procedure. Duplicate samples are usually analyzed with methods that do not require matrix spike analysis. LCSD's are normally not performed except when regulatory agencies or client specifications require them. The recoveries for the spiked duplicate samples must meet the same laboratory established recovery limits as the accuracy QC samples. If an LCSD is analyzed both the LCS and LCSD must meet the same recovery criteria and be included in the final report. The precision measurement is reported as "Relative Percent Difference" (RPD). Poor precision between duplicates (except LCS/LCSD) may indicate non-homogeneous matrix or sampling.

- 25.5.3.2 Precision Calculation** (Relative Percent Difference - RPD)

$$RPD = \frac{|S - D|}{\frac{(S + D)}{2}} \times 100$$

Where: S=Sample Concentration
D=Duplicate Concentration

25.5.4 Internal Standards

25.5.4.1 In most organic analyses, internal standards are spiked into all environmental and quality control samples (including the initial calibration standards). An internal standard is also used with some metals analyses. It is added to sample extracts after the extraction (post-prep). The acceptance criteria in most methods are 50% to 200% of the responses in the mid-point of the corresponding calibration curve. Consult the method-specific SOPs for details on the internal standard compounds, calculations and acceptance criteria.

25.5.4.2 When the internal standard recoveries fall outside these limits, if there are not obvious chromatographic interferences, reanalyze the sample to confirm a possible matrix effect. If the recoveries confirm or there was obvious interference, results are reported from the original analysis and a qualifier is added. If the reanalysis meets internal standard recovery criteria, the second run is reported (or both are reported if requested by the client).

25.6 ACCEPTANCE CRITERIA (CONTROL LIMITS)

25.6.1 Each individual analyte in the LCS, MS, or Surrogate Spike are evaluated against the control limits as published in the test method. Where there are no established acceptance criteria, the laboratory calculates control limits with the use of control charts or, in some cases, utilizes client project specific or regulatory mandated control limits. When this occurs, the regulatory or project limits will supersede the laboratory's in-house limits.

Note: For methods, analytes and matrices with very limited data (e.g., unusual matrices not analyzed often), interim limits are established using available data or by analogy to similar methods or matrices.

25.6.2 Once control limits have been established, they are verified, reviewed, and updated if necessary on an annual basis unless the method requires more frequent updating (e.g. EPA SW846 8000 series methods). Control limits are established per method (as opposed to per instrument) regardless of the number of instruments utilized.

25.6.2.1 The lab should consider the effects of the spiking concentration control limits, and to avoid censoring of data. The acceptance criteria for recovery and precision are often a function of the spike concentration used. Therefore, caution must be used when pooling data to generate control limits.

25.6.2.2 Not only should the results all be from a similar matrix, but the spiking levels should also be approximately the same (within a factor of 2). Similarly, the matrix spike and surrogate results should all be generated using the same set of extraction, cleanup and analysis techniques. For example, results from solid samples extracted by ultrasonic extraction are not mixed with those extracted by Soxhlet.

- 25.6.2.3** The laboratory should try and avoid discarding data that do not meet a preconceived notion of acceptable performance. This results in a censored data set, which, when used to develop acceptance criteria, will lead to unrealistically narrow criteria. For a 99% confidence interval, 1 out of every 100 observations likely will still fall outside the limits. For methods with long analyte lists this may mean occasional failures every batch or two. While professional judgment is important in evaluating data to be used to develop acceptance criteria, specific results are not discarded simply because they do not meet one's expectations. However, data points shall be discarded if they were the result of human or mechanical error or sample concentration exceeded spike level by $> 4x$.
- 25.6.3** Laboratory generated % Recovery acceptance (control) limits are generally established by taking ± 3 Standard Deviations (99% confidence level) from the average recovery of a minimum of 20-30 data points (more points are preferred).
- 25.6.3.1** Regardless of the calculated limit, the limit should be no tighter than the Calibration Verification (ICV/CCV). (Unless the analytical method specifies a tighter limit).
- 25.6.3.2** In-house limits cannot be any wider than those mandated in a regulated analytical method.
- 25.6.3.3** The lowest acceptable recovery limit will be 10% (the analyte must be detectable). Exception: The lowest acceptable recovery limit for Benzidine will be 5% and the analyte must be detectable.
- 25.6.3.4** The maximum acceptable recovery limit will be 150%.
- 25.6.3.5** The maximum acceptable RPD limit will be 35% for waters and 40% for soils. The minimum RPD limit is 10%.
- 25.6.3.6** If either the high or low end of the control limit changes by $\leq 5\%$ from previous, the control chart is visually inspected and, using professional judgment, they may be left unchanged if there is no affect on laboratory ability to meet the existing limits.
- 25.6.4** The lab must be able to generate a current listing of their control limits and track when the updates are performed. In addition, the laboratory must be able to recreate historical control limits.
- 25.6.4.1** The QA department generates a Quality Control Limit Summary that contains tables that summarize the precision and accuracy acceptability limits for analyses performed at TestAmerica Irvine. This summary includes an effective date, is updated each time new limits are generated and is located in the QA directory of the laboratory computer network. Unless otherwise noted, limits within these tables are laboratory generated. The analysts are instructed to use the current limits in the laboratory (dated and approved by the Technical Director and QA Manager) and entered into the Laboratory Information Management System (LIMS). The Quality Assurance department maintains an archive of all limits used within the laboratory.

25.6.5 A LCS that is within the acceptance criteria establishes that the analytical system is in control and is used to validate the process. Samples that are analyzed with an LCS with recoveries outside of the acceptance limits may be determined as out of control and should be reanalyzed if possible. If reanalysis is not possible, then the results for all affected analytes for samples within the same batch must be qualified when reported. The internal corrective action process (see Section 13) is also initiated if an LCS exceeds the acceptance limits. Sample results may be qualified and reported without reanalysis if:

25.6.5.1 The analyte results are below the reporting limit and the LCS is above the upper control limit.

25.6.5.2 If the analytical results are above the relevant regulatory limit and the LCS is below the lower control limit.

[DD17]

25.6.6 If the MS/MSDs do not meet acceptance limits, the MS/MSD and the associated spiked sample is reported with a qualifier for those analytes that do not meet limits. If obvious preparation errors are suspected, or if requested by the client, unacceptable MS/MSDs are reprocessed and reanalyzed to prove matrix interference. A more detailed discussion of acceptance criteria and corrective action can be found in [Appendix 4](#) and in Section 13.

25.6.7 If a surrogate standard falls outside the acceptance limits, if there is not obvious chromatographic matrix interference, reanalyze the sample to confirm a possible matrix effect. If the recoveries confirm or there was obvious chromatographic interference, results are reported from the original analysis and a qualifier is added. If the reanalysis meets surrogate recovery criteria, the second run is reported (or both are reported if requested by the client). [Under certain circumstances, where all of the samples are from the same location and share similar chromatography, the reanalysis may be performed on a single sample rather than all of the samples and if the surrogate meets the recovery criteria in the reanalysis, all of the affected samples would require reanalysis.](#)

25.7 METHOD DETECTION LIMITS (MDLs)

MDLs, calculated as described in Section 20.7, are updated or verified annually, or more often if required by the method.

25.8 ADDITIONAL PROCEDURES TO ASSURE QUALITY CONTROL

25.8.1 The laboratory has written procedures to assure the accuracy of the test method including calibration (see Section 21), use of certified reference materials (see Section 22) and use of PT samples (see Section 16).

25.8.2 A discussion regarding MDLs, Limit of Detection (LOD) and Limit of Quantitation (LOQ) can be found in Section 20.

25.8.3 Use of formulae to reduce data is discussed in the method standard operating procedures and in Section 21.

25.8.4 Selection of appropriate reagents and standards is included in Section 9 and 22.

- 25.8.5** A discussion on selectivity of the test is included in Section 5.
- 25.8.6** Constant and consistent test conditions are discussed in Section 19.
- 25.8.7** The laboratories sample acceptance policy is included in Section 24.
- 25.8.8** A listing of the type of test result correlations that are looked at during report review (e.g. Total Chromium should be greater or equal to Hexavalent Chromium) is included in Section 20.13.4.5.

SECTION 26.0

REPORTING RESULTS (NELAC 5.5.10)

26.1 OVERVIEW

The results of each test are reported accurately, clearly, unambiguously, and objectively in accordance with State and Federal regulations as well as client requirements. Analytical results are issued in a format that is intended to satisfy customer and laboratory accreditation requirements as well as provide the end user with the information needed to properly evaluate the results. Where there is a conflict between the client requested formats and accreditation requirements or data usability information, accreditation requirements and data usability information will take precedence over client requests. A variety of report formats are available to meet specific needs.

In cases where a client asks for simplified reports, there must be a written request from the client. There still must be enough information that would show any analyses that were out of conformance (QC out of limits) and there should be a reference to a full report that is made available to the client.

Review of reported data is included in Section 20.

26.2 TEST REPORTS

Analytical results are reported in a format that is satisfactory to the client and meets all requirements of applicable accrediting authorities and agencies. A variety of report formats are available to meet specific needs. The report is printed [on laboratory letterhead](#), reviewed, and signed by the appropriate [project manager](#). At a minimum, the standard laboratory report shall contain the following information:

26.2.1 A report title (e.g. [Analytical Report For Samples](#)) with a “[sample results](#)” column header.

26.2.2 Each report page printed [on company letterhead](#), which includes the laboratory name, address and telephone number.

26.2.3 A unique identification of the report ([e.g. work order number](#)) and on each page an identification in order to ensure the page is recognized as part of the report and a clear identification of the end.

Note: Page numbers of report are represented [as page # of ##](#). [Where the first number is the page number and the second is the total number of pages.](#)

26.2.4 A copy of the chain of custody (COC).

- Any COCs involved with Subcontracting are included.
- In most cases, the applicable COC is not paginated but is an integral part of the report. If the COC is not a paginated portion of the report then there will be a statement on the front of the report to effect of "The Chain of Custody, X page(s), is included and is an integral part of this report.". The number of pages of the CoC (X) is entered into Element so that it is correct for each report.
- Any additional addenda to the report must be treated in a similar fashion so it is a recognizable part of the report and cannot accidentally get separated from the report (eg. Sampling information).

26.2.5 The name and address of client and a project name/number, if applicable.

26.2.6 Client project manager or other contact

26.2.7 Description and unambiguous identification of the tested sample(s) including the client identification code.

26.2.8 Date of receipt of sample, date and time of collection, and date(s) of test preparation and performance, and time of preparation or analysis if the required holding time for either activity is less than or equal to 72 hours.

26.2.9 Date reported or date of revision, if applicable.

26.2.10 Method of analysis including method code (EPA, Standard Methods, etc).

26.2.11 Reporting limit.

26.2.12 Method detection limits (if requested)

26.2.13 Definition of Data qualifiers and reporting acronyms (e.g. ND).

26.2.14 Sample results.

26.2.15 QC data consisting of method blank, surrogate, LCS, and MS/MSD recoveries and control limits.

26.2.16 Condition of samples at receipt including temperature (noted on COC.) This may also be accomplished in a narrative or by attaching sample login sheets (Refer to Sec. 26.2.4 – Item 3 regarding additional addenda).

26.2.17 A statement expressing the validity of the results, that the source methodology was followed and all results were reviewed for error.

26.2.18 A statement to the effect that the results relate only to the items tested and the sample as received by the laboratory.

26.2.19 A statement that the report shall not be reproduced except in full, without prior express written approval by the laboratory coordinator.

26.2.20 A signature and title of the person(s) accepting responsibility for the content of the report and date of issue. Signatories are appointed by the Lab Director. For applying an electronic signature refer to the Electronic Signature Policy (Section 26.4).

26.2.21 When NELAC accreditation is required, the lab shall certify that the test results meet all requirements of NELAC or provide reasons and/or justification if they do not. **Examples: At the time of analysis the laboratory was in compliance with the current NELAC standards and held accreditation for all analyses performed unless noted by a qualifier. The labs accreditation number is _____.** OR The report meets all applicable NELAC standards and shall not be reproduced except in full, without the written approval of the laboratory.

26.2.22 Where applicable, a narrative to the report that explains the issue(s) and corrective action(s) taken in the event that a specific accreditation or certification requirement was not met.

26.2.23 When Soil samples are analyzed, a specific identification as to whether soils are reported on a “wet weight” or “dry weight” basis.

26.2.24 Appropriate laboratory certification number for the state of origin of the sample, if applicable.

26.2.25 If only part of the report is provided to the client (client requests some results before all of it is complete), it must be clearly indicated on the report (e.g., **partial report, or how your lab identifies it**), and that a complete report will follow once all of the work has been completed.

26.2.26 Any out of network subcontracted analysis results are provided as a separate report on the official letterhead of the subcontractor. All in-network subcontracting is clearly identified on the report as to which laboratory performed a specific analysis.

26.3 REPORTING LEVEL OR REPORT TYPE

TestAmerica Irvine offers three levels of quality control reporting. Each level, in addition to its own specific requirements, contains all the information provided in the preceding level. The packages provide the following information in addition to the information described above:

- Level II is a report with the features described in Section 26.2 above plus summary information, including results for the method blank reported to the laboratory MDL, percent recovery for laboratory control samples and matrix spike samples, and the RPD values for all MSD and sample duplicate analyses.
- Level III contains all the information supplied in Level II, but presented on the CLP-like summary forms, and relevant calibration information. No raw data is provided.
- Level IV is the same as Level III with the addition of all raw supporting data.

In addition to the various levels of QC packaging, the laboratory also provides reports in diskette deliverable form. Initial reports may be provided to clients by facsimile. All faxed reports are followed by hardcopy. Procedures used to ensure client confidentiality are outlined in Section 26.7.

26.3.1 Electronic Data Deliverables (EDDs)

EDDs are routinely offered as part of TestAmerica's services. TestAmerica Irvine offers a variety of EDD formats including Environmental Restoration Information Management System (ERPIMS), New Agency Standard (NAS), Format A, Excel, Dbase, GISKEY, and Text Files.

EDD specifications are submitted to the IT department by the PM for review and undergo the contract review process. Once the facility has committed to providing data in a specific electronic format, the coding of the format may need to be performed. This coding is documented and validated. The validation of the code is retained by the IT staff coding the EDD.

[DD18]

EDDs shall be subject to a review to ensure their accuracy and completeness. If EDD generation is automated, review may be reduced to periodic screening if the laboratory can demonstrate that it can routinely generate that EDD without errors. Any revisions to the EDD format must be reviewed until it is demonstrated that it can routinely be generated without errors. If the EDD can be reproduced accurately and if all subsequent EDDs can be produced error-free, each EDD does not necessarily require a review.

26.4 ELECTRONIC REPORTING AND SIGNATURE POLICY

Following the lead of the Federal Paperwork Reduction Act, TestAmerica has implemented policies and procedures to help reduce paper usage. One of these procedures is to generate final reports and provide them to clients in pdf format.

Laboratory Director appointed representatives may approve final reports using an electronic signature that is applied to the report at the time of generation. This policy is prepared to state that the electronically applied signatures on TestAmerica Analytical Testing Corp. reports are as legally binding as a handwritten "wet signature". This policy is intended to prevent the possibility of non-repudiation (denial that an individual signed the document) and to insure authenticity and security. In order to ensure the electronic signatures are valid and unequivocally represent the identity of the signer, TestAmerica uses 21 CFR Part 11 "Electronic Records; Electronic Signatures" from the FDA as well as EPA's procurement policy (EPS 00-01) as guidance documents for this policy.

In order to ensure authenticity of the reports, the following conditions must be met:

26.4.1 Report Content

- State that the report was electronically signed.
- The printed name and title of the signer must be underneath the signature

- The date **and time** when the signature was executed is represented in the “Report Issued” entry on the cover page of the report.
- The meaning of the signature: (e.g. reviewed and approved)

In order to insure the integrity of the signatures, the following security features have been implemented.

26.4.2 General Requirements

- The identity of the signatory must be verified before an electronic signature can be created for that person.
- Each electronic signature shall be unique to a single individual and shall not be reused by or assigned to another individual
- Persons using an electronic signature shall certify that the electronic signatures in the system are intended to be the legally binding equivalent to their traditional handwritten signature. On this certification, the signatory will state that their passwords are to remain completely confidential and can only be used by the genuine owner of the password and the sign-off may not take place until each page has been viewed. Refer to Figure 26-1.

26.4.3 Components and Controls

Two distinct identification components are utilized for each individual. The components are a) user name b) password. Each signing will require the entry of the username and the password must be reentered. The signatures may not be copied, excised or transferred from the report by ordinary means.

The report may not be changed once the signature has been applied and the pdf files are stored on the file server with security **as well as password protected** to ensure no changes may be made to the file.

In the case where a client requests that the pdf be unsecure so that the report may be inserted into their reports, the client must sign an agreement stating that they will not alter the report. This can be achieved by requiring agreement each time it is accessed on the web or by signing off on an agreement (refer to Figure 26-2). **The lab can determine the best approach for this to be done:**

- **On a report by report basis**
- **On a client basis (all reports to a client would be an exception)**
- **On a project basis (all reports for a project would be an exception)**

Pdf reports must be backed up on a Magnetic tape or other durable storage media (e.g., DVD) and maintained secure for up to 5 years.

26.5 SUPPLEMENTAL INFORMATION FOR TEST

The lab identifies any unacceptable QC analyses or any other unusual circumstances or observations such as environmental conditions and any non-standard conditions that may have affected the quality of a result. This is typically in the form of a footnote or a qualifier and/or a narrative explaining the discrepancy in the front of the report. Refer to Appendix 7 for a list of the laboratory's standard footnotes and qualifiers.

26.5.1 Numeric results with values outside of the calibration range, either high or low are qualified as 'estimated'.

26.5.2 Where quality system requirements are not met, a statement of compliance/non-compliance with requirements and/or specifications, including identification of test results derived from any sample that did not meet NELAC sample acceptance requirements such as improper container, holding time, or temperature.

26.5.3 Where applicable, a statement on the estimated uncertainty of measurements; information on uncertainty is needed when a client's instructions so require.

26.5.4 Opinions and Interpretations - The test report contains objective information, and generally does not contain subjective information such as opinions and interpretations. If such information is required by the client, the Laboratory Director will determine if a response can be prepared. If so, the Laboratory Director will designate the appropriate member of the management team to prepare a response. The response will be fully documented, and reviewed by the Laboratory Director, before release to the client. There may be additional fees charged to the client at this time, as this is a non-routine function of the laboratory.

Note: Review of data deliverable packages for submittal to regulatory authorities requires responses to non-conforming data concerning potential impact on data quality. This necessitates a limited scope of interpretation, and this work is performed by the QA Department. This is the only form of "interpretation" of data that is routinely performed by the laboratory.

When opinions or interpretations are included in the report, the laboratory provides an explanation as to the basis upon which the opinions and interpretations have been made. Opinions and interpretations are clearly noted as such and where applicable, a comment should be added suggesting that the client verify the opinion or interpretation with their regulator.

26.6 ENVIRONMENTAL TESTING OBTAINED FROM SUBCONTRACTORS

If TestAmerica Irvine is not able to provide the client the requested analysis, the samples would be subcontracted following the procedures outlined in Section 8.

Data reported from analyses performed by a subcontractor laboratory are clearly identified as such on the analytical report provided to the client. Results from a subcontract laboratory outside of the TestAmerica network are reported to the client on the subcontract laboratory's original report stationary and the report includes any accompanying documentation.

26.7 CLIENT CONFIDENTIALITY

In situations involving the transmission of environmental test results by telephone, facsimile or other electronic means, client confidentiality must be maintained.

TestAmerica will not intentionally divulge to any person (other than the Client or any other person designated by the Client in writing) any information regarding the services provided by TestAmerica or any information disclosed to TestAmerica by the Client. Furthermore, information known to be potentially endangering to national security or an entity's proprietary rights will not be released.

Note: This shall not apply to the extent that the information is required to be disclosed by TestAmerica under the compulsion of legal process. TestAmerica will, to the extent feasible, provide reasonable notice to the client before disclosing the information.

Note: Authorized representatives of an accrediting authority are permitted to make copies of any analyses or records relevant to the accreditation process, and copies may be removed from the laboratory for purposes of assessment.

26.7.1 Report deliverable formats are discussed with each new client. If a client requests that reports be faxed or e-mailed, the reports are faxed with a cover sheet or e-mailed with the following note that includes a confidentiality statement similar to the following:

This material is intended only for the use of the individual(s) or entity to whom it is addressed, and may contain information that is privileged and confidential. If you are not the intended recipient, or the employee or agent responsible for delivering this material to the intended recipient, you are hereby notified that any dissemination, distribution or copying of this communication is strictly prohibited. If you have received this communication in error, please notify us immediately by telephone at the 1-800-765-0980 (or for e-mails: please notify us immediately by e-mail or by phone (1-800-765-0980) and delete this material from any computer).

26.8 FORMAT OF REPORTS

The format of reports are designed to accommodate each type of environmental test carried out and to minimize the possibility of misunderstanding or misuse.

26.9 AMENDMENTS TO TEST REPORTS

Corrections, additions, or deletions to reports are only made when justification arises through supplemental documentation. Justification is documented using the laboratory's corrective action system (refer to Section 13).

The revised report is retained on the Archive data server, as is the original report. The revised report is stored in the Archive data server under the sample number followed by "Revision". The revised report will have the word "revised" or "amended" next to the date rather than the word "reported".

When the report is re-issued, a notation of "revised " is placed on the cover/signature page of the report *or at the top of the narrative page* with a brief explanation of reason for the re-issue.

26.10 POLICIES ON CLIENT REQUESTS FOR AMENDMENTS

26.10.1 Sample Reanalysis Policy

Because there is a certain level of uncertainty with any analytical measurement a sample reanalysis may result in either a higher or lower value from an initial sample analysis. There are also variables that may be present (e.g. sample homogeneity, analyte precipitation over time, etc.) that may affect the results of a reanalysis. Based on the above comments, the laboratory will reanalyze samples at a client's request with the following caveats. Client specific arrangements for reanalysis protocols can be established.

- Homogenous samples: If a reanalysis agrees with the original result to within the RPD limits for MS/MSD or Duplicate analyses, or within ± 1 reporting limit for samples $\leq 5x$ the reporting limit, the original analysis will be reported. At the client's request, both results may be reported on the same report but not on two separate reports.
- If the reanalysis does not agree (as defined above) with the original result, then the laboratory will investigate the discrepancy and reanalyze the sample a third time for confirmation if sufficient sample is available.
- Any potential charges related to reanalysis are discussed in the contract terms and conditions or discussed at the time of the request. The client will typically be charged for reanalysis unless it is determined that the lab was in error.
- Due to the potential for increased variability, reanalysis may not be applicable to Non-homogenous, Encore, and Sodium Bisulfate preserved samples. See the [QA Manager](#) or Laboratory Director if unsure.

26.10.2 Policy on Data Omissions or Reporting Limit Increases

Fundamentally, our policy is simply to not omit previously reported results (including data qualifiers) or to not raise reporting limits and report sample results as ND. This policy has few exceptions. Exceptions are:

- Laboratory error.
- Sample identification is indeterminate (confusion between COC and sample labels).
- An incorrect analysis (not analyte) was requested (e.g., COC lists 8315 but client wanted 8310). A written request for the change is required.
- Incorrect limits reported based on regulatory requirements.
- The requested change has absolutely no possible impact on the interpretation of the analytical results and there is no possibility of the change being interpreted as misrepresentation by anyone inside or outside of our company.

26.10.3 Multiple Reports

TestAmerica does not issue multiple reports for the same workorder where there is different information on each report (this does not refer to copies of the same report) unless required to meet regulatory needs and approved by QA.

Figure 26-1.

Read and Understand Memo for
Electronic Reporting and Electronic Signatures Policy

I have read and understand the TestAmerica Policy on Electronic Reporting and Electronic Signatures and agree to follow procedures stated in this document. Furthermore, I agree to maintain my password secure and confidential and will not divulge this password to anyone. I am aware that my electronic signature is as legally binding as that of my signature signed with a pen. I will not apply my signature until I have reviewed each page.

Employee:

Signature: _____

Date: _____

Return this signed form to HR within 5 days for filing in your Personnel File

Figure 26-2.

AGREEMENT FOR ELECTRONIC REPORTS

TestAmerica provides laboratory services and certified lab reports (“Reports”) to the undersigned client (“Client”). Client desires to receive the Reports in both written hard copy and electronic format. Both TestAmerica and the Client desire to protect and preserve the integrity of the Reports.

TestAmerica agrees to provide Client with the Reports in both hard copy and electronic format. Client agrees to accept all responsibility for and indemnify and hold TestAmerica harmless from all claims or demands from third parties, including attorneys’ fees and costs incurred by TestAmerica, due to alterations or deletions to the Reports by Client, or the use of incomplete Reports by Client.

Client agrees not to alter any Reports whether in the hard copy or electronic format and to use reasonable efforts to preserve the Reports in the form and substance originally provided by TestAmerica.

Date: _____ **Company Name:** _____

Completed By: _____

Title/Position: _____

Client Signature: _____

Date: _____ Company Name: _____ TestAmerica Location

Received By: _____

Title/Position: _____

Signature: _____

Please sign and FAX to [xxx-xxx-xxxx](tel:xxx-xxx-xxxx)

Appendix 1.

**TESTAMERICA
ETHICS POLICY No. CA-L-P-001**

Refer to CA-L-P-001 for complete policy.

**TestAmerica
EMPLOYEE ETHICS STATEMENT**

I understand that TestAmerica is committed to ensuring the highest standard of quality and integrity of the data and services provided to our clients. I have read the Ethics Policy of the Company.

- *With regard to the duties I perform and the data I report in connection with my employment at the Company, I agree that:*
- *I will not intentionally report data values that are inconsistent with the actual values observed or measured.*
- *I will not intentionally report the dates, times, sample or QC identifications, or method citations of data analyses that are not the actual dates, times, sample or QC identifications, or method citations.*
- *I will not intentionally misrepresent another individual's work as my own or represent my own work as someone else's.*
- *I will not intentionally misrepresent any data where data does not meet Method or QC requirements. If it is to be reported, I will report it with all appropriate notes and/or qualifiers; I shall not modify data (either sample or QC data) unless the modification can be technically justified through a measurable analytical process, such as one deemed acceptable to the laboratory's Standard Operating Procedures, Quality Assurance Manual or Technical Director. All such modifications must be clearly and thoroughly documented in the appropriate laboratory notebooks/worksheets and/or raw data and include my initials or signature and date.*
- *I shall not make false statements to, or seek to otherwise deceive, members of Management or their representatives, agents, or clients/customers. I will not, through acts of commission, omission, erasure, or destruction, improperly report measurement standards, quality control data, test results or conclusions.*
- *I shall not compare or disclose results for any Performance Testing (PT) sample, or other similar QA or QC requirements, with any employee of any other laboratory, including any other TestAmerica laboratory, prior to the required submission date of the results to the person, organization, or entity supplying the PT sample.*
- *I shall immediately inform my supervisor or other member of management regarding any intentional or unintentional reporting of my own inauthentic data. Such report shall be given both orally and in writing to the supervisor or other member of management contacted and to the local Quality Assurance Manager. The Quality Assurance Manager will initial and date the information and return a copy to me. I shall not condone any accidental or intentional reporting of inauthentic data by other employees and will immediately report its occurrence. If I have actual knowledge of such acts committed by any other employees, and I do not report such information to designated members of Management, it shall be considered as serious as if I personally committed the offense. Accordingly, in that event, I understand that I may be subject to immediate termination of employment.*
- *I understand that if any supervisor, manager, or representative of TestAmerica management instructs, requests, or directs me to perform any of the aforementioned improper laboratory practices, or if I am in doubt or uncertain as to whether or not such laboratory practices are proper, I will not*

comply. In fact, I must report such event to all appropriate members of Management including, but not limited to, the Lab Director, all supervisors and managers with direct line reporting relationship between me and the Lab Director, and the local Quality Assurance representative, excluding such individuals who participated in such perceived improper instruction, request, or directive. In addition, I may contact Corporate Quality Assurance / Ethics Compliance Officer(s) for assistance.

- I understand the critical importance of accurately reporting data, measurements, and results, whether initially requested by a client, or retained by TestAmerica and submitted to a client at a later date, or retained by TestAmerica for subsequent internal use;*
- I will not share the pricing or cost data of Vendors or Suppliers with anyone outside of the TestAmerica family of companies.*
- I shall not accept gifts of a value that would adversely influence judgment.*
- I shall avoid conflicts of interest and report any potential conflicts to the management (e.g. employment or consulting with competitors, clients, or vendors).*
- I shall not participate in unfair competition practices (e.g. slandering competitors, collusion with other labs to restrict others from bidding on projects).*
- I shall not misrepresent certifications and status of certifications to clients or regulators.*
- I shall not intentionally discharge wastes illegally down the drain or onto the ground.*
- I understand that any attempt by management or an employee to circumvent these policies will be subject to disciplinary action.*

As a TestAmerica employee, I understand that I have the responsibility to conduct myself with integrity in accordance with the ethical standards described in the Ethics Policy. I will also report any information relating to possible kickbacks or violations of the Procurement Integrity Act, or other questionable conduct in the course of sales or purchasing activities. I will not knowingly participate in any such activity and will report any actual or suspected violation of this policy to management.

I understand that if my job includes supervisory responsibilities, I shall not instruct, request, or direct any subordinate to perform any laboratory practice which is unethical or improper. Also, I shall not discourage, intimidate, or inhibit an employee who may choose to appropriately appeal my supervisory instruction, request, or directive which the employee perceives to be improper, nor retaliate against those who do.

The Ethics Policy has been explained to me by my supervisor or at a training session, and I have had the opportunity to ask questions if I did not understand any part of it. I understand that any violation of this policy subjects me to disciplinary action, which can include termination of my employment. In addition, I understand that any violation of this policy which relates to work under a government contract or subcontract could also subject me to the potential for prosecution under federal law.

EMPLOYEE SIGNATURE _____

Date _____

Supervisor/Trainer: _____

Date _____

Work Instruction No. CA-WI-005

TestAmerica
CONFIDENTIALITY AND PROPRIETARY INFORMATION AGREEMENT

TestAmerica and their predecessors, in their businesses, have developed and use commercially valuable technical and non-technical information and to guard the legitimate interests of TestAmerica and its clients, it is necessary to protect certain information as confidential and proprietary.

I, _____, understand and acknowledge that during the term of my employment by TestAmerica, I will be privy to and entrusted with certain confidential information and trade secrets of TestAmerica and its clients.

Confidential information and trade secrets include, but are not limited to: customer and client lists; price lists; marketing and sales strategies and procedures; operational and equipment techniques; standard operating procedures; business plans and systems; quality control procedures and systems; special projects and technological research, including projects, research and reports for any government entity or client; client's plans and processes; client's manner of operation; the trade secrets of clients; client's data; vendor or supplier pricing; employee lists and personal information, and any other records, data, files, drawings, inventions, discoveries, applications, or processes which are not in the public domain.

I agree as follows:

1. I will not in any way, during the term of my employment, or at any time thereafter, except as authorized in writing by the Legal Department of TestAmerica or the client where client data is involved, disclose to others, use for my own benefit, remove from TestAmerica's premises (except to the extent off-site work is approved by my supervisor), copy or make notes of any confidential information and/or trade secrets of TestAmerica or its clients, excepting only that information which may be public knowledge. Technical and business information of any previous employer or other third party which I may disclose to TestAmerica shall be limited to that which was acquired legitimately and disclosed to me without restriction as to secrecy.
2. I agree that all inventions (whether or not patentable) conceived or made by me during the period of my employment by TestAmerica shall belong to TestAmerica, provided such inventions grow out of my work for TestAmerica and are related to the business of TestAmerica. I agree to disclose and assign such inventions to TestAmerica. In California, this provision shall not apply to any invention which qualifies fully under Section 2870 of the California Labor Code.
3. On termination of my employment from TestAmerica, I will deliver to TestAmerica all documents, records, notes, data, memoranda, files, manuals, equipment and things of any nature which relate in any way to confidential information and/or trade secrets of TestAmerica or its clients and which are in my possession or under my control.
4. I agree that during the period of my employment and for one (1) year from and after the termination (for any reason) of my employment with TestAmerica, I shall not directly or indirectly (without first obtaining the written permission of TestAmerica), recruit for employment, or induce to terminate his or her employment with TestAmerica, any person who is an active employee of TestAmerica on the last day of my employment with TestAmerica.
5. I acknowledge that if I were to breach any provision of this Confidentiality Agreement, money damages will be inadequate, and I hereby agree that TestAmerica shall be entitled, where appropriate, to specific performance and/or injunctive relief (i.e. to require me to comply with this Agreement). I further acknowledge that the willingness of TestAmerica to hire me or to continue my employment constitutes full and adequate consideration for the agreements, and obligations to which I have agreed as set forth in this document.

I have executed this Agreement, intending to be legally bound.

Printed Name

Signature


Date

Work Instruction No. CA-WI-006

Appendix 2.


Example Laboratory Organization Chart

(The most current chart can be obtained from the QA Manager or Lab Director)

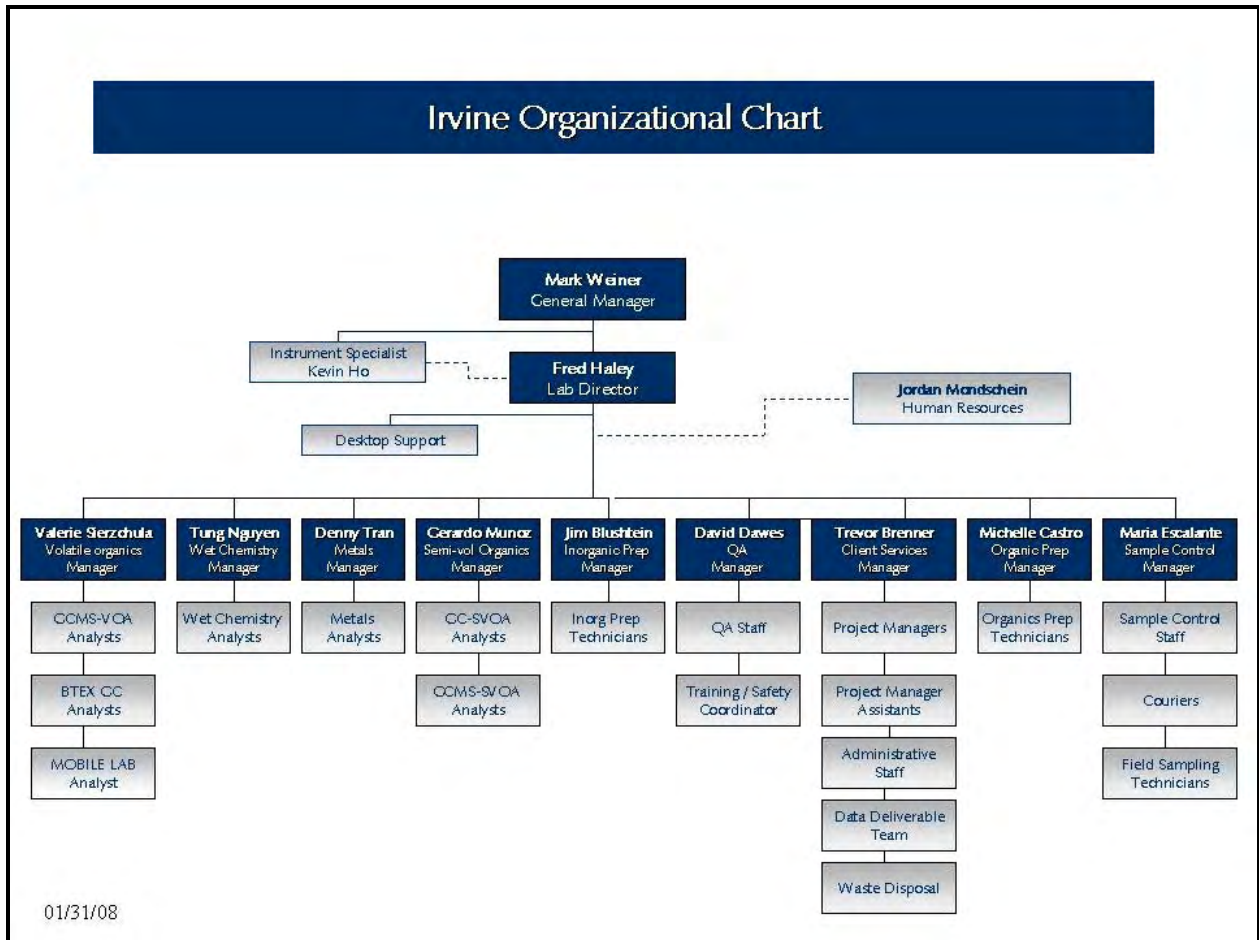

Appendix 3.

Laboratory Floor Plan

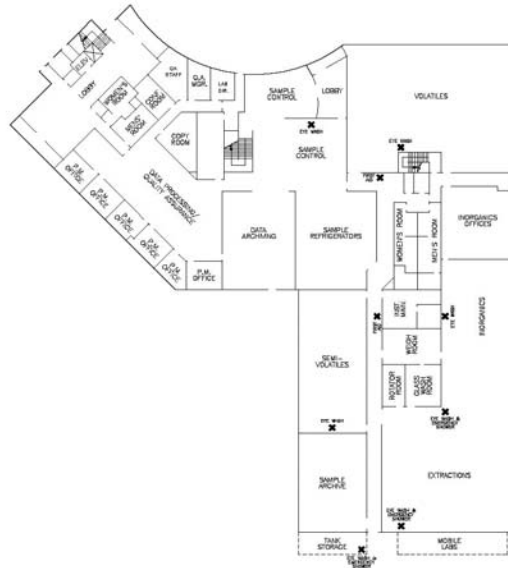

FIRST FLOOR
IRVINE LABORATORY



SECOND FLOOR
CORPORATE OFFICES

Appendix 4: Summary of Calibration and QC Procedures

The following tables are summaries of select method-specified calibration and QC requirements for select laboratory methods. For more information, actual limits, and any method-deviations, please see the current revision of the laboratory's SOP.

QC Acceptance Criteria for Method EPA 8260B					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 8260B	Volatile Organic Compounds	BFB tuning	Prior to initial calibration and calibration verification	Table 2 criteria met (Method 8260B – Table4)	Retune instrument and verify
		5-point initial calibration for all analytes. (6-point for quadratic regression)	Initial calibration prior to sample analysis.	SPCCs minimum RFs: > 0.10 (BF, CM, DM) and > 0.30 (CB, TE). %RSD of RFs: < 30(for CCCs, Ketone and Alcohols); < 15for others. Calibration Curve (If %RSD > 15): coefficient factor, r > 0.99	Correct problem then repeat initial calibration.
		Retention time window calculated for each analyte	Each initial calibration and calibration verifications	± 3 times standard deviation for each analyte retention time from 72-hour study	Correct problem then reanalyze all samples analyzed since the last retention time check
		2nd source Calibration verification (same as LCS)	Daily, before sample analysis and every 12 hours of analysis time	SPCCs minimum RFs met. CCCs: < 20% drift from initial calibration. Others: in-house recovery limits.	Correct problem then repeat initial calibration
		Method blank	One per analytical batch of 20 samples	No analytes detected ≥ RL.	Correct problem and re-analyze method blank and all samples processed with the contaminated blank unless sample results are

QC Acceptance Criteria for Method EPA 8260B					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 8260B	Volatile Organic Compounds				ND for the contamination compound or sample results are > 20 times the level found in the blank
		LCS for all analytes (2nd source)	One LCS per analytical batch	In-house statistical limits	If sufficient sample is available for re-analysis, correct problem and re-analyze the LCS and all samples in the affected analytical batch unless samples are ND for the affected compound(s) and LCS is biased high
		MS/MSD	One MS/MSD per every 20 project samples per matrix	In-house statistical limits	Qualifier to indicate matrix interference
		Internal standard	Every sample, calibration check, method blank, LCS, MS/MSD	Retention time within ± 30 seconds from last mid-point calibration standard Absolute areas within 50-200% of level in last mid-point calibration standard	Determine, correct problem and re-analyze samples
		Surrogate spike	Every sample, calibration check, method blank, LCS, MS/MSD	In-house statistical limits	Determine, correct problem and re-analyze samples. For matrix effect, flag result accordingly. For other causes, fill out a CAR
		MDL study	One full MDL run originally. Verification every quarter.	MDLs established per 40CFR – Part 136	None

QC Acceptance Criteria for Method EPA 8260B					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
		Initial Demonstration of Capability (4 replicates of LCS)	Once per analyst	Average recovery and precision within in-house statistical limits	Recalculate results; determine and correct problem with the system and then rerun demonstration for those analytes that did not meet criteria

QC Acceptance Criteria for Method EPA 8270C					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 8270C	Volatile Organic Compounds	DFTPP tuning	Prior to initial calibration and calibration verification	Table 3 of method 8270C DDT degradation < 20%, Benzidine and Pentachlorophenol tailing factors < 3 and < 5 respectively	Retune instrument and verify
		5-point initial calibration for all analytes. (6-point for quadratic regression)	Initial calibration prior to sample analysis.	SPCCs minimum RFs: > 0.05 %RSD of RFs: < 30(for CCCs); < 15 for others. Calibration Curve (If %RSD > 15): coefficient factor, r > 0.99	Correct problem then repeat initial calibration.
		Retention time window calculated for each analyte	Each initial calibration and calibration verifications	± 3 times standard deviation for each analyte retention time from 72-hour study	Correct problem then reanalyze all samples analyzed since the last retention time check
		2nd source Calibration verification (same as LCS)	Once, after ICAL	SPCCs minimum RFs met. CCCs: < 20% drift from initial calibration. Others: in-house recovery limits.	Correct problem then repeat initial calibration
		Method blank	One per analytical	No analytes detected ≥ RL.	Correct problem, re-extract and/or re-analyze

QC Acceptance Criteria for Method EPA 8270C					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
			batch of 20 samples		method blank and all samples processed with the contaminated blank unless sample results are ND for the contamination compound or sample results are > 20 times the level found in the blank
		LCS for all analytes (2nd source)	One LCS per analytical batch	In-house statistical limits	If sufficient sample is available for re-analysis, correct problem and re-analyze the LCS and all samples in the affected analytical batch unless samples are ND for the affected compound(s) and LCS is biased high
		MS/MSD	One MS/MSD per every 20 project samples per matrix	In-house statistical limits	Qualifier to indicate matrix interference
		Internal standard	Every sample, calibration check, method blank, LCS, MS/MSD	Retention time within ± 30 seconds from last mid-point calibration standard Absolute areas within 50-200% of level in last mid-point calibration standard	Determine, correct problem and re-analyze samples
		Surrogate spike	Every sample, calibration check, method blank, LCS, MS/MSD	In-house statistical limits	Determine, correct problem and re-analyze samples. For matrix effect, flag result accordingly. For other causes, fill out a CAR
		MDL study	One full MDL run originally. Verification every quarter.	MDLs established per 40CFR – Part 136	None

QC Acceptance Criteria for Method EPA 8270C					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
		Initial Demonstration of Capability (4 replicates of LCS)	Once per analyst	Average recovery and precision within in-house statistical limits	Recalculate results; determine and correct problem with the system and then rerun demonstration for those analytes that did not meet criteria

QC Acceptance Criteria for Method EPA 8081A					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 8081A	DDT, BHC and other Organochlorine Pesticides	5-point initial calibration for all analytes.	Initial calibration prior to sample analysis.	%RSD of RFs (or Average of %RSD): < 20 for all compounds Calibration Curve (If %RSD > 20 and <50): Correlation coefficient, r > 0.99	1. % RSD may be used if the average % RSD of all compounds is 20% and sample results are ND for any target compound with %RSD > 20% 2. Correct problem then repeat initial calibration
		Second-source calibration verification for all analytes	Once per five-point initial calibration	All target analytes within $\pm 15\%$ of expected value	1. If the average recovery of all compounds is within 15% and sample results are ND, then the results will be reported with an additional form indicating the individual compounds exceeding the 15% limit 2. Otherwise, correct problem then repeat initial calibration
		Retention time window calculated for each analyte	Every 6 months	± 3 times standard deviation for each analyte retention time from 72-hour study	None
		Continuing calibration verification	After every 20 samples and at the end of the analysis sequence	All target analytes within $\pm 15\%$ of expected value and all compounds correctly identified by RT	1. If the average recovery of all compounds is within 15% and sample results are ND, then the results will be reported with an additional form indicating the individual compounds exceeding the 15% limit.

QC Acceptance Criteria for Method EPA 8081A					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
					2. Correct problem then repeat initial calibration verification and reanalyze all samples since last successful calibration verification.
EPA 8081A	DDT, BHC and other Organochlorine Pesticides	Method blank	One per analytical batch	No analytes detected \geq RL	Correct problem then reprep and analyze method blank and all associated samples unless sample results are ND for the contamination compound or sample results are $>x$ 10 times the level found in the blank
		LCS for all analytes	One LCS per analytical batch	In-house statistical limits	If sufficient sample is available for re-extraction correct problem then reprep and analyze the LCS and all samples in the affected analytical batch unless samples are ND for the affected compound(s) and LCS is biased high
		Surrogate spike	Every sample, spiked sample, standard, and method blank	In-house statistical limits	<ol style="list-style-type: none"> 1. Re-analyze the sample one time. Evaluate data and, if matrix effects are indicated, report results and Flag surrogate recovery 2. If sample is available for re-extraction, correct problem then re-extract and analyze samples 3. Otherwise report results with a corrective action report indicating the cause of the problem
		MS/MSD	One MS/MSD per every 20 project samples per matrix	In-house statistical limits	Qualify samples to indicate matrix interference

QC Acceptance Criteria for Method EPA 8081A					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
		MDL study	One full MDL run originally. Verified every quarter	MDLs established per 40CFR – Part 136	None
		Initial Demonstration of Capability (4 replicates of LCS)	Once per analyst	Average recovery and precision within in-house statistical limits	Recalculate results; locate and fix problem with system and then rerun demonstration for those analytes that did not meet criteria

QC Acceptance Criteria for Method EPA 8082					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 8082	PCBs	Minimum 5-point initial calibration Aroclors 1016 and 1260 (Additional 3-point calibrations are to be created and maintained whenever other Aroclors are identified in samples)	Initial calibration prior to sample analysis.	<u>%RSD of RFs</u> : ≤ 20 for each compound <u>Calibration Curve (If %RSD > 20):</u> Linear, NOT forced through zero, $r \geq 0.990$	Correct problem then repeat initial calibration.
		Retention time window calculated for each analyte	Each initial calibration	± 3 times standard deviation for each analyte retention time from 72-hour study	None

QC Acceptance Criteria for Method EPA 8082					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
		Second-source calibration verification for all analytes	Once per initial calibration	All analytes within $\pm 15\%$ of expected value	<ol style="list-style-type: none"> 4. Re-analyze once to confirm. 5. Correct problem then repeat initial calibration.
		Retention time window check	All CCVs	Each congener is within established absolute RT window	Determine the cause, correct the problem and reanalyze all affected samples.
		Continuing calibration verification	After every 10-20 samples and at the end of the analysis sequence	All analytes within $\pm 15\%$ of expected value	<ol style="list-style-type: none"> 1. If the ICV/CCV result is $> 115\%$ of the expected value and all samples are ND for the compound then report the results with a CAR and flag the results with a 'C' qualifier. 2. If the CCV result is $< 85\%$ of the expected value, reanalyze the samples against an acceptable calibration curve one time. 3. If the CCV fails again due to matrix interference and the sample is ND or a hit, report results with a CAR and flag 'C4'. If there is a PCB hit in the sample at or below the RL, then analyze a standard at the RL. If the area count of the sample is $<$ the area count of the RL standard, report as ND and flag 'C4.'
		Second Column Confirmation	Every sample	Results agree within 40%	If the second column does not agree within 40% but still confirms the presence of the analyte then confirmation is qualitative. The higher result must be reported or the sample reanalyzed under a new calibration or on another instrument
		Method blank	One per analytical batch	No analytes detected \geq RL	Correct problem then reprep and analyze method blank and all associated samples unless sample results are ND for the contamination compound or sample results are $> x20$ times the level found in the blank

QC Acceptance Criteria for Method EPA 8082					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
		LCS for all analytes	One LCS per analytical batch	In-house statistical limits	If sufficient sample is available for re-extraction correct problem then reprep and analyze the LCS and all samples in the affected analytical batch unless samples are ND for the affected compound(s) and LCS is biased high
		Surrogate spike	Every sample, spiked sample, standard, and method blank	In-house statistical limits	<ol style="list-style-type: none"> 2. Re-analyze the sample one time. Evaluate data and, if matrix effects are indicated, report results and Flag surrogate recovery 3. If sample is available for re-extraction, correct problem then re-extract and analyze samples 6. Otherwise report results with a corrective action report indicating the cause of the problem
		MS/MSD	One MS/MSD per every 20 project samples per matrix	In-house statistical limits	Qualify samples to indicate matrix interference
		MDL study	One full MDL run originally. Verified every quarter	MDLs established per 40CFR – Part 136	None
		Initial Demonstration of Capability (4 replicates of LCS)	Once per analyst	Average recovery and precision within in-house statistical limits	Recalculate results; locate and fix problem with system and then rerun demonstration for those analytes that did not meet criteria

QC Acceptance Criteria for Method EPA 8015					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 8015	Volatile Fuel Hydrocarbons (VFH, C6-C12)	5-point initial calibration	Initial calibration prior to sample analysis.	20% RSD for calibration point RFs	Correct problem then repeat initial calibration
		Second-source calibration verification (ICV/CCV)	Initially and every 12 hours or 10 samples	±15% of expected value	7. Re-analyzed once 8. Correct problem and re-analyze all affected samples.
		Retention time window calculated for each analyte	Every 6 months	± 3 times standard deviation for each analyte retention time from 72-hour study	None
		Method blank	One per analytical batch	No analytes detected ≥ RL	Correct problem then reprep and analyze method blank and all associated samples unless sample results are ND for the contamination compound or sample results are >20 times the level found in the blank
		LCS for all analytes	One LCS per analytical batch	In-house statistical limits	If sufficient sample is available, correct problem and analyze the LCS and all samples in the affected analytical batch unless samples are ND and LCS is biased high
		Surrogate spike	Every sample, spiked sample, standard, and	In-house statistical limits	3. Evaluate secondary surrogate. 4. If matrix effects are indicated, report results

QC Acceptance Criteria for Method EPA 8015					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 8015	Volatile Fuel Hydrocarbons (VFH, C6-C12)		method blank		and flag surrogate recovery
		MS/MSD	One MS/MSD per every 20 project samples per matrix	In-house statistical limits	Qualify samples to indicate matrix interference
		MDL study	One full MDL run originally. Verified every quarter	MDLs established per 40CFR – Part 136	None
		Initial Demonstration of Capability (4 replicates of LCS)	Once per analyst	Average recovery and precision within in-house statistical limits	Recalculate results; locate and fix problem with system and then rerun demonstration for those analytes that did not meet criteria

QC Acceptance Criteria for Method EPA 6010B					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 6010B	ICP Metals	Initial multipoint calibration (minimum 3 standards and a blank)	Daily initial calibration prior to sample analysis	Correlation coefficient ≥ 0.995 for linear regression	Correct problem then repeat initial calibration
		2 nd source initial calibration verification	Immediately after initial calibration	All analytes within $\pm 10\%$ of expected value	1) Reanalyze once 2) If still out, correct problem then repeat initial calibration
		Calibration blank	After every 10 samples and at end of the analysis sequence	No analytes beyond $\geq \pm RL$	Reanalyze the blank. If it still fails, correct problem then analyze calibration blank and previous 10 samples unless sample results >10 times the absolute level found in the blank
		Continuing calibration verification (Instrument Check Standard)	After every 10 samples and at end of the analysis sequence	All analyte(s) within $\pm 10\%$ of expected value	Repeat calibration and reanalyze all samples since last successful CCV
		Interference check solution (ICSA)	At least weekly, before sample analysis	Interfering elements (Al, Ca, Fe, Mg) within $\pm 20\%$ of expected value . Target elements: ± 2 Reporting Limit.	Dilute ICSA and/or samples
		Method blank	One per analytical batch	No analytes detected $\geq RL$	Correct problem then reprep and analyze method blank and all samples processed with the contaminated blank unless sample results are ND for the contaminatate compound or sample results are > x 10 times the level found in the blank

QC Acceptance Criteria for Method EPA 6010B					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
		LCS for all elements	One LCS per analytical batch	All elements within $\pm 20\%$ of expected value	If sufficient sample is available for re-extraction correct problem then reprep and analyze the LCS and all samples in the affected analytical batch unless samples are ND for the affected element(s) and the LCS is biased high
		MS/MSD	One MS/MSD per every 20 project samples per matrix	Within 75-125% of expected results	None
		Internal standard	Each sample	Within 30-120% of the intensity level in the initial calibration standard	Correct problem and/or dilute sample
		MDL study	One full MDL run originally. Verification every quarter	MDLs established per CFR 40 – Part 136	None
		Initial Demonstration of Capability (4 replicates of LCS)	Once per analyst	Average and precision within in-house statistical limits	Recalculate results; locate and fix problem with system and then rerun demonstration for those analytes that did not meet criteria

Summary of Calibration and QC Procedures for Method EPA 6020

Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 6020	ICPMS Metals	Pre-calibration mass tuning & performance check	Daily, before initial calibration	See ICPMS – Mass tuning and performance check	Correct problem then retune instrument and verify
		Initial multipoint calibration (3 standards and a blank in triplicate)	Daily initial calibration prior to sample analysis	Correlation coefficient ≥ 0.995 for linear regression	Correct problem then repeat initial calibration
		2 nd source initial calibration verification (ICV)	Immediately after initial calibration	All analytes within $\pm 10\%$ of expected value	1) Reanalyze once 2) If still out, correct problem then repeat initial calibration
		Calibration blank (ICB / CCB)	After ICV and CCV	No analytes $\geq \pm RL$	Reanalyze the blank. If it still fails, correct problem then analyze calibration blank and previous 10 samples unless sample results are $>10x$ the absolute level found in the blank
		Interference check solution (ICSA / ICSAB)	Daily, before sample analysis and every 12 hours	Target elements: within $\pm 5ppb$ (Zn: 15ppb) in ICSA and $\pm 30\%$ (Zn: $\pm 50\%$) of expected value in ICSAB. Interfering elements: NA (above linear range)	Terminate analysis; correct problem; reanalyze ICS; reanalyze all affected samples
		Continuing calibration verification (CCV)	After every 10 samples and at the end of the analysis sequence	All analytes within $\pm 10\%$ of expected value	Repeat calibration and reanalyze all samples since last successful calibration
		LCS for all elements	One LCS per	All elements within $\pm 20\%$ of expected value	If sufficient sample is available for re-extraction

Summary of Calibration and QC Procedures for Method EPA 6020

Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
			analytical batch of 20 samples		correct problem then reprep and analyze the LCS and all samples in the affected analytical batch unless samples are ND for the affected element(s) and the LCS is biased high
		Method blank	One per analytical batch	No analytes detected \geq RL	Correct problem then reprep and analyze method blank and all samples processed with the contaminated blank unless sample results are ND for the contaminatate compound or sample results are > 10 times the level found in the blank
		MS/MSD	One MS/MSD per analytical batch	Within 75-125% of expected results	Perform Post-digestion spike
		Post-digestion spike	When MS/MSD fails	Within 75-125% of expected results	Qualifier to indicate matrix interference. Issue a CAR for other causes
		Internal standard	Each sample	Within 30-120% of the intensity level in the initial calibration standard	Correct problem and/or dilute sample
		Initial Demonstration of Capability (4 replicates of LCS)	Once per analyst	Average recovery of all elements within $\pm 20\%$ of expected value and precision within 20%	Recalculate results; locate and fix problem with system and then rerun demonstration for those analytes that did not meet criteria
		IDL Study	Quarterly	IDLs calculated from the average standard deviations of three blanks run on three non-consecutive days (each blank run 7 consecutive times)	None
		MDL study	Biannually	MDLs established per CFR 40 – Part 13	None

QC Acceptance Criteria for Method EPA 300.0					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 300.0	Common Anions	Multipoint calibration for all analytes (minimum 3 standards and one calibration blank)	Initial calibration prior to sample analysis	Correlation coefficient ≥ 0.995 for linear regression	Correct problem then repeat initial calibration
		Second-source calibration verification	Once per multipoint calibration	All analytes within $\pm 10\%$ of expected value	Correct problem then repeat initial calibration
		Retention time window calculated for each analyte	Annually	± 3 times standard deviation for each analyte retention time from 72-hour study	Correct problem then reanalyze all samples analyzed since the last retention time check
		Instrument Performance Check (IPC)	Daily, before sample analysis or when eluent is changed	All analytes within $\pm 10\%$ of expected value	Correct problem then repeat initial calibration
		Continuing calibration verification (CCV)	After every 10 samples and at the end of the analysis sequence (second source standard)	All analytes within $\pm 10\%$ of expected value	<ol style="list-style-type: none"> 1. Correct problem then repeat initial calibration verification and reanalyze all samples since last successful calibration verification 2. If the recovery is $> 110\%$ and sample results are ND results may be reported without re-analysis
		Method blank	One per analytical batch	No analytes detected \geq RL	Correct problem then reprep and analyze method blank and all samples processed with the contaminated blank unless sample results are ND for the contamination compound or sample results are > 10 times the level found in the blank

QC Acceptance Criteria for Method EPA 300.0					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
		LCS for all analytes. ICV or CCVs are reported as LCS since it is a second source standard.	One LCS per analytical batch	All analytes within +/- 10% of expected value	If sufficient sample is available for re-extraction correct problem then reprep and analyze the LCS and all samples in the affected analytical batch unless samples are ND and LCS is biased high.
		MS/MSD	One MS/MSD per every 20 project samples per matrix	In-house statistical limits	None
		Initial Demonstration of Capability (4 replicates of LCS)	Once per analyst	Average recovery within +/- 10% of expected value and precision within $\pm 20\%$	Recalculate results; locate and fix problem with system and then rerun demonstration for those analytes that did not meet criteria
		MDL study	One full MDL run originally. Verified quarterly.	MDLs established per 40CFR – Part 136	None

Acceptance Criteria for Method EPA 7470A/7471A - Mercury					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 7470A/ 7471A	Mercury	Initial calibration (5 points and a blank)	Daily	Linear regression and forced through zero curve , $r \geq 0.995$	Correct problem and repeat calibration
		2 nd source initial calibration verification (ICV)	Immediately after calibration	Recovery within 90-110% of expected value	Reprep and re-analyze ICV. If still outs, reprep calibration standards and re-calibrate
		Calibration Blank (ICB and CCB)	After ICV and CCV	Free of mercury or below reporting limit	Re-analyze samples bracketed by affected ICB and/or CCBs unless results are not detected or >10x the level found in the calibration blank
		Method blank	One per analytical batch of 20 samples	Free of mercury or below reporting limit	Re-digest and re-analyze the batch unless sample results are not detected or >10x the level found in the method blank
		LCS	One per analytical batch of 20 samples	Within in-house statistical limits	Re-digest and re-analyze the batch unless sample results are not detected and LCS is biased high
		MS / MSD	One MS/MSD set per batch	Within in-house statistical limits	Qualify samples to indicate matrix interference or issue a CAR for other causes
		Continuous calibration verification (CCV)	After every 10 sample analysis	Recovery within 80-120%	Re-analyze all samples bracketed by non-compliant CCVs
		MDL	One full MDL study originally. Verified quarterly	Established per 40CFR – Part 136	None
		Initial Demonstration of Capability (4 replicates of LCS)	Per analyst	Average recovery within in-house statistical limits	Correct problem and repeat the process

QC Acceptance Criteria for Method EPA 7196A – Hexavalent Chromium					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
EPA 7196A/ SM 3500Cr D	Hexavalent Chromium (Cr+6)	Initial Calibration (4-point and a blank)	Daily	Correlation coefficient (r) > 0.995	Reprep standards and recalibrate
		2 nd source calibration verification (ICV)	Immediately after calibration	Recovery within 90-110% of expected value	Reprep, rerun and verify result. Otherwise recalibrate
		Continuing calibration verification (CCV)	Every 10 samples and at end of run	EPA 7169A: recovery within 80-120% SM 3500Cr D: recovery within 90-110%	Reanalyzed once. If still fails, recalibrate and reanalyze all samples bracketed by the failed CCV.
		LCS	One per analytical batch	Recovery within in-house statistical limits	Correct problem, re-extract and rerun all associated samples unless sample results are not detected and LCS is biased high
		MS/MSD-soluble	One MS/MSD per analytical batch	Recovery within in-house statistical limits	Perform a post-digestion spike (PDS). Perform a PDS on all samples with results above the RL. If PDS ≥ 85% then flag as matrix interference (MI). If <85 and ≥ 50%, dilute and re-analyze if dilution still >RL otherwise use PDS as single-point MSA and flag as MI (no MSA for SM3500). If <50%, dilute and reanalyze with PDS and flag as MI
		MS-insoluble	One MS per analytical batch (SOILS ONLY)	Recovery within in-house statistical limits	Perform a post-digestion spike (PDS)
		MDL study	One full MDL study originally, reviewed after significant instrument maintenance or method modification	Established per 40 CFR – Part 136	None
	Initial Demonstration of Capability (4 replicates)	One per analyst	Average recovery and RSD within in-house statistical limits	Identify, correct problem and repeat process	

QC Acceptance Criteria for Method EPA 7196A – Hexavalent Chromium					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
		of LCS)			

QC Acceptance Criteria for Method EPA 9014 - Cyanide					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
9014	Cyanide	Initial Calibration 5-point and a blank)	Daily, prior to sample analysis	Linear regression, $r \geq 0.995$	Correct problem then repeat initial calibration
		2 nd source initial and continuous calibration verification (ICV / CCV)	Immediately after calibration and after every 10 samples	Within $\pm 15\%$ of expected value	Re-prepare / re-run ICV or CCV and verify recovery. Otherwise, recalibrate and re-run samples not bracketed between compliant CCVs
		Method blank (distilled)	One per analytical batch of 20 samples	Not detected or below Reporting Limit	Redistill method blank and all associated samples, unless sample results are not detected or $> 10x$ the blank level
		LCS (distilled)	One LCS per analytical batch	Within $\pm 10\%$ of the undistilled standard and true value	Correct the problem and redistill all associated samples, unless LCS is biased high and samples are not detected
		MS / MSD	One MS / MSD per analytical batch	Within in-house statistical limit	Qualify sample to indicate matrix interference

QC Acceptance Criteria for Method EPA 9014 - Cyanide					
Method	Applicable Parameter	QC Check	Minimum Frequency	Acceptance Criteria	Corrective Action
		MDL	Initially and after extensive instrument maintenance	Established per 40CFR – Part 136	None
		Demonstration of Capability (4 replicates of QC check)	Per analyst	Within in-house statistical limits	Identify, correct problem and repeat process

Appendix 5. Glossary/Acronyms

Glossary:

Acceptance Criteria:

Specified limits placed on characteristics of an item, process, or service defined in requirement documents. (ASQC)

Accreditation:

The process by which an agency or organization evaluates and recognizes a laboratory as meeting certain predetermined qualifications or standards, thereby accrediting the laboratory. In the context of the National Environmental Laboratory Accreditation Program (NELAP), this process is a voluntary one. (NELAC)

Accrediting Authority:

The Territorial, State, or Federal Agency having responsibility and accountability for environmental laboratory accreditation and which grants accreditation (NELAC) [1.5.2.3]

Accuracy:

The degree of agreement between an observed value and an accepted reference value. Accuracy includes a combination of random error (precision) and systematic error (bias) components which are due to sampling and analytical operations; a data quality indicator. (QAMS)

Analyst:

The designated individual who performs the “hands-on” analytical methods and associated techniques and who is the one responsible for applying required laboratory practices and other pertinent quality controls to meet the required level of quality. (NELAC)

Assessment:

The evaluation process used to measure or establish the performance, effectiveness, and conformance of an organization and/or its systems to defined criteria (to the standards and requirements of NELAC). (NELAC)

Assessment Criteria:

The measures established by NELAC and applied in establishing the extent to which an applicant is in conformance with NELAC requirements. (NELAC)

Assessment Team:

The group of people authorized to perform the on-site inspection and proficiency testing data evaluation required to establish whether an applicant meets the criteria for NELAP accreditation. (NELAC)

Assessor:

One who performs on-site assessments of accrediting authorities and laboratories' capability and capacity for meeting NELAC requirements by examining the records and other physical evidence for each one of the tests for which accreditation has been requested. (NELAC)

Audit:

A systematic evaluation to determine the conformance to quantitative and qualitative specifications of some operational function or activity. (EPA-QAD)

Batch:

Environmental samples which are prepared and/or analyzed together with the same process and personnel, using the same lot(s) of reagents. A preparation batch is composed of one to 20 environmental samples of the same matrix, meeting the above mentioned criteria and with a maximum time between the start of processing of the first and last sample in the batch to be 24 hours. An analytical batch is composed of prepared environmental samples (extracts, digestates or concentrates) and /or those samples not requiring preparation, which are analyzed together as a group using the same calibration curve or factor. An analytical batch can include samples originating from various environmental matrices and can exceed 20 samples. (NELAC Quality Systems Committee)

Blank:

A sample that has not been exposed to the analyzed sample stream in order to monitor contamination during sampling, transport, storage or analysis. The blank is subjected to the usual analytical and measurement process to establish a zero baseline or background value and is sometimes used to adjust or correct routine analytical results. (ASQC)

Blind Sample:

A sample for analysis with a composition known to the submitter. The analyst/laboratory may know the identity of the sample but not its composition. It is used to test the analyst's or laboratory's proficiency in the execution of the measurement process.

Calibration:

To determine, by measurement or comparison with a standard, the correct value of each scale reading on a meter, instrument, or other device. The levels of the applied calibration standard should bracket the range of planned or expected sample measurements. (NELAC)

Calibration Curve:

The graphical relationship between the known values, such as concentrations, of a series of calibration standards and their instrument response. (NELAC)

Calibration Method:

A defined technical procedure for performing a calibration. (NELAC)

Calibration Standard:

A substance or reference material used to calibrate an instrument (QAMS)

Certified Reference Material (CRM):

A reference material one or more of whose property values are certified by a technically valid procedure, accompanied by or traceable to a certificate or other documentation which is issued by a certifying body. (ISO Guide 30-2.2)

Chain of Custody:

An unbroken trail of accountability that ensures the physical security of samples and includes the signatures of all who handle the samples. (NELAC) [5.12.4]

Clean Air Act:

The enabling legislation in 42 U.S.C. 7401 et seq., Public Law 91-604, 84 Stat. 1676 Pub. L. 95-95, 91 Stat., 685 and Pub. L. 95-190, 91 Stat., 1399, as amended, empowering EPA to promulgate air quality standards, monitor and enforce them. (NELAC)

Comprehensive Environmental Response, Compensation and Liability Act (CERCLA/SUPERFUND):

The enabling legislation in 42 U.S.C. 9601-9675 et seq., as amended by the Superfund Amendments and Reauthorization Act of 1986 (SARA), 42 U.S.C. 9601 et seq., to eliminate the health and environmental threats posed by hazardous waste sites. (NELAC)

Compromised Samples:

Those samples which are improperly sampled, insufficiently documented (chain of custody and other sample records and/or labels), improperly preserved, collected in improper containers, or exceeding holding times when delivered to a laboratory. Under normal conditions, compromised samples are not analyzed. If emergency situation require analysis, the results must be appropriately qualified. (NELAC)

Confidential Business Information (CBI):

Information that an organization designates as having the potential of providing a competitor with inappropriate insight into its management, operation or products. NELAC and its representatives agree to safeguarding identified CBI and to maintain all information identified as such in full confidentiality.

Confirmation:

Verification of the identity of a component through the use of an approach with a different scientific principle from the original method. These may include, but are not limited to:

- Second column confirmation
- Alternate wavelength
- Derivatization
- Mass spectral interpretation
- Alternative detectors or
- Additional Cleanup procedures

(NELAC)

Conformance:

An affirmative indication or judgement that a product or service has met the requirements of the relevant specifications, contract, or regulation; also the state of meeting the requirements. (ANSI/ASQC E4-1994)

Corrective Action:

The action taken to eliminate the causes of an existing nonconformity, defect or other undesirable situation in order to prevent recurrence. (ISO 8402)

Data Audit:

A qualitative and quantitative evaluation of the documentation and procedures associated with environmental measurements to verify that the resulting data are of acceptable quality (i.e., that they meet specified acceptance criteria). (NELAC)

Data Reduction:

The process of transforming raw data by arithmetic or statistical calculations, standard curves, concentration factors, etc., and collation into a more useable form. (EPA-QAD)

Deficiency:

An unauthorized deviation from acceptable procedures or practices, or a defect in an item. (ASQC)

Detection Limit:

The lowest concentration or amount of the target analyte that can be identified, measured, and reported with confidence that the analyte concentration is not a false positive value. See Method Detection Limit. (NELAC)

Document Control:

The act of ensuring that documents (and revisions thereto) are proposed, reviewed for accuracy, approved for release by authorized personnel, distributed properly, and controlled to ensure use of the correct version at the location where the prescribed activity is performed. (ASQC)

Duplicate Analyses:

The analyses or measurements of the variable of interest performed identically on two subsamples of the same sample. The results from duplicate analyses are used to evaluate analytical or measurement precision but not the precision of sampling, preservation or storage internal to the laboratory. (EPA-QAD)

Environmental Detection Limit (EDL):

The smallest level at which a radionuclide in an environmental medium can be unambiguously distinguished for a given confidence interval using a particular combination of sampling and measurement procedures, sample size, analytical detection limit, and processing procedure. The EDL shall be specified for the 0.95 or greater confidence interval. The EDL shall be established initially and verified annually for each test method and sample matrix. (NELAC Radioanalysis Subcommittee)

Equipment Blank:

Sample of analyte-free media which has been used to rinse common sampling equipment to check effectiveness of decontamination procedures. (NELAC)

External Standard Calibration:

Calibrations for methods that do not utilize internal standards to compensate for changes in instrument conditions.

Federal Insecticide, Fungicide and Rodenticide Act (FIFRA):

The enabling legislation under 7 U.S.C. 135 et seq., as amended, that empowers the EPA to register insecticides, fungicides, and rodenticides. (NELAC)

Federal Water Pollution Control Act (Clean Water Act, CWA):

The enabling legislation under 33 U.S.C. 1251 et seq., Public Law 92-50086 Stat 816, that empowers EPA to set discharge limitations, write discharge permits, monitor, and bring enforcement action for non-compliance. (NELAC)

Field Blank:

Blank prepared in the field by filling a clean container with pure de-ionized water and appropriate preservative, if any, for the specific sampling activity being undertaken (EPA OSWER)

Field of Testing:

NELAC's approach to accrediting laboratories by program, method and analyte. Laboratories requesting accreditation for a program-method-analyte combination or for an up-dated/improved method are required to submit to only that portion of the accreditation process not previously addressed (see NELAC, section 1.9ff). (NELAC)

Finding:

An assessment conclusion that identifies a condition having a significant effect on an item or activity. An assessment finding is normally a deficiency and is normally accompanied by specific examples of the observed condition. (NELAC)

Holding Times (Maximum Allowable Holding Times):

The maximum times that samples may be held prior to analyses and still be considered valid or not compromised. (40 CFR Part 136)

Inspection:

An activity such as measuring, examining, testing, or gauging one or more characteristics of an entity and comparing the results with specified requirements in order to establish whether conformance is achieved for each characteristic. (ANSI/ASQC E4-1994)

Internal Standard:

A known amount of standard added to a test portion of a sample and carried through the entire measurement process as a reference for evaluating and controlling the precision and bias of the applied analytical test method. (NELAC)

Internal Standard Calibration:

Calibrations for methods that utilize internal standards to compensate for changes in instrument conditions.

Instrument Blank:

A clean sample (e.g., distilled water) processed through the instrumental steps of the measurement process; used to determine instrument contamination. (EPA-QAD)

Instrument Response:

Instrument response is normally expressed as either peak area or peak height however it may also reflect a numerical representation of some type of count on a detector (e.g. Photomultiplier tube, or Diode array detector) and is used in this document to represent all types.

Laboratory:

A defined facility performing environmental analyses in a controlled and scientific manner. (NELAC)

Laboratory Control Sample (however named, such as laboratory fortified blank, spiked blank, or QC check sample):

A sample matrix, free from the analytes of interest, spiked with verified known amounts of analytes or a material containing known and verified amounts of analytes, taken through all preparation and analysis steps. Where there is no preparation taken for an analysis (such as in

aqueous volatiles), or when all samples and standards undergo the same preparation and analysis process (such as Phosphorus), there is no LCS. It is generally used to establish intra-laboratory or analyst specific precision and bias or to assess the performance of all or a portion of the measurement system.

An LCS shall be prepared at a minimum of 1 per batch of 20 or less samples per matrix type per sample extraction or preparation method except for analytes for which spiking solutions are not available such as total suspended solids, total dissolved solids, total volatile solids, total solids, pH, color, odor, temperature, dissolved oxygen or turbidity. The results of these samples shall be used to determine batch acceptance.

Note: NELAC standards allow a matrix spike to be used in place of this control as long as the acceptance criteria are as stringent as for the LCS. (NELAC)

Laboratory Duplicate:

Aliquots of a sample taken from the same container under laboratory conditions and processed and analyzed independently. (NELAC)

Least Squares Regression (1st Order Curve):

The least squares regression is a mathematical calculation of a straight line over two axes. The y axis represents the instrument response (or Response ratio) of a standard or sample and the x axis represents the concentration. The regression calculation will generate a correlation coefficient (r) that is a measure of the "goodness of fit" of the regression line to the data. A value of 1.00 indicates a perfect fit. In order to be used for quantitative purposes, r must be greater than or equal to 0.99 for organics and 0.995 for inorganics.

Limit of Detection (LOD):

An estimate of the minimum amount of a substance that an analytical process can reliably detect. An LOD is analyte- and matrix-specific and may be laboratory dependent. (Analytical Chemistry, 55, p.2217, December 1983, modified) See also Method Detection Limit.

Manager (however named):

The individual designed as being responsible for the overall operation, all personnel, and the physical plant of the environmental laboratory. A supervisor may report to the manager. In some cases, the supervisor and the manager may be the same individual. (NELAC)

Matrix:

The component or substrate that contains the analyte of interest. For purposes of batch and QC requirement determinations, the following matrix distinctions shall be used:

Aqueous: Any aqueous sample excluded from the definition of Drinking Water matrix or Saline/Estuarine source. Includes surface water, groundwater, effluents, and TCLP or other extracts.

Drinking Water: any aqueous sample that has been designated as a potable or potential potable water source.

Saline/Estuarine: any aqueous sample from an ocean or estuary, or other salt water source such as the Great Salt Lake.

Non-aqueous Liquid: any organic liquid with ,<15% settleable solids.

Biological Tissue: any sample of a biological origin such as fish tissue, shellfish, or plant material. Such samples shall be grouped according to origin.

Solids: includes soils, sediments, sludges, and other matrices with >15% settleable solids.

Chemical Waste: a product or by-product of an industrial process that results in a matrix not previously defined.

Air: whole gas or vapor samples including those contained in flexible or rigid wall containers and the extracted concentrated analytes of interest from a gas or vapor that are collected with a sorbant tube, impinger solution, filter, or other device. (NELAC)

Matrix Spike (spiked sample or fortified sample):

Prepared by adding a known mass of target analyte to a specified amount of matrix sample for which an independent estimate of target analyte concentration is available. Matrix spikes are used, for example, to determine the effect of the matrix on a method's recovery efficiency.

Matrix spikes shall be performed at a frequency of one in 20 samples per matrix type per sample extraction or preparation method except for analytes for which spiking solutions are not available such as, total suspended solids, total dissolved solids, total volatile solids, total solids, pH, color, odor, temperature, dissolved oxygen or turbidity. The selected sample(s) shall be rotated among client samples so that various matrix problems may be noted and/or addressed. Poor performance in a matrix spike may indicate a problem with the sample composition and shall be reported to the client whose sample was used for the spike. (QAMS)

Matrix Spike Duplicate (spiked sample or fortified sample duplicate):

A second replicate matrix spike is prepared in the laboratory and analyzed to obtain a measure of the precision of the recovery for each analyte.

Matrix spike duplicates or laboratory duplicates shall be analyzed at a minimum of 1 in 20 samples per matrix type per sample extraction or preparation method. The laboratory shall document their procedure to select the use of an appropriate type of duplicate. The selected sample(s) shall be rotated among client samples so that various matrix problems may be noted and/or addressed. Poor performance in the duplicates may indicate a problem with the sample composition and shall be reported to the client whose sample was used for the duplicate. (QAMS)

Method Blank:

A sample of a matrix similar to the batch of associated samples (when available) that is free from the analytes of interest and is processed simultaneously with and under the same conditions as samples through all steps of the analytical procedures, and in which no target analytes or interferences are present at concentrations that impact the analytical results for sample analyses. (NELAC)

Method Detection Limit:

The minimum concentration of a substance (an analyte) that can be measured and reported with 99% confidence that the analyte concentration is greater than zero and is determined from analysis of a sample in a given matrix containing the analyte. (40 CFR Part 136, Appendix B)

National Environmental Laboratory Accreditation Conference (NELAC):

A voluntary organization of State and Federal environmental officials and interest groups purposed primarily to establish mutually acceptable standards for accrediting environmental laboratories. A subset of NELAP. (NELAC)

National Environmental Laboratory Accreditation Program (NELAP):

The overall National Environmental Laboratory Accreditation Program of which NELAC is a part. (NELAC)

Negative Control:

Measures taken to ensure that a test, its components, or the environment do not cause undesired effects, or produce incorrect test results. (NELAC)

NELAC Standards:

The plan of procedures for consistently evaluating and documenting the ability of laboratories performing environmental measurements to meet nationally defined standards established by the National Environmental Laboratory Accreditation Conference. (NELAC)

Performance Audit:

The routine comparison of independently obtained qualitative and quantitative measurement system data with routinely obtained data in order to evaluate the proficiency of an analyst or laboratory. (NELAC)

Performance Based Measurement System (PBMS):

A set of processes wherein the data quality needs, mandates or limitations of a program or project are specified and serve as criteria for selecting appropriate test methods to meet those needs in a cost-effective manner. (NELAC)

Positive Control:

Measures taken to ensure that a test and/or its components are working properly and producing correct or expected results from positive test subjects. (NELAC)

Precision:

The degree to which a set of observations or measurements of the same property, obtained under similar conditions, conform to themselves; a data quality indicator. Precision is usually expressed as standard deviation, variance or range, in either absolute or relative terms. (NELAC)

Preservation:

Refrigeration and/or reagents added at the time of sample collection (or later) to maintain the chemical and/or biological integrity of the sample. (NELAC)

Proficiency Testing:

A means of evaluating a laboratory's performance under controlled conditions relative to a given set of criteria through analysis of unknown samples provided by an external source. (NELAC)
[2.1]

Proficiency Testing Program:

The aggregate of providing rigorously controlled and standardized environmental samples to a laboratory for analysis, reporting of results, statistical evaluation of the results and the collective demographics and results summary of all participating laboratories. (NELAC)

Proficiency Test Sample (PT):

A sample, the composition of which is unknown to the analyst and is provided to test whether the analyst/laboratory can produce analytical results within specified acceptance criteria. (QAMS)

Quality Assurance:

An integrated system of activities involving planning, quality control, quality assessment, reporting and quality improvement to ensure that a product or service meets defined standards of quality with a stated level of confidence. (QAMS)

Quality Assurance [Project] Plan (QAPP):

A formal document describing the detailed quality control procedures by which the quality requirements defined for the data and decisions pertaining to a specific project are to be achieved. (EAP-QAD)

Quality Control:

The overall system of technical activities which purpose is to measure and control the quality of a product or service so that it meets the needs of users. (QAMS)

Quality Control Sample:

An uncontaminated sample matrix spiked with known amounts of analytes from a source independent from the calibration standards. It is generally used to establish intra-laboratory or analyst specific precision and bias or to assess the performance of all or a portion of the measurement system. (EPA-QAD)

Quality Manual:

A document stating the management policies, objectives, principles, organizational structure and authority, responsibilities, accountability, and implementation of an agency, organization, or laboratory, to ensure the quality of its product and the utility of its product to its users. (NELAC)

Quality System:

A structured and documented management system describing the policies, objectives, principles, organizational authority, responsibilities, accountability, and implementation plan of an organization for ensuring quality in its work processes, products (items), and services. The quality system provides the framework for planning, implementing, and assessing work performed by the organization and for carrying out required QA and QC (ANSI/ASQC-E-41994)

Quantitation Limits:

The maximum or minimum levels, concentrations, or quantities of a target variable (e.g., target analyte) that can be quantified with the confidence level required by the data user. (NELAC)

Range:

The difference between the minimum and the maximum of a set of values. (EPA-QAD)

Reagent Blank (method reagent blank):

A sample consisting of reagent(s), without the target analyte or sample matrix, introduced into the analytical procedure at the appropriate point and carried through all subsequent steps to determine the contribution of the reagents and of the involved analytical steps. (QAMS)

Reference Material:

A material or substance one or more properties of which are sufficiently well established to be used for the calibration of an apparatus, the assessment of a measurement method, or for assigning values to materials. (ISO Guide 30-2.1)

Reference Method:

A method of known and documented accuracy and precision issued by an organization recognized as competent to do so. (NELAC)

Reference Standard:

A standard, generally of the highest metrological quality available at a given location, from which measurements made at that location are derived. (VIM-6.0-8)

Replicate Analyses:

The measurements of the variable of interest performed identically on two or more sub-samples of the same sample within a short time interval. (NELAC)

Requirement:

Denotes a mandatory specification; often designated by the term "shall". (NELAC)

Resource Conservation and Recovery Act (RCRA):

The enabling legislation under 42 USC 321 et seq. (1976), that gives EPA the authority to control hazardous waste from the "cradle-to-grave", including its generation, transportation, treatment, storage, and disposal. (NELAC)

Safe Drinking Water Act (SDWA):

The enabling legislation, 42 USC 300f et seq. (1974), (Public Law 93-523), that requires the EPA to protect the quality of drinking water in the U.S. by setting maximum allowable contaminant levels, monitoring, and enforcing violations. (NELAC)

Sample Duplicate:

Two samples taken from and representative of the same population and carried through all steps of the sampling and analytical procedures in an identical manner. Duplicate samples are used to assess variance of the total method including sampling and analysis. (EPA-QAD)

Second Order Polynomial Curve (Quadratic): The 2nd order curves are a mathematical calculation of a slightly curved line over two axis. The y axis represents the instrument response (or Response ratio) of a standard or sample and the x axis represents the concentration. The 2nd order regression will generate a coefficient of determination (COD or r²) that is a measure of the "goodness of fit" of the quadratic curvature the data. A value of 1.00 indicates a perfect fit. In order to be used for quantitative purposes, r² must be greater than or equal to 0.99.

Selectivity:

(Analytical chemistry) the capability of a test method or instrument to respond to a target substance of constituent in the presence of non-target substances. (EPA-QAD)

Sensitivity:

The capability of a method or instrument to discriminate between measurement responses representing different levels (e.g., concentrations) of a variable of interest. (NELAC)

Spike:

A known mass of target analyte added to a blank, sample or sub-sample; used to determine recovery efficiency or for other quality control purposes.

If the mandated or requested test method does not specify the spiking components, the laboratory shall spike all reportable components to be reported in the Laboratory Control Sample and Matrix Spike. However, in cases where the components interfere with accurate assessment (such as simultaneously spiking chlordane, toxaphene and PCBs in Method 608), the test method has an extremely long list of components or components are incompatible, a representative number (at a minimum 10%) of the listed components may be used to control the test method. The selected components of each spiking mix shall represent all chemistries, elution patterns and masses permit specified analytes and other client requested components. However, the laboratory shall ensure that all reported components are used in the spike mixture within a two-year time period.. (NELAC)

Standard:

The document describing the elements of laboratory accreditation that has been developed and established within the consensus principles of NELAC and meets the approval requirements of NELAC procedures and policies. (ASQC)

Standard Operating Procedures (SOPs):

A written document which details the method of an operation, analysis, or action whose techniques and procedures are thoroughly prescribed and which is accepted as the method for performing certain routine or repetitive tasks. (QAMS)

Standardized Reference Material (SRM):

A certified reference material produced by the U.S. National Institute of Standards and Technology or other equivalent organization and characterized for absolute content, independent of analytical method. (EPA-QAD)

Supervisor (however named):

The individual(s) designated as being responsible for a particular area or category of scientific analysis. This responsibility includes direct day-to-day supervision of technical employees, supply and instrument adequacy and upkeep, quality assurance/quality control duties, and ascertaining that technical employees have the required balance of education, training and experience to perform the required analyses. (NELAC)

Surrogate:

A substance with properties that mimic the analyte of interest. It is unlikely to be found in environment samples and is added to them for quality control purposes.

Surrogate compounds must be added to all samples, standards, and blanks, for all organic chromatography methods except when the matrix precludes its use or when a surrogate is not available. Poor surrogate recovery may indicate a problem with sample composition and shall be reported to the client whose sample produced poor recovery. (QAMS)

Systems Audit (also Technical Systems Audit):

A thorough, systematic, qualitative on-site assessment of the facilities, equipment, personnel, training, procedures, record keeping, data validation, data management, and reporting aspects of a total measurement system. (EPA-QAD)

Technical Director:

Individuals(s) who has overall responsibility for the technical operation of the environmental testing laboratory. (NELAC)

Test:

A technical operation that consists of the determination of one or more characteristics or performance of a given product, material, equipment, organism, physical phenomenon, process, or service according to a specified procedure. The result of a test is normally recorded in a document sometimes called a test report or a test certificate. (ISO/IEC Guide 2-12.1, amended)

Test Method:

An adoption of a scientific technique for a specific measurement problem, as documented in a laboratory SOP. (NELAC)

Toxic Substances Control Act (TSCA):

The enabling legislation in 15 USC 2601 et seq., (1976) that provides for testing, regulating, and screening all chemicals produced or imported into the United States for possible toxic effects prior to commercial manufacture. (NELAC)

Traceability:

The property of a result of a measurement whereby it can be related to appropriate standards, generally international or national standards, through an unbroken chain of comparisons. (VIM-6.12)

Uncertainty:

A parameter associated with the result of a measurement that characterizes the dispersion of the value that could reasonably be attributed to the measured value.

United States Environmental Protection Agency (EPA):

The Federal governmental agency with responsibility for protecting public health and safeguarding and improving the natural environment (i.e., the air, water, and land) upon which human life depends. (US-EPA)

Validation:

The process of substantiating specified performance criteria. (EPA-QAD)

Verification:

Confirmation by examination and provision of evidence that specified requirements have been met. (NELAC)

NOTE: In connection with the management of measuring equipment, verification provides a means for checking that the deviations between values indicated by a measuring instrument and corresponding known values of a measured quantity are consistently smaller than the maximum allowable error defined in a standard, regulation or specification peculiar to the management of the measuring equipment.

The result of verification leads to a decision either to restore in service, to perform adjustment, to repair, to downgrade, or to declare obsolete. In all cases, it is required that a written trace of the verification performed shall be kept on the measuring instrument's individual record.

Work Cell:

A well-defined group of analysts that together perform the method analysis. The members of the group and their specific functions within the work cell must be fully documented. (NELAC)

Acronyms:

BS – Blank Spike
BSD – Blank Spike Duplicate
CAR – Corrective Action Report
CCV – Continuing Calibration Verification
CF – Calibration Factor
CFR – Code of Federal Regulations
COC – Chain of Custody
CRS – Change Request Form
DOC – Demonstration of Capability
DQO – Data Quality Objectives
DU – Duplicate
DUP - Duplicate
EHS – Environment, Health and Safety
EPA – Environmental Protection Agency
GC - Gas Chromatography
GC/MS - Gas Chromatography/Mass Spectrometry
HPLC - High Performance Liquid Chromatography
ICP - Inductively Coupled Plasma Atomic Emission Spectroscopy
ICV – Initial Calibration Verification
IDL – Instrument Detection Limit
IH – Industrial Hygiene
IS – Internal Standard
LCS – Laboratory Control Sample
LCSD – Laboratory Control Sample Duplicate
LIMS – Laboratory Information Management System
MDL – Method Detection Limit
MS – Matrix Spike
MSD – Matrix Spike Duplicate
MSDS - Material Safety Data Sheet
NELAC - National Environmental Laboratory Accreditation Conference
NELAP - National Environmental Laboratory Accreditation Program
PT – Performance Testing
QAM – Quality Assurance Manual
QA/QC – Quality Assurance / Quality Control
QAPP – Quality Assurance Project Plan
RF – Response Factor
RPD – Relative Percent Difference
RSD – Relative Standard Deviation
SD – Standard Deviation
SOP: Standard Operating Procedure
TAT – Turn-Around-Time
VOA – Volatiles
VOC – Volatile Organic Compound

Appendix 6.

Laboratory Certifications, Accreditations, Validations

TestAmerica Irvine maintains certifications, accreditations, certifications, and validations with numerous state and national entities. Programs vary but may include on-site audits, reciprocal agreements with another entity, performance testing evaluations, review of the QA Manual, Standard Operating Procedures, Method Detection Limits, training records, etc. At the time of this QA Manual revision, the laboratory has accreditation/certification/licensing with the following organizations:

State	Agency	Program	License Number
CA	DHS-ELAP	HW	1197
CA	DHS-ELAP	WW, HW	17941 ¹
CA	DHS-ELAP	WW, HW	25362
CA	DHS-NELAP	DW, WW, HW	01108CA
AZ	DHS	DW, WW, HW	AZ0671
NV	DEP	DW, WW, RCRA	CA72
UT	DHS-ELCP	DW, WW,HW	DEL9492611022
WA	DOE	WW, HW	C2025
NM	DWB	DW	--
CNMI	DEQ	DW	--
GUAM	EPA	DW	--
HI	DOH	DW	--
--	ACIL	Seal Of Excellence	300
--	USDA	Foreign Soil	S-669307

¹ for Mobile lab (EPA # CA01103)

The certificates and parameter lists (which may differ) for each organization may be found on the corporate web site, the laboratory's public server, the final report review table, and in the following offices: QA, marketing, and project management.

Claims of Accreditation Status

TestAmerica Irvine has agreed to make only valid claims as to its accreditation/certification status by any authority by ensuring that the expiration dates are not exceeded and the method-specific scope or parameter lists are supportable, as required by each. Any false claims would be reported to that authority. The agreement covers the use of the authority's name, such as "Authority-Accredited," logo, or certificate number. The only valid proof of accreditation/certification is the current certificate and scope of the authority. It is the responsibility of the laboratory to make these documents available to all staff, and it is the staff's duty to reference only the current documents.

A report with scope and non-scope analytes may only be presented on the same report if the non-accredited results are clearly and unambiguously identified. No report with non-scope analytes may be associated with the logo, "Authority accredited" phrase, or the certificate number. Only the analytes specified by a unique method are valid within the scope. There shall be no intentional misleading of the users of the laboratory's services in this regard.

No opinions and/or interpretations based on results outside the laboratory's scope may be presented on a document referenced by "Authority-accredited, the logo, or the certificate number. If these are made, they must be written in a separate letter which is not endorsed by the authority.

The "Authority-accredited" logo may only be affixed to equipment calibrated by a laboratory that is accredited by the authority. If calibration labels contain the logo, they must also show the calibration laboratory's name or its certificate number, the instrument's unique identification, the date of the last calibration, and a cross-reference to the last calibration certificate.

Should the company decide to use the "Authority-accredited" logo in marketing activities, no misrepresentation may occur. Only reference to the accredited scope at a specific laboratory site is allowed. If any "Authority-accredited" language is used in proposals or quotations, any non-scope analytes must be clearly denoted as not accredited by that authority. The same is true for any use of laboratory letterhead with the "Authority-accredited" wording or logo. The logo may not be affixed to any material, item, product, part, or packaging, thereby implying accreditation status to that piece. In literature, any use of the logo must be positioned adjacent to the accredited laboratory's name and clearly state that the presence of the logo does not imply certification/approval of the products tested. At no time may the logo appear to suggest that a person is accredited. Misrepresentation of accreditation status is never allowed and must be reported if it occurs. If in doubt, the idea of the logo's use may be presented to the authority for approval.

If accreditation is terminated or suspended, the laboratory will immediately cease to use the "Authority-accredited" wording, the logo, or the certificate number reference in any way and inform clients impacted by the change.

Appendix 7. Data Qualifiers

Qualifier	Text	Usage Comments
-	Negative Ion Balance	
+	Positive Ion Balance	
<	Result is less than the indicated value.	Used only for Flashpoint
>	Result is greater than the indicated value.	Used only for Flashpoint
A-01	[Custom Value]	Type the qualifier in full sentences without abbreviations or uncommon acronyms. DO NOT USE ALL CAPS. AZ requires narrative.
A1	Too numerous to count.	Microbiology only (Put 'TNTC' in CSTM qualifier)
A10	Results based upon colony counts outside the acceptable range.	
A12	Atypical growth	
A13	Atypical growth appears to have a toxic effect on surrounding growth, thus affecting the plate count.	
A2	Sample incubation period exceeded method requirement.	Microbiology only (NDs ONLY)
A3	Sample incubation period was shorter than method requirement.	Microbiology only
A4	Target organism detected in associated method blank.	Microbiology only (NDs ONLY)
A5	Incubator/water bath temperature was outside method requirements.	Microbiology only
A6	Target organism not detected in associated positive control.	Microbiology only
A7	Micro sample received without adequate headspace.	Microbiology only (Coliforms)
A8	Result is greater than or equal to the indicated value.	Microbiology only. Won't really be used, 'CSTM' qualifier is used instead.
A9	Bacterial results confirmed	
B	Analyte was detected in the associated Method Blank.	Requires internal CAR. Flag method blank and all associated samples with positive hits. Do not flag blank for J-flag hits unless regulatory limit has been exceeded..
B-1	Analyte was detected in the associated method blank. Analyte concentration in the sample is greater than 10x the concentration found in the method blank.	20x for organics; Requires internal CAR.
B2	Non-target analyte detected in method blank and sample, producing interference.	Requires internal CAR.
B3	Target analyte detected in calibration blank at or above the method reporting limit.	Requires internal CAR.
B4	Target analyte detected in blank at/above method acceptance criteria.	AZ - Metals and IC only. Requires internal CAR
B5	Target analyte detected in method blank at or above the method reporting limit, but below the trigger level or MCL.	

Qualifier	Text	Usage Comments
B6	Target analyte detected in calibration blank at or above the method reporting limit, but below the trigger level or MCL.	
BQC	Reported for batch QC purposes only. See re-analysis (RE) for final result.	AZ requires narrative.
BQC1	Reported for batch QC purposes only. See original analysis for final result.	AZ requires narrative.
C	Calibration Verification recovery was above the method control limit for this analyte. Analyte not detected, data not impacted.	Flag all affected sample results. Corrective action, such as re-calibration, is required. Not to be used on a continuous basis.
C-1	Calibration Verification recovery was above the method control limit for this analyte, however the average % difference for all analytes met method criteria. See Calibration Summary form. [Custom Value]	Used for NDs unless reanalysis confirms sample causing interference. 8000B series methods only. Flag all affected sample results.
C-2	Calibration Verification recovery was below the method control limit for this analyte, however the average % difference for all analytes met method criteria. See Calibration Summary form. [Custom Value]	Used for NDs unless reanalysis confirms sample causing interference. 8000B series methods only. Flag all affected sample results.
C4	Calibration Verification recovery was below the method control limit for this analyte.	Corrective Action, such as re-calibration, is required. Not to be used on a continuous basis. Requires internal CAR.
C5	Calibration Verification recovery was below the method control limit for this analyte. An additional check standard was analyzed at the reporting limit to ensure instrument sensitivity at the reporting limit. Samples ND.	Corrective Action, such as re-calibration, is required. Not to be used on a continuous basis. CAR not required for 8000 methods if average %R meets criteria. AZ requires narrative.
C6	CCV recovery was below method acceptance limits. The sample could not be reanalyzed due to insufficient sample.	CAR required.
C-7	Calibration Verification recovery was below the method control limit due to matrix interference carried over from analytical samples. The matrix interference was confirmed by reanalysis with the same result.	Re-extraction and/or re-analysis required for all bracketed samples. Needs internal CAR.
C8	Calibration Verification recovery was above the method control limit for this analyte. A high bias may be indicated.	Requires internal CAR.
CBP	Calibration verification recovery for this analyte is outside of limits as stated in BP-GCLN Technical Requirements however the calibration verification meets the requirements as stated in the analytical method.	BP work only.
CE	Sample not homogenous.	
CF1	Confirmatory analysis not performed as required by the method.	Always use with N1
CF2	Confirmatory analysis was past holding time.	
CF3	Confirmatory analysis was past holding time. Original result not confirmed.	

Qualifier	Text	Usage Comments
CF5	The sample was originally analyzed with a positive result, however the reanalysis did not confirm the presence of the analyte.	Use for BP Ethanol Reporting
CIG	The % RSD for this compound was above 20%. The average % RSD for all compounds in the calibration met the 20% criteria specified in EPA method 8000B. See the attached Initial Calibration Criteria form.	For GC or HPLC 8000B series only. Used for NDs only.
CIN	The % RSD for this compound was above 15%. The average % RSD for all compounds in the calibration met the 15% criteria specified in EPA methods 8260B/8270C. See the attached Initial Calibration Criteria form.	For GCMS 8000B series only. Used for NDs only.
cl	Compound reported based on total Chlordane result being less than the reporting limit.	Special qualifier for client specific requirements. Do not use for Arizona clients.
CN1	The cyanide value was greater after chlorination than before chlorination due to the sample matrix. An additional Weak Acid Dissociable Cyanide analysis was performed.	AZ requires narrative.
CN2	The cyanide value was greater after chlorination than before chlorination due to the sample matrix.	AZ requires narrative.
CN3	Reactive sulfide results reported from total determination method.	
CN4	Amenable cyanide results reported from total determination method.	
CR	The carbon range of the fuel found in the sample = [Custom Value]	When requested, enter Carbon range of fuel at the prompt.
CSTM	[Cutom Value]	Use when results need to be reported as '<' or '>' or negative values. Enter exactly as it should appear on the report (e.g "> 50" or "-3.2", or "DNQ")
DNQ	Detected but not quantified.	For Boeing Project to use in conjunction with J flag. PM to add to report.
DR	Sample dried prior to screening.	
E	Concentration exceeds the calibration range and therefore result is semi-quantitative.	Use when re-analysis is for multiple dilutions.
E1	Concentration estimated. Analyte exceeded calibration range. Reanalysis not possible due to insufficient sample.	
E3	Concentration estimated. Analyte exceeded calibration range. Reanalysis not performed due to holding time requirements.	
E8	Analyte reported to the MDL per project specification. Target analyte was not detected in the sample	
FT	This analysis was performed in the field by the sampler whose name appears on the attached Chain of Custody form.	

Qualifier	Text	Usage Comments
H	Sample analysis performed past method-specified holding time.	Requires client notification prior to release of data. Requires internal CAR.
H-1	Sample analysis performed past the method-specified holding time per client's approval.	MUST HAVE DOCUMENTED CLIENT APPROVAL. Requires internal CAR
H2	Initial analysis within holding time. Reanalysis for the required dilution was past holding time.	Requires client notification prior to release of data.
H3	Sample was received and analyzed past holding time.	Requires client notification prior to release of data.
H4	Sample was extracted past holding time, but analyzed within analysis holding time.	Requires client notification prior to release of data. Requires internal CAR.
H5	The sample was prepared outside of the required 8 hour holding time, however it was stored at >0° and <4°C and prepared within the method allowed 24 hour holding time.	For HPC only
H6	The sample was received at the laboratory either past, or with insufficient time remaining on, the required 8 hour holding time. However, it was stored at >0° and <4°C and prepared within the method allowed 24 hour hold time.	For HPC only
H8	The sample was extracted past the holding time.	
H9	Sample analysis performed past the EPA recommended holding time.	
H10	The holding time calculation is based on a sampling time of 00:00 on the sampling date noted on the Chain of Custody. No sampling time was provided to the laboratory.	For clients that won't give a sampling time
HFT	The holding time for this test is immediate. It was analyzed in the laboratory as soon as possible after receipt.	
HS	HS = Sample container contained headspace.	
HTI	The holding time for this test is immediate. The laboratory measurement, therefore, cannot be used for compliance purposes.	Arizona clients only (at this time). Use for pH, Temperature, Residual Chlorine, Dissolved Oxygen and Free Carbon Dioxide. AZ requires narrative.
I	Internal Standard recovery was outside of method limits. Matrix interference was confirmed.	
I2	Internal Standard recovery was outside of method limits.	Requires internal CAR
ID	Due to the low levels of analyte found in the sample, the analyte was qualitatively identified based on the compound's retention time and the presence of a single mass ion.	For GCMS when 2 mass ions cannot be detected. (e.g. low level TBA) AZ requires narrative.
ID2	Secondary ion abundance outside of method requirements. Identification based on analytical judgment	
J	Estimated value. Analyte detected at a level less than the Reporting Limit (RL) and greater than or equal to the Method Detection Limit (MDL). The user of this data should be aware that this data is	When, on a project specific basis, reporting results down to the MDL is required.

Qualifier	Text	Usage Comments
	of limited reliability.	
K	The sample dilutions set-up for the BOD analysis did not meet the oxygen depletion criteria of at least 2 mg/l. Therefore the reported result is an estimated value only.	
K-1	The sample dilutions set up for the BOD analysis failed to meet the criteria of a residual dissolved oxygen of at least 1 mg/l. Therefore the reported result is an estimated value only.	
K-2	The seed depletion was outside the method acceptance limits. Therefore, the reported result is an estimated value only.	
K-3	The dilution water D.O. depletion was > 0.2 mg/L.	
K-4	The seed depletion was not within method recommended limits. The LCS, which is a means of checking dilution water quality and seed effectiveness, was within acceptance limits. The acceptable LCS demonstrates that the data is valid.	
L	Laboratory Control Sample and/or Laboratory Control Sample Duplicate recovery was above the acceptance limits. Analyte not detected, data not impacted.	Flag all affected sample results. Requires internal CAR.
L1	Laboratory Control Sample and/or Laboratory Control Sample Duplicate recovery was above acceptance limits.	When there are positive hits. Requires internal CAR. Add N-1 or N-2 if for any additional clarification.
L2	Laboratory Control Sample and/or Laboratory Control Sample Duplicate recovery was below acceptance limits.	Use only if samples cannot be reanalyzed. Requires internal CAR. Add N-1 or N-2 if for any additional clarification.
L4	Laboratory Control Sample and/or Laboratory Control Sample Duplicate recovery was below the acceptance limits. A low bias to sample results is indicated.	Generally for BOD only. However it could be used for BP-Amoco if technical requirements are met and local clients are o.k. with it.
L6	Per the EPA methods, benzidine is known to be subject to oxidative losses during solvent concentration.	To be used for high or low recoveries.
M1	The MS and/or MSD were above the acceptance limits due to sample matrix interference. See Blank Spike (LCS).	Flag source sample AND MS and/or MSD only.
M2	The MS and/or MSD were below the acceptance limits due to sample matrix interference. See Blank Spike (LCS).	Flag source sample AND MS and/or MSD only.
M-3	Results exceeded the linear range in the MS/MSD and therefore are not available for reporting. The batch was accepted based on acceptable recovery in the Blank Spike (LCS).	Analyte Qualifier in the LCS. AZ requires narrative.

Qualifier	Text	Usage Comments
M4	The sample required a dilution due to matrix interference. Because of this dilution, the matrix spike concentrations in the sample were reduced to a level where the recovery calculation does not provide useful information. See Blank Spike (LCS).	Must be diluted below Reporting Limit.
M5	Due to CCV failure, the MS/MSD results were not available for reporting. The batch was accepted based on acceptable recovery in the Blank Spike (LCS).	Generally a sample qualifier though it could be used as an analyte qualifier if some analytes are to be reported. AZ requires narrative.
M6	Matrix Spike recovery was outside the method control limits.	Do Not Use Anymore
M7	The MS and/or MSD were above the acceptance limits. See Blank Spike (LCS).	Internal CAR required. Add N-2 if Client CAR is needed.
M8	The MS and/or MSD were below the acceptance limits. See Blank Spike (LCS).	Internal CAR required. Add N-2 if Client CAR is needed.
M9	Matrix Spike recovery was high. Data Reported per ADEQ policy 0154.000	AZ Only. Use only if BS/BSD have acceptable Recovery AND RPD.
M10	Matrix Spike recovery was low. Data Reported per ADEQ policy 0154.000	AZ Only. Use only if BS/BSD have acceptable Recovery AND RPD.
M13	The sample spiked had a pH of less than 2. 2-Chloroethylvinylether degrades under acidic conditions.	
MCP	No results were reported for the MS and/or MSD due to a clogged autosampler port. Batch was accepted based on Blank Spike (LCS) recoveries.	Requires internal CAR. AZ requires narrative.
MEN	Unspiked sample results were determined from the sample portion received in an Encore sampler. The sample portions used for the MS/MSD were taken from an additional sample sleeve due to an insufficient number of Encore samplers supplied.	When insufficient Encores are available for MS/MSD. AZ requires narrative.
MHA	Due to high levels of analyte in the sample, the MS/MSD calculation does not provide useful spike recovery information. See Blank Spike (LCS).	Sample results > 4x spike level. Use whether or not the QC passes.
MNR	No results were reported for the MS/MSD. The sample used for the MS/MSD required dilution due to the sample matrix. Because of this, the spike compounds were diluted below the detection limit.	Use as sample qualifier on the LCS. AZ requires narrative.
MNR1	There was no MS/MSD analyzed with this batch due to insufficient sample volume. See Blank Spike/Blank Spike Duplicate.	Use when there is not enough sample available to analyze MS/MSD. Use as a sample qualifier on the LCS. LCS must be analyzed too.
MNR2	Insufficient sample received to meet method QC requirements. See case narrative.	FOR AZ DRINKING WATERS ONLY.
MNR3	Insufficient sample received to meet method QC requirements.	
N1	See case narrative.	

Qualifier	Text	Usage Comments
N2	See corrective action report.	
Neg	The reported result is a negative value.	For Redox Potential only.
NFP	Non-fuel pattern present.	
P	The sample, as received, was not preserved in accordance to the referenced analytical method.	except for metals
P1	Sample received and analyzed without chemical preservation.	
P2	Sample received without chemical preservation, but preserved by the laboratory.	
P3	Sample was received above recommended temperature	
P4	Sample received in inappropriate sample container.	
P5	Insufficient sample received to meet method QC requirements.	
P6	Sample received unpreserved, however the sample was analyzed within 7 days per EPA recommendation.	For EPA 624
P7	Sample filtered in lab.	
P8	Sample unable to be adjusted to correct pH due to matrix.	
P9	This analyte has been shown to degrade upon preservation with HCl and cannot accurately be quantitated.	
P10	Sample received with chemical preservation; pH measured in lab >2	
P12	Sample received with chemical preservation; pH measured in lab >2	
pH	pH = [Custom value]	AZ requires narrative.
P-HS	Sample container contained headspace.	
QB	Quantitated against a Bunker C Oil standard.	Use as "Analyte Qualifier"
QC4	Quantitation begun immediately before the retention time of tert-Butanol (TBA).	Only for TPH when C4 carbon range is requested. Use as Analyte qualifier.
QCM	Quantitation begun immediately following the methanol peak.	Only for TPH when C4 carbon range is requested. Use as Analyte qualifier.
QD	Quantitated against a diesel fuel standard.	Use as "Sample Qualifier"
QG	Carbon range C6-C12 quantitated against a gasoline standard.	Use as "Analyte Qualifier" To be used with the analyte "Volatile Fuel Hydrocarbons".
QG1	Quantitated against a gasoline standard.	Use as "Analyte Qualifier" for any carbon range other than C6-C12
QJ	Quantitated against a jet fuel standard.	Use as "Sample Qualifier"
QM	Quantitated against a motor oil standard.	Use as "Sample Qualifier"
QMS	Quantitated against a mineral spirits standard.	Use as "Analyte Qualifier"
QP	Hydrocarbon result partly due to individual peak(s) in quantitation range.	Use when individual non-HC peaks are present.

Qualifier	Text	Usage Comments
qr	Qualitative result based on chromatographic comparison with a known standard.	
QS	Quantitated against a Stoddard solvent standard.	Use as "Sample Qualifier"
QT	Quantitated against a therminol standard.	Use as "Sample Qualifier"
QU	Unquantitated hydrocarbons present in the sample outside of the reported carbon range.	Use for EFH when there are HCs above the quantitation range.
QV	The molecular weight of 100 was used to convert Volatile Fuel Hydrocarbons from mg/m ³ to ppm by volume (ppmv).	
R	The RPD exceeded the method control limit due to sample matrix effects. The individual analyte QA/QC recoveries, however, were within acceptance limits.	Apply to MSD only
R-1	The RPD between the primary and confirmatory analysis exceeded 40%. Per method 8000B, the higher value was reported.	
R-2	The RPD exceeded the acceptance limit.	Narrative required for AZ. (narrative likely for all). Add N-2 if Client CAR is needed.
R-3	The RPD exceeded the acceptance limit due to sample matrix effects.	
R-4	Due to the low levels of analyte in the sample, the duplicate RPD calculation does not provide useful information.	Duplicates Only. NOT for MS/MSD.
R-6	The RPD calculation does not provide useful information due to varying sample weights when Encore samplers are used.	Encore Samples only.
R-7	LFB/LFBD RPD exceeded the method control limit. Recovery met acceptance criteria.	Apply to LCSD only.
R-9	Sample RPD exceeded the laboratory control limit.	For Sample Duplicates
R-10	The RPD between the primary and confirmatory analysis exceeded 40%. Per method 8000B, the lower value was reported due to apparent chromatographic problems.	
R-11	RPD exceeded the laboratory control limit. See case narrative.	When there are no "Method" Limits.
R-12	The RPD between the primary and confirmatory analysis exceeded 40%. Per method 8000C, the lower value was reported.	For labs referenceing 8000C-series methods.
RL1	Reporting limit raised due to sample matrix effects.	
RL2	Reporting limit raised due to high concentrations of hydrocarbons.	
RL3	Reporting limit raised due to high concentrations of non-target analytes.	
RL4	Reporting limit raised due to insufficient sample volume.	
RL5	Reporting raised due to high single peak analyte.	For TPH (DRO or GRO) only.

Qualifier	Text	Usage Comments
RL6	Reporting limit raised due to high toxaphene concentrations.	
RL7	Sample required dilution due to high concentration of target analyte.	
S	Analyzed by standard addition.	Will probably only be used for metals in rare instances.
S10	Insufficient sample available for reanalysis.	
SB	Sustained burning when exposed to open flame.	For Ignitability only. For all positive hits.
SC	Analytical results not reliable due to potential sample container contamination.	For low level Volatiles when contamination is the likely cause of the result.
SF	Reactive sulfide results reported from total determination method.	
T1	Method promulgated by EPA, but not by ADHS at this time	AZDHS only
T2	Cited ADHS licensed method does not contain this analyte as part of method compound list.	AZDHS only
T3	Method not promulgated by EPA or ADHS.	AZDHS only
T4	The cited licensed method does not contain this analyte as part of the method compound list.	Not for AZ work
T5	Less than the prescribed sample amount was available to perform the leachate extraction. The volume of extraction fluid was adjusted proportionately based on the method prescribed ratio of extraction fluid to sample weight.	Internal CAR not required if documented in extraction log.
T6	The temperature during the 18 hour TCLP extraction exceeded the 21-25 degrees C range stated in EPA Method 1311. The temperature range during the extraction was [Custom Value] degrees C.	Enter the temperature range during the extraction when prompted (e.g. 20-27)
T7	Tentatively identified compound. Concentration is estimated based on the closest internal standard.	
TMP	Temperature taken in the field at the time of sampling.	Only when lab is reporting temperature into an ELMNT analysis code.
TRM	Per client request, the sample was digested according to section 4.1.4 of "Methods for the Chemical Analysis of Water and Wastes 1983". The sample was subsequently prepared and analyzed by EPA Method 245.1.	Boeing Total Recoverable Mercury ONLY.
TRM	Per client request, the sample was digested according to section 4.1.4 of "Methods for the Chemical Analysis of Water and Wastes 1983". The sample was subsequently prepared and analyzed by EPA Method 245.1.	
TVO	Based on the sum of the concentrations of the compounds in the EPA 8010/8020 list.	Client Specific for special Air test code.
X	Exceeds regulatory limit.	PM to apply as an "Analyte" Qualifier.
X1	Exceeds specified permit limit.	PM to apply as an "Analyte" Qualifier.

Qualifier	Text	Usage Comments
Z	Due to sample matrix effects, the surrogate recovery was below the acceptance limits.	Re-extraction and/or re-analysis required unless chromatographic interference is clearly evident
Z1	Surrogate recovery was above acceptance limits.	AZ requires narrative. Requires internal CAR.
Z2	Surrogate recovery was above the acceptance limits. Data not impacted.	Only use if sample results are ND. Requires internal CAR
Z3	The sample required a dilution due to the nature of the sample matrix. Because of this dilution, the surrogate spike concentration in the sample was reduced to a level where the recovery calculation does not provide useful information.	Only if diuted below calibration range for surrogate. Surrogates in MB and LCS must pass to use this qualifier.
Z5	Due to sample matrix effects, the surrogate recovery was outside acceptance limits. Secondary surrogate recovery was within the acceptance limits.	For PCBs only. AZ requires narrative.
Z6	Surrogate recovery was below acceptance limits.	When reanalysis not performed. Rerquires internal CAR.
Z7	Surrogate recovery was high. Data reported per ADEQ policy 0154.000.	For AZDHS only. Surrogate passes in LCS but not in sample.
Z8	Surrogate recovery was low. Data reported per ADEQ policy 0154.000.	For AZDHS only. Surrogate passes in LCS but not in sample.
Z9	Unable to calculate surrogate recovery due to matrix interference.	Chromatographic interference must be clearly evident.
ZX	Due to sample matrix effects, the surrogate recovery was outside acceptance limits.	Use for High bias. Re-extraction and/or re-analysis required (Narrate for AZ)