

APPENDIX G

Section 13

Outfall 003, January 25, 2008

MEC^X Data Validation Reports



DATA VALIDATION REPORT

Boeing SSFL NPDES

SAMPLE DELIVERY GROUP: IRA2500

Prepared by

MEC^X, LLC
12269 East Vassar Drive
Aurora, CO 80014

I. INTRODUCTION

Task Order Title: Boeing SSFL NPDES
 Contract Task Order: 1261.100D.00
 Sample Delivery Group: IRA2500
 Project Manager: B. Kelly
 Matrix: Soil
 QC Level: IV
 No. of Samples: 1
 No. of Reanalyses/Dilutions: 0
 Laboratory: TestAmerica-Irvine

Table 1. Sample Identification

Client ID	Laboratory ID	Sub-Laboratory ID	Matrix	Collected	Method
Outfall 003	IRA2500-01	30210-001	Water	01/25/08 0825	245.1, 200.8, 900.0, 901.1, 903.1, 904.0, 905.0, 906.0, 1613, ASTM D-5174

II. Sample Management

No anomalies were observed regarding sample management. The sample in this SDG was received at TestAmerica-Irvine and Eberline within the temperature limits of 4°C \pm 2°C. The sample was received below the temperature limit at Vista; however, the sample was not noted to have been frozen. The sample was received above the temperature limit at Weck; however, mercury is not considered volatile. According to the case narrative for this SDG, the sample was received intact at all laboratories. The COCs were appropriately signed and dated by field and/or laboratory personnel. As the sample was couriered to TestAmerica-Irvine, custody seals were not required. Custody seals were intact upon arrival at Eberline and Vista. Custody seals were not present upon receipt at Weck. If necessary, the client ID was added to the sample result summary by the reviewer.

Data Qualifier Reference Table

Qualifier	Organics	Inorganics
U	The analyte was analyzed for, but was not detected above the reported sample quantitation limit. The associated value is the quantitation limit or the estimated detection limit for dioxins.	The material was analyzed for, but was not detected above the level of the associated value. The associated value is either the sample quantitation limit or the sample detection limit. The associated value is the sample detection limit or the quantitation limit for perchlorate only.
J	The analyte was positively identified; the associated numerical value is the approximate concentration of the analyte in the sample.	The associated value is an estimated quantity.
N	The analysis indicates the presence of an analyte for which there is presumptive evidence to make a "tentative identification."	Not applicable.
NJ	The analysis indicates the presence of an analyte that has been "tentatively identified" and the associated numerical value represents its approximate concentration.	Not applicable.
UJ	The analyte was not deemed above the reported sample quantitation limit. However, the reported quantitation limit is approximate and may or may not represent the actual limit of quantitation necessary to accurately and precisely measure the analyte in the sample.	The material was analyzed for, but was not detected. The associated value is an estimate and may be inaccurate or imprecise.
R	The data are unusable. The sample results are rejected due to serious deficiencies in the ability to analyze the sample and to meet quality control criteria. The presence or absence of the analyte cannot be verified.	The data are unusable. The sample results are rejected due to serious deficiencies in the ability to analyze the sample and to meet quality control criteria. The presence or absence of the analyte cannot be verified.

Qualification Code Reference Table

Qualifier	Organics	Inorganics
H	Holding times were exceeded.	Holding times were exceeded.
S	Surrogate recovery was outside QC limits.	The sequence or number of standards used for the calibration was incorrect
C	Calibration %RSD or %D was noncompliant.	Correlation coefficient is <0.995.
R	Calibration RRF was <0.05.	%R for calibration is not within control limits.
B	Presumed contamination as indicated by the preparation (method) blank results.	Presumed contamination as indicated by the preparation (method) or calibration blank results.
L	Laboratory Blank Spike/Blank Spike Duplicate %R was not within control limits.	Laboratory Control Sample %R was not within control limits.
Q	MS/MSD recovery was poor or RPD high.	MS recovery was poor.
E	Not applicable.	Duplicates showed poor agreement.
I	Internal standard performance was unsatisfactory.	ICP ICS results were unsatisfactory.
A	Not applicable.	ICP Serial Dilution %D were not within control limits.
M	Tuning (BFB or DFTPP) was noncompliant.	Not applicable.
T	Presumed contamination as indicated by the trip blank results.	Not applicable.
+	False positive – reported compound was not present.	Not applicable.
-	False negative – compound was present but not reported.	Not applicable.
F	Presumed contamination as indicated by the FB or ER results.	Presumed contamination as indicated by the FB or ER results.
\$	Reported result or other information was incorrect.	Reported result or other information was incorrect.
?	TIC identity or reported retention time has been changed.	Not applicable.

Qualification Code Reference Table Cont.

D	The analysis with this flag should not be used because another more technically sound analysis is available.	The analysis with this flag should not be used because another more technically sound analysis is available.
P	Instrument performance for pesticides was poor.	Post Digestion Spike recovery was not within control limits.
DNQ	The reported result is above the method detection limit but is less than the reporting limit.	The reported result is above the method detection limit but is less than the reporting limit.
*II, *III	Unusual problems found with the data that have been described in Section II, "Sample Management," or Section III, "Method Analyses." The number following the asterisk (*) will indicate the report section where a description of the problem can be found.	Unusual problems found with the data that have been described in Section II, "Sample Management," or Section III, "Method Analyses." The number following the asterisk (*) will indicate the report section where a description of the problem can be found.

III. Method Analyses

A. EPA METHOD 1613—Dioxin/Furans

Reviewed By: K. Shadowlight

Date Reviewed: March 1, 2008

The sample listed in Table 1 for this analysis was validated based on the guidelines outlined in the *MEC^X Data Validation Procedure for Dioxins and Furans (DVP-19, Rev. 0)*, *USEPA Method 1613*, and the *National Functional Guidelines Chlorinated Dioxin/Furan Data Review (8/02)*.

- Holding Times: Extraction and analytical holding times were met. The water sample was extracted and analyzed within one year of collection.
- Instrument Performance: Instrument performance criteria were met. Following are findings associated with instrument performance.
 - GC Column Performance: A Windows Defining Mix (WDM) containing the first and last eluting congeners of each descriptor and isomer specificity compounds was not analyzed prior to the initial calibration sequence or at the beginning of each analytical sequence; however, the first and last eluting congeners and isomer specificity compounds were added to the midpoint of the initial calibration and to the continuing calibration standards. The GC column performance in the calibrations was acceptable, with the height of the valley between the closely eluting isomers and 2,3,7,8-TCDD reported as less than 25%.
 - Mass Spectrometer Performance: The mass spectrometer performance was acceptable with the static resolving power greater than 10,000.
- Calibration: Calibration criteria were met.
 - Initial Calibration: Initial calibration criteria were met. The initial calibration was acceptable with %RSDs $\leq 20\%$ for the 16 native compounds (calibration by isotope dilution) and $\leq 35\%$ for the one native and all labeled compounds (calibration by internal standard). The relative retention times and ion abundance ratios were within the Method 1613 QC limits for all standards.
 - Continuing Calibration: Calibration verification (VER) consisted of a mid-level standard (CS3) analyzed at the beginning of each analytical sequence. The VERs were acceptable with the concentrations within the acceptance criteria listed in Table 6 of EPA Method 1613. The ion abundance ratios and relative retention times were within the method QC limits.
- Blanks: Total HpCDD was detected in the method blank above the EDL. The result in the sample was qualified as estimated, "J," as a portion of the reported total HpCDD was

considered to be method blank contamination. The method blank had no other target compound detects above the EDL.

- Blank Spikes and Laboratory Control Samples: Recoveries were within the acceptance criteria listed in Table 6 of Method 1613.
- Field QC Samples: Field QC samples were evaluated, and if necessary, qualified based on method blanks and other laboratory QC results affecting the usability of the field QC data. Any remaining detects were used to evaluate the associated site samples. Following are findings associated with field QC samples:
 - Field Blanks and Equipment Rinsates: This SDG had no identified field blank or equipment rinsate samples.
 - Field Duplicates: There were no field duplicate samples identified for this SDG.
- Internal Standards Performance: The labeled standard recoveries were within the acceptance criteria listed in Table 7 of Method 1613.
- Compound Identification: Compound identification was verified. The laboratory analyzed for polychlorinated dioxins/furans by EPA Method 1613.
- Compound Quantification and Reported Detection Limits: Compound quantitation was verified by recalculating any sample detects and a representative number of blank spike concentrations. The laboratory calculated and reported compound-specific detection limits. Any detects below the laboratory lower calibration level were qualified as estimated, “J,” and coded with “DNQ,” in order to comply with the NPDES permit. Nondetects are valid to the estimated detection limit (EDL).

B. EPA METHODS 200.8, 245.1—Metals and Mercury

Reviewed By: P. Meeks

Date Reviewed: March 7, 2008

The sample listed in Table 1 for this analysis was validated based on the guidelines outlined in the *MEC^X Data Validation Procedure for Metals (DVP-5, Rev. 0 and DVP-21, Rev. 0)*, *EPA Methods 200.8, 245.1*, and the *National Functional Guidelines for Inorganic Data Review (2/94)*.

- Holding Times: The analytical holding times, 6 months for metals and 28 days for mercury, were met.
- Tuning: The mass calibration and resolution checks criteria were met. All tuning solution %RSDs were $\leq 5\%$, and all masses of interest were calibrated to ≤ 0.1 amu and ≤ 0.9 amu at 10% peak height.

- Calibration: Calibration criteria were met. Mercury initial calibration r^2 values were ≥ 0.995 and all initial and continuing calibration recoveries were within 90-110% for the ICP-MS metals and 85-115% for mercury.
- Blanks: There were no applicable detects in the method blanks or CCBs.
- Interference Check Samples: ICSA/B analyses were performed in association with the metals analyses. Recoveries were within the method-established control limits. Most analytes were reported in the ICSA solution; however, the reviewer was not able to ascertain if the detection was indicative of matrix interference.
- Blank Spikes and Laboratory Control Samples: The recoveries were within laboratory-established QC limits.
- Laboratory Duplicates: No laboratory duplicate analyses were performed.
- Matrix Spike/Matrix Spike Duplicate: MS/MSD analyses were not performed on the sample in this SDG. Evaluation of method accuracy was based on LCS results.
- Serial Dilution: No serial dilution analyses were performed.
- Internal Standards Performance: All sample internal standard intensities were within 30-120% of the internal standard intensities measured in the initial calibration. The bracketing CCV and CCB internal standard intensities were within 80-120% of the internal standard intensities measured in the initial calibration.
- Sample Result Verification: Calculations were verified and the sample results reported on the sample result summary were verified against the raw data. No transcription errors or calculation errors were noted. Detects reported below the reporting limit were qualified as estimated, "J," and coded with "DNQ," in order to comply with the NPDES permit. Reported nondetects are valid to the MDL.
- Field QC Samples: Field QC samples were evaluated, and if necessary, qualified based on method blanks and other laboratory QC results affecting the usability of the field QC data. Any remaining detects were used to evaluate the associated site samples. Following are findings associated with field QC samples:
 - Field Blanks and Equipment Rinsates: This SDG had no identified field blank or equipment rinsate samples.
 - Field Duplicates: There were no field duplicate samples identified for this SDG.

C. VARIOUS EPA METHODS — Radionuclides

Reviewed By: P. Meeks

Date Reviewed: March 5, 2008

The sample listed in Table 1 for this analysis was validated based on the guidelines outlined in the *EPA Methods 900.0, 901.1, 903.1, 904.0, 905.0, and 906.0, ASTM Method D-5174, and the National Functional Guidelines for Inorganic Data Review (2/94)*.

- **Holding Times:** The tritium sample was analyzed within 180 days of collection. Aliquots for gross alpha and, gross beta were prepared within the five-day analytical holding time for unpreserved samples. The aliquots for radium-226, radium-228, strontium-90, gamma spectroscopy, and total uranium were prepared beyond the five-day holding time for unpreserved samples; therefore, these results were qualified as estimated, "J," for detects and, "UJ," for nondetects.
- **Calibration:** The laboratory calibration information included the standard certificates and applicable preparation/dilutions logs for NIST-traceability.

The gross alpha detector efficiency was less than 20%; therefore, gross alpha detected in the sample was qualified as an estimated detect, "J." The gross beta detector efficiency was greater than 20%.

The tritium aliquot was spiked for efficiency determination; therefore, no calibration was necessary. The tritium detector efficiency for the sample was at least 20% and was considered acceptable. The internal spike efficiency to default efficiency ratios was near 1, indicating that quenching did not occur.

The strontium chemical yield was at least 70% and was considered acceptable. The strontium continuing calibration results were within the laboratory control limits.

The radium-226 cell efficiencies were determined in September 2006. The radium-226 continuing calibration results were within the laboratory-established control limits. The radium-228 calibration utilized actinium-228 and was verified in February 2001. The radium-228 tracer, yttrium oxalate yields were greater than 70%.

The gamma spectroscopy geometry-specific, detector efficiencies were determined in September 1999 and February 2007. All analytes were determined at the maximum photopeak energy.

The kinetic phosphorescence analyzer (KPA) was calibrated immediately prior to the sample analysis. All calibration check standard recoveries were within 90-110% and were deemed acceptable.

- **Blanks:** There were no analytes detected in the method blank.

- Blank Spikes and Laboratory Control Samples: The recoveries were within laboratory-established control limits.
- Laboratory Duplicates: No laboratory duplicate analyses were performed on the sample in this SDG.
- Matrix Spike/Matrix Spike Duplicate: No MS/MSD analyses were performed for the sample in this SDG. Method accuracy was evaluated based on the LCS results.
- Sample Result Verification: An EPA Level IV review was performed for the sample in this data package. The sample results and MDAs reported on the sample result form were verified against the raw data and no calculation or transcription errors were noted. Reported nondetects are valid to the MDA.
- Field QC Samples: Field QC samples were evaluated, and if necessary, qualified based on method blanks and other laboratory QC results affecting the usability of the field QC data. Any remaining detects were used to evaluate the associated site samples. Following are findings associated with field QC samples:
 - Field Blanks and Equipment Rinsates: This SDG had no identified field blank or equipment rinsate samples.
 - Field Duplicates: There were no field duplicate samples identified for this SDG.

Sample ID: IRA2500-01 *Out-fall 003*

EPA Method 1613

Client Data
 Name: Test America-Irvine, CA
 Project: IRA2500
 Date Collected: 25-Jan-08
 Time Collected: 0825

Sample Data
 Matrix: Aqueous
 Sample Size: 1.00 L

Laboratory Data
 Lab Sample: 30210-001
 QC Batch No.: 9921
 Date Analyzed DB-5: 7-Feb-08
 Date Received: 29-Jan-08
 Date Extracted: 2-Feb-08
 Date Analyzed DB-225: NA

Analyte	Conc. (ug/L)	DL ^a	EMPC ^b	Qualifiers	Labeled Standard	%R	LCL-UCL ^d	Qualifiers
2,3,7,8-TCDD	ND	0.00000105			IS 13C-2,3,7,8-TCDD	79.6	25 - 164	
1,2,3,7,8-PeCDD	ND	0.000000764			13C-1,2,3,7,8-PeCDD	69.2	25 - 181	
1,2,3,4,7,8-HxCDD	ND	0.00000190			13C-1,2,3,4,7,8-HxCDD	67.9	32 - 141	
1,2,3,6,7,8-HxCDD	ND	0.00000191			13C-1,2,3,6,7,8-HxCDD	70.3	28 - 130	
1,2,3,7,8,9-HxCDD	ND	0.00000183			13C-1,2,3,4,6,7,8-HpCDD	71.6	23 - 140	
1,2,3,4,6,7,8-HpCDD	0.00000816			J	13C-OCDD	57.7	17 - 157	
OCDD	0.0000552				13C-2,3,7,8-TCDF	79.1	24 - 169	
2,3,7,8-TCDF	ND	0.000000724			13C-1,2,3,7,8-PeCDF	76.0	24 - 185	
1,2,3,7,8-PeCDF	ND	0.000000757			13C-2,3,4,7,8-PeCDF	64.4	21 - 178	
2,3,4,7,8-PeCDF	ND	0.000000932			13C-1,2,3,4,7,8-HxCDF	72.1	26 - 152	
1,2,3,4,7,8-HxCDF	ND	0.000000686			13C-1,2,3,6,7,8-HxCDF	66.1	26 - 123	
1,2,3,6,7,8-HxCDF	ND	0.000000784			13C-2,3,4,6,7,8-HxCDF	61.3	28 - 136	
2,3,4,6,7,8-HxCDF	ND	0.000000968			13C-1,2,3,7,8,9-HxCDF	65.8	29 - 147	
1,2,3,7,8,9-HxCDF	ND	0.00000120			13C-1,2,3,4,6,7,8-HpCDF	60.1	28 - 143	
1,2,3,4,6,7,8-HpCDF	ND	0.00000174			13C-1,2,3,4,7,8,9-HpCDF	65.3	26 - 138	
1,2,3,4,7,8,9-HpCDF	ND	0.00000179			13C-OCDF	62.2	17 - 157	
OCDF	ND	0.0000101			CRS 37Cl-2,3,7,8-TCDD	88.4	35 - 197	

Totals

Total TCDD	ND	0.00000105						
Total PeCDD	ND	0.00000231						
Total HxCDD	ND	0.00000273						
Total HpCDD	0.0000173			B				
Total TCDF	ND	0.000000724						
Total PeCDF	ND	0.000000836						
Total HxCDF	ND	0.000000890						
Total HpCDF	ND	0.00000243						

Footnotes
 a. Sample specific estimated detection limit.
 b. Estimated maximum possible concentration.
 c. Method detection limit.
 d. Lower control limit - upper control limit.

Analyst: *Level IV* Approved By: William J. Luksemburg 08-Feb-2008 12:17

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Routine Outfall 003
Report Number: IRA2500

Sampled: 01/25/08
Received: 01/25/08

METALS

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRA2500-01 (Outfall 003 - Water)									
Reporting Units: ug/l									
Antimony J/DNR	EPA 200.8	8A28076	0.20	2.0	0.26	1	01/28/08	01/28/08	J
Cadmium ↓	EPA 200.8	8A28076	0.11	1.0	0.19	1	01/28/08	01/28/08	J
Copper	EPA 200.8	8A28076	0.75	2.0	3.3	1	01/28/08	01/28/08	J
Lead J/DNR	EPA 200.8	8A28076	0.30	1.0	0.44	1	01/28/08	01/28/08	J
Thallium U	EPA 200.8	8A28076	0.20	1.0	ND	1	01/28/08	01/28/08	J

LEVEL IV

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRA2500 <Page 2 of 15>

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08

Received: 01/25/08

DISSOLVED METALS

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRA2500-01 (Outfall 003 - Water) - cont.									
Reporting Units: ug/l									
Antimony	EPA 200.8-Diss	8A25156	0.20	2.0	0.26	1	01/25/08	01/26/08	J
Cadmium	EPA 200.8-Diss	8A25156	0.11	1.0	0.16	1	01/25/08	01/26/08	J
Copper	EPA 200.8-Diss	8A25156	0.75	2.0	2.8	1	01/25/08	01/26/08	
Lead	EPA 200.8-Diss	8A25156	0.30	1.0	ND	1	01/25/08	01/26/08	
Thallium	EPA 200.8-Diss	8A25156	0.20	1.0	ND	1	01/25/08	01/28/08	

LEVEL IV

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRA2500 <Page 3 of 15>

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Routine Outfall 003
Report Number: IRA2500

Sampled: 01/25/08
Received: 01/25/08

Metals by EPA 200 Series Methods

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRA2500-01 (Outfall 003 - Water) - cont.									
Reporting Units: ug/l									
Mercury, Dissolved	U	EPA 245.1	W8A1076	0.050	0.20	ND	1	01/30/08	01/31/08
Mercury, Total	↓	EPA 245.1	W8A1076	0.050	0.20	ND	1	01/30/08	01/31/08

LEVEL IV

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRA2500 <Page 5 of 15>

Eberline Services

ANALYSIS RESULTS

SDG <u>8690</u>	Client <u>TA IRVINE</u>
Work Order <u>R801173-01</u>	Contract <u>PROJECT# IRA2500</u>
Received Date <u>01/29/08</u>	Matrix <u>WATER</u>

Client	Lab	Sample ID	Collected	Analyzed	Nuclide	Results + 2σ	Units	MDA
Outfall 003 IRA2500-01	8690-001	01/25/08	02/16/08	GrossAlpha	1.34 ± 0.61	pCi/L	0.60	J/R
			02/16/08	Gross Beta	4.34 ± 0.66	pCi/L	0.91	
			02/20/08	Ra-228	0.449 ± 0.20	pCi/L	0.48	U/J/H
			02/15/08	K-40 (G)	U	pCi/L	21	↓
			02/15/08	Cs-137 (G)	U	pCi/L	0.81	U
			02/21/08	H-3	-60.6 ± 92	pCi/L	160	U
			02/20/08	Ra-226	0.001 ± 0.47	pCi/L	0.90	U/J/H
			02/14/08	Sr-90	0.269 ± 0.28	pCi/L	0.55	↓
			02/19/08	Total U	0.380 ± 0.043	pCi/L	0.022	J/H

LEVEL IV

Certified by <u>nd</u>
Report Date <u>02/27/08</u>
Page 1

APPENDIX G

Section 14

Outfall 003, January 25, 2008

Test America Analytical Laboratory Report

LABORATORY REPORT

Prepared For: MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project: Routine Outfall 003

Sampled: 01/25/08
Received: 01/25/08
Issued: 02/28/08 09:50

NELAP #01108CA California ELAP#1197 CSDLAC #10256

The results listed within this Laboratory Report pertain only to the samples tested in the laboratory. The analyses contained in this report were performed in accordance with the applicable certifications as noted. All soil samples are reported on a wet weight basis unless otherwise noted in the report. This Laboratory Report is confidential and is intended for the sole use of TestAmerica and its client. This report shall not be reproduced, except in full, without written permission from TestAmerica. The Chain of Custody, 1 page, is included and is an integral part of this report.

This entire report was reviewed and approved for release.

SAMPLE CROSS REFERENCE

SUBCONTRACTED: Refer to the last page for specific subcontract laboratory information included in this report.

ADDITIONAL INFORMATION: This is a final report to include all subcontract data.

LABORATORY ID
IRA2500-01

CLIENT ID
Outfall 003

MATRIX
Water

Reviewed By:



TestAmerica Irvine

Joseph Doak
Project Manager

MWH-Pasadena/Boeing
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007
 Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08

Received: 01/25/08

METALS

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRA2500-01 (Outfall 003 - Water)									
Reporting Units: ug/l									
Antimony	EPA 200.8	8A28076	0.20	2.0	0.26	1	01/28/08	01/28/08	J
Cadmium	EPA 200.8	8A28076	0.11	1.0	0.19	1	01/28/08	01/28/08	J
Copper	EPA 200.8	8A28076	0.75	2.0	3.3	1	01/28/08	01/28/08	
Lead	EPA 200.8	8A28076	0.30	1.0	0.44	1	01/28/08	01/28/08	J
Thallium	EPA 200.8	8A28076	0.20	1.0	ND	1	01/28/08	01/28/08	

TestAmerica Irvine

Joseph Doak
 Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

MWH-Pasadena/Boeing
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007
 Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08

Received: 01/25/08

DISSOLVED METALS

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRA2500-01 (Outfall 003 - Water) - cont.									
Reporting Units: ug/l									
Antimony	EPA 200.8-Diss	8A25156	0.20	2.0	0.26	1	01/25/08	01/26/08	J
Cadmium	EPA 200.8-Diss	8A25156	0.11	1.0	0.16	1	01/25/08	01/26/08	J
Copper	EPA 200.8-Diss	8A25156	0.75	2.0	2.8	1	01/25/08	01/26/08	
Lead	EPA 200.8-Diss	8A25156	0.30	1.0	ND	1	01/25/08	01/26/08	
Thallium	EPA 200.8-Diss	8A25156	0.20	1.0	ND	1	01/25/08	01/28/08	

TestAmerica Irvine

Joseph Doak
 Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

MWH-Pasadena/Boeing
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007
 Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08
 Received: 01/25/08

INORGANICS

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRA2500-01 (Outfall 003 - Water) - cont.									
Reporting Units: mg/l									
Hexane Extractable Material (Oil & Grease)	EPA 1664A	8B04061	1.3	4.8	ND	1	02/04/08	02/04/08	
Chloride	EPA 300.0	8A25053	0.25	0.50	9.4	1	01/25/08	01/25/08	
Nitrate/Nitrite-N	EPA 300.0	8A25053	0.15	0.26	2.4	1	01/25/08	01/25/08	
Sulfate	EPA 300.0	8A25053	0.20	0.50	18	1	01/25/08	01/25/08	
Total Dissolved Solids	SM2540C	8A31077	10	10	170	1	01/31/08	01/31/08	

TestAmerica Irvine

Joseph Doak
 Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08

Received: 01/25/08

Metals by EPA 200 Series Methods

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRA2500-01 (Outfall 003 - Water) - cont.									
Reporting Units: ug/l									
Mercury, Dissolved	EPA 245.1	W8A1076	0.050	0.20	ND	1	01/30/08	01/31/08	
Mercury, Total	EPA 245.1	W8A1076	0.050	0.20	ND	1	01/30/08	01/31/08	

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRA2500 <Page 5 of 15>
NPDES - 690

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08
Received: 01/25/08

SHORT HOLD TIME DETAIL REPORT

	Hold Time (in days)	Date/Time Sampled	Date/Time Received	Date/Time Extracted	Date/Time Analyzed
Sample ID: Outfall 003 (IRA2500-01) - Water EPA 300.0	2	01/25/2008 08:25	01/25/2008 18:20	01/25/2008 19:00	01/25/2008 20:00

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRA2500 <Page 6 of 15>
NPDES - 691

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08
Received: 01/25/08

METHOD BLANK/QC DATA

METALS

Analyte	Result	Reporting Limit	MDL	Units	Spike Level	Source Result	%REC %REC	%REC Limits	RPD	RPD Limit	Data Qualifiers
Batch: 8A28076 Extracted: 01/28/08											
Blank Analyzed: 01/28/2008 (8A28076-BLK1)											
Antimony	ND	2.0	0.20	ug/l							
Cadmium	ND	1.0	0.11	ug/l							
Copper	ND	2.0	0.75	ug/l							
Lead	ND	1.0	0.30	ug/l							
Thallium	ND	1.0	0.20	ug/l							
LCS Analyzed: 01/28/2008 (8A28076-BS1)											
Antimony	83.1	2.0	0.20	ug/l	80.0		104	85-115			
Cadmium	82.2	1.0	0.11	ug/l	80.0		103	85-115			
Copper	83.7	2.0	0.75	ug/l	80.0		105	85-115			
Lead	82.0	1.0	0.30	ug/l	80.0		102	85-115			
Thallium	81.4	1.0	0.20	ug/l	80.0		102	85-115			
Matrix Spike Analyzed: 01/28/2008 (8A28076-MS1) Source: IRA2324-01											
Antimony	83.5	2.0	0.20	ug/l	80.0	ND	104	70-130			
Cadmium	81.0	1.0	0.11	ug/l	80.0	ND	101	70-130			
Copper	85.4	2.0	0.75	ug/l	80.0	2.97	103	70-130			
Lead	81.3	1.0	0.30	ug/l	80.0	0.484	101	70-130			
Thallium	83.7	1.0	0.20	ug/l	80.0	ND	105	70-130			
Matrix Spike Analyzed: 01/28/2008 (8A28076-MS2) Source: IRA2432-04											
Antimony	87.0	2.0	0.20	ug/l	80.0	ND	109	70-130			
Cadmium	78.5	1.0	0.11	ug/l	80.0	ND	98	70-130			
Copper	80.3	2.0	0.75	ug/l	80.0	1.94	98	70-130			
Lead	80.4	1.0	0.30	ug/l	80.0	0.376	100	70-130			
Thallium	81.2	1.0	0.20	ug/l	80.0	ND	102	70-130			
Matrix Spike Dup Analyzed: 01/28/2008 (8A28076-MSD1) Source: IRA2324-01											
Antimony	83.3	2.0	0.20	ug/l	80.0	ND	104	70-130	0	20	
Cadmium	80.8	1.0	0.11	ug/l	80.0	ND	101	70-130	0	20	
Copper	84.6	2.0	0.75	ug/l	80.0	2.97	102	70-130	1	20	
Lead	81.9	1.0	0.30	ug/l	80.0	0.484	102	70-130	1	20	
Thallium	83.5	1.0	0.20	ug/l	80.0	ND	104	70-130	0	20	

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08
Received: 01/25/08

METHOD BLANK/QC DATA

DISSOLVED METALS

Analyte	Result	Reporting Limit	MDL	Units	Spike Level	Source Result	%REC %REC	RPD Limits	RPD RPD	RPD Limit	Data Qualifiers
Batch: 8A25156 Extracted: 01/25/08											
Blank Analyzed: 01/26/2008-01/28/2008 (8A25156-BLK1)											
Antimony	ND	2.0	0.20	ug/l							
Cadmium	ND	1.0	0.11	ug/l							
Copper	ND	2.0	0.75	ug/l							
Lead	ND	1.0	0.30	ug/l							
Thallium	ND	1.0	0.20	ug/l							
LCS Analyzed: 01/26/2008-01/28/2008 (8A25156-BS1)											
Antimony	80.7	2.0	0.20	ug/l	80.0		101	85-115			
Cadmium	80.4	1.0	0.11	ug/l	80.0		101	85-115			
Copper	80.8	2.0	0.75	ug/l	80.0		101	85-115			
Lead	84.6	1.0	0.30	ug/l	80.0		106	85-115			
Thallium	77.6	1.0	0.20	ug/l	80.0		97	85-115			
Matrix Spike Analyzed: 01/26/2008-01/28/2008 (8A25156-MS1) Source: IRA2497-01											
Antimony	85.0	2.0	0.20	ug/l	80.0	0.221	106	70-130			
Cadmium	83.4	1.0	0.11	ug/l	80.0	ND	104	70-130			
Copper	85.3	2.0	0.75	ug/l	80.0	2.94	103	70-130			
Lead	84.7	1.0	0.30	ug/l	80.0	0.920	105	70-130			
Thallium	76.5	1.0	0.20	ug/l	80.0	ND	96	70-130			
Matrix Spike Dup Analyzed: 01/26/2008-01/28/2008 (8A25156-MSD1) Source: IRA2497-01											
Antimony	83.0	2.0	0.20	ug/l	80.0	0.221	103	70-130	2	20	
Cadmium	83.4	1.0	0.11	ug/l	80.0	ND	104	70-130	0	20	
Copper	83.7	2.0	0.75	ug/l	80.0	2.94	101	70-130	2	20	
Lead	86.0	1.0	0.30	ug/l	80.0	0.920	106	70-130	2	20	
Thallium	77.3	1.0	0.20	ug/l	80.0	ND	97	70-130	1	20	

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08
Received: 01/25/08

METHOD BLANK/QC DATA

INORGANICS

Analyte	Result	Reporting Limit	MDL	Units	Spike Level	Source Result	%REC %REC	RPD Limits	RPD RPD	RPD Limit	Data Qualifiers
Batch: 8A25053 Extracted: 01/25/08											
Blank Analyzed: 01/25/2008 (8A25053-BLK1)											
Chloride	ND	0.50	0.25	mg/l							
Nitrate/Nitrite-N	ND	0.26	0.15	mg/l							
Sulfate	ND	0.50	0.20	mg/l							
LCS Analyzed: 01/25/2008 (8A25053-BS1)											
Chloride	4.93	0.50	0.25	mg/l	5.00		99	90-110			
Sulfate	10.2	0.50	0.20	mg/l	10.0		102	90-110			
Matrix Spike Analyzed: 01/25/2008 (8A25053-MS1)											
						Source: IRA2375-01					
Chloride	9.73	0.50	0.25	mg/l	5.00	4.99	95	80-120			
Sulfate	25.6	0.50	0.20	mg/l	10.0	15.9	96	80-120			
Matrix Spike Analyzed: 01/25/2008 (8A25053-MS2)											
						Source: IRA2478-01					
Chloride	12.3	0.50	0.25	mg/l	5.00	7.60	95	80-120			
Sulfate	19.9	0.50	0.20	mg/l	10.0	9.44	104	80-120			
Matrix Spike Dup Analyzed: 01/25/2008 (8A25053-MSD1)											
						Source: IRA2375-01					
Chloride	9.76	0.50	0.25	mg/l	5.00	4.99	95	80-120	0	20	
Sulfate	25.7	0.50	0.20	mg/l	10.0	15.9	98	80-120	1	20	

Batch: 8A31077 Extracted: 01/31/08

Blank Analyzed: 01/31/2008 (8A31077-BLK1)

Total Dissolved Solids ND 10 10 mg/l

LCS Analyzed: 01/31/2008 (8A31077-BS1)

Total Dissolved Solids 1000 10 10 mg/l 1000 100 90-110

TestAmerica Irvine

Joseph Doak
Project Manager

MWH-Pasadena/Boeing
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007
 Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08
 Received: 01/25/08

METHOD BLANK/QC DATA

INORGANICS

Analyte	Result	Reporting Limit	MDL	Units	Spike Level	Source Result	%REC %REC	%REC Limits	RPD	RPD Limit	Data Qualifiers
<u>Batch: 8A31077 Extracted: 01/31/08</u>											
Duplicate Analyzed: 01/31/2008 (8A31077-DUP1)						Source: IRA2619-03					
Total Dissolved Solids	ND	10	10	mg/l		ND				10	
<u>Batch: 8B04061 Extracted: 02/04/08</u>											
Blank Analyzed: 02/04/2008 (8B04061-BLK1)											
Hexane Extractable Material (Oil & Grease)	1.40	5.0	1.4	mg/l							J
LCS Analyzed: 02/04/2008 (8B04061-BS1)											
Hexane Extractable Material (Oil & Grease)	19.5	5.0	1.4	mg/l	20.2		97	78-114			MNR1
LCS Dup Analyzed: 02/04/2008 (8B04061-BSD1)											
Hexane Extractable Material (Oil & Grease)	18.2	5.0	1.4	mg/l	20.2		90	78-114	7	11	

TestAmerica Irvine

Joseph Doak
 Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

MWH-Pasadena/Boeing
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007
 Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08
 Received: 01/25/08

METHOD BLANK/QC DATA

Metals by EPA 200 Series Methods

Analyte	Result	Reporting Limit	MDL	Units	Spike Level	Source Result	%REC	%REC Limits	RPD	RPD Limit	Data Qualifiers
Batch: W8A1076 Extracted: 01/30/08											
Blank Analyzed: 01/31/2008 (W8A1076-BLK1)											
Mercury, Dissolved	ND	0.20	0.050	ug/l							
Mercury, Total	ND	0.20	0.050	ug/l							
LCS Analyzed: 01/31/2008 (W8A1076-BS1)											
Mercury, Dissolved	0.913	0.20	0.050	ug/l	1.00		91	85-115			
Mercury, Total	0.913	0.20	0.050	ug/l	1.00		91	85-115			
Matrix Spike Analyzed: 01/31/2008 (W8A1076-MS1) Source: 8012935-01											
Mercury, Dissolved	0.971	0.20	0.050	ug/l	1.00	0.0450	93	70-130			
Mercury, Total	0.971	0.20	0.050	ug/l	1.00	0.0450	93	70-130			
Matrix Spike Analyzed: 01/31/2008 (W8A1076-MS2) Source: 8012939-01											
Mercury, Dissolved	2.01	0.20	0.050	ug/l	1.00	1.18	83	70-130			
Mercury, Total	2.01	0.20	0.050	ug/l	1.00	1.18	83	70-130			
Matrix Spike Dup Analyzed: 01/31/2008 (W8A1076-MSD1) Source: 8012935-01											
Mercury, Dissolved	0.957	0.20	0.050	ug/l	1.00	0.0450	91	70-130	1	20	
Mercury, Total	0.957	0.20	0.050	ug/l	1.00	0.0450	91	70-130	1	20	
Matrix Spike Dup Analyzed: 01/31/2008 (W8A1076-MSD2) Source: 8012939-01											
Mercury, Dissolved	1.99	0.20	0.050	ug/l	1.00	1.18	81	70-130	1	20	
Mercury, Total	1.99	0.20	0.050	ug/l	1.00	1.18	81	70-130	1	20	

TestAmerica Irvine

Joseph Doak
 Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

MWH-Pasadena/Boeing
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007
 Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08
 Received: 01/25/08

Compliance Check

The results obtained from the analytical testing of this data set were checked against compliance limits received from the client. Any results at or above the compliance limits appear in bold on this page.

LabNumber	Analysis	Analyte	Units	Result	MRL	Compliance Limit
IRA2500-01	1664-HEM	Hexane Extractable Material (Oil & Greas	mg/l	0.67	4.8	15
IRA2500-01	Antimony-200.8	Antimony	ug/l	0.26	2.0	6
IRA2500-01	Cadmium-200.8	Cadmium	ug/l	0.19	1.0	4
IRA2500-01	Chloride - 300.0	Chloride	mg/l	9.42	0.50	150
IRA2500-01	Copper-200.8	Copper	ug/l	3.26	2.0	14
IRA2500-01	Hg_w 245.1	Mercury, Total	ug/l	0.033	0.20	0.13
IRA2500-01	Lead-200.8	Lead	ug/l	0.44	1.0	5.2
IRA2500-01	Nitrogen, NO3+NO2 -N	Nitrate/Nitrite-N	mg/l	2.39	0.26	10
IRA2500-01	Sulfate-300.0	Sulfate	mg/l	18	0.50	250
IRA2500-01	TDS - SM 2540C	Total Dissolved Solids	mg/l	167	10	850
IRA2500-01	Thallium-200.8	Thallium	ug/l	0.0024	1.0	2

TestAmerica Irvine

Joseph Doak
 Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08
Received: 01/25/08

DATA QUALIFIERS AND DEFINITIONS

- J** Estimated value. Analyte detected at a level less than the Reporting Limit (RL) and greater than or equal to the Method Detection Limit (MDL). The user of this data should be aware that this data is of limited reliability.
- MNR1** There was no MS/MSD analyzed with this batch due to insufficient sample volume. See Blank Spike/Blank Spike Duplicate.
- ND** Analyte NOT DETECTED at or above the reporting limit or MDL, if MDL is specified.
- RPD** Relative Percent Difference

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRA2500 <Page 13 of 15>
NPDES - 698

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08
Received: 01/25/08

Certification Summary

TestAmerica Irvine

Method	Matrix	Nelac	California
EPA 1664A	Water		
EPA 200.8-Diss	Water	X	X
EPA 200.8	Water	X	X
EPA 300.0	Water	X	X
SM2540C	Water	X	

Nevada and NELAP provide analyte specific accreditations. Analyte specific information for TestAmerica may be obtained by contacting the laboratory or visiting our website at www.testamericainc.com

Subcontracted Laboratories

Aquatic Testing Laboratories-SUB *California Cert #1775*

4350 Transport Street, Unit 107 - Ventura, CA 93003

Analysis Performed: Bioassay-7 dy Chrnrc
Samples: IRA2500-01

Eberline Services - SUB

2030 Wright Avenue - Richmond, CA 94804

Analysis Performed: Gamma Spec
Samples: IRA2500-01

Analysis Performed: Gross Alpha
Samples: IRA2500-01

Analysis Performed: Gross Beta
Samples: IRA2500-01

Analysis Performed: Radium, Combined
Samples: IRA2500-01

Analysis Performed: Strontium 90
Samples: IRA2500-01

Analysis Performed: Tritium
Samples: IRA2500-01

Analysis Performed: Uranium, Combined
Samples: IRA2500-01

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Routine Outfall 003

Report Number: IRA2500

Sampled: 01/25/08

Received: 01/25/08

Vista Analytical *NELAC Cert #02102CA, California Cert #1640, Nevada Cert #CA-413*

1104 Windfield Way - El Dorado Hills, CA 95762

Analysis Performed: 1613-Dioxin-HR-Alta
Samples: IRA2500-01

Weck Laboratories, Inc

14859 E. Clark Avenue - City of Industry, CA 91745

Method Performed: EPA 245.1
Samples: IRA2500-01

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

CHAIN OF CUSTODY FORM

Test America Version 12/20/07

ANALYSIS REQUIRED

Client Name/Address
MWH-Arcadia
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007
 Test America Contact Joseph Doak

Project
 Boeing-SSFL NPDES
Routine Outfall 003
 Stormwater at RMHF

Project Manager: **Bronwyn Kelly**
 Phone Number:
 (626) 568-6691
 Fax Number:
 (626) 568-6515

Sampler: **MARISCALLO, J. BARRAO, R.**

Field readings:
 Temp = **47.7°**
 pH = **7.6**
 Time of readings = **8:25**


Sample Description	Sample Matrix	Container Type	# of Cont.	Preservative	Sampling Date/Time	Bottle #	Total Recoverable Metals: Sb, Cd, Cu, Pb, Hg, Ti	TCDD (and all congeners)	Oil & Grease (1664-HEM)	Cl ⁻ , SO ₄ ²⁻ , NO ₃ ⁻ +NO ₂ ⁻	TDS	Gross Alpha(900.0), Gross Beta(90.0), Tritium (H-3) (906.0), Sr-90 (905.0), Total Combined Radium 226 (903.0 or 903.1) & Radium 228 (904.0), Uranium (908.0), K-40, CS-137 (901.0 or 901.1)	Chronic Toxicity	Total Dissolved Metals: Sb, Cd, Cu, Pb, Hg, Ti	Field readings	Comments	
Outfall 003	W	1L Poly	1	HNO ₃	1-25-08 8:25	1A	X										
Outfall 003-Dup	W	1L Poly	1	HNO ₃		1B	X										
Outfall 003	W	1L Amber	2	None		2A, 2B		X									
Outfall 003	W	1L Amber	2	HCl		3A, 3B		X									
Outfall 003	W	500 ml Poly	2	None		4A, 4B				X							
Outfall 003	W	500 ml Poly	1	None		5					X						
Outfall 003	W	2.5 Gal Cube 500 ml Amber	1	None		6A											
Outfall 003	W	500 ml Amber	1	None		6B											
Outfall 003	W	1 Gal Poly	1	None	1-25-08 8:25	7							X				Unfiltered and unpreserved analysis
Outfall 003	W	1L Poly	1	None		8								X			Only test if second rain event of the year Filter w/in 24hrs of receipt at lab

Relinquished By	Date/Time	Received By	Date/Time
<i>Joe Barron</i>	1-25-08 15:10	<i>Joe Barron</i>	1/25/08 15:10
<i>Joe Barron</i>	1-25-08 15:10	<i>Joe Barron</i>	1/25/08 15:10
<i>Joe Barron</i>	1-25-08 15:10	<i>Joe Barron</i>	1/25/08 15:10

Turn around Time: (check)
 24 Hours _____ 5 Days _____
 48 Hours _____ 10 Days _____
 72 Hours _____ Normal _____ X
 Sample Integrity: (check) On Ice: _____
 Intact _____ 44724

TR
 1/25/08
 1915

LABORATORY REPORT



**Aquatic
Testing
Laboratories**

"dedicated to providing quality aquatic toxicity testing"

4350 Transport Street, Unit 107
Ventura, CA 93003
(805) 650-0546 FAX (805) 650-0756
CA DOHS ELAP Cert. No.: 1775

Date: February 3, 2008
Client: TestAmerica - Irvine
17461 Derian Ave., Suite 100
Irvine, CA 92614
Attn: Joseph Doak

Laboratory No.: A-08012607-001
Sample ID.: IRA2500-01 (Outfall 003)

Sample Control: The sample was received by ATL within the recommended hold time, in a chilled state, and with the chain of custody record attached. Testing was conducted on only one sample per client instruction.

Date Sampled: 01/25/08
Date Received: 01/26/08
Temp. Received: 6°C
Chlorine (TRC): 0.0 mg/l
Date Tested: 01/26/08 to 02/02/08

Sample Analysis: The following analyses were performed on your sample:


Ceriodaphnia dubia Survival and Reproduction Test (EPA Method 1002).

Attached are the test data generated from the analysis of your sample.

Result Summary:

Chronic:	<u>NOEC</u>	<u>TUc</u>
<i>Ceriodaphnia</i> Survival:	100%	1.0
<i>Ceriodaphnia</i> Reproduction:	100%	1.0

Quality Control: Reviewed and approved by:

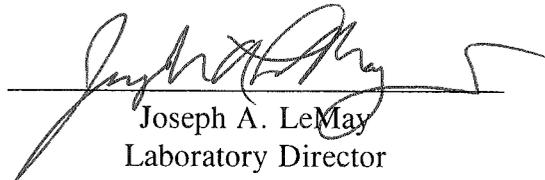
Joseph A. LeMay
Laboratory Director

**CERIODAPHNIA CHRONIC BIOASSAY
EPA METHOD 1002.0**



Lab No.: A-08012607-001
Client/ID: Test America – Outfall 003

Date Tested: 01/26/08 to 02/02/08

TEST SUMMARY

Test type: Daily static-renewal.
Species: *Ceriodaphnia dubia*.
Age: < 24 hrs; all released within 8 hrs.
Test vessel size: 30 ml.
Number of test organisms per vessel: 1.
Temperature: 25 +/- 1°C.
Dilution water: Mod. hard reconstituted (MHRW).
QA/QC Batch No.: RT-080106.

Endpoints: Survival and Reproduction.
Source: In-laboratory culture.
Food: .1 ml YTC, algae per day.
Test solution volume: 15 ml.
Number of replicates: 10.
Photoperiod: 16/8 hrs. light/dark cycle.
Test duration: 7 days.
Statistics: ToxCalc computer program.

RESULTS SUMMARY

Sample Concentration	Percent Survival	Mean Number of Young Per Female
Control	100%	24.8
100% Sample	100%	29.6
Sample not statistically significantly less than Control for either endpoint.		

CHRONIC TOXICITY

Survival NOEC	100%
Survival TUC	1.0
Reproduction NOEC	100%
Reproduction TUC	1.0

QA/QC TEST ACCEPTABILITY

Parameter	Result
Control survival ≥ 80%	Pass (100% survival)
≥ 15 young per surviving control female	Pass (24.8 young)
≥ 60% surviving controls had 3 broods	Pass (100% with 3 broods)
PMSD < 47% for reproduction; if > 47% and no toxicity at IWC, the test must be repeated	Pass (PMSD = 7.4%)
Statistically significantly different concentrations relative difference > 13%	Pass (no concentration significantly different)
Concentration response relationship acceptable	Pass (no significant response at concentration tested)

Ceriodaphnia Survival and Reproduction Test-7 Day Survival

Start Date: 1/26/2008 15:30 Test ID: 8012607 Sample ID: OUTFALL 003
 End Date: 2/2/2008 14:30 Lab ID: CAATL-Aquatic Testing Labs Sample Type: EFF2-Industrial
 Sample Date: 1/25/2008 08:25 Protocol: EPA-821-R-02-013 Test Species: CD-Ceriodaphnia dubia


Comments:

Conc-%	1	2	3	4	5	6	7	8	9	10
D-Control	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000
100	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000

Conc-%	Mean	N-Mean	Resp	Not Resp	Total	N	Fisher's Exact P	1-Tailed Critical	Isotonic	
									Mean	N-Mean
D-Control	1.0000	1.0000	0	10	10	10			1.0000	1.0000
100	1.0000	1.0000	0	10	10	10	1.0000	0.0500	1.0000	1.0000

Hypothesis Test (1-tail, 0.05)	NOEC	LOEC	ChV	TU
Fisher's Exact Test	100	>100		1
Treatments vs D-Control				

Linear Interpolation (200 Resamples)				
Point	%	SD	95% CL	Skew
IC05	>100			
IC10	>100			
IC15	>100			
IC20	>100			
IC25	>100			
IC40	>100			
IC50	>100			

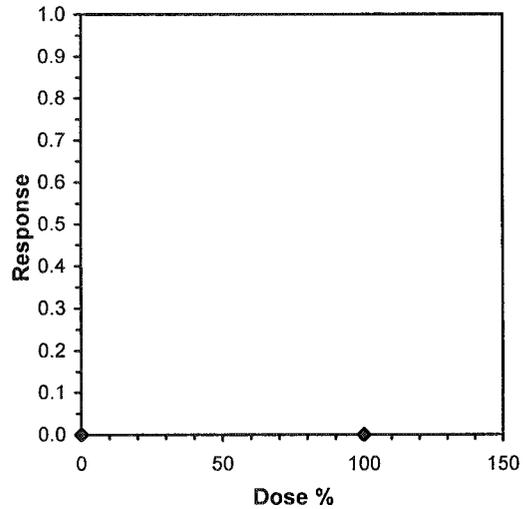

Ceriodaphnia Survival and Reproduction Test-Reproduction

Start Date: 1/26/2008 15:30 Test ID: 8012607 Sample ID: OUTFALL 003
 End Date: 2/2/2008 14:30 Lab ID: CAATL-Aquatic Testing Labs Sample Type: EFF2-Industrial
 Sample Date: 1/25/2008 08:25 Protocol: EPA-821-R-02-013 Test Species: CD-Ceriodaphnia dubia


Comments:

Conc-%	1	2	3	4	5	6	7	8	9	10
D-Control	26.000	22.000	24.000	26.000	24.000	25.000	26.000	27.000	26.000	22.000
100	28.000	31.000	28.000	27.000	35.000	27.000	29.000	34.000	29.000	28.000

Conc-%	Mean	N-Mean	Transform: Untransformed					N	t-Stat	1-Tailed Critical	MSD	Isotonic	
			Mean	Min	Max	CV%	Mean					N-Mean	
D-Control	24.800	1.0000	24.800	22.000	27.000	7.061	10				27.200	1.0000	
100	29.600	1.1935	29.600	27.000	35.000	9.582	10	-4.554	1.734	1.828	27.200	1.0000	

Auxiliary Tests	Statistic	Critical	Skew	Kurt		
Shapiro-Wilk's Test indicates normal distribution (p > 0.05)	0.916354	0.905	0.824122	0.36145		
F-Test indicates equal variances (p = 0.17)	2.623188	6.541086				
Hypothesis Test (1-tail, 0.05)	MSDu	MSDp	MSB	MSE	F-Prob	df
Homoscedastic t Test indicates no significant differences Treatments vs D-Control	1.827863	0.073704	115.2	5.555556	2.5E-04	1, 18

Linear Interpolation (200 Resamples)				
Point	%	SD	95% CL	Skew
IC05	>100			
IC10	>100			
IC15	>100			
IC20	>100			
IC25	>100			
IC40	>100			
IC50	>100			

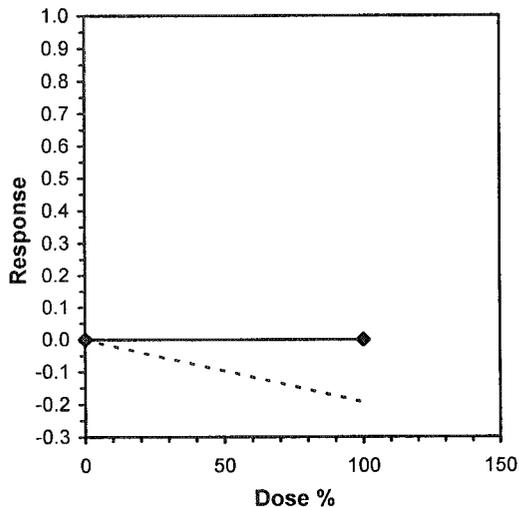

CERIODAPHNIA DUBIA CHRONIC BIOASSAY
EPA METHOD 1002.0 Raw Data Sheet



Lab No.: A-08012607-001

Client ID: TestAmerica - IRA2500-01 (Outfall 003)

Start Date: 01/26/2008

		DAY 1		DAY 2		DAY 3		DAY 4		DAY 5		DAY 6		DAY 7	
		0 hr	24hr												
Analyst Initials:		Rm	h	h	h	h	Rm	Rm	Rm	Rm	Rm	Rm	Rm	Rm	h
Time of Readings:		1530	1430	1430	1500	1500	1500	1500	1500	1600	1600	1500	1500	1500	1430
Control	DO	8.0	7.8	7.7	8.1	7.9	7.7	8.9	8.2	8.1	7.9	8.2	7.8	8.0	8.2
	pH	7.8	7.6	7.4	7.6	7.8	8.0	8.0	7.9	7.8	7.9	7.7	7.8	7.6	7.6
	Temp	25.4	24.7	25.1	24.4	25.0	24.6	24.6	24.8	24.6	24.5	25.1	24.7	25.0	24.3
100%	DO	10.3	7.7	9.7	8.0	9.4	7.9	10.2	8.5	10.3	8.2	9.6	8.3	11.6	8.6
	pH	7.3	7.4	7.0	7.4	7.1	7.5	7.1	7.5	7.0	7.5	7.1	7.5	7.0	7.4
	Temp	24.3	24.5	24.8	24.2	25.3	24.9	24.8	24.5	25.0	24.4	24.8	24.8	25.2	24.3

Additional Parameters	Control	100% Sample
Conductivity (umohms)	290	197
Alkalinity (mg/l CaCO ₃)	66	58
Hardness (mg/l CaCO ₃)	98	76
Ammonia (mg/l NH ₃ -N)	<0.2	0.4

Source of Neonates											
Replicate:	A	B	C	D	E	F	G	H	I	J	
Brood ID:	B1	E1	G2	H2	I3	J3	A6	C5	G4	I5	

Sample	Day	Number of Young Produced										Total Live Young	No. Live Adults	Analyst Initials
		A	B	C	D	E	F	G	H	I	J			
Control	1	0	0	0	0	0	0	0	0	0	0	0	10	h
	2	0	0	0	0	0	0	0	0	0	0	0	10	
	3	0	0	0	0	0	3	4	0	4	0	11	10	
	4	4	3	5	3	4	0	0	5	0	4	28	10	
	5	8	7	9	9	8	7	8	9	9	8	82	10	
	6	14	12	10	0	0	15	0	0	0	0	51	10	
	7	0	0	0	14	12	0	14	13	13	10	76	10	
	Total	26	22	24	26	24	25	26	27	26	22	248	10	
100%	1	0	0	0	0	0	0	0	0	0	0	0	10	h
	2	0	0	0	0	0	0	0	0	0	0	0	10	
	3	0	0	3	5	0	4	3	0	4	3	22	10	
	4	3	5	0	0	5	0	0	5	0	0	18	10	
	5	8	10	9	8	13	7	8	12	7	9	91	10	
	6	17	16	16	14	17	16	18	17	18	16	165	10	
	7	0	0	0	0	0	14	16	0	0	0	0	10	
	Total	28	31	28	27	35	27	29	34	29	28	296	10	

Circled fourth brood not used in statistical analysis.

7th day only used if <60% of the surviving control females have produced their third brood.

SUBCONTRACT ORDER

TestAmerica Irvine

IRA2500

SENDING LABORATORY:

TestAmerica Irvine
17461 Derian Avenue. Suite 100
Irvine, CA 92614
Phone: (949) 261-1022
Fax: (949) 260-3297
Project Manager: Joseph Doak

RECEIVING LABORATORY:

Aquatic Testing Laboratories-SUB
4350 Transport Street, Unit 107
Ventura, CA 93003
Phone : (805) 650-0546
Fax: (805) 650-0756
Project Location: California
Receipt Temperature: 6 °C Ice: Y N

Analysis	Units	Due	Expires	Comments
Sample ID: IRA2500-01	Water			Sampled: 01/25/08 08:25 pH=7.6, temp=47.7
Bioassay-7 dy Chrmic	N/A	02/05/08	01/26/08 20:25	Cerio, EPA/821-R02-013, Sub to Aquatic testing
Level 4 + EDD-OUT	N/A	02/05/08	02/22/08 08:25	**LEVEL IV QC, ACCESS 7 EDD**
<i>Containers Supplied:</i> 1 gal Poly (L)				

Joseph Doak
Released By

Released By

1/26/08
Date/Time
1/26/08 1445
Date/Time

Received By

Received By

1/26/08 1255
Date/Time
1-26-08 1445
Date/Time



***REFERENCE
TOXICANT
DATA***

CERIODAPHNIA CHRONIC BIOASSAY
EPA METHOD 1002.0
REFERENCE TOXICANT - NaCl



QA/QC Batch No.: RT-080106

Date Tested: 01/06/08 to 01/12/08

TEST SUMMARY

Test type: Daily static-renewal.
 Species: *Ceriodaphnia dubia*.
 Age: <24 hrs; all released within 8 hrs.
 Test vessel size: 30 ml.
 Number of test organisms per vessel: 1.
 Temperature: 25 +/- 1°C.
 Dilution water: Mod. hard reconstituted (MHRW).
 Reference Toxicant: Sodium chloride (NaCl).

Endpoints: Survival and Reproduction.
 Source: In-laboratory culture.
 Food: .1 ml YTC, algae per day.
 Test solution volume: 20 ml.
 Number of replicates: 10.
 Photoperiod: 16/8 hrs. light/dark cycle.
 Test duration: 6 days.
 Statistics: ToxCalc computer program.

RESULTS SUMMARY

Sample Concentration	Percent Survival		Mean Number of Young Per Female	
Control	100%		20.5	
0.25 g/l	100%		19.5	
0.5 g/l	100%		19.5	
1.0 g/l	100%		14.0	*
2.0 g/l	80%		3.2	*
4.0 g/l	0%	*	0	**

* Statistically significantly less than control at P = 0.05 level
 ** Reproduction data from concentrations greater than survival NOEC are excluded from statistical analysis.

CHRONIC TOXICITY

Survival LC50	2.5 g/l
Reproduction IC25	0.88 g/l

QA/QC TEST ACCEPTABILITY

Parameter	Result
Control survival ≥80%	Pass (100% Survival)
≥15 young per surviving control female	Pass (20.5 young)
≥60% surviving controls had 3 broods	Pass (90% with 3 broods)
PMSD <47% for reproduction	Pass (PMSD = 19.1%)
Stat. sig. diff. conc. relative difference >13%	Pass (Stat. sig. diff. conc. = 31.7%)
Concentration response relationship acceptable	Pass (Response curve normal)

Ceriodaphnia Survival and Reproduction Test-Survival Day 6


Start Date: 1/6/2008 13:00 Test ID: RT-080106c Sample ID: REF-Ref Toxicant
 End Date: 1/12/2008 13:00 Lab ID: CAATL-Aquatic Testing Labs Sample Type: NACL-Sodium chloride
 Sample Date: 1/6/2008 Protocol: FWCH-EPA-821-R-02-013 Test Species: CD-Ceriodaphnia dubia
 Comments:

Conc-gm/L	1	2	3	4	5	6	7	8	9	10
D-Control	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000
0.25	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000
0.5	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000
1	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000
2	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	1.0000	0.0000	0.0000
4	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000

Conc-gm/L	Mean	N-Mean	Resp	Not Resp	Total	N	Fisher's Exact P	1-Tailed Critical	Number Resp	Total Number
D-Control	1.0000	1.0000	0	10	10	10			0	10
0.25	1.0000	1.0000	0	10	10	10	1.0000	0.0500	0	10
0.5	1.0000	1.0000	0	10	10	10	1.0000	0.0500	0	10
1	1.0000	1.0000	0	10	10	10	1.0000	0.0500	0	10
2	0.8000	0.8000	2	8	10	10	0.2368	0.0500	2	10
4	0.0000	0.0000	10	0	10	10			10	10


Hypothesis Test (1-tail, 0.05)	NOEC	LOEC	ChV	TU
Fisher's Exact Test	2	4	2.82843	
Treatments vs D-Control				

Trimmed Spearman-Kärber			
Trim Level	EC50	95% CL	
0.0%	2.4623	2.0663	2.9342
5.0%	2.5108	2.0545	3.0683
10.0%	2.5519	1.9976	3.2599
20.0%	2.5937	2.2616	2.9745
Auto-0.0%	2.4623	2.0663	2.9342

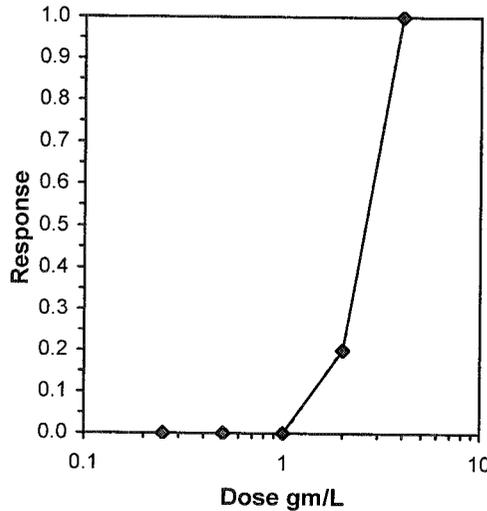

Ceriodaphnia dubia Chronic Survival Laboratory Control Chart

CV% = 5.46

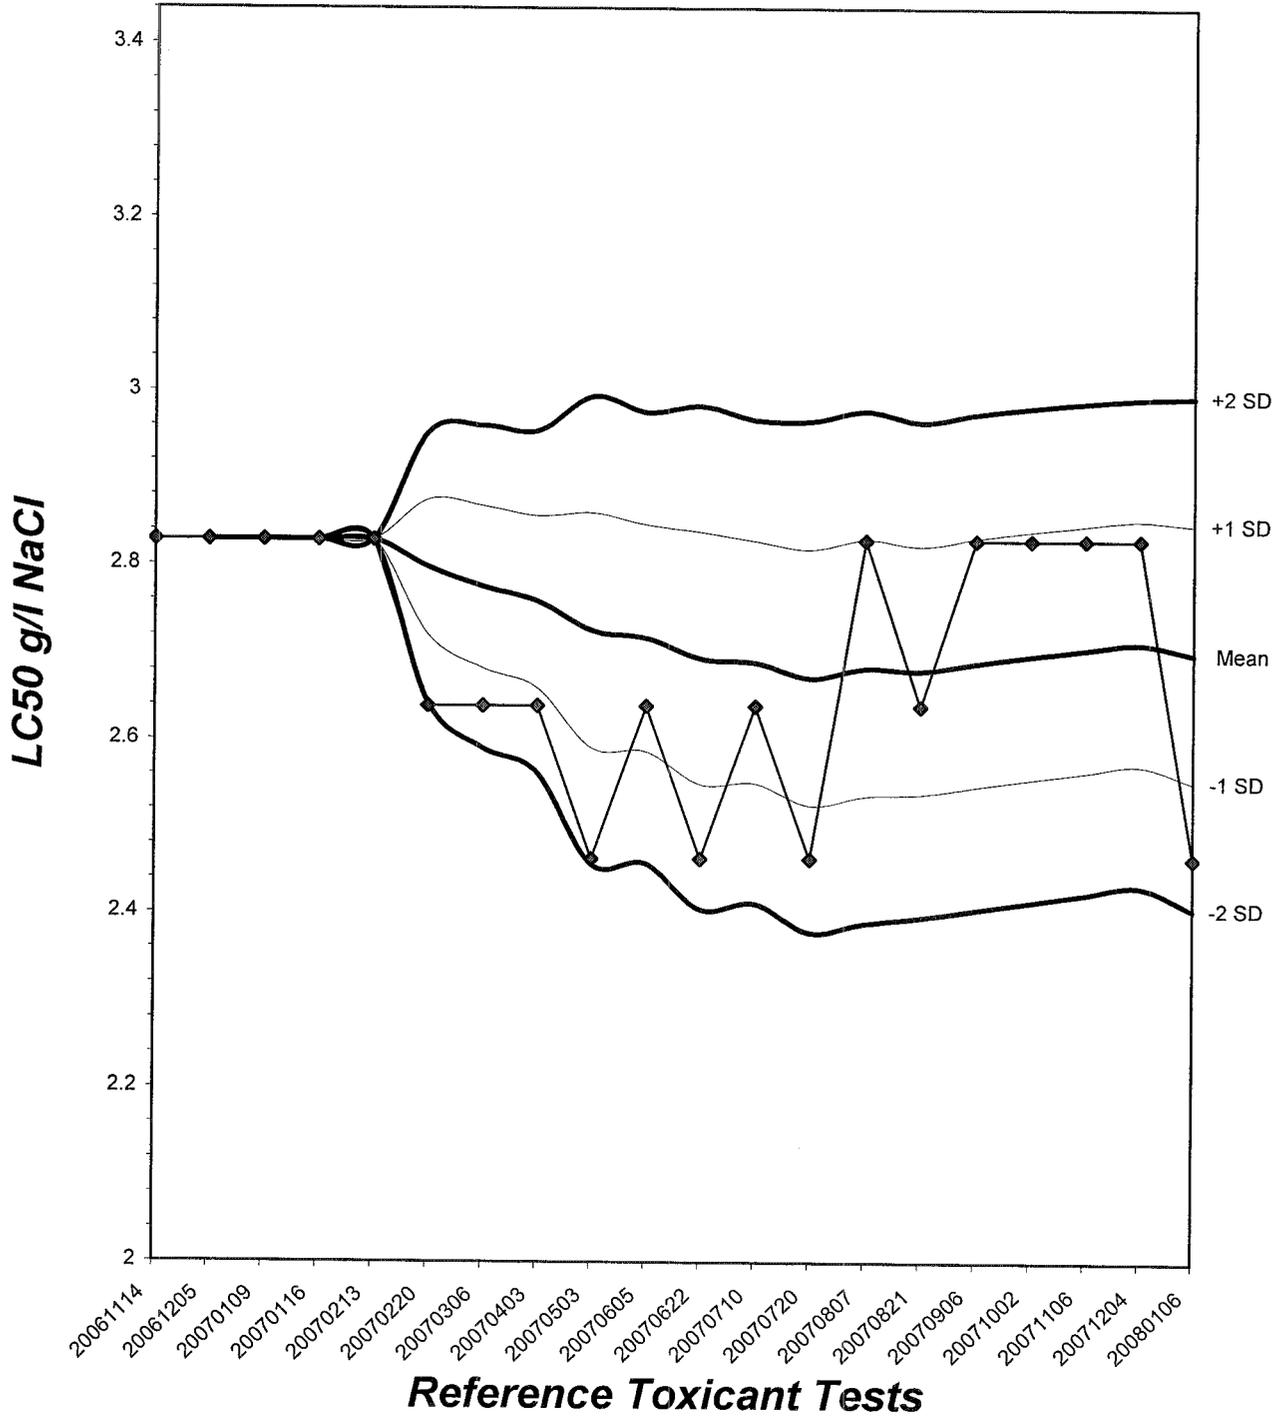

Ceriodaphnia Survival and Reproduction Test-Reproduction


Start Date: 1/6/2008 13:00 Test ID: RT-080106c Sample ID: REF-Ref Toxicant
 End Date: 1/12/2008 13:00 Lab ID: CAATL-Aquatic Testing Labs Sample Type: NACL-Sodium chloride
 Sample Date: 1/6/2008 Protocol: FWCH-EPA-821-R-02-013 Test Species: CD-Ceriodaphnia dubia
 Comments:

Conc-gm/L	1	2	3	4	5	6	7	8	9	10
D-Control	23.000	11.000	21.000	21.000	23.000	20.000	19.000	22.000	20.000	25.000
0.25	12.000	24.000	19.000	22.000	9.000	20.000	21.000	21.000	22.000	25.000
0.5	21.000	19.000	21.000	22.000	16.000	12.000	22.000	21.000	22.000	19.000
1	19.000	9.000	9.000	19.000	14.000	10.000	16.000	17.000	19.000	8.000
2	8.000	2.000	2.000	5.000	4.000	3.000	3.000	5.000	0.000	0.000
4	0.000	0.000	0.000	0.000	0.000	0.000	0.000	0.000	0.000	0.000

Conc-gm/L	Transform: Untransformed							Rank Sum	1-Tailed Critical	Isotonic	
	Mean	N-Mean	Mean	Min	Max	CV%	N			Mean	N-Mean
D-Control	20.500	1.0000	20.500	11.000	25.000	18.432	10			20.500	1.0000
0.25	19.500	0.9512	19.500	9.000	25.000	26.177	10	102.00	76.00	19.500	0.9512
0.5	19.500	0.9512	19.500	12.000	22.000	16.617	10	94.50	76.00	19.500	0.9512
*1	14.000	0.6829	14.000	8.000	19.000	32.819	10	62.50	76.00	14.000	0.6829
*2	3.200	0.1561	3.200	0.000	8.000	76.263	10	55.00	76.00	3.200	0.1561
4	0.000	0.0000	0.000	0.000	0.000	0.000	10			0.000	0.0000


Auxiliary Tests	Statistic	Critical	Skew	Kurt
Shapiro-Wilk's Test indicates non-normal distribution (p <= 0.05)	0.91281	0.947	-0.9793	0.67912
Bartlett's Test indicates equal variances (p = 0.25)	5.39	13.2767		
Hypothesis Test (1-tail, 0.05)	NOEC	LOEC	ChV	TU
Steel's Many-One Rank Test	0.5	1	0.70711	
Treatments vs D-Control				

Linear Interpolation (200 Resamples)					
Point	gm/L	SD	95% CL	Skew	
IC05	0.5023	0.1876	0.0809	0.6178	-0.0659
IC10	0.5955	0.1768	0.1617	0.7497	-0.5184
IC15	0.6886	0.1424	0.2426	0.9253	-0.5389
IC20	0.7818	0.1259	0.4995	1.0352	0.2728
IC25	0.8750	0.1224	0.6413	1.1094	0.3153
IC40	1.1574	0.1139	0.9216	1.3331	-0.0890
IC50	1.3472	0.0972	1.1197	1.4847	-0.4227

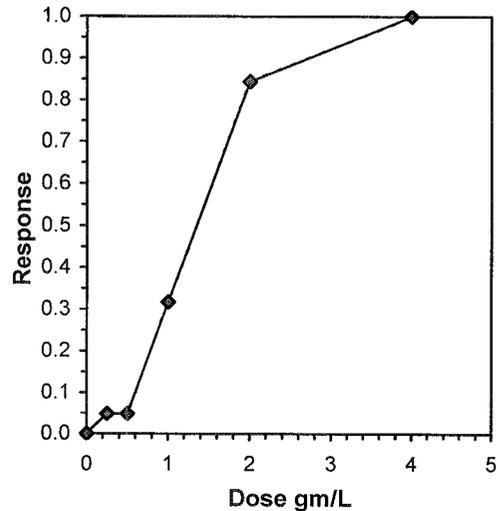

***Ceriodaphnia dubia* Chronic Reproduction Laboratory Control Chart**

CV% = 13.5

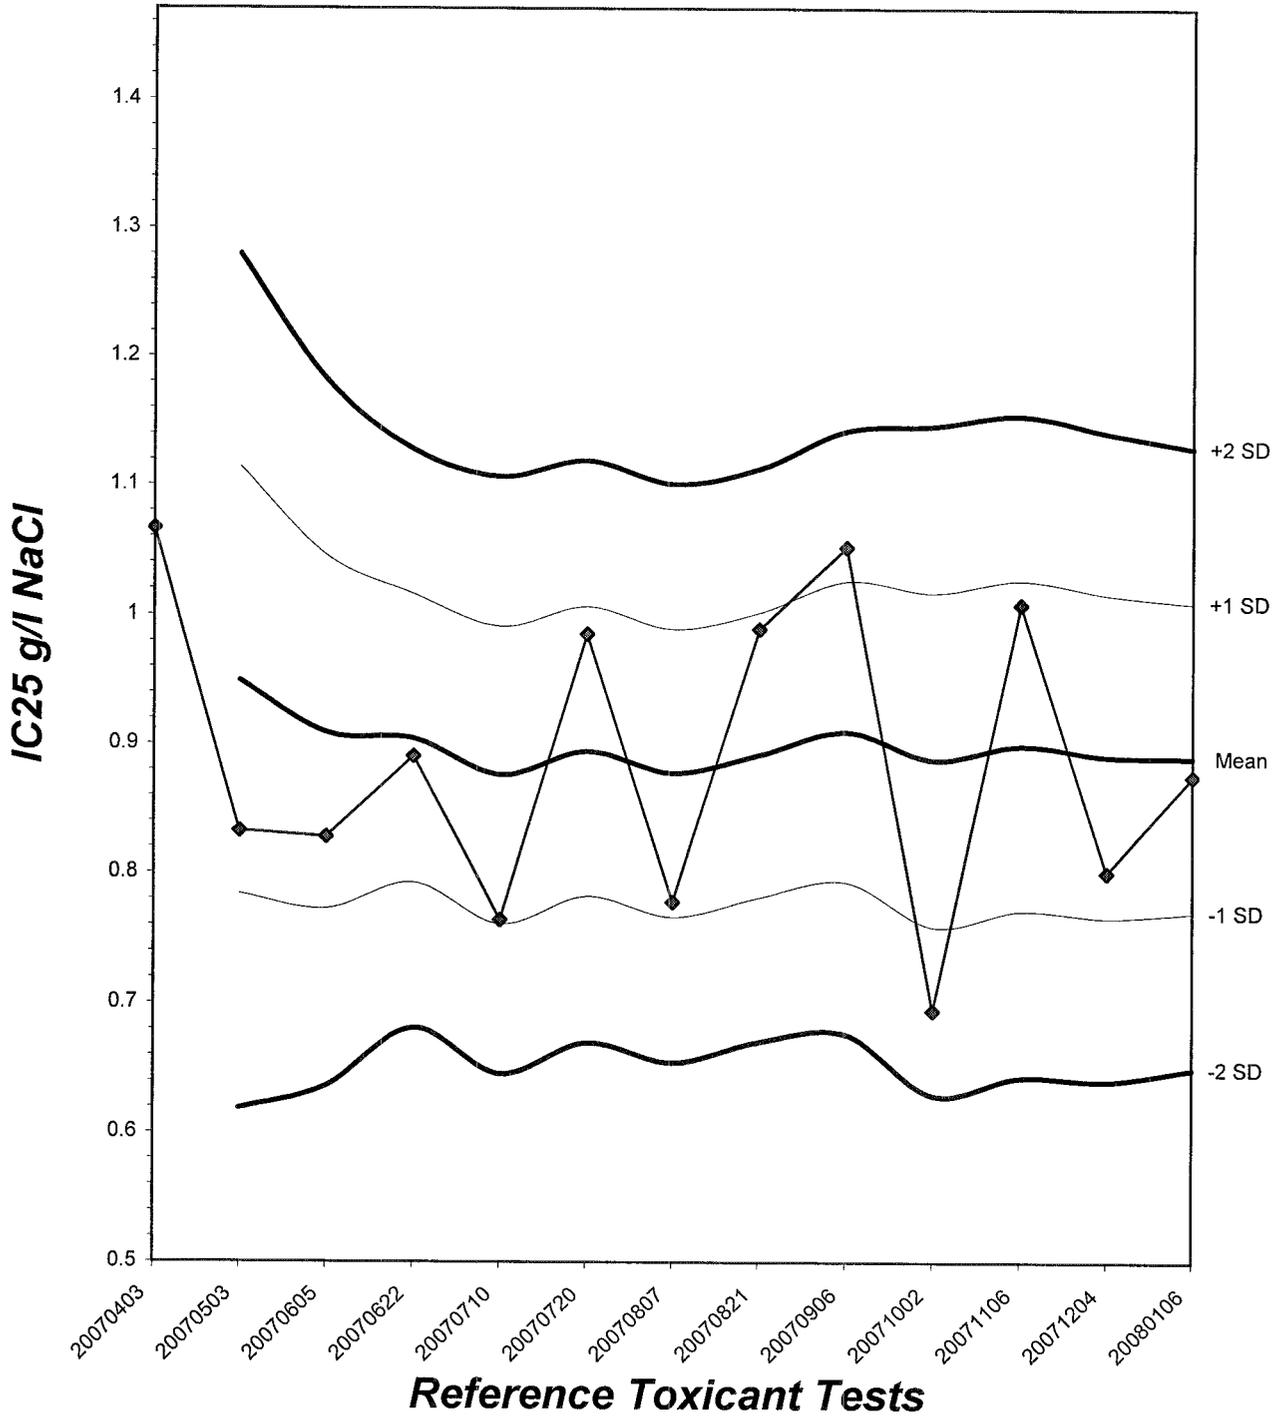

CERIODAPHNIA DUBIA CHRONIC BIOASSAY

Reference Toxicant - NaCl

Reproduction and Survival Raw Data Sheet



QA/QC No.: RT-080106

Start Date: 01/06/2008

Sample	Day	Number of Young Produced										Total Live Young	No. Live Adults	Analyst Initials
		A	B	C	D	E	F	G	H	I	J			
Control	1	0	0	0	0	0	0	0	0	0	0	0	10	h
	2	0	0	0	0	0	0	0	0	0	0	0	10	
	3	0	0	2	0	0	0	3	0	3	0	8	10	
	4	4	3	0	4	3	2	0	2	0	3	21	10	
	5	9	8	7	7	6	7	6	7	6	7	70	10	
	6	10	0	12	10	14	11	10	13	11	15	106	10	
	7	-	-	-	-	-	-	-	-	-	-	-	-	
	Total	23	11	21	21	23	20	19	22	20	25	205	10	
0.25 g/l	1	0	0	0	0	0	0	0	0	0	0	0	10	h
	2	0	0	0	0	0	0	0	0	0	0	0	10	
	3	0	3	0	3	0	2	0	0	3	0	11	10	
	4	4	0	2	0	3	6	4	2	0	3	24	10	
	5	8	8	7	5	6	0	7	6	7	8	62	10	
	6	0	13	10	14	0	12	10	13	12	14	98	10	
	7	-	-	-	-	-	-	-	-	-	-	-	-	
	Total	12	24	19	22	9	20	21	21	22	25	195	10	
0.5 g/l	1	0	0	0	0	0	0	0	0	0	0	0	10	h
	2	0	0	0	0	0	0	0	0	0	0	0	10	
	3	2	0	2	0	0	0	3	2	0	0	9	10	
	4	0	3	0	3	4	3	0	0	3	3	19	10	
	5	9	6	7	7	0	9	8	7	7	6	66	10	
	6	10	10	12	12	12	0	11	12	12	10	101	10	
	7	-	-	-	-	-	-	-	-	-	-	-	-	
	Total	21	19	21	22	16	12	22	21	22	19	195	10	

Circled fourth brood not used in statistical analysis.

7th day only used if <60% of the surviving control females have produced their third brood.

CERIODAPHNIA DUBIA CHRONIC BIOASSAY

Reference Toxicant - NaCl

Reproduction and Survival Raw Data Sheet



QA/QC No.: RT-080106

Start Date: 01/06/2008

Sample	Day	Number of Young Produced										Total Live Young	No. Live Adults	Analyst Initials
		A	B	C	D	E	F	G	H	I	J			
1.0 g/l	1	0	0	0	0	0	0	0	0	0	0	0	10	h
	2	0	0	0	0	0	0	0	0	0	0	0	10	
	3	0	0	0	0	0	3	0	0	2	0	5	10	
	4	3	2	2	3	0	0	3	2	0	2	17	10	
	5	5	7	7	4	5	7	5	4	7	6	57	10	
	6	11	0	0	12	9	0	8	11	10	0	61	10	
	7	-	-	-	-	-	-	-	-	-	-	-	-	
	Total	19	9	9	19	14	10	16	17	19	8	140	10	
2.0 g/l	1	0	0	0	0	0	0	0	X	0	0	9	h	
	2	0	0	0	0	0	0	0	-	0	0	9		
	3	0	0	0	0	0	0	0	-	0	0	9		
	4	2	0	2	3	0	0	0	2	-	0	9		9
	5	3	0	0	2	2	3	3	0	-	0	13		9
	6	3	2	0	0	2	0	0	3	-	X	10		8
	7	-	-	-	-	-	-	-	-	-	-	-		-
	Total	8	2	2	5	4	3	3	5	0	0	32		8
4.0 g/l	1	X	X	X	X	X	X	X	X	X	0	0	h	
	2	-	-	-	-	-	-	-	-	-	-	-		
	3	-	-	-	-	-	-	-	-	-	-	-		
	4	-	-	-	-	-	-	-	-	-	-	-		
	5	-	-	-	-	-	-	-	-	-	-	-		
	6	-	-	-	-	-	-	-	-	-	-	-		
	7	-	-	-	-	-	-	-	-	-	-	-		
	Total	0	0	0	0	0	0	0	0	0	0	0		0

Circled fourth brood not used in statistical analysis.

7th day only used if <60% of the surviving control females have produced their third brood.

CERIODAPHNIA DUBIA CHRONIC BIOASSAY

Reference Toxicant - NaCl Water Chemistries Raw Data Sheet



QA/QC No.: RT-080106

Start Date: 01/06/2008

		DAY 1		DAY 2		DAY 3		DAY 4		DAY 5		DAY 6		DAY 7	
		Initial	Final												
Analyst Initials:		[Signature]		[Signature]		[Signature]		[Signature]		[Signature]		[Signature]		[Signature]	
Time of Readings:		1300	1330	1330	1300	1300	1230	1230	1300	1300	1300	1300	1300	1300	1300
Control	DO	7.6	7.2	7.4	7.7	7.4	7.6	7.4	7.5	8.2	7.8	7.9	7.7	-	-
	pH	7.6	7.4	7.4	7.3	7.3	7.2	7.2	7.7	7.5	7.6	7.9	7.6	-	-
	Temp	24.3	25.1	25.4	24.8	24.1	24.9	24.9	25.1	24.4	25.0	24.6	25.1	-	-
0.25 g/l	DO	7.5	7.3	7.5	7.5	7.5	7.7	7.3	7.4	8.2	7.8	7.9	7.7	-	-
	pH	7.5	7.3	7.4	7.4	7.4	7.2	7.3	7.4	7.6	7.5	7.6	7.7	-	-
	Temp	24.4	25.2	25.3	24.9	24.2	24.9	24.7	25.0	24.4	25.1	24.6	25.1	-	-
0.5 g/l	DO	7.4	7.2	7.4	7.6	7.4	7.5	7.4	7.6	8.5	7.6	8.0	7.8	-	-
	pH	7.5	7.3	7.4	7.4	7.4	7.2	7.3	7.5	7.6	7.5	7.7	7.7	-	-
	Temp	24.3	25.1	25.3	24.9	24.1	25.2	24.6	24.9	24.4	24.9	24.4	24.9	-	-
1.0 g/l	DO	7.5	7.2	7.6	7.7	7.3	7.8	7.4	7.4	8.4	7.8	7.7	7.7	-	-
	pH	7.5	7.3	7.6	7.5	7.4	7.2	7.3	7.5	7.6	7.6	7.4	7.6	-	-
	Temp	24.4	25.2	25.1	24.7	24.2	25.2	24.6	25.0	24.4	24.9	24.6	25.0	-	-
2.0 g/l	DO	7.4	7.4	7.6	7.5	7.4	7.8	7.2	7.6	8.2	7.6	7.6	7.7	-	-
	pH	7.5	7.4	7.6	7.6	7.4	7.3	7.2	7.6	7.5	7.6	7.9	7.6	-	-
	Temp	24.5	25.1	25.0	24.6	24.2	25.3	24.8	25.2	24.4	24.8	24.6	25.1	-	-
4.0 g/l	DO	7.5	7.8	-	-	-	-	-	-	-	-	-	-	-	-
	pH	7.6	7.8	-	-	-	-	-	-	-	-	-	-	-	-
	Temp	24.3	24.6	-	-	-	-	-	-	-	-	-	-	-	-

Dissolved Oxygen (DO) readings are in mg/l O₂; Temperature (Temp) readings are in °C.

Additional Parameters	Control			High Concentration		
	Day 1	Day 3	Day 5	Day 1	Day 3	Day 5
Conductivity (µS)	350	348	305	6400	3100	3210
Alkalinity (mg/l CaCO ₃)	66	65	63	65	66	64
Hardness (mg/l CaCO ₃)	98	97	98	98	97	98

Source of Neonates


Replicate:	A	B	C	D	E	F	G	H	I	J
Brood ID:	2B	1B	3C	2C	2A	3D	3E	2H	3F	2G

Laboratory Temperature Chart

QA/QC Batch No: RT-080106

Date Tested: 01/06/08 to 01/12/08

Acceptable Range: 25 +/- 1°C

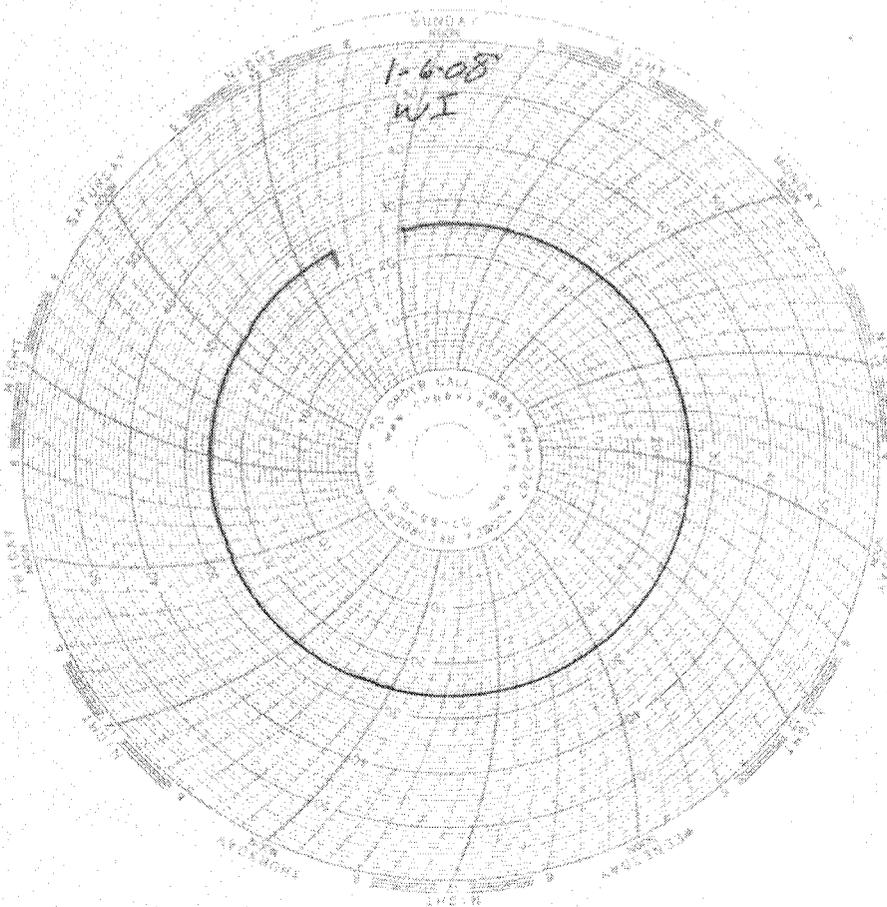



February 27 2008

Mr. Joseph Doak
Test America, Inc.
17461 Derian Avenue, Suite 100
Irvine, CA 92614

Reference: Eberline Services NELAP Cert #01120CA
Test America Project Nos. IRA2496, IRA2497, IRA2499, IRA2500
IRA2506, IRA2565
Eberline Services Reports R801170-8687, R801171-8688, R801172-8689
R801173-8690, R801174-8691, R801175-8692

Dear Mr. Doak:

Enclosed are results from the analyses of six water samples received on January 29, 2008. The samples were analyzed according to the accompanying Test America Subcontract Order Forms, the requested analyses were: gross alpha/gross beta (EPA 900.0), tritium (H-3, EPA906.0), Sr-90 (EPA905.0), Ra-226 (EPA903.1), Ra-228 (EPA 904.0), total uranium (ASTM D-5174), and gamma spectroscopy (EPA901.1, K-40 and Cs-137 only). The parenthetical G after a nuclide indicates that the result was obtained by gamma spectroscopy; a "U" in the results column indicates that the nuclide was not detected greater than the indicated minimum detectable activity (MDA). The samples were not filtered prior to analysis. The samples were analyzed in batches with common QC samples. All samples were batched with QC samples 8687-002, 003, 004, and 005, except for total uranium analysis; the QC samples for total-U analysis are 8682-002, 003, 004, and 005. Batch quality control samples consisted of LCS's, blank analyses, duplicate analyses, and matrix spike analyses (gross alpha/gross beta, H-3, Ra-226, Total-U only). All QC sample results were within the limits defined in Eberline Services Quality Control Procedures Manual.

Please call me if you have any questions concerning this report.

Regards,

Melissa Mannion
Senior Program Manager

MCM/njv

Enclosure: Reports/CoC's

Analytical Services
2030 Wright Avenue
P.O. Box 4040
Richmond, California 94804-0040
(510) 235-2633 Fax (510) 235-0438
Toll Free (800) 841-5487
www.eberlineservices.com

NPDES-718

Eberline Services

ANALYSIS RESULTS

SDG <u>8690</u>	Client <u>TA IRVINE</u>
Work Order <u>R801173-01</u>	Contract <u>PROJECT# IRA2500</u>
Received Date <u>01/29/08</u>	Matrix <u>WATER</u>

<u>Client</u>	<u>Lab</u>	<u>Collected</u>	<u>Analyzed</u>	<u>Nuclide</u>	<u>Results + 2σ</u>	<u>Units</u>	<u>MDA</u>
<u>IRA2500-01</u>	<u>8690-001</u>	<u>01/25/08</u>	<u>02/16/08</u>	GrossAlpha	1.34 ± 0.61	pCi/L	0.60
			<u>02/16/08</u>	Gross Beta	4.34 ± 0.66	pCi/L	0.91
			<u>02/20/08</u>	Ra-228	0.449 ± 0.20	pCi/L	0.48
			<u>02/15/08</u>	K-40 (G)	U	pCi/L	21
			<u>02/15/08</u>	Cs-137 (G)	U	pCi/L	0.81
			<u>02/21/08</u>	H-3	-60.6 ± 92	pCi/L	160
			<u>02/20/08</u>	Ra-226	0.001 ± 0.47	pCi/L	0.90
			<u>02/14/08</u>	Sr-90	0.269 ± 0.28	pCi/L	0.55
			<u>02/19/08</u>	Total U	0.380 ± 0.043	pCi/L	0.022

Certified by <u></u>
Report Date <u>02/27/08</u>
Page 1

SUBCONTRACT ORDER
TestAmerica Irvine
IRA2500

8690

SENDING LABORATORY:

TestAmerica Irvine
 17461 Derian Avenue, Suite 100
 Irvine, CA 92614
 Phone: (949) 261-1022
 Fax: (949) 260-3297
 Project Manager: Joseph Doak

RECEIVING LABORATORY:

Eberline Services - SUB
 2030 Wright Avenue
 Richmond, CA 94804
 Phone : (510) 235-2633
 Fax: (510) 235-0438
 Project Location: California
 Receipt Temperature: 6 °C Ice: (Y) / N

Analysis	Units	Due	Expires	Comments
Sample ID: IRA2500-01	Water	Sampled: 01/25/08 08:25 pH=7.6, temp=47.7		
Gamma Spec-O	mg/kg	02/05/08	01/24/09 08:25	Boeing, permit, J flags, K-40 and CS-137 only
Gross Alpha-O	pCi/L	02/05/08	07/23/08 08:25	Boeing, permit, J flags
Gross Beta-O	pCi/L	02/05/08	07/23/08 08:25	Boeing, permit, J flags
Level 4 Data Package	N/A	02/05/08	02/22/08 08:25	
Radium, Combined-O	pCi/L	02/05/08	01/24/09 08:25	Boeing, permit, J flags
Strontium 90-O	pCi/L	02/05/08	01/24/09 08:25	Boeing, permit, J flags
Tritium-O	pCi/L	02/05/08	01/24/09 08:25	Boeing, permit, J flags
Uranium, Combined-O	pCi/L	02/05/08	01/24/09 08:25	Boeing, permit, J flags
<i>Containers Supplied:</i>				
2.5 gal Poly (J)	500 mL Amber (K)			

J. May Ryan 1/28/08 17:00
 Released By Date/Time

 Released By Date/Time

FedEx 1/28/08 17:00
 Received By Date/Time

MPW 02/29/08 10:15
 Received By Date/Time

JK 12/1/08

Client: TEST AMERICA City: IRVINE State: CA
 Date/Time received: 01/24/08 10:15 CoC No: IRA 2500
 Container ID No: 16 CTEST Requested TAT (Days): _____ P.C. Received Yes: No:

INSPECTION

1 Custody seals on shipping container intact? Yes: No: N/A:
 2 Custody seals on shipping container dated & signed? Yes: No: N/A:
 3 Custody seals on sample containers intact? Yes: No: N/A:
 4 Custody seals on sample containers dated & signed? Yes: No: N/A:
 5 Packing material is _____ Yes: Dry:
 6 Number of samples in shipping container: 1 Sample Matrix: W
 7 Number of containers per sample: 2 (Or see CoC) _____
 8 Samples are in correct container? Yes: No:
 9 Paperwork agrees with samples? Yes: No:
 10 Samples have Tape: Hazard labels: Rad labels: Appropriate sample labels:
 11 Samples are in good condition: Leaking: Broken Containers: Missing:
 12 Samples are Preserved: Not preserved: Preservative: _____
 13 Describe any anomalies: _____

 14 Was F.M. notified of any anomalies? Yes: No: Date: _____
 15 Inspected by: [Signature] Date: 01/24/08 Time: 10:30

Customer Sample No.	Beta/Gamma Coeff	Ion Chamber mR/hr	Wide	Customer Sample No.	Beta/Gamma Coeff	Ion Chamber mR/hr	Wide
IRA 2500-1	460						

Ion Chamber Ser. No: _____ Calibration date: _____
 Alpha Meter Ser. No: _____ Calibration date: _____
 Beta/Gamma Meter Ser. No: 100482 Calibration date: 09 MAY 07

February 11, 2008

Vista Project I.D.: 30210

Mr. Joseph Doak
Test America-Irvine, CA
17461 Derian Avenue
Suite 100
Irvine, CA 92614

Dear Mr. Doak,

Enclosed are the results for the one aqueous sample received at Vista Analytical Laboratory on January 29, 2008 under your Project Name "IRA2500". This sample was extracted and analyzed using EPA Method 1613 for tetra-through-octa chlorinated dioxins and furans. A standard turnaround time was provided for this work.

The following report consists of a Sample Inventory (Section I), Analytical Results (Section II) and the Appendix, which contains the chain-of-custody, a list of data qualifiers and abbreviations, Vista's current certifications, and copies of the raw data (if requested).

Vista Analytical Laboratory is committed to serving you effectively. If you require additional information, please contact me at 916-673-1520 or by email at mmaier@vista-analytical.com. Thank you for choosing Vista as part of your analytical support team.

Sincerely,



Martha M. Maier
Laboratory Director



Vista Analytical Laboratory certifies that the report herein meets all the requirements set forth by NELAC for those applicable test methods. Results relate only to the samples as received by the laboratory. This report should not be reproduced except in full without the written approval of Vista Analytical Laboratory.



Section I: Sample Inventory Report

Date Received: 1/29/2008

Vista Lab. ID

Client Sample ID

30210-001

IRA2500-01

SECTION II

Method Blank					EPA Method 1613				
Matrix:	Aqueous	QC Batch No.:	9921	Lab Sample:	0-MB001	Date Analyzed DB-5:	6-Feb-08	Date Analyzed DB-225:	NA
Sample Size:	1.00 L	Date Extracted:	2-Feb-08						
Analyte	Conc. (ug/L)	DL ^a	EMPC ^b	Qualifiers	Labeled Standard	%R	LCL-UCL ^d	Qualifiers	
2,3,7,8-TCDD	ND	0.00000165			IS 13C-2,3,7,8-TCDD	73.6	25 - 164		
1,2,3,7,8-PeCDD	ND	0.00000120			13C-1,2,3,7,8-PeCDD	76.1	25 - 181		
1,2,3,4,7,8-HxCDD	ND	0.00000316			13C-1,2,3,4,7,8-HxCDD	74.4	32 - 141		
1,2,3,6,7,8-HxCDD	ND	0.00000300			13C-1,2,3,6,7,8-HxCDD	73.5	28 - 130		
1,2,3,7,8,9-HxCDD	ND	0.00000295			13C-1,2,3,4,6,7,8-HpCDD	77.2	23 - 140		
1,2,3,4,6,7,8-HpCDD	ND	0.00000197			13C-OCDD	65.9	17 - 157		
OCDD	ND	0.00000682			13C-2,3,7,8-TCDF	72.7	24 - 169		
2,3,7,8-TCDF	ND	0.000000988			13C-1,2,3,7,8-PeCDF	80.3	24 - 185		
1,2,3,7,8-PeCDF	ND	0.00000123			13C-2,3,4,7,8-PeCDF	66.6	21 - 178		
2,3,4,7,8-PeCDF	ND	0.00000151			13C-1,2,3,4,7,8-HxCDF	95.5	26 - 152		
1,2,3,4,7,8-HxCDF	ND	0.000000596			13C-1,2,3,6,7,8-HxCDF	77.3	26 - 123		
1,2,3,6,7,8-HxCDF	ND	0.000000816			13C-2,3,4,6,7,8-HxCDF	67.6	28 - 136		
2,3,4,6,7,8-HxCDF	ND	0.000000976			13C-1,2,3,7,8,9-HxCDF	76.1	29 - 147		
1,2,3,7,8,9-HxCDF	ND	0.00000111			13C-1,2,3,4,6,7,8-HpCDF	72.0	28 - 143		
1,2,3,4,6,7,8-HpCDF	ND	0.00000146			13C-1,2,3,4,7,8,9-HpCDF	75.2	26 - 138		
1,2,3,4,7,8,9-HpCDF	ND	0.00000154			13C-OCDF	71.7	17 - 157		
OCDF	ND	0.00000455			CRS 37Cl-2,3,7,8-TCDD	77.0	35 - 197		
Totals					Footnotes				
Total TCDD	ND	0.00000165			a. Sample specific estimated detection limit.				
Total PeCDD	ND	0.00000209			b. Estimated maximum possible concentration.				
Total HxCDD	ND	0.00000304			c. Method detection limit.				
Total HpCDD	0.00000138				d. Lower control limit - upper control limit.				
Total TCDF	ND	0.000000988							
Total PeCDF	ND	0.00000136							
Total HxCDF	ND	0.000000843							
Total HpCDF	ND	0.00000150							

Analyst: MAS

Approved By: William J. Luksemburg 09-Feb-2008 13:10

OPR Results				EPA Method 1613			
Matrix:	Aqueous	QC Batch No.:	9921	Lab Sample:	0-OPR001		
Sample Size:	1.00 L	Date Extracted:	2-Feb-08	Date Analyzed DB-5:	6-Feb-08	Date Analyzed DB-225:	NA
Analyte	Spike Conc.	Conc. (ng/mL)	OPR Limits	Labeled Standard	%R	LCL-UCL	Qualifier
2,3,7,8-TCDD	10.0	11.2	6.7 - 15.8	IS 13C-2,3,7,8-TCDD	77.8	25 - 164	
1,2,3,7,8-PeCDD	50.0	55.0	35 - 71	13C-1,2,3,7,8-PeCDD	74.8	25 - 181	
1,2,3,4,7,8-HxCDD	50.0	54.7	35 - 82	13C-1,2,3,4,7,8-HxCDD	74.8	32 - 141	
1,2,3,6,7,8-HxCDD	50.0	54.1	38 - 67	13C-1,2,3,6,7,8-HxCDD	75.4	28 - 130	
1,2,3,7,8,9-HxCDD	50.0	54.8	32 - 81	13C-1,2,3,4,6,7,8-HpCDD	80.9	23 - 140	
1,2,3,4,6,7,8-HpCDD	50.0	54.0	35 - 70	13C-OCDD	71.4	17 - 157	
OCDD	100	113	78 - 144	13C-2,3,7,8-TCDF	77.3	24 - 169	
2,3,7,8-TCDF	10.0	10.7	7.5 - 15.8	13C-1,2,3,7,8-PeCDF	73.3	24 - 185	
1,2,3,7,8-PeCDF	50.0	55.0	40 - 67	13C-2,3,4,7,8-PeCDF	66.3	21 - 178	
2,3,4,7,8-PeCDF	50.0	55.4	34 - 80	13C-1,2,3,4,7,8-HxCDF	90.2	26 - 152	
1,2,3,4,7,8-HxCDF	50.0	54.4	36 - 67	13C-1,2,3,6,7,8-HxCDF	73.1	26 - 123	
1,2,3,6,7,8-HxCDF	50.0	56.0	42 - 65	13C-2,3,4,6,7,8-HxCDF	69.8	28 - 136	
2,3,4,6,7,8-HxCDF	50.0	56.1	35 - 78	13C-1,2,3,7,8,9-HxCDF	74.7	29 - 147	
1,2,3,7,8,9-HxCDF	50.0	55.4	39 - 65	13C-1,2,3,4,6,7,8-HpCDF	71.2	28 - 143	
1,2,3,4,6,7,8-HpCDF	50.0	55.5	41 - 61	13C-1,2,3,4,7,8,9-HpCDF	77.2	26 - 138	
1,2,3,4,7,8,9-HpCDF	50.0	55.7	39 - 69	13C-OCDF	72.9	17 - 157	
OCDF	100	106	63 - 170	CRS 37Cl-2,3,7,8-TCDD	86.5	35 - 197	

Analyst: MAS

Approved By: William J. Luksemburg 08-Feb-2008 12:17

Sample ID: IRA2500-01					EPA Method 1613			
Client Data			Sample Data		Laboratory Data			
Name:	Test America-Irvine, CA		Matrix:	Aqueous	Lab Sample:	30210-001	Date Received:	29-Jan-08
Project:	IRA2500		Sample Size:	1.00 L	QC Batch No.:	9921	Date Extracted:	2-Feb-08
Date Collected:	25-Jan-08				Date Analyzed DB-5:	7-Feb-08	Date Analyzed DB-225:	NA
Time Collected:	0825							
Analyte	Conc. (ug/L)	DL ^a	EMPC ^b	Qualifiers	Labeled Standard	%R	LCL-UCL ^d	Qualifiers
2,3,7,8-TCDD	ND	0.00000105			IS 13C-2,3,7,8-TCDD	79.6	25 - 164	
1,2,3,7,8-PeCDD	ND	0.000000764			13C-1,2,3,7,8-PeCDD	69.2	25 - 181	
1,2,3,4,7,8-HxCDD	ND	0.00000190			13C-1,2,3,4,7,8-HxCDD	67.9	32 - 141	
1,2,3,6,7,8-HxCDD	ND	0.00000191			13C-1,2,3,6,7,8-HxCDD	70.3	28 - 130	
1,2,3,7,8,9-HxCDD	ND	0.00000183			13C-1,2,3,4,6,7,8-HpCDD	71.6	23 - 140	
1,2,3,4,6,7,8-HpCDD	0.00000816			J	13C-OCDD	57.7	17 - 157	
OCDD	0.0000552				13C-2,3,7,8-TCDF	79.1	24 - 169	
2,3,7,8-TCDF	ND	0.000000724			13C-1,2,3,7,8-PeCDF	76.0	24 - 185	
1,2,3,7,8-PeCDF	ND	0.000000757			13C-2,3,4,7,8-PeCDF	64.4	21 - 178	
2,3,4,7,8-PeCDF	ND	0.000000932			13C-1,2,3,4,7,8-HxCDF	72.1	26 - 152	
1,2,3,4,7,8-HxCDF	ND	0.000000686			13C-1,2,3,6,7,8-HxCDF	66.1	26 - 123	
1,2,3,6,7,8-HxCDF	ND	0.000000784			13C-2,3,4,6,7,8-HxCDF	61.3	28 - 136	
2,3,4,6,7,8-HxCDF	ND	0.000000968			13C-1,2,3,7,8,9-HxCDF	65.8	29 - 147	
1,2,3,7,8,9-HxCDF	ND	0.00000120			13C-1,2,3,4,6,7,8-HpCDF	60.1	28 - 143	
1,2,3,4,6,7,8-HpCDF	ND	0.00000174			13C-1,2,3,4,7,8,9-HpCDF	65.3	26 - 138	
1,2,3,4,7,8,9-HpCDF	ND	0.00000179			13C-OCDF	62.2	17 - 157	
OCDF	ND	0.0000101			CRS 37Cl-2,3,7,8-TCDD	88.4	35 - 197	
Totals					Footnotes			
Total TCDD	ND	0.00000105			a. Sample specific estimated detection limit.			
Total PeCDD	ND	0.00000231			b. Estimated maximum possible concentration.			
Total HxCDD	ND	0.00000273			c. Method detection limit.			
Total HpCDD	0.0000173			B	d. Lower control limit - upper control limit.			
Total TCDF	ND	0.000000724						
Total PeCDF	ND	0.000000836						
Total HxCDF	ND	0.000000890						
Total HpCDF	ND	0.00000243						

Analyst:

Approved By: William J. Luksemburg 08-Feb-2008 12:17

APPENDIX

DATA QUALIFIERS & ABBREVIATIONS

B	This compound was also detected in the method blank.
D	Dilution
E	The amount detected is above the High Calibration Limit.
P	The amount reported is the maximum possible concentration due to possible chlorinated diphenylether interference.
H	The signal-to-noise ratio is greater than 10:1.
I	Chemical Interference
J	The amount detected is below the Low Calibration Limit.
*	See Cover Letter
Conc.	Concentration
DL	Sample-specific estimated detection limit
MDL	The minimum concentration of a substance that can be measured and reported with 99% confidence that the analyte concentration is greater than zero in the matrix tested.
EMPC	Estimated Maximum Possible Concentration
NA	Not applicable
RL	Reporting Limit – concentrations that correspond to low calibration point
ND	Not Detected
TEQ	Toxic Equivalency

Unless otherwise noted, solid sample results are reported in dry weight. Tissue samples are reported in wet weight.

CERTIFICATIONS

Accrediting Authority	Certificate Number
State of Alaska, DEC	CA413-02
State of Arizona	AZ0639
State of Arkansas, DEQ	05-013-0
State of Arkansas, DOH	Reciprocity through CA
State of California – NELAP Primary AA	02102CA
State of Colorado	
State of Connecticut	PH-0182
State of Florida, DEP	E87777
Commonwealth of Kentucky	90063
State of Louisiana, Health and Hospitals	LA050001
State of Louisiana, DEQ	01977
State of Maine	CA0413
State of Michigan	81178087
State of Mississippi	Reciprocity through CA
Naval Facilities Engineering Service Center	
State of Nevada	CA413
State of New Jersey	CA003
State of New Mexico	Reciprocity through CA
State of New York, DOH	11411
State of North Carolina	06700
State of North Dakota, DOH	R-078
State of Oklahoma	D9919
State of Oregon	CA200001-002
State of Pennsylvania	68-00490
State of South Carolina	87002001
State of Tennessee	02996
State of Texas	TX247-2005A
U.S. Army Corps of Engineers	
State of Utah	9169330940
Commonwealth of Virginia	00013
State of Washington	C1285
State of Wisconsin	998036160
State of Wyoming	8TMS-Q

SUBCONTRACT ORDER

TestAmerica Irvine

IRA2500

30210 1.8°C

SENDING LABORATORY:

TestAmerica Irvine
17461 Derian Avenue. Suite 100
Irvine, CA 92614
Phone: (949) 261-1022
Fax: (949) 260-3297
Project Manager: Joseph Doak

RECEIVING LABORATORY:

Vista Analytical Laboratory- SUB
1104 Windfield Way
El Dorado Hills, CA 95762
Phone : (916) 673-1520
Fax: (916) 673-0106
Project Location: California
Receipt Temperature: _____ °C Ice: Y / N

Analysis	Units	Due	Expires	Comments
Sample ID: IRA2500-01	Water			Sampled: 01/25/08 08:25 pH=7.6, temp=47.7
1613-Dioxin-HR-Alta	ug/l	02/05/08	02/01/08 08:25	J flags,17 congeners,no TEQ,ug/L,sub=Vista
Level 4 Data Package - Out	N/A	02/05/08	02/22/08 08:25	
<i>Containers Supplied:</i>				
1 L Amber (C)		1 L Amber (D)		

J. Joseph Doak 1/28/08 17:00
Released By Date/Time

FedEx 1/28/08 17:00
Received By Date/Time

Released By Date/Time

Bethina Benedict 1/29/08 1505
Received By Date/Time

SAMPLE LOG-IN CHECKLIST



Vista Project #: 30210

TAT unspecified

Samples Arrival:	Date/Time 1/29/08 0905	Initials: YBSP	Location: WR-2
			Shelf/Rack: N/A
Logged In:	Date/Time 1/29/08 1507	Initials: YBSP	Location: WR-2
			Shelf/Rack: C 2
Delivered By:	<input checked="" type="checkbox"/> FedEx	<input type="checkbox"/> UPS	<input type="checkbox"/> Cal
		<input type="checkbox"/> DHL	<input type="checkbox"/> Hand Delivered
	<input type="checkbox"/> Other		
Preservation:	<input checked="" type="checkbox"/> Ice	<input type="checkbox"/> Blue Ice	<input type="checkbox"/> Dry Ice
	<input type="checkbox"/> None		
Temp °C	1.8°C	Time: 0911	Thermometer ID: IR-1

	YES	NO	NA
Adequate Sample Volume Received?	<input checked="" type="checkbox"/>		
Holding Time Acceptable?	<input checked="" type="checkbox"/>		
Shipping Container(s) Intact?	<input checked="" type="checkbox"/>		
Shipping Custody Seals Intact?	<input checked="" type="checkbox"/>		
Shipping Documentation Present?	<input checked="" type="checkbox"/>		
Airbill	Trk # 7904 34539950	<input checked="" type="checkbox"/>	
Sample Container Intact?	<input checked="" type="checkbox"/>		
Sample Custody Seals Intact?			<input checked="" type="checkbox"/>
Chain of Custody / Sample Documentation Present?	<input checked="" type="checkbox"/>		
COC Anomaly/Sample Acceptance Form completed?		<input checked="" type="checkbox"/>	
If Chlorinated or Drinking Water Samples, Acceptable Preservation?			<input checked="" type="checkbox"/>
Na ₂ S ₂ O ₃ Preservation Documented?	COC	Sample Container	<input checked="" type="checkbox"/> None
Shipping Container	Vista	<input checked="" type="checkbox"/> Client	Retain
		<input checked="" type="checkbox"/> Return	Dispose

Comments:

SUBCONTRACT ORDER

TestAmerica Irvine

IRA2500

8012813


SENDING LABORATORY:



TestAmerica Irvine
17461 Derian Avenue. Suite 100
Irvine, CA 92614
Phone: (949) 261-1022
Fax: (949) 260-3297
Project Manager: Joseph Doak

RECEIVING LABORATORY:

Weck Laboratories, Inc-SUB
14859 E. Clark Avenue
City of Industry, CA 91745
Phone : (626) 336-2139
Fax: (626) 336-2634
Project Location: California
Receipt Temperature: _____ °C Ice: Y / N

Analysis	Units	Due	Expires	Comments
Sample ID: IRA2500-01	Water		Sampled: 01/25/08 08:25	pH=7.6, temp=47.7
Level 4 Data Package - Wec	N/A	02/05/08	02/22/08 08:25	
Mercury - 245.1, Diss -OUT	mg/l	02/05/08	02/22/08 08:25	
Mercury - 245.1-OUT	mg/l	02/05/08	02/22/08 08:25	Boeing, permit, J flags
<i>Containers Supplied:</i>				
125 mL Poly w/HNO3	125 mL Poly (O)			
(N)				


 Released By _____ Date/Time 01/28/08 0700

 Released By _____ Date/Time 01/28/08 0700


 Received By _____ Date/Time TAI 01/28/08 0700

 Received By _____ Date/Time 01/28/08 0700



CERTIFICATE OF ANALYSIS

Client: TestAmerica, Inc. - Irvine
17461 Derian Ave, Suite 100
Irvine, CA 92614
Attention: Joseph Doak

Report Date: 02/04/08 10:39
Received Date: 01/28/08 08:45
Turn Around: 6 days

Phone: (949) 261-1022
Fax: (949) 260-3297

Work Order #: 8012813
Client Project: IRA2500

NELAP #04229CA ELAP#1132 NEVADA #CA211 HAWAII LACSD #10143

The results in this report apply to the samples analyzed in accordance with the Chain of Custody document. Weck Laboratories, Inc. certifies that the test results meet all NELAC requirements unless noted in the case narrative. This analytical report is confidential and is only intended for the use of Weck Laboratories, Inc. and its client. This report contains the Chain of Custody document, which is an integral part of it, and can only be reproduced in full with the authorization of Weck Laboratories, Inc.

Dear Joseph Doak :

Enclosed are the results of analyses for samples received 01/28/08 08:45 with the Chain of Custody document. The samples were received in good condition. The samples were received at 7.9 °C and on ice. All analysis met the method criteria except as noted below or in the report with data qualifiers.

Reviewed by:

Kim G Tu

Project Manager



Page 1 of 6





Weck Laboratories, Inc.
14859 E. Clark Ave.
Industry, CA 91745
Phone 626.336.2139 Fax 626.336.2634


TestAmerica, Inc. - Irvine
17461 Derian Ave, Suite 100
Irvine CA, 92614

Report ID: 8012813
Project ID: IRA2500

Date Received: 01/28/08 08:45
Date Reported: 02/04/08 10:39

ANALYTICAL REPORT FOR SAMPLES

Sample ID	Sampled by:	Sample Comments	Laboratory	Matrix	Date Sampled
IRA2500-01	Client		8012813-01	Water	01/25/08 08:25



Weck Laboratories, Inc.
14859 E. Clark Ave.
Industry, CA 91745
Phone 626.336.2139 Fax 626.336.2634

TestAmerica, Inc. - Irvine
17461 Derian Ave, Suite 100
Irvine CA, 92614

Report ID: 8012813
Project ID: IRA2500

Date Received: 01/28/08 08:45
Date Reported: 02/04/08 10:39

IRA2500-01 8012813-01 (Water)

Date Sampled: 01/25/08 08:25

Metals by EPA 200 Series Methods

Analyte	Result	MDL	Units	Reporting Limit	Dilution Factor	Method	Batch Number	Date Prepared	Date Analyzed	Data Qualifiers
Mercury, Dissolved	ND	0.050	ug/l	0.20	1	EPA 245.1	W8A1076	01/30/08	01/31/08	jlp
Mercury, Total	ND	0.050	ug/l	0.20	1	EPA 245.1	W8A1076	01/30/08	01/31/08	jlp



Weck Laboratories, Inc.
14859 E. Clark Ave.
Industry, CA 91745
Phone 626.336.2139 Fax 626.336.2634

TestAmerica, Inc. - Irvine
17461 Derian Ave, Suite 100
Irvine CA, 92614

Report ID: 8012813
Project ID: IRA2500

Date Received: 01/28/08 08:45
Date Reported: 02/04/08 10:39

QUALITY CONTROL SECTION



Weck Laboratories, Inc.
 14859 E. Clark Ave.
 Industry, CA 91745
 Phone 626.336.2139 Fax 626.336.2634

TestAmerica, Inc. - Irvine
 17461 Derian Ave, Suite 100
 Irvine CA, 92614

Report ID: 8012813
 Project ID: IRA2500

Date Received: 01/28/08 08:45
 Date Reported: 02/04/08 10:39

Metals by EPA 200 Series Methods - Quality Control

%REC

Analyte	Result	Reporting Limit	Units	Spike Level	Source Result	%REC	%REC Limits	RPD	RPD Limit	Data Qualifiers
Batch W8A1076 - EPA 245.1										
Blank (W8A1076-BLK1)										
				Analyzed: 01/31/08						
Mercury, Dissolved	ND	0.20	ug/l							
Mercury, Total	ND	0.20	ug/l							
LCS (W8A1076-BS1)										
				Analyzed: 01/31/08						
Mercury, Dissolved	0.913	0.20	ug/l	1.00		91	85-115			
Mercury, Total	0.913	0.20	ug/l	1.00		91	85-115			
Matrix Spike (W8A1076-MS1)										
				Source: 8012935-01			Analyzed: 01/31/08			
Mercury, Dissolved	0.971	0.20	ug/l	1.00	0.0450	93	70-130			
Mercury, Total	0.971	0.20	ug/l	1.00	0.0450	93	70-130			
Matrix Spike (W8A1076-MS2)										
				Source: 8012939-01			Analyzed: 01/31/08			
Mercury, Dissolved	2.01	0.20	ug/l	1.00	1.18	83	70-130			
Mercury, Total	2.01	0.20	ug/l	1.00	1.18	83	70-130			
Matrix Spike Dup (W8A1076-MSD1)										
				Source: 8012935-01			Analyzed: 01/31/08			
Mercury, Dissolved	0.957	0.20	ug/l	1.00	0.0450	91	70-130	1	20	
Mercury, Total	0.957	0.20	ug/l	1.00	0.0450	91	70-130	1	20	
Matrix Spike Dup (W8A1076-MSD2)										
				Source: 8012939-01			Analyzed: 01/31/08			
Mercury, Dissolved	1.99	0.20	ug/l	1.00	1.18	81	70-130	1	20	
Mercury, Total	1.99	0.20	ug/l	1.00	1.18	81	70-130	1	20	



Weck Laboratories, Inc.
14859 E. Clark Ave.
Industry, CA 91745
Phone 626.336.2139 Fax 626.336.2634

TestAmerica, Inc. - Irvine
17461 Derian Ave, Suite 100
Irvine CA, 92614

Report ID: 8012813
Project ID: IRA2500

Date Received: 01/28/08 08:45
Date Reported: 02/04/08 10:39

Notes and Definitions

ND	NOT DETECTED at or above the Reporting Limit. If J-value reported, then NOT DETECTED at or above the Method Detection Limit (MDL)
dry	Sample results reported on a dry weight basis
RPD	Relative Percent Difference
% Rec	Percent Recovery
Sub	Subcontracted analysis, original report available upon request
MDL	Method Detection Limit
MDA	Minimum Detectable Activity

Any remaining sample(s) will be disposed of one month from the final report date unless other arrangements are made in advance.

An Absence of Total Coliform meets the drinking water standards as established by the California Department of Health Services.

The Reporting Limit (RL) is referenced as the Laboratory's Practical Quantitation Limit (PQL) or the Detection Limit for Reporting Purposes (DLR).

All samples collected by Weck Laboratories have been sampled in accordance to laboratory SOP Number MIS002.

APPENDIX G

Section 15

Outfall 003 – BMP Effectiveness, January 26, 2008

Test America Analytical Laboratory Report

LABORATORY REPORT

Prepared For: MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project: BMP Effectiveness
Monitoring Program

Sampled: 01/26/08
Received: 01/26/08
Issued: 02/06/08 17:08

NELAP #01108CA California ELAP#1197 CSDLAC #10256

The results listed within this Laboratory Report pertain only to the samples tested in the laboratory. The analyses contained in this report were performed in accordance with the applicable certifications as noted. All soil samples are reported on a wet weight basis unless otherwise noted in the report. This Laboratory Report is confidential and is intended for the sole use of TestAmerica and its client. This report shall not be reproduced, except in full, without written permission from TestAmerica. The Chain of Custody, 1 page, is included and is an integral part of this report.

This entire report was reviewed and approved for release.

SAMPLE CROSS REFERENCE

LABORATORY ID

IRA2558-01

CLIENT ID

003 EFF-1

MATRIX

Water

Reviewed By:



TestAmerica Irvine

Joseph Doak
Project Manager

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: BMP Effectiveness
Monitoring Program
Report Number: IRA2558

Sampled: 01/26/08
Received: 01/26/08

INORGANICS

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRA2558-01 (003 EFF-1 - Water)									
Reporting Units: g/cc									
Density	Displacement	8B01112	N/A	NA	0.99	1	02/01/08	02/01/08	
Sample ID: IRA2558-01 (003 EFF-1 - Water)									
Reporting Units: mg/l									
Sediment	ASTM D3977	8B04100	10	10	ND	1	02/04/08	02/04/08	
Total Suspended Solids	EPA 160.2	8A30131	10	10	ND	1	01/30/08	01/30/08	

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRA2558 <Page 2 of 5>
NPDES - 744

MWH-Pasadena/Boeing
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007
 Attention: Bronwyn Kelly

Project ID: BMP Effectiveness
 Monitoring Program
 Report Number: IRA2558

Sampled: 01/26/08
 Received: 01/26/08

METHOD BLANK/QC DATA

INORGANICS

Analyte	Result	Reporting Limit	MDL	Units	Spike Level	Source Result	%REC	%REC Limits	RPD	RPD Limit	Data Qualifiers
<u>Batch: 8A30131 Extracted: 01/30/08</u>											
Blank Analyzed: 01/30/2008 (8A30131-BLK1)											
Total Suspended Solids	ND	10	10	mg/l							
LCS Analyzed: 01/30/2008 (8A30131-BS1)											
Total Suspended Solids	953	10	10	mg/l	1000		95	85-115			
Duplicate Analyzed: 01/30/2008 (8A30131-DUP1)											
Total Suspended Solids	3120	10	10	mg/l		Source: IRA2772-01 3060			2	10	
<u>Batch: 8B01112 Extracted: 02/01/08</u>											
Duplicate Analyzed: 02/01/2008 (8B01112-DUP1)											
Density	0.996	NA	N/A	g/cc		Source: IRA2560-01 0.997			0	20	

TestAmerica Irvine

Joseph Doak
 Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: BMP Effectiveness
Monitoring Program
Report Number: IRA2558

Sampled: 01/26/08
Received: 01/26/08

DATA QUALIFIERS AND DEFINITIONS

ND Analyte NOT DETECTED at or above the reporting limit or MDL, if MDL is specified.
RPD Relative Percent Difference

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRA2558 <Page 4 of 5>
NPDES - 746

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: BMP Effectiveness
Monitoring Program
Report Number: IRA2558

Sampled: 01/26/08
Received: 01/26/08

Certification Summary

TestAmerica Irvine

Method	Matrix	Nelac	California
ASTM D3977	Water		
Displacement	Water		
EPA 160.2	Water	X	X

Nevada and NELAP provide analyte specific accreditations. Analyte specific information for TestAmerica may be obtained by contacting the laboratory or visiting our website at www.testamericainc.com

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

Test America Version 12/20/07
CHAIN OF CUSTODY FORM

IRA 2558
 ANALYSIS REQUIRED

Client Name/Address:
MWH-Arcadia
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007

Project: **Boeing BMP Effectiveness Monitoring Program**

Test America Contact: Joseph Doak
 Project Manager: Bronwyn Kelly
 Sampler: **R O A - 060**
J M A N I S C A L

Phone Number: (626) 568-6691
 Fax Number: (626) 568-6515

Field readings:

Temp = **NA**
 pH = **NA**
 Time of readings = **NA**

Comments

Turn around Time: (check)
 24 Hours _____ 5 Days _____
 48 Hours _____ 10 Days _____
 72 Hours _____ Normal _____
 Sample Integrity: (check)
 Intact On Ice:

7.6/5.6
 CB30

Suspended Sediment Concentration (SSC, ASTM D3977-1997)

Sample Description	Sample Matrix	Container Type	# of Cont.	Sampling Date/Time	Preservative	Bottle #
003 EFF-1	W	500 mL Poly	1	01/26/08- 1033	None	1
003 EFF-2	W	500 mL Poly	1		None	2
003 EFF-3	W	500 mL Poly	1		None	3
003 EFF-4	W	500 mL Poly	1		None	4
003 EFF-5	W	500 mL Poly	1		None	5
003 EFF-6	W	500 mL Poly	1		None	6
003 EFF-7	W	500 mL Poly	1		None	7
003 EFF-8	W	500 mL Poly	1		None	8
003 EFF-9	W	500 mL Poly	1		None	9
003 EFF-10	W	500 mL Poly	1		None	10
003 EFF-11	W	500 mL Poly	1		None	11
003 EFF-12	W	500 mL Poly	1		None	12
003 EFF-13	W	500 mL Poly	1		None	13
003 EFF-14	W	500 mL Poly	1		None	14
003 EFF-15	W	500 mL Poly	1		None	15
003 EFF-16	W	500 mL Poly	1		None	16
003 EFF-17	W	500 mL Poly	1		None	17
003 EFF-18	W	500 mL Poly	1		None	18
003 EFF-19	W	500 mL Poly	1		None	19
003 EFF-20	W	500 mL Poly	1		None	20
003 EFF-21	W	500 mL Poly	1		None	21
003 EFF-22	W	500 mL Poly	1		None	22
003 EFF-23	W	500 mL Poly	1		None	23
003 EFF-24	W	500 mL Poly	1		None	24

EW

Relinquished By: **Kim Bin** Date/Time: **1-26-08 1245**
 Relinquished By: **[Signature]** Date/Time: **1-26-08 1530**
 Relinquished By: **[Signature]** Date/Time: **1-26-08 1530**

Received By: **[Signature]** Date/Time: **1-26-08 1245**
 Received By: **[Signature]** Date/Time: **1-26-08 1530**
 Received By: **[Signature]** Date/Time: **1-26-08 1530**

1-28-08
 CB30

APPENDIX G

Section 16

Outfall 003, February 3, 2008

MEC^X Data Validation Reports



DATA VALIDATION REPORT

Boeing SSFL NPDES

SAMPLE DELIVERY GROUP: IRB0148

Prepared by

MEC^X, LLC
12269 East Vassar Drive
Aurora, CO 80014

I. INTRODUCTION

Task Order Title: Boeing SSFL NPDES
 Contract Task Order: 1261.100D.00
 Sample Delivery Group: IRB0148
 Project Manager: B. Kelly
 Matrix: Water
 QC Level: IV
 No. of Samples: 1
 No. of Reanalyses/Dilutions: 0
 Laboratory: TestAmerica-Irvine

Table 1. Sample Identification

Client ID	Laboratory ID	Sub-Laboratory ID	Matrix	Collected	Method
Outfall 003	IRB0148-01	30226-001, 8020459-01, CRA0034-01, 8696-001	Water	02/03/08 1445	200.7, 200.8, 245.1, 525.2, 624, 900.0, 901.1, 903.0, 904.0, 905.0, 906.0, 1613, ASTM D-5174
Trip Blank	IRB0148-02	N/A	Water	02/03/08	624

II. Sample Management

No anomalies were observed regarding sample management. The samples in this SDG were received at TestAmerica-Irvine above the temperature limits; however, the samples had insufficient time to cool. The samples were received marginally below the temperature limit at Vista and Weck; however, the samples were not noted to be damaged or frozen. The samples were received within the temperature limits at Eberline and TestAmerica-Colton. According to the case narrative for this SDG, the sample was received intact at all laboratories. The FedEx courier did not relinquish custody of the sample to Eberline. The remaining COCs were appropriately signed and dated by field and/or laboratory personnel. As the sample was couriered to TestAmerica-Irvine, and Weck custody seals were not required. Custody seals were intact upon arrival at Eberline and Vista. If necessary, the client ID was added to the sample result summary by the reviewer.

Data Qualifier Reference Table

Qualifier	Organics	Inorganics
U	The analyte was analyzed for, but was not detected above the reported sample quantitation limit. The associated value is the quantitation limit or the estimated detection limit for dioxins.	The material was analyzed for, but was not detected above the level of the associated value. The associated value is either the sample quantitation limit or the sample detection limit. The associated value is the sample detection limit or the quantitation limit for perchlorate only.
J	The analyte was positively identified; the associated numerical value is the approximate concentration of the analyte in the sample.	The associated value is an estimated quantity.
N	The analysis indicates the presence of an analyte for which there is presumptive evidence to make a "tentative identification."	Not applicable.
NJ	The analysis indicates the presence of an analyte that has been "tentatively identified" and the associated numerical value represents its approximate concentration.	Not applicable.
UJ	The analyte was not deemed above the reported sample quantitation limit. However, the reported quantitation limit is approximate and may or may not represent the actual limit of quantitation necessary to accurately and precisely measure the analyte in the sample.	The material was analyzed for, but was not detected. The associated value is an estimate and may be inaccurate or imprecise.
R	The data are unusable. The sample results are rejected due to serious deficiencies in the ability to analyze the sample and to meet quality control criteria. The presence or absence of the analyte cannot be verified.	The data are unusable. The sample results are rejected due to serious deficiencies in the ability to analyze the sample and to meet quality control criteria. The presence or absence of the analyte cannot be verified.

Qualification Code Reference Table

Qualifier	Organics	Inorganics
H	Holding times were exceeded.	Holding times were exceeded.
S	Surrogate recovery was outside QC limits.	The sequence or number of standards used for the calibration was incorrect
C	Calibration %RSD or %D was noncompliant.	Correlation coefficient is <0.995.
R	Calibration RRF was <0.05.	%R for calibration is not within control limits.
B	Presumed contamination as indicated by the preparation (method) blank results.	Presumed contamination as indicated by the preparation (method) or calibration blank results.
L	Laboratory Blank Spike/Blank Spike Duplicate %R was not within control limits.	Laboratory Control Sample %R was not within control limits.
Q	MS/MSD recovery was poor or RPD high.	MS recovery was poor.
E	Not applicable.	Duplicates showed poor agreement.
I	Internal standard performance was unsatisfactory.	ICP ICS results were unsatisfactory.
A	Not applicable.	ICP Serial Dilution %D were not within control limits.
M	Tuning (BFB or DFTPP) was noncompliant.	Not applicable.
T	Presumed contamination as indicated by the trip blank results.	Not applicable.
+	False positive – reported compound was not present.	Not applicable.
-	False negative – compound was present but not reported.	Not applicable.
F	Presumed contamination as indicated by the FB or ER results.	Presumed contamination as indicated by the FB or ER results.
\$	Reported result or other information was incorrect.	Reported result or other information was incorrect.
?	TIC identity or reported retention time has been changed.	Not applicable.

Qualification Code Reference Table Cont.

D	The analysis with this flag should not be used because another more technically sound analysis is available.	The analysis with this flag should not be used because another more technically sound analysis is available.
P	Instrument performance for pesticides was poor.	Post Digestion Spike recovery was not within control limits.
DNQ	The reported result is above the method detection limit but is less than the reporting limit.	The reported result is above the method detection limit but is less than the reporting limit.
*II, *III	Unusual problems found with the data that have been described in Section II, "Sample Management," or Section III, "Method Analyses." The number following the asterisk (*) will indicate the report section where a description of the problem can be found.	Unusual problems found with the data that have been described in Section II, "Sample Management," or Section III, "Method Analyses." The number following the asterisk (*) will indicate the report section where a description of the problem can be found.

III. Method Analyses

A. EPA METHOD 1613—Dioxin/Furans

Reviewed By: K. Shadowlight

Date Reviewed: March 22, 2008

The sample listed in Table 1 for this analysis was validated based on the guidelines outlined in the *MEC^x Data Validation Procedure for Dioxins and Furans (DVP-19, Rev. 0)*, *USEPA Method 1613*, and the *National Functional Guidelines Chlorinated Dioxin/Furan Data Review (8/02)*.

- Holding Times: Extraction and analytical holding times were met. The water sample was extracted and analyzed within one year of collection.
- Instrument Performance: Instrument performance criteria were met. Following are findings associated with instrument performance.
 - GC Column Performance: A Windows Defining Mix (WDM) containing the first and last eluting congeners of each descriptor and isomer specificity compounds was not analyzed prior to the initial calibration sequence or at the beginning of each analytical sequence; however, the first and last eluting congeners and isomer specificity compounds were added to the midpoint of the initial calibration and to the continuing calibration standards. The GC column performance in the calibrations was acceptable, with the height of the valley between the closely eluting isomers and 2,3,7,8-TCDD reported as less than 25%.
 - Mass Spectrometer Performance: The mass spectrometer performance was acceptable with the static resolving power greater than 10,000.
- Calibration: Calibration criteria were met.
 - Initial Calibration: Initial calibration criteria were met. The initial calibration was acceptable with %RSDs $\leq 20\%$ for the 16 native compounds (calibration by isotope dilution) and $\leq 35\%$ for the one native and all labeled compounds (calibration by internal standard). The relative retention times and ion abundance ratios were within the Method 1613 QC limits for all standards.
 - Continuing Calibration: Calibration verification (VER) consisted of a mid-level standard (CS3) analyzed at the beginning of each analytical sequence. The VERs were acceptable with the concentrations within the acceptance criteria listed in Table 6 of EPA Method 1613. The ion abundance ratios and relative retention times were within the method QC limits.
- Blanks: OCDD was reported in the method blank at 0.00000899 μ /L. The detect for OCDD in the sample was less than five times the concentration reported in the method blank; therefore, the OCDD detect was qualified as an estimated nondetect, "UJ," and raised to

the reporting limit in sample Outfall 003. The method blank had no other target compound detects above the EDL.

- Blank Spikes and Laboratory Control Samples: Recoveries were within the acceptance criteria listed in Table 6 of Method 1613.
- Field QC Samples: Field QC samples were evaluated, and if necessary, qualified based on method blanks and other laboratory QC results affecting the usability of the field QC data. Any remaining detects were used to evaluate the associated site samples. Following are findings associated with field QC samples:
 - Field Blanks and Equipment Rinsates: This SDG had no identified field blank or equipment rinsate samples.
 - Field Duplicates: There were no field duplicate samples identified for this SDG.
- Internal Standards Performance: The labeled standard recoveries were within the acceptance criteria listed in Table 7 of Method 1613.
- Compound Identification: Compound identification was verified. The laboratory analyzed for polychlorinated dioxins/furans by EPA Method 1613.
- Compound Quantification and Reported Detection Limits: Compound quantitation was verified by recalculating any sample detects and a representative number of blank spike concentrations. The laboratory calculated and reported compound-specific detection limits. Any detects below the laboratory lower calibration level were qualified as estimated, “J,” and coded with “DNQ,” in order to comply with the NPDES permit. Nondetects are valid to the estimated detection limit (EDL).

B. EPA METHODS 200.7, 200.8, 245.1—Metals and Mercury

Reviewed By: P. Meeks

Date Reviewed: March 26, 2008

The sample listed in Table 1 for this analysis was validated based on the guidelines outlined in the *MEC^X Data Validation Procedure for Metals (DVP-5, Rev. 0 and DVP-21, Rev. 0)*, *EPA Methods 200.7, 200.8, and 245.1*, and the *National Functional Guidelines for Inorganic Data Review (2/94)*.

- Holding Times: The analytical holding times, 6 months for metals and 28 days for mercury, were met.
- Tuning: The mass calibration and resolution checks criteria were met. All tuning solution %RSDs were $\leq 5\%$, and all masses of interest were calibrated to ≤ 0.1 amu and ≤ 0.9 amu at 10% peak height, except for cerium associated with the dissolved metals fraction. The cerium mass calibration marginally exceeded the control limit; therefore, antimony, lead,

and thallium were qualified as estimated in the dissolved metals fraction, "J," for detects and, "UJ," for nondetects.

- Calibration: Calibration criteria were met. Mercury initial calibration r^2 values were ≥ 0.995 and all initial and continuing calibration recoveries were within 90-110% for the ICP-MS metals and 85-115% for mercury. All CRI/CRA and check standard recoveries were within the control limits of 70-130%.
- Blanks: Selenium was reported in the method blank associated with the total metals fraction at $-8.4 \mu\text{g/L}$; therefore, nondetected selenium in the total metals fraction was qualified as an estimated nondetect, "UJ." There were no other applicable detects in the method blanks or CCBs.
- Interference Check Samples: ICSA/B analyses were performed in association with all analyses except total antimony. Recoveries were within the method-established control limits. Most analytes were reported in the ICSA solutions. No 6010 analytes required qualification as the concentrations of the interferents were not significant. For the 6020 analytes, the reviewer was not able to ascertain if the detections were indicative of matrix interference.
- Blank Spikes and Laboratory Control Samples: The recoveries were within laboratory-established QC limits.
- Laboratory Duplicates: No laboratory duplicate analyses were performed.
- Matrix Spike/Matrix Spike Duplicate: No MS/MSD analyses were performed on the sample in this SDG. Evaluation of method accuracy was based on LCS results.
- Serial Dilution: No serial dilution analyses were performed.
- Internal Standards Performance: All sample internal standard intensities were within 30-120% of the internal standard intensities measured in the initial calibration. The bracketing CCV and CCB internal standard intensities were within 80-120% of the internal standard intensities measured in the initial calibration.
- Sample Result Verification: Calculations were verified and the sample results reported on the sample result summary were verified against the raw data. No transcription errors or calculation errors were noted. Detects reported below the reporting limit were qualified as estimated, "J," and coded with "DNQ," in order to comply with the NPDES permit. Reported nondetects are valid to the MDL.

The reviewer noted that nickel was detected at a slightly higher concentration in the dissolved metals sample fraction and that vanadium was detected marginally above the MDL in the dissolved metals fraction but was not detected in the total metals fraction. In both cases the difference between the dissolved and total results was within the sensitivity

limits of the analytical instruments and, therefore, the reviewer considered the total and dissolved results to be equivalent.

- Field QC Samples: Field QC samples were evaluated, and if necessary, qualified based on method blanks and other laboratory QC results affecting the usability of the field QC data. Any remaining detects were used to evaluate the associated site samples. Following are findings associated with field QC samples:
 - Field Blanks and Equipment Rinsates: This SDG had no identified field blank or equipment rinsate samples.
 - Field Duplicates: There were no field duplicate samples identified for this SDG.

C. EPA METHOD 525.2 — Pesticides

Reviewed By: P. Meeks

Date Reviewed: March 27, 2008

The sample listed in Table 1 for this analysis was validated based on the guidelines outlined in the *MEC^X Data Validation Procedure for Organochlorine Pesticides by GC (DVP-4, Rev. 0)*, *EPA Method 525.2*, and the *National Functional Guidelines for Organic Data Review (02/94)*.

- Holding Times: Extraction and analytical holding times were met. The water sample pH was not adjusted within 24 hours; therefore, nondetected diazinon was qualified as an estimated nondetect, "UJ." The sample was analyzed within 30 days of extraction.
- GC/MS Tuning: The DFTPP tunes met the method abundance criteria. The sample was analyzed within 12 hours of the DFTPP injection time.
- Calibration: Calibration criteria were met. For both target compounds, initial calibration average RRFs were ≥ 0.05 and %RSDs $\leq 30\%$. Continuing calibration RRFs were ≥ 0.05 and applicable target compound responses were within the method QC limits of 70-130%.
- Blanks: The method blank had no target compound detects above the MDL.
- Blank Spikes and Laboratory Control Samples: Recoveries and RPDs were within laboratory-established QC limits.
- Surrogate Recovery: Recoveries were within laboratory-established QC limits.
- Matrix Spike/Matrix Spike Duplicate: MS/MSD analyses were not performed on the sample from this SDG. Evaluation of method accuracy and precision was based on the LCS/LCSD results.
- Field QC Samples: Field QC samples were evaluated, and if necessary, qualified based on method blanks and other laboratory QC results affecting the usability of the field QC

data. Any remaining detects were used to evaluate the associated site samples. Following are findings associated with field QC samples:

- Field Blanks and Equipment Rinsates: This SDG had no identified field blank or equipment rinsate samples.
- Field Duplicates: There were no field duplicate samples identified for this SDG.
- Internal Standards Performance: The internal standard area counts and retention times were within the method control limits established by the continuing calibration standards of $\pm 30\%$.
- Compound Identification: Compound identification was verified. The laboratory analyzed for chlorpyrifos and diazinon by Method 525.2. Review of the sample chromatogram, retention times, and spectra indicated no problems with target compound identification.
- Compound Quantification and Reported Detection Limits: Compound quantification was verified. The reporting limits were supported by the low point of the initial calibration and the laboratory MDLs. Reported nondetects are valid to the reporting limit.
- System Performance: Review of the raw data indicated no problems with system performance.

D. VARIOUS EPA METHODS — Radionuclides

Reviewed By: P. Meeks

Date Reviewed: March 28, 2008

The sample listed in Table 1 for this analysis was validated based on the guidelines outlined in the *EPA Methods 900.0, 901.1, 903.1, 904.0, 905.0, and 906.0, ASTM Method D-5174*, and the *National Functional Guidelines for Inorganic Data Review (2/94)*.

- Holding Times: The tritium sample was analyzed within 180 days of collection. Aliquots for gross alpha and gross beta, were prepared within the five-day analytical holding time for unpreserved samples. Aliquots for radium-226, radium-228, strontium-90, total uranium, and gamma spectroscopy were prepared beyond the five-day holding time for unpreserved samples; therefore, results for these analytes were qualified as estimated, "J," for detects and, "UJ," for nondetects.
- Calibration: The laboratory calibration information included the standard certificates and applicable preparation/dilutions logs for NIST-traceability.

The gross alpha detector efficiency was less than 20%; therefore, nondetected gross alpha in the sample was qualified as an estimated nondetect, "UJ." The gross beta detector efficiency was greater than 20%.

The tritium aliquot was spiked for efficiency determination; therefore, no calibration was necessary. The tritium detector efficiency for the sample was at least 20% and was considered acceptable. The strontium chemical yield was at least 70% and was considered acceptable. The strontium continuing calibration results were within the laboratory control limits. The radium-226 continuing calibration results were within the laboratory-established control limits. The radium-228 tracer, yttrium oxalate, yields were greater than 70%. The gamma spectroscopy analytes were determined at the maximum photopeak energy. The kinetic phosphorescence analyzer (KPA) was calibrated immediately prior to the sample analysis. All KPA calibration check standard recoveries were within 90-110% and were deemed acceptable.

- Blanks: There were no analytes detected in the method blanks.
- Blank Spikes and Laboratory Control Samples: The recoveries were within laboratory-established control limits.
- Laboratory Duplicates: No laboratory duplicate analyses were performed on the sample in this SDG.
- Matrix Spike/Matrix Spike Duplicate: No MS/MSD analyses were performed for the sample in this SDG. Method accuracy was evaluated based on the LCS results.
- Sample Result Verification: An EPA Level IV review was performed for the sample in this data package. The sample results and MDAs reported on the sample result form were verified against the raw data and no calculation or transcription errors were noted. Reported nondetects are valid to the MDA.
- Field QC Samples: Field QC samples were evaluated, and if necessary, qualified based on method blanks and other laboratory QC results affecting the usability of the field QC data. Any remaining detects were used to evaluate the associated site samples. Following are findings associated with field QC samples:
 - Field Blanks and Equipment Rinsates: This SDG had no identified field blank or equipment rinsate samples.
 - Field Duplicates: There were no field duplicate samples identified for this SDG.

E. EPA METHOD 624—Volatile Organic Compounds (VOCs)

Reviewed By: L. Calvin

Date Reviewed: April 2, 2008

The samples listed in Table 1 for this analysis were validated based on the guidelines outlined in the *MEC^X Data Validation Procedure for Volatile Organics (DVP-2, Rev. 0)*, *EPA Method 8260B*, and the *National Functional Guidelines for Organic Data Review (2/94)*.

- Holding Times: Analytical holding times were met. The preserved water samples were analyzed within 14 days of collection, and the unpreserved aliquots were analyzed within seven days of collection.
- GC/MS Tuning: The BFB tunes met the method abundance criteria. Samples were analyzed within 12 hours of the BFB injection time.
- Calibration: For applicable target compounds, initial calibration average RRFs were ≥ 0.05 , with the exception of the average RRF for acrolein. Nondetect results for acrolein were rejected, "R," in both samples. Initial calibration %RSDs were $\leq 35\%$. Continuing calibration RRFs were ≥ 0.05 and %Ds $\leq 20\%$, with the exception of %Ds for 1,1,1-trichloroethane, carbon tetrachloride, trichlorofluoromethane, acrolein, and acrylonitrile. As acrolein was previously rejected for the initial calibration average RRF, it was not further qualified for the %D outlier. Nondetect results for the remaining %D outliers were qualified as estimated, "UJ," in site sample Outfall 003. Sample Trip Blanks was identified as field QC and required no qualification for the %D outliers.
- Blanks: The method blank had no target compound detects above the MDL.
- Blank Spikes and Laboratory Control Samples: Recoveries were within laboratory-established QC limits. The reviewer noted that acrolein and acrylonitrile were not included in the LCS,
- Surrogate Recovery: Recoveries were within laboratory-established QC limits.
- Matrix Spike/Matrix Spike Duplicate: MS/MSD analyses were not performed on the site sample in this SDG. Evaluation of method accuracy was based on the LCS results.
- Field QC Samples: Field QC samples were evaluated, and if necessary, qualified based on method blanks and other laboratory QC results affecting the usability of the field QC data. Any remaining detects were used to evaluate the associated site samples. Following are findings associated with field QC samples:
 - Trip Blanks: Sample Trip Blanks was the trip blank associated with site sample Outfall 003. Methylene chloride was detected above the reporting limit in the trip blank at 1.2 $\mu\text{g/L}$. The sample detect above the reporting limit was qualified as an estimated nondetect, "UJ," at the level of contamination in sample Outfall 003. The trip blank had no target other compound detects above the MDL.
 - Field Blanks and Equipment Rinsates: This SDG had no identified field blank or equipment rinsate samples.
 - Field Duplicates: There were no field duplicate samples identified for this SDG.

- Internal Standards Performance: The internal standard area counts and retention times were within the control limits established by the continuing calibration standards: -50%/+100% for internal standard areas and ± 30 seconds for retention times.
- Compound Identification: Compound identification was verified. The laboratory analyzed for volatile target compounds by EPA Method 624. Review of the sample chromatogram, retention times, and spectra indicated no problems with target compound identification.
- Compound Quantification and Reported Detection Limits: Compound quantification was verified. The reporting limits were supported by the low point of the initial calibration and the laboratory MDLs. Reported nondetects are valid to the reporting limit.
- Tentatively Identified Compounds: TICs were not reported by the laboratory for this SDG.
- System Performance: Review of the raw data indicated no problems with system performance.

Sample ID: IRB0148-01		EPA Method 1613						
Client Data		Laboratory Data						
Name: Test America-Irvine, CA	Lab Sample: 30226-001	Date Received: 5-Feb-08						
Project: IRB0148	QC Batch No.: 9953	Date Extracted: 15-Feb-08						
Date Collected: 3-Feb-08	Date Analyzed DB-5: 19-Feb-08	Date Analyzed DB-225: NA						
Time Collected: 1445								
Analyte	Conc. (ug/L)	DL ^a	EMPC ^b	Qualifiers	Labeled Standard	%R	LCL-UCL ^d	Qualifiers
2,3,7,8-TCDD	ND	0.000000433			IS 13C-2,3,7,8-TCDD	87.4	25 - 164	
1,2,3,7,8-PeCDD	ND	0.000000534			13C-1,2,3,7,8-PeCDD	78.0	25 - 181	
1,2,3,4,7,8-HxCDD	ND	0.00000110			13C-1,2,3,4,7,8-HxCDD	82.4	32 - 141	
1,2,3,6,7,8-HxCDD	ND	0.00000112			13C-1,2,3,6,7,8-HxCDD	82.0	28 - 130	
1,2,3,7,8,9-HxCDD	ND	0.00000106			13C-1,2,3,4,6,7,8-HpCDD	85.6	23 - 140	
1,2,3,4,6,7,8-HpCDD	0.00000442			J	13C-OCDD	73.8	17 - 157	
OCDD	0.0000240			J,B	13C-2,3,7,8-TCDF	92.7	24 - 169	
2,3,7,8-TCDF	ND	0.000000522			13C-1,2,3,7,8-PeCDF	76.0	24 - 185	
1,2,3,7,8-PeCDF	ND	0.000000731			13C-2,3,4,7,8-PeCDF	78.7	21 - 178	
2,3,4,7,8-PeCDF	ND	0.000000723			13C-1,2,3,4,7,8-HxCDF	77.3	26 - 152	
1,2,3,4,7,8-HxCDF	ND	0.000000471			13C-1,2,3,6,7,8-HxCDF	77.5	26 - 123	
1,2,3,6,7,8-HxCDF	ND	0.000000493			13C-2,3,4,6,7,8-HxCDF	77.4	28 - 136	
2,3,4,6,7,8-HxCDF	ND	0.000000533			13C-1,2,3,7,8,9-HxCDF	81.2	29 - 147	
1,2,3,7,8,9-HxCDF	ND	0.000000703			13C-1,2,3,4,6,7,8-HpCDF	76.0	28 - 143	
1,2,3,4,6,7,8-HpCDF	ND	0.00000121			13C-1,2,3,4,7,8,9-HpCDF	80.5	26 - 138	
1,2,3,4,7,8,9-HpCDF	ND	0.00000107			13C-OCDF	77.6	17 - 157	
OCDF	ND	0.00000387			CRS 37Cl-2,3,7,8-TCDD	87.2	35 - 197	
Totals								
Total TCDD	ND	0.000000433						
Total PeCDD	ND	0.00000130						
Total HxCDD	ND	0.00000163						
Total HpCDD	0.00000781							
Total TCDF	ND							
Total PeCDF	ND	0.000000727						
Total HxCDF	ND	0.000000545						
Total HpCDF	ND	0.00000202						

Footnotes

a. Sample specific estimated detection limit.

b. Estimated maximum possible concentration.

c. Method detection limit.

d. Lower control limit - upper control limit.

Analyst: MAS *level 17* Approved By: William J. Luksemburg 22-Feb-2008 15:48

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Annual Outfall 003
Report Number: IRB0148

Sampled: 02/03/08
Received: 02/03/08

METALS

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRB0148-01 (Outfall 003 - Water) - cont.									
Reporting Units: mg/l									
Hardness as CaCO3	SM2340B	[CALC]	N/A	0.33	160	1	02/04/08	02/04/08	
Boron	EPA 200.7	8B04079	0.020	0.050	0.12	1	02/04/08	02/04/08	
Calcium	EPA 200.7	8B04079	0.050	0.10	44	1	02/04/08	02/04/08	
Iron	EPA 200.7	8B04079	0.015	0.040	0.081	1	02/04/08	02/04/08	
Magnesium	EPA 200.7	8B04079	0.012	0.020	12	1	02/04/08	02/04/08	

LEVEL IV

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRB0148 <Page 9 of 50>

MWH-Pasadena/Boeing
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007
 Attention: Bronwyn Kelly

Project ID: Annual Outfall 003

Report Number: IRB0148

Sampled: 02/03/08
 Received: 02/03/08

METALS

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRB0148-01 (Outfall 003 - Water) - cont.									
Reporting Units: ug/l									
Aluminum	EPA 200.7	8B04079	40	50	61	1	02/04/08	02/04/08	
Antimony <i>J/DNA</i>	EPA 200.8	8B04080	0.20	2.0	0.42	1	02/04/08	02/05/08	J
Arsenic <i>U</i>	EPA 200.7	8B04079	7.0	10	ND	1	02/04/08	02/04/08	
Beryllium <i>↓</i>	EPA 200.7	8B04079	0.90	2.0	ND	1	02/04/08	02/04/08	
Cadmium <i>J/DNA</i>	EPA 200.8	8B04080	0.11	1.0	0.19	1	02/04/08	02/04/08	J
Chromium <i>↓</i>	EPA 200.7	8B04079	2.0	5.0	2.2	1	02/04/08	02/04/08	J
Copper	EPA 200.8	8B04080	0.75	2.0	3.4	1	02/04/08	02/04/08	
Lead <i>U</i>	EPA 200.8	8B04080	0.30	1.0	ND	1	02/04/08	02/04/08	
Nickel <i>J/DNA</i>	EPA 200.7	8B04079	2.0	10	2.3	1	02/04/08	02/04/08	J
Selenium <i>U/J/B</i>	EPA 200.7	8B04079	8.0	10	ND	1	02/04/08	02/04/08	
Silver <i>U</i>	EPA 200.7	8B04079	6.0	10	ND	1	02/04/08	02/04/08	
Thallium <i>↓</i>	EPA 200.8	8B04080	0.20	1.0	ND	1	02/04/08	02/04/08	
Vanadium <i>↓</i>	EPA 200.7	8B04079	3.0	10	ND	1	02/04/08	02/04/08	
Zinc <i>J/DNA</i>	EPA 200.7	8B04079	6.0	20	14	1	02/04/08	02/04/08	J

LEVEL IV

TestAmerica Irvine

Joseph Doak
 Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRB0148 <Page 10 of 50>

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Annual Outfall 003

Report Number: IRB0148

Sampled: 02/03/08
Received: 02/03/08

DISSOLVED METALS

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRB0148-01 (Outfall 003 - Water) - cont.									
Reporting Units: mg/l									
Boron	EPA 200.7-Diss	8B05111	0.020	0.050	0.11	1	02/05/08	02/06/08	
Calcium	EPA 200.7-Diss	8B05111	0.050	0.10	44	1	02/05/08	02/06/08	
Iron <i>J/DNG</i>	EPA 200.7-Diss	8B05111	0.015	0.040	0.026	1	02/05/08	02/06/08	J
Magnesium	EPA 200.7-Diss	8B05111	0.012	0.020	12	1	02/05/08	02/06/08	
Hardness (as CaCO3)	SM2340B	8B05111	1.0	1.0	160	1	02/05/08	02/06/08	

LEVEL IV

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRB0148 <Page 11 of 50>

MWH-Pasadena/Boeing
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007
 Attention: Bronwyn Kelly

Project ID: Annual Outfall 003

Report Number: IRB0148

Sampled: 02/03/08
 Received: 02/03/08

DISSOLVED METALS

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRB0148-01 (Outfall 003 - Water) - cont.									
Reporting Units: ug/l									
Aluminum	EPA 200.7-Diss	8B05111	40	50	ND	1	02/05/08	02/06/08	
Antimony	EPA 200.8-Diss	8B04144	0.20	2.0	0.33	1	02/04/08	02/05/08	J
Arsenic	EPA 200.7-Diss	8B05111	7.0	10	ND	1	02/05/08	02/06/08	
Beryllium	EPA 200.7-Diss	8B05111	0.90	2.0	ND	1	02/05/08	02/06/08	
Cadmium	EPA 200.8-Diss	8B04144	0.11	1.0	ND	1	02/04/08	02/05/08	
Chromium	EPA 200.7-Diss	8B05111	2.0	5.0	ND	1	02/05/08	02/06/08	
Copper	EPA 200.8-Diss	8B04144	0.75	2.0	2.5	1	02/04/08	02/05/08	
Lead	EPA 200.8-Diss	8B04144	0.30	1.0	ND	1	02/04/08	02/05/08	
Nickel	EPA 200.7-Diss	8B05111	2.0	10	2.4	1	02/05/08	02/06/08	J
Selenium	EPA 200.7-Diss	8B05111	8.0	10	ND	1	02/05/08	02/06/08	
Silver	EPA 200.7-Diss	8B05111	6.0	10	ND	1	02/05/08	02/06/08	
Thallium	EPA 200.8-Diss	8B04144	0.20	1.0	ND	1	02/04/08	02/05/08	
Vanadium	EPA 200.7-Diss	8B05111	3.0	10	3.3	1	02/05/08	02/06/08	J
Zinc	EPA 200.7-Diss	8B05111	6.0	20	11	1	02/05/08	02/06/08	J

pm 3/26/08

LEVEL 1U

TestAmerica Irvine

Joseph Doak
 Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRB0148 <Page 12 of 50>

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Annual Outfall 003

Report Number: IRB0148

Sampled: 02/03/08
Received: 02/03/08

Metals by EPA 200 Series Methods

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRB0148-01 (Outfall 003 - Water) - cont.									
Reporting Units: ug/l									
Mercury, Dissolved	EPA 245.1	W8B0171	0.050	0.20	ND	1	02/06/08	02/07/08	
Mercury, Total	EPA 245.1	W8B0171	0.050	0.20	ND	1	02/06/08	02/07/08	

LEVEL IV

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRB0148 <Page 16 of 50>

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Annual Outfall 003
Report Number: IRB0148

Sampled: 02/03/08
Received: 02/03/08

ORGANIC COMPOUNDS BY GC/MS (EPA 525.2)

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRB0148-01 (Outfall 003 - Water) - cont.									
Reporting Units: ug/l									
Chlorpyrifos	U	EPA 525.2	C8B0516	0.10	1.0	ND	1.01	02/05/08	02/07/08
Diazinon	UJ/4	EPA 525.2	C8B0516	0.24	0.25	ND	1.01	02/05/08	02/07/08
<i>Surrogate: 1,3-Dimethyl-2-nitrobenzene (70-130%)</i>						90 %			
<i>Surrogate: Triphenylphosphate (70-130%)</i>						107 %			
<i>Surrogate: Perylene-d12 (70-130%)</i>						88 %			

LEVEL IV

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRB0148 <Page 15 of 50>

Eberline Services

ANALYSIS RESULTS

SDG <u>8696</u> Work Order <u>R802042-01</u> Received Date <u>02/05/08</u>	Client <u>TA IRVINE</u> Contract <u>PROJECT# IRB0148</u> Matrix <u>WATER</u>
--	--

Client	Lab						
<u>Sample ID</u>	<u>Sample ID</u>	<u>Collected</u>	<u>Analyzed</u>	<u>Nuclide</u>	<u>Results ± 2σ</u>	<u>Units</u>	<u>MDA</u>
IRB0148-01 Outfall 003	8696-001	02/03/08	02/27/08	GrossAlpha	0.628 ± 0.82	pCi/L	1.2
			02/27/08	Gross Beta	6.13 ± 1.0	pCi/L	1.4
			02/27/08	Ra-228	1.36 ± 0.92	pCi/L	0.64
			02/23/08	K-40 (G)	U	pCi/L	54
			02/23/08	Cs-137 (G)	U	pCi/L	2.0
			02/28/08	H-3	31.6 ± 84	pCi/L	150
			03/03/08	Ra-226	0.807 ± 0.54	pCi/L	0.74
			02/18/08	Sr-90	1.50 ± 0.50	pCi/L	0.66
			02/26/08	Total U	1.26 ± 0.14	pCi/L	0.022

UJ/R
 J/H
 UJ/H
 ↓
 U
 J/H
 ↓

LEVEL IV

Certified by <u></u> Report Date <u>03/11/08</u> Page 1

MWH-Pasadena/Boeing
618 Michillinda Avenue, Suite 200
Arcadia, CA 91007
Attention: Bronwyn Kelly

Project ID: Annual Outfall 003

Report Number: IRB0148

Sampled: 02/03/08
Received: 02/03/08

PURGEABLES BY GC/MS (EPA 624)

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRB0148-02 (Trip Blanks - Water)									
Reporting Units: ug/l									
1,1,1-Trichloroethane	EPA 624	8B04007	0.30	0.50	ND	1	02/04/08	02/04/08	
1,1,2,2-Tetrachloroethane	EPA 624	8B04007	0.24	0.50	ND	1	02/04/08	02/04/08	
1,1,2-Trichloroethane	EPA 624	8B04007	0.30	0.50	ND	1	02/04/08	02/04/08	
1,1-Dichloroethane	EPA 624	8B04007	0.27	0.50	ND	1	02/04/08	02/04/08	
1,1-Dichloroethene	EPA 624	8B04007	0.42	0.50	ND	1	02/04/08	02/04/08	
1,2-Dichloroethane	EPA 624	8B04007	0.28	0.50	ND	1	02/04/08	02/04/08	
1,2-Dichlorobenzene	EPA 624	8B04007	0.32	0.50	ND	1	02/04/08	02/04/08	
1,2-Dichloropropane	EPA 624	8B04007	0.35	0.50	ND	1	02/04/08	02/04/08	
1,3-Dichlorobenzene	EPA 624	8B04007	0.35	0.50	ND	1	02/04/08	02/04/08	
1,4-Dichlorobenzene	EPA 624	8B04007	0.37	0.50	ND	1	02/04/08	02/04/08	
Benzene	EPA 624	8B04007	0.28	0.50	ND	1	02/04/08	02/04/08	
Bromodichloromethane	EPA 624	8B04007	0.30	0.50	ND	1	02/04/08	02/04/08	
Bromoform	EPA 624	8B04007	0.40	0.50	ND	1	02/04/08	02/04/08	
Bromomethane	EPA 624	8B04007	0.42	1.0	ND	1	02/04/08	02/04/08	
Carbon tetrachloride	EPA 624	8B04007	0.28	0.50	ND	1	02/04/08	02/04/08	
Chlorobenzene	EPA 624	8B04007	0.36	0.50	ND	1	02/04/08	02/04/08	
Chloroethane	EPA 624	8B04007	0.40	1.0	ND	1	02/04/08	02/04/08	
Chloroform	EPA 624	8B04007	0.33	0.50	ND	1	02/04/08	02/04/08	
Chloromethane	EPA 624	8B04007	0.40	0.50	ND	1	02/04/08	02/04/08	
cis-1,3-Dichloropropene	EPA 624	8B04007	0.22	0.50	ND	1	02/04/08	02/04/08	
Dibromochloromethane	EPA 624	8B04007	0.28	0.50	ND	1	02/04/08	02/04/08	
Ethylbenzene	EPA 624	8B04007	0.25	0.50	ND	1	02/04/08	02/04/08	
Methylene chloride	EPA 624	8B04007	0.95	1.0	1.2	1	02/04/08	02/04/08	
Tetrachloroethene	EPA 624	8B04007	0.32	0.50	ND	1	02/04/08	02/04/08	
Toluene	EPA 624	8B04007	0.36	0.50	ND	1	02/04/08	02/04/08	
trans-1,2-Dichloroethene	EPA 624	8B04007	0.27	0.50	ND	1	02/04/08	02/04/08	
trans-1,3-Dichloropropene	EPA 624	8B04007	0.32	0.50	ND	1	02/04/08	02/04/08	
Trichloroethene	EPA 624	8B04007	0.26	0.50	ND	1	02/04/08	02/04/08	
Trichlorofluoromethane	EPA 624	8B04007	0.34	0.50	ND	1	02/04/08	02/04/08	
Trichlorotrifluoroethane (Freon 113)	EPA 624	8B04007	0.50	5.0	ND	1	02/04/08	02/04/08	
Vinyl chloride	EPA 624	8B04007	0.30	0.50	ND	1	02/04/08	02/04/08	
Xylenes, Total	EPA 624	8B04007	0.90	1.5	ND	1	02/04/08	02/04/08	
Surrogate: Dibromofluoromethane (80-120%)					111 %				
Surrogate: Toluene-d8 (80-120%)					102 %				
Surrogate: 4-Bromofluorobenzene (80-120%)					94 %				

Level IV

TestAmerica Irvine

Joseph Doak
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRB0148 <Page 3 of 50>

MWH-Pasadena/Boeing
 618 Michillinda Avenue, Suite 200
 Arcadia, CA 91007
 Attention: Bronwyn Kelly

Project ID: Annual Outfall 003

Report Number: IRB0148

Sampled: 02/03/08
 Received: 02/03/08

PURGEABLES-- GC/MS (EPA 624)

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IRB0148-01 (Outfall 003 - Water)									
Reporting Units: ug/l									
Acrolein	EPA 624	8B04007	4.0	5.0	ND	1	02/04/08	02/04/08	
Acrylonitrile	EPA 624	8B04007	0.70	2.0	ND	1	02/04/08	02/04/08	
2-Chloroethyl vinyl ether	EPA 624	8B04007	1.8	5.0	ND	1	02/04/08	02/04/08	
Surrogate: Dibromofluoromethane (80-120%)					113 %				
Surrogate: Toluene-d8 (80-120%)					102 %				
Surrogate: 4-Bromofluorobenzene (80-120%)					93 %				
Sample ID: IRB0148-02 (Trip Blanks - Water)									
Reporting Units: ug/l									
Acrolein	EPA 624	8B04007	4.0	5.0	ND	1	02/04/08	02/04/08	
Acrylonitrile	EPA 624	8B04007	0.70	2.0	ND	1	02/04/08	02/04/08	
2-Chloroethyl vinyl ether	EPA 624	8B04007	1.8	5.0	ND	1	02/04/08	02/04/08	
Surrogate: Dibromofluoromethane (80-120%)					111 %				
Surrogate: Toluene-d8 (80-120%)					102 %				
Surrogate: 4-Bromofluorobenzene (80-120%)					94 %				

Level IV

TestAmerica Irvine

Joseph Doak
 Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IRB0148 <Page 4 of 50>